

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022406.D
 Acq On : 30 Sep 2021 02:56
 Operator : SY/MD
 Sample : M3979-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A07

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

Signal : TIC: VV022406.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	95	rVB	111922	115732	11.08%	1.393%
2	1.565	156	163	176	rVB	107746	120890	11.58%	1.455%
3	2.105	321	331	341	rBV	195251	279042	26.72%	3.360%
4	2.368	411	413	415	rBV	410	183	0.02%	0.002%
5	2.606	482	487	490	rBV4	1430	1433	0.14%	0.017%
6	2.728	523	525	528	rBV3	436	299	0.03%	0.004%
7	2.767	528	537	550	rVV3	5308	11483	1.10%	0.138%
8	2.831	553	557	561	rBV4	305	303	0.03%	0.004%
9	2.915	579	583	585	rBV3	390	276	0.03%	0.003%
10	3.027	613	618	621	rBV2	482	393	0.04%	0.005%
11	3.114	642	645	649	rBV3	252	309	0.03%	0.004%
12	3.208	671	674	678	rBV2	231	194	0.02%	0.002%
13	3.323	707	710	712	rBV2	451	244	0.02%	0.003%
14	3.423	739	741	747	rVB2	258	181	0.02%	0.002%
15	3.449	747	749	752	rBV	218	131	0.01%	0.002%
16	3.494	760	763	765	rBV	250	171	0.02%	0.002%
17	3.581	788	790	793	rVV	658	356	0.03%	0.004%
18	3.699	822	827	831	rBV2	193	208	0.02%	0.003%
19	3.738	836	839	844	rVB3	268	200	0.02%	0.002%
20	3.799	855	858	861	rVB	307	174	0.02%	0.002%
21	3.847	871	873	876	rVB	290	149	0.01%	0.002%
22	3.902	877	890	938	rBV2	76679	315614	30.22%	3.800%
23	4.349	1014	1029	1049	rBV	151664	380396	36.42%	4.580%
24	4.622	1111	1114	1115	rBV	473	249	0.02%	0.003%
25	4.687	1132	1134	1136	rVB2	323	134	0.01%	0.002%
26	4.712	1140	1142	1143	rBV2	320	141	0.01%	0.002%
27	4.767	1157	1159	1161	rVB2	348	122	0.01%	0.001%
28	4.812	1167	1173	1177	rBV2	400	423	0.04%	0.005%
29	4.944	1211	1214	1216	rBV2	315	136	0.01%	0.002%
30	5.047	1229	1246	1297	rBV2	375416	984158	94.24%	11.849%
31	5.339	1335	1337	1339	rBV2	508	222	0.02%	0.003%
32	5.481	1378	1381	1385	rVV2	314	274	0.03%	0.003%
33	5.516	1389	1392	1394	rBV	503	345	0.03%	0.004%
34	5.571	1407	1409	1411	rBV	258	159	0.02%	0.002%
35	5.616	1411	1423	1459	rBV	260338	542849	51.98%	6.536%
36	5.915	1504	1516	1529	rBV5	8811	20444	1.96%	0.246%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022406.D
 Acq On : 30 Sep 2021 02:56
 Operator : SY/MD
 Sample : M3979-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A07

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

37	5.995	1539	1541	1543	rBV	311	154	0.01%	0.002%
38	6.069	1549	1564	1601	rBV	213329	452108	43.29%	5.443%
39	6.362	1651	1655	1656	rBV2	421	227	0.02%	0.003%
40	6.410	1667	1670	1671	rBV	284	158	0.02%	0.002%
41	6.452	1679	1683	1686	rVB3	370	255	0.02%	0.003%
42	6.465	1686	1687	1691	rVB2	344	202	0.02%	0.002%
43	6.529	1695	1707	1713	rBV7	1330	2904	0.28%	0.035%
44	6.613	1729	1733	1735	rBV	341	228	0.02%	0.003%
45	6.645	1741	1743	1746	rBV2	434	249	0.02%	0.003%
46	6.719	1763	1766	1769	rBV2	364	211	0.02%	0.003%
47	6.735	1769	1771	1774	rVB2	409	163	0.02%	0.002%
48	6.760	1777	1779	1782	rVB3	509	227	0.02%	0.003%
49	6.915	1825	1827	1830	rBV2	276	160	0.02%	0.002%
50	6.989	1839	1850	1873	rBV	104117	195052	18.68%	2.348%
51	7.317	1940	1952	1972	rBV	426715	762373	73.00%	9.179%
52	7.622	2038	2047	2067	rBV	71235	130946	12.54%	1.577%
53	7.805	2101	2104	2108	rVB3	402	223	0.02%	0.003%
54	7.841	2113	2115	2119	rVB3	414	230	0.02%	0.003%
55	7.976	2144	2157	2183	rBV	610335	1044364	100.00%	12.574%
56	8.092	2183	2193	2235	rVV	273372	511007	48.93%	6.152%
57	8.378	2279	2282	2286	rVB3	841	538	0.05%	0.006%
58	8.403	2286	2290	2294	rBV3	349	307	0.03%	0.004%
59	8.500	2317	2320	2323	rBV3	455	304	0.03%	0.004%
60	8.539	2327	2332	2334	rBV2	471	446	0.04%	0.005%
61	8.612	2354	2355	2360	rVB3	521	320	0.03%	0.004%
62	8.635	2360	2362	2366	rBV2	473	291	0.03%	0.004%
63	8.719	2386	2388	2390	rBV2	267	182	0.02%	0.002%
64	8.764	2399	2402	2405	rBV2	307	199	0.02%	0.002%
65	8.796	2409	2412	2413	rBV	343	161	0.02%	0.002%
66	8.854	2418	2430	2453	rBV	393032	660147	63.21%	7.948%
67	9.281	2560	2563	2565	rBV2	305	172	0.02%	0.002%
68	9.304	2567	2570	2573	rBV2	315	176	0.02%	0.002%
69	9.436	2608	2611	2614	rBV2	370	273	0.03%	0.003%
70	9.493	2626	2629	2633	rBV2	336	256	0.02%	0.003%
71	9.680	2685	2687	2693	rBV2	200	166	0.02%	0.002%
72	9.751	2707	2709	2711	rBV	451	246	0.02%	0.003%
73	10.085	2809	2813	2817	rBV2	242	225	0.02%	0.003%
74	10.124	2822	2825	2827	rBV2	539	376	0.04%	0.005%
75	10.165	2831	2838	2839	rBV2	490	318	0.03%	0.004%
76	10.217	2842	2854	2876	rBV	321608	509055	48.74%	6.129%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022406.D
 Acq On : 30 Sep 2021 02:56
 Operator : SY/MD
 Sample : M3979-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A07

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

77	10.825	3041	3043	3050	rVB	409	339	0.03%	0.004%
78	10.860	3050	3054	3056	rBV2	487	313	0.03%	0.004%
79	10.924	3067	3074	3080	rBV5	946	1393	0.13%	0.017%
80	11.159	3145	3147	3151	rVB	279	180	0.02%	0.002%
81	11.252	3164	3176	3200	rBV	356930	567104	54.30%	6.828%
82	11.419	3225	3228	3230	rBV	460	296	0.03%	0.004%
83	11.571	3271	3275	3278	rBV3	551	352	0.03%	0.004%
84	11.625	3280	3292	3310	rBV	424696	677991	64.92%	8.163%
85	11.866	3365	3367	3370	rBV2	471	293	0.03%	0.004%
86	11.944	3389	3391	3392	rBV	318	121	0.01%	0.001%
87	12.095	3435	3438	3440	rBV	363	196	0.02%	0.002%
88	12.255	3485	3488	3493	rBV2	428	412	0.04%	0.005%
89	12.355	3516	3519	3522	rBV3	501	304	0.03%	0.004%
90	12.368	3522	3523	3529	rVB2	377	212	0.02%	0.003%
91	12.455	3546	3550	3553	rBV3	331	270	0.03%	0.003%
92	12.593	3591	3593	3597	rVB	476	223	0.02%	0.003%
93	13.259	3798	3800	3804	rBV2	348	195	0.02%	0.002%
94	13.333	3821	3823	3824	rBV	352	128	0.01%	0.002%
95	13.384	3836	3839	3842	rVB2	456	258	0.02%	0.003%
96	13.551	3890	3891	3896	rBV3	369	300	0.03%	0.004%
97	13.876	3986	3992	3993	rBV2	482	422	0.04%	0.005%
98	14.030	4038	4040	4042	rBV	496	223	0.02%	0.003%
99	14.358	4139	4142	4150	rVB2	528	586	0.06%	0.007%
100	14.390	4150	4152	4156	rBV2	333	298	0.03%	0.004%




Sum of corrected areas: 8306025

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022406.D
Acq On : 30 Sep 2021 02:56
Operator : SY/MD
Sample : M3979-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
F4A07

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

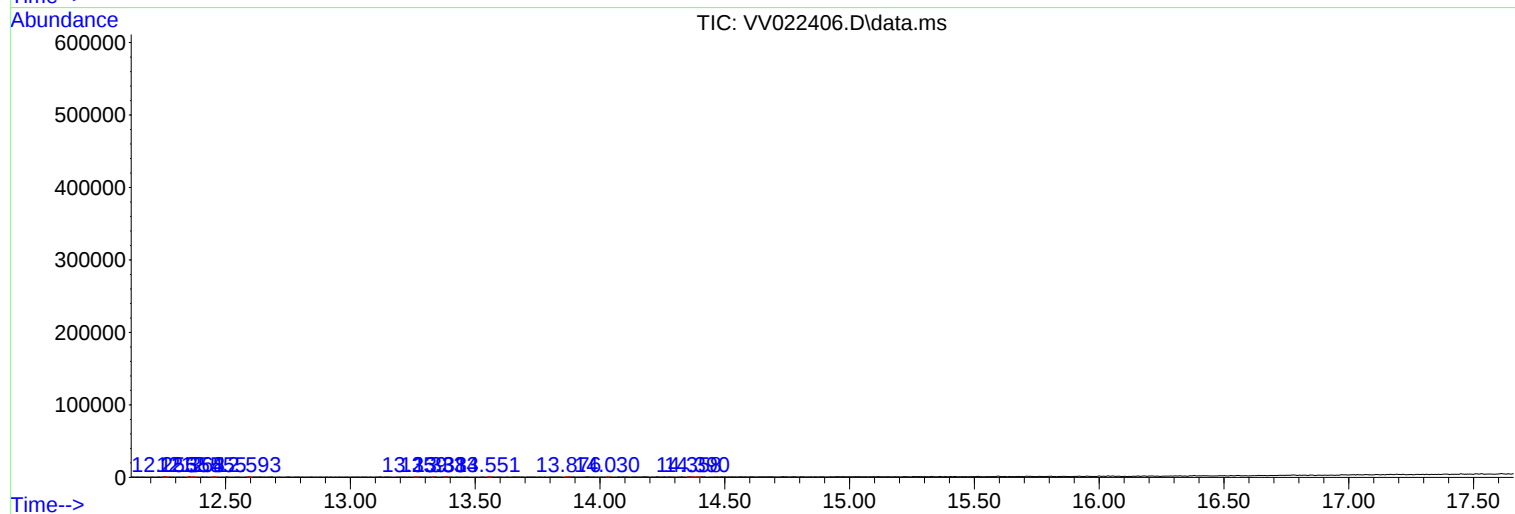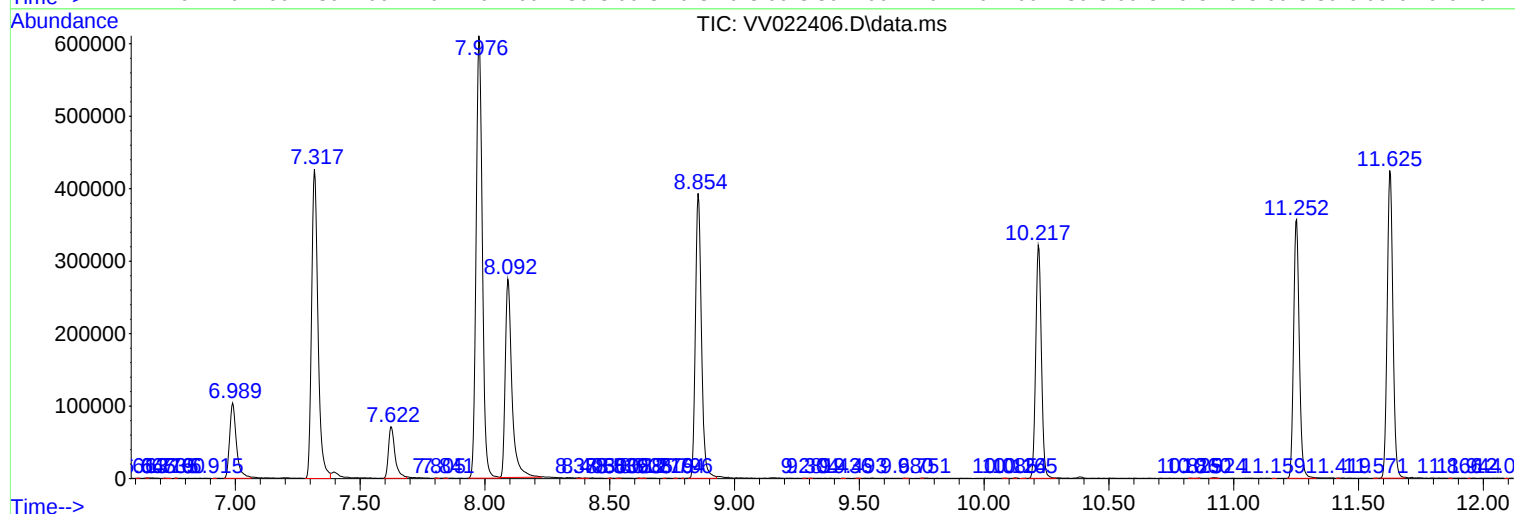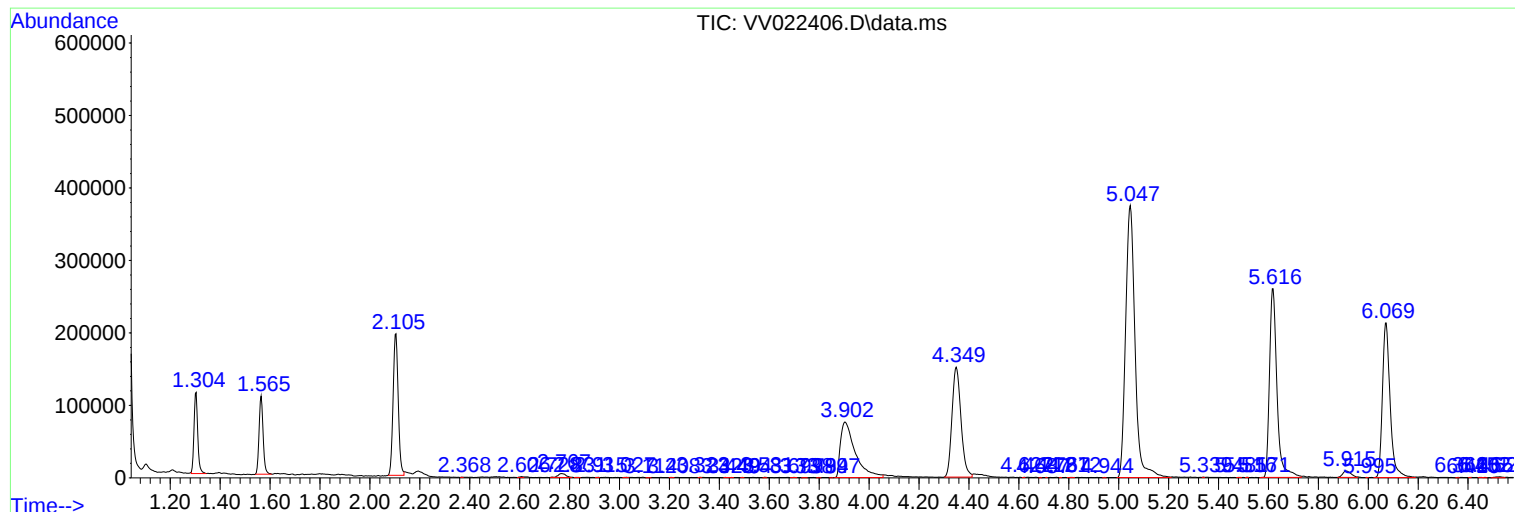

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022406.D
Acq On : 30 Sep 2021 02:56
Operator : SY/MD
Sample : M3979-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A07

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022406.D
Acq On : 30 Sep 2021 02:56
Operator : SY/MD
Sample : M3979-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A07

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
