

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022407.D
 Acq On : 30 Sep 2021 03:20
 Operator : SY/MD
 Sample : M3979-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A08

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

Signal : TIC: VV022407.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	76	81	98	rVB	111922	116352	1.88%	0.853%
2	1.564	156	163	176	rVB	109537	123901	2.01%	0.908%
3	2.101	321	330	345	rBV	199561	289218	4.68%	2.119%
4	2.507	454	456	461	rVB3	937	663	0.01%	0.005%
5	2.606	483	487	488	rBV3	724	510	0.01%	0.004%
6	2.767	531	537	548	rVB6	2988	5257	0.09%	0.039%
7	2.835	555	558	564	rVB2	495	350	0.01%	0.003%
8	2.918	582	584	589	rVB	324	223	0.00%	0.002%
9	2.950	592	594	597	rBV2	388	228	0.00%	0.002%
10	3.079	632	634	636	rVB	718	252	0.00%	0.002%
11	3.101	638	641	643	rBV2	449	220	0.00%	0.002%
12	3.233	679	682	686	rVB2	325	245	0.00%	0.002%
13	3.310	703	706	709	rVB2	439	266	0.00%	0.002%
14	3.452	748	750	753	rVB3	545	257	0.00%	0.002%
15	3.487	753	761	764	rBV2	406	361	0.01%	0.003%
16	3.642	803	809	811	rBV	320	256	0.00%	0.002%
17	3.744	838	841	845	rBV2	243	172	0.00%	0.001%
18	3.806	855	860	863	rBV2	337	288	0.00%	0.002%
19	3.822	863	865	869	rVB	383	199	0.00%	0.001%
20	3.905	878	891	932	rBV2	83737	324100	5.25%	2.375%
21	4.349	1015	1029	1053	rBV	151004	375099	6.07%	2.749%
22	4.635	1113	1118	1119	rBV3	426	280	0.00%	0.002%
23	4.722	1144	1145	1149	rVB2	395	236	0.00%	0.002%
24	4.767	1156	1159	1161	rBV3	425	327	0.01%	0.002%
25	4.809	1168	1172	1174	rBV	424	322	0.01%	0.002%
26	5.047	1227	1246	1267	rBV2	381611	967715	15.67%	7.091%
27	5.294	1321	1323	1328	rBV2	525	304	0.00%	0.002%
28	5.478	1376	1380	1383	rBV3	225	211	0.00%	0.002%
29	5.619	1412	1424	1442	rBV	270042	544867	8.82%	3.993%
30	5.915	1504	1516	1544	rBV5	56944	129942	2.10%	0.952%
31	6.072	1551	1565	1601	rBV	214995	459014	7.43%	3.364%
32	6.320	1641	1642	1647	rVB2	504	243	0.00%	0.002%
33	6.580	1720	1723	1724	rBV	378	201	0.00%	0.001%
34	6.641	1738	1742	1744	rBV	720	539	0.01%	0.004%
35	6.731	1765	1770	1772	rVB3	334	265	0.00%	0.002%
36	6.748	1773	1775	1778	rBV2	286	186	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022407.D
 Acq On : 30 Sep 2021 03:20
 Operator : SY/MD
 Sample : M3979-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A08

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

37	6.793	1787	1789	1793	rBV2	254	204	0.00%	0.001%
38	6.812	1793	1795	1803	rVB2	637	470	0.01%	0.003%
39	6.912	1824	1826	1830	rBV	272	193	0.00%	0.001%
40	6.989	1838	1850	1877	rBV	104426	198426	3.21%	1.454%
41	7.317	1940	1952	1973	rBV	431681	774611	12.54%	5.676%
42	7.625	2037	2048	2067	rBV	73986	133014	2.15%	0.975%
43	7.799	2100	2102	2104	rVB2	478	193	0.00%	0.001%
44	7.815	2104	2107	2110	rBV	540	318	0.01%	0.002%
45	7.976	2143	2157	2183	rVV	3646924	6176481	100.00%	45.260%
46	8.092	2184	2193	2228	rVB	280277	528513	8.56%	3.873%
47	8.420	2291	2295	2298	rBV2	825	601	0.01%	0.004%
48	8.571	2340	2342	2345	rBV3	361	246	0.00%	0.002%
49	8.690	2377	2379	2381	rBV	342	219	0.00%	0.002%
50	8.702	2381	2383	2388	rVV4	375	314	0.01%	0.002%
51	8.854	2418	2430	2458	rBV	409229	686996	11.12%	5.034%
52	9.098	2503	2506	2507	rBV	326	173	0.00%	0.001%
53	9.124	2512	2514	2517	rBV2	367	209	0.00%	0.002%
54	9.413	2601	2604	2607	rVB	446	214	0.00%	0.002%
55	9.432	2607	2610	2614	rBV4	420	382	0.01%	0.003%
56	9.654	2676	2679	2680	rBV2	311	188	0.00%	0.001%
57	9.741	2703	2706	2709	rBV3	274	223	0.00%	0.002%
58	9.796	2719	2723	2728	rVB3	223	221	0.00%	0.002%
59	9.821	2728	2731	2734	rVB3	228	185	0.00%	0.001%
60	9.905	2754	2757	2759	rBV2	440	303	0.00%	0.002%
61	9.918	2759	2761	2764	rVV3	382	249	0.00%	0.002%
62	10.120	2818	2824	2826	rBV4	843	915	0.01%	0.007%
63	10.217	2842	2854	2874	rBV	318367	503024	8.14%	3.686%
64	10.336	2889	2891	2895	rVB3	474	285	0.00%	0.002%
65	10.583	2966	2968	2970	rBV2	431	193	0.00%	0.001%
66	10.599	2970	2973	2975	rBV3	266	189	0.00%	0.001%
67	10.680	2995	2998	3001	rBV2	245	188	0.00%	0.001%
68	10.722	3007	3011	3017	rVB4	250	268	0.00%	0.002%
69	10.911	3065	3070	3071	rBV3	557	451	0.01%	0.003%
70	10.976	3085	3090	3094	rBV2	289	220	0.00%	0.002%
71	11.001	3096	3098	3101	rVV	298	179	0.00%	0.001%
72	11.017	3101	3103	3108	rVB2	235	194	0.00%	0.001%
73	11.095	3123	3127	3130	rBV2	206	183	0.00%	0.001%
74	11.153	3142	3145	3153	rVB3	636	713	0.01%	0.005%
75	11.204	3153	3161	3165	rBV3	508	661	0.01%	0.005%
76	11.252	3165	3176	3200	rBV	373500	591886	9.58%	4.337%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022407.D
 Acq On : 30 Sep 2021 03:20
 Operator : SY/MD
 Sample : M3979-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A08

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

77	11.381	3213	3216	3218	rBV3	456	261	0.00%	0.002%
78	11.429	3229	3231	3232	rBV	509	246	0.00%	0.002%
79	11.625	3280	3292	3313	rBV	445381	695243	11.26%	5.095%
80	11.770	3335	3337	3340	rBV2	399	267	0.00%	0.002%
81	12.021	3413	3415	3419	rVB2	411	230	0.00%	0.002%
82	12.230	3476	3480	3482	rBV	373	238	0.00%	0.002%
83	12.374	3523	3525	3526	rBV	448	172	0.00%	0.001%
84	12.796	3653	3656	3659	rBV2	355	218	0.00%	0.002%
85	12.850	3670	3673	3679	rVB4	388	354	0.01%	0.003%
86	12.882	3680	3683	3686	rBV2	445	272	0.00%	0.002%
87	13.056	3734	3737	3739	rBV	364	216	0.00%	0.002%
88	13.500	3871	3875	3876	rBV	350	212	0.00%	0.002%
89	13.574	3893	3898	3899	rBV	441	291	0.00%	0.002%
90	13.824	3972	3976	3978	rBV2	357	210	0.00%	0.002%
91	13.860	3985	3987	3989	rBV	338	205	0.00%	0.002%
92	13.953	4013	4016	4019	rVB	346	218	0.00%	0.002%
93	13.979	4020	4024	4025	rBV2	364	263	0.00%	0.002%
94	14.252	4105	4109	4112	rBV3	457	439	0.01%	0.003%
95	14.294	4121	4122	4127	rBV2	288	218	0.00%	0.002%
96	14.445	4167	4169	4171	rBV	601	248	0.00%	0.002%
97	14.506	4186	4188	4189	rBV	556	201	0.00%	0.001%
98	14.689	4243	4245	4250	rBV2	292	198	0.00%	0.001%
99	14.821	4284	4286	4291	rBV2	290	261	0.00%	0.002%
100	14.985	4335	4337	4340	rBV3	395	268	0.00%	0.002%



Sum of corrected areas: 13646713

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022407.D
Acq On : 30 Sep 2021 03:20
Operator : SY/MD
Sample : M3979-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A08

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

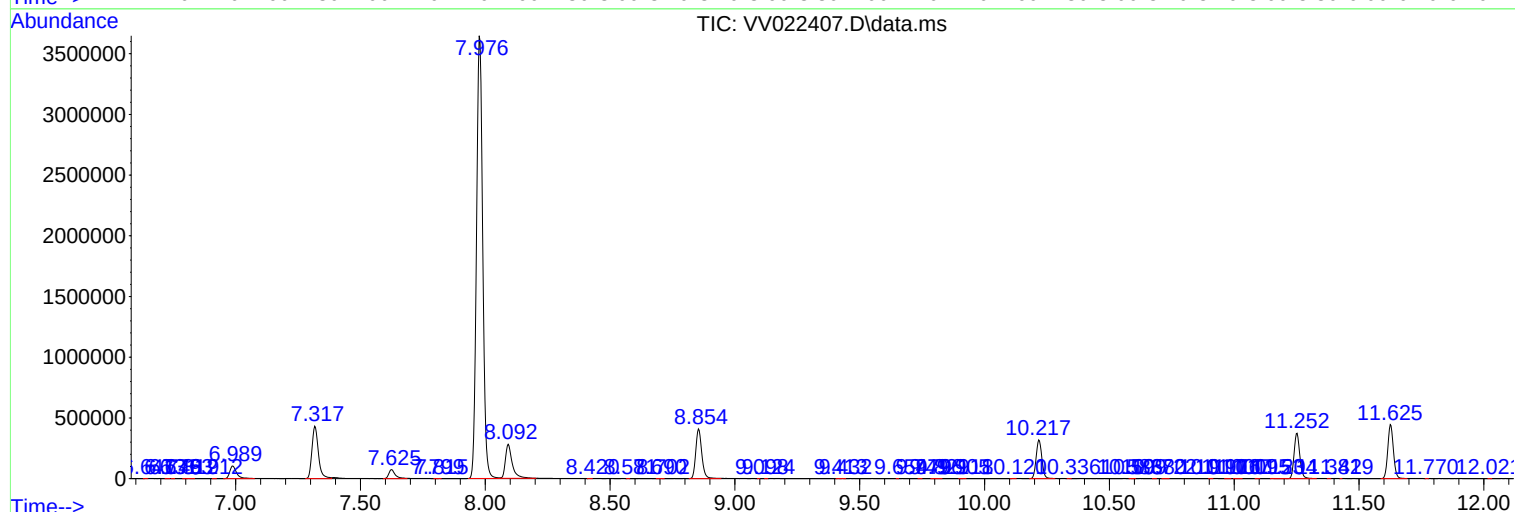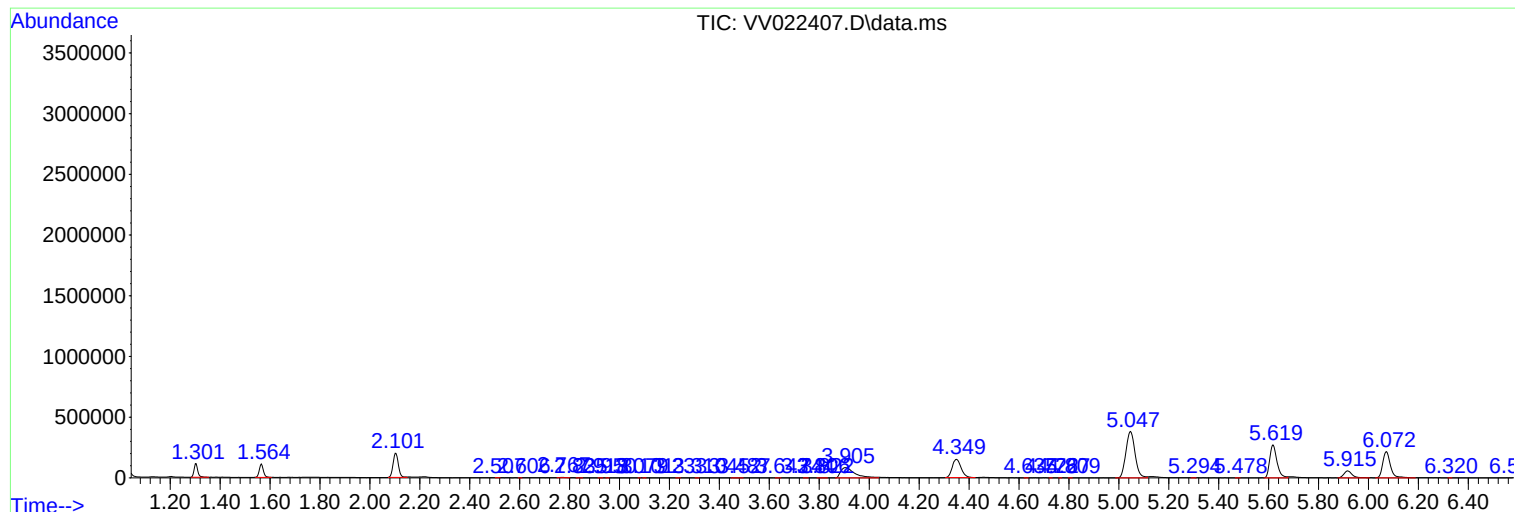

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022407.D
Acq On : 30 Sep 2021 03:20
Operator : SY/MD
Sample : M3979-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A08

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022407.D
Acq On : 30 Sep 2021 03:20
Operator : SY/MD
Sample : M3979-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A08

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------