

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022408.D
 Acq On : 30 Sep 2021 03:45
 Operator : SY/MD
 Sample : M3979-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A09

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

Signal : TIC: VV022408.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	96	rVB	113940	117540	4.28%	1.138%
2	1.564	156	163	178	rVB	109654	122740	4.47%	1.189%
3	2.105	321	331	342	rBV	194421	283131	10.32%	2.742%
4	2.886	572	574	578	rBV2	363	255	0.01%	0.002%
5	2.925	584	586	588	rBV3	417	214	0.01%	0.002%
6	2.989	604	606	608	rBV	341	195	0.01%	0.002%
7	3.076	629	633	638	rBV2	273	287	0.01%	0.003%
8	3.317	705	708	713	rVB3	356	290	0.01%	0.003%
9	3.343	714	716	724	rVB2	395	257	0.01%	0.002%
10	3.400	731	734	739	rBV3	247	193	0.01%	0.002%
11	3.423	739	741	746	rVB2	397	260	0.01%	0.003%
12	3.452	746	750	757	rBV4	650	590	0.02%	0.006%
13	3.642	806	809	813	rBV	351	264	0.01%	0.003%
14	3.732	834	837	842	rVB2	225	219	0.01%	0.002%
15	3.780	846	852	856	rVB2	191	178	0.01%	0.002%
16	3.809	856	861	864	rBV2	279	219	0.01%	0.002%
17	3.908	875	892	924	rBV3	130421	425591	15.51%	4.121%
18	4.349	1013	1029	1050	rBV	150896	381649	13.91%	3.696%
19	4.677	1121	1131	1138	rBV8	1578	3219	0.12%	0.031%
20	4.751	1151	1154	1156	rBB	356	193	0.01%	0.002%
21	4.773	1156	1161	1166	rVB2	425	466	0.02%	0.005%
22	4.802	1166	1170	1173	rBV3	249	200	0.01%	0.002%
23	4.899	1195	1200	1202	rBV2	247	209	0.01%	0.002%
24	4.960	1213	1219	1221	rBV2	420	413	0.02%	0.004%
25	5.047	1229	1246	1265	rBV2	383706	958757	34.95%	9.284%
26	5.304	1324	1326	1330	rVB3	463	261	0.01%	0.003%
27	5.413	1355	1360	1362	rBV3	498	428	0.02%	0.004%
28	5.477	1377	1380	1381	rBV	424	226	0.01%	0.002%
29	5.555	1400	1404	1405	rBV3	297	231	0.01%	0.002%
30	5.619	1411	1424	1441	rBV	265649	538574	19.63%	5.215%
31	5.915	1504	1516	1550	rVB4	78462	174405	6.36%	1.689%
32	6.069	1550	1564	1580	rBV	213966	440370	16.05%	4.264%
33	6.481	1689	1692	1695	rVB3	393	278	0.01%	0.003%
34	6.497	1695	1697	1700	rVB2	284	192	0.01%	0.002%
35	6.519	1700	1704	1709	rBV3	556	535	0.02%	0.005%
36	6.542	1709	1711	1714	rBV2	294	198	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022408.D
 Acq On : 30 Sep 2021 03:45
 Operator : SY/MD
 Sample : M3979-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A09

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

37	6.577	1719	1722	1723	rBV2	717	404	0.01%	0.004%
38	6.709	1761	1763	1768	rVB3	387	278	0.01%	0.003%
39	6.928	1829	1831	1835	rBV	325	199	0.01%	0.002%
40	6.989	1839	1850	1878	rBV	102174	198421	7.23%	1.921%
41	7.140	1895	1897	1898	rBV	540	193	0.01%	0.002%
42	7.317	1939	1952	1970	rBV	432482	771817	28.14%	7.474%
43	7.577	2031	2033	2035	rBV3	394	221	0.01%	0.002%
44	7.622	2038	2047	2069	rBV	71962	132367	4.83%	1.282%
45	7.821	2106	2109	2111	rVV3	285	193	0.01%	0.002%
46	7.847	2114	2117	2119	rVV3	402	288	0.01%	0.003%
47	7.857	2119	2120	2127	rVB4	717	452	0.02%	0.004%
48	7.931	2141	2143	2144	rBV	511	237	0.01%	0.002%
49	7.976	2144	2157	2183	rVV	1585657	2743129	100.00%	26.564%
50	8.092	2184	2193	2227	rVB	273069	509393	18.57%	4.933%
51	8.522	2325	2327	2330	rBV	390	245	0.01%	0.002%
52	8.628	2358	2360	2365	rVB3	518	211	0.01%	0.002%
53	8.654	2365	2368	2371	rBV3	647	347	0.01%	0.003%
54	8.725	2387	2390	2394	rBV3	630	379	0.01%	0.004%
55	8.854	2418	2430	2463	rBV	409561	690125	25.16%	6.683%
56	9.021	2479	2482	2485	rBV4	437	346	0.01%	0.003%
57	9.201	2536	2538	2543	rBV3	333	206	0.01%	0.002%
58	9.336	2577	2580	2582	rBV2	382	239	0.01%	0.002%
59	9.381	2592	2594	2597	rBV2	360	201	0.01%	0.002%
60	9.403	2597	2601	2605	rBV3	520	372	0.01%	0.004%
61	9.477	2620	2624	2626	rBV2	258	184	0.01%	0.002%
62	9.509	2632	2634	2639	rVB2	457	251	0.01%	0.002%
63	9.542	2639	2644	2645	rBV2	396	278	0.01%	0.003%
64	9.776	2714	2717	2721	rBV3	312	221	0.01%	0.002%
65	9.834	2731	2735	2738	rVB3	387	308	0.01%	0.003%
66	10.098	2814	2817	2820	rBV2	228	208	0.01%	0.002%
67	10.127	2820	2826	2828	rBV3	1035	959	0.03%	0.009%
68	10.169	2835	2839	2842	rVB2	251	190	0.01%	0.002%
69	10.217	2843	2854	2875	rVV	318353	502578	18.32%	4.867%
70	10.593	2969	2971	2974	rVB2	412	207	0.01%	0.002%
71	10.654	2988	2990	2993	rBV2	337	193	0.01%	0.002%
72	10.921	3066	3073	3081	rVV3	1696	2232	0.08%	0.022%
73	10.953	3081	3083	3085	rBV	372	192	0.01%	0.002%
74	11.056	3113	3115	3118	rBV2	381	228	0.01%	0.002%
75	11.075	3118	3121	3125	rBV3	292	222	0.01%	0.002%
76	11.201	3153	3160	3163	rBV2	384	482	0.02%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022408.D
 Acq On : 30 Sep 2021 03:45
 Operator : SY/MD
 Sample : M3979-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A09

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

77	11.252	3164	3176	3197	rBV	379166	593935	21.65%	5.752%
78	11.416	3225	3227	3230	rBV3	499	358	0.01%	0.003%
79	11.535	3256	3264	3275	rBV8	2332	4740	0.17%	0.046%
80	11.625	3280	3292	3315	rBV	449107	707981	25.81%	6.856%
81	11.979	3397	3402	3404	rBV3	525	454	0.02%	0.004%
82	12.050	3421	3424	3428	rVB2	318	196	0.01%	0.002%
83	12.085	3430	3435	3437	rBV2	453	322	0.01%	0.003%
84	12.101	3438	3440	3443	rBV	358	185	0.01%	0.002%
85	12.197	3466	3470	3477	rVB3	513	644	0.02%	0.006%
86	12.435	3541	3544	3549	rBV2	286	257	0.01%	0.002%
87	12.686	3613	3622	3627	rBV5	838	1433	0.05%	0.014%
88	12.718	3630	3632	3635	rBV	365	278	0.01%	0.003%
89	12.796	3652	3656	3662	rBV2	358	389	0.01%	0.004%
90	13.062	3737	3739	3745	rBV2	249	198	0.01%	0.002%
91	13.197	3779	3781	3784	rBV2	329	227	0.01%	0.002%
92	13.509	3875	3878	3881	rBV	263	218	0.01%	0.002%
93	13.783	3959	3963	3966	rBV3	511	421	0.02%	0.004%
94	14.114	4062	4066	4070	rBV2	378	342	0.01%	0.003%
95	14.271	4113	4115	4119	rBV2	288	179	0.01%	0.002%
96	14.419	4159	4161	4166	rVB3	509	348	0.01%	0.003%
97	14.522	4191	4193	4195	rBV	326	188	0.01%	0.002%
98	14.802	4277	4280	4285	rBV3	398	416	0.02%	0.004%
99	14.930	4318	4320	4322	rBV2	539	180	0.01%	0.002%
100	15.310	4436	4438	4440	rBV	485	219	0.01%	0.002%



Sum of corrected areas: 10326531

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022408.D
Acq On : 30 Sep 2021 03:45
Operator : SY/MD
Sample : M3979-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A09

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

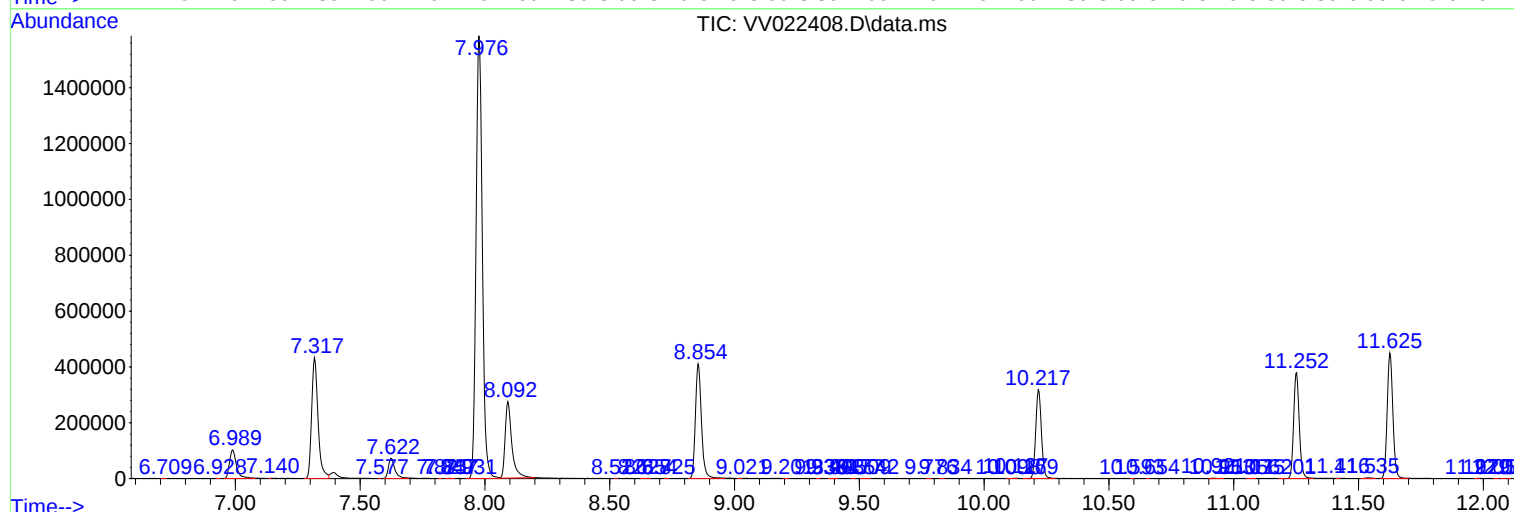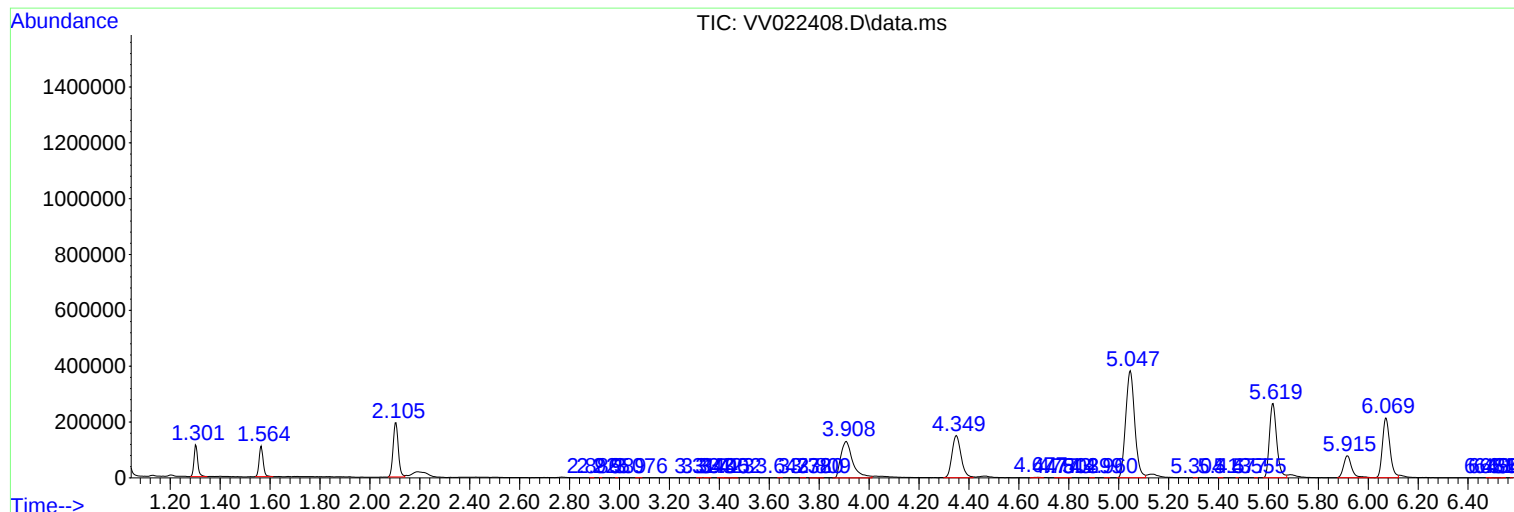

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022408.D
Acq On : 30 Sep 2021 03:45
Operator : SY/MD
Sample : M3979-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A09

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022408.D
Acq On : 30 Sep 2021 03:45
Operator : SY/MD
Sample : M3979-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A09

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
