

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022409.D
 Acq On : 30 Sep 2021 04:09
 Operator : SY/MD
 Sample : M3979-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A10

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M

Title : VOC Analysis

Signal : TIC: VV022409.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	97	rVB	109463	114888	7.17%	1.322%
2	1.565	156	163	175	rBV	104854	117808	7.36%	1.356%
3	2.102	321	330	345	rBV	193159	279143	17.43%	3.213%
4	2.343	403	405	408	rBV2	777	373	0.02%	0.004%
5	2.548	466	469	472	rBV2	416	339	0.02%	0.004%
6	2.651	498	501	503	rBV2	347	178	0.01%	0.002%
7	2.716	516	521	523	rBV2	503	461	0.03%	0.005%
8	2.806	544	549	554	rBV4	405	433	0.03%	0.005%
9	2.831	554	557	561	rBV2	379	259	0.02%	0.003%
10	3.002	606	610	614	rBV2	347	262	0.02%	0.003%
11	3.108	641	643	647	rVB4	485	200	0.01%	0.002%
12	3.259	687	690	696	rVB2	380	273	0.02%	0.003%
13	3.519	768	771	776	rBV3	270	218	0.01%	0.003%
14	3.558	779	783	784	rBV2	350	210	0.01%	0.002%
15	3.568	784	786	789	rVB	410	220	0.01%	0.003%
16	3.793	852	856	858	rBV	339	178	0.01%	0.002%
17	3.902	879	890	926	rBV	71958	262272	16.38%	3.018%
18	4.349	1013	1029	1050	rBV	146660	371206	23.18%	4.272%
19	4.687	1131	1134	1139	rBV3	466	405	0.03%	0.005%
20	4.751	1151	1154	1156	rVB	504	245	0.02%	0.003%
21	4.838	1178	1181	1182	rBV2	340	190	0.01%	0.002%
22	5.047	1224	1246	1266	rBV2	375021	940149	58.71%	10.820%
23	5.326	1329	1333	1335	rBV2	364	286	0.02%	0.003%
24	5.407	1355	1358	1360	rVV2	420	180	0.01%	0.002%
25	5.439	1365	1368	1371	rBV	349	206	0.01%	0.002%
26	5.468	1375	1377	1381	rBV2	439	318	0.02%	0.004%
27	5.558	1403	1405	1408	rBV	353	181	0.01%	0.002%
28	5.619	1411	1424	1440	rBV	258618	523194	32.67%	6.021%
29	5.841	1491	1493	1500	rVB4	376	263	0.02%	0.003%
30	5.912	1505	1515	1533	rVB8	9852	23397	1.46%	0.269%
31	5.982	1535	1537	1539	rVB8	706	274	0.02%	0.003%
32	6.005	1539	1544	1549	rVB3	555	352	0.02%	0.004%
33	6.069	1549	1564	1598	rBV	209672	448897	28.03%	5.166%
34	6.449	1676	1682	1684	rBV2	204	191	0.01%	0.002%
35	6.519	1695	1704	1706	rBV3	1288	1505	0.09%	0.017%
36	6.648	1741	1744	1745	rVV2	393	209	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022409.D
 Acq On : 30 Sep 2021 04:09
 Operator : SY/MD
 Sample : M3979-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A10

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

37	6.670	1749	1751	1755	rVV5	442	301	0.02%	0.003%
38	6.703	1759	1761	1766	rBV2	360	312	0.02%	0.004%
39	6.841	1800	1804	1807	rBV	260	224	0.01%	0.003%
40	6.886	1817	1818	1822	rVB	389	184	0.01%	0.002%
41	6.989	1836	1850	1882	rBV	100810	196022	12.24%	2.256%
42	7.166	1902	1905	1907	rBV2	278	202	0.01%	0.002%
43	7.269	1935	1937	1940	rBV2	365	225	0.01%	0.003%
44	7.317	1940	1952	1972	rBV	416535	752763	47.01%	8.663%
45	7.622	2038	2047	2068	rBV2	70310	126813	7.92%	1.459%
46	7.889	2128	2130	2135	rVB2	320	218	0.01%	0.003%
47	7.918	2135	2139	2141	rBV3	263	248	0.02%	0.003%
48	7.976	2144	2157	2183	rBV	922375	1601349	100.00%	18.429%
49	8.092	2184	2193	2220	rBV	266743	490134	30.61%	5.641%
50	8.400	2287	2289	2291	rBV2	357	186	0.01%	0.002%
51	8.429	2295	2298	2299	rBV	373	223	0.01%	0.003%
52	8.606	2349	2353	2355	rBV3	556	344	0.02%	0.004%
53	8.677	2372	2375	2376	rBV3	410	209	0.01%	0.002%
54	8.776	2402	2406	2408	rBV2	405	384	0.02%	0.004%
55	8.854	2417	2430	2458	rBV	398308	666877	41.64%	7.675%
56	9.076	2497	2499	2504	rVB2	519	464	0.03%	0.005%
57	9.108	2504	2509	2510	rBV2	513	385	0.02%	0.004%
58	9.156	2521	2524	2526	rBV2	413	249	0.02%	0.003%
59	9.432	2609	2610	2614	rVB2	400	198	0.01%	0.002%
60	9.481	2623	2625	2628	rVB2	327	196	0.01%	0.002%
61	9.548	2644	2646	2648	rBV	521	258	0.02%	0.003%
62	9.674	2682	2685	2688	rVB3	417	315	0.02%	0.004%
63	9.985	2776	2782	2784	rBV2	455	442	0.03%	0.005%
64	10.124	2817	2825	2826	rBV3	1110	1023	0.06%	0.012%
65	10.217	2843	2854	2876	rVV	321820	504439	31.50%	5.805%
66	10.329	2887	2889	2893	rVB3	500	301	0.02%	0.003%
67	10.375	2900	2903	2906	rBV2	523	429	0.03%	0.005%
68	10.426	2913	2919	2923	rBV3	483	600	0.04%	0.007%
69	10.452	2924	2927	2929	rVB2	497	319	0.02%	0.004%
70	10.532	2950	2952	2958	rVB3	328	193	0.01%	0.002%
71	10.629	2978	2982	2987	rBV2	277	295	0.02%	0.003%
72	10.786	3026	3031	3032	rBV	218	181	0.01%	0.002%
73	10.796	3032	3034	3038	rVB2	323	210	0.01%	0.002%
74	10.915	3068	3071	3073	rBV	521	359	0.02%	0.004%
75	11.252	3164	3176	3202	rBV	358549	569985	35.59%	6.560%
76	11.384	3215	3217	3223	rBV3	622	720	0.04%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022409.D
 Acq On : 30 Sep 2021 04:09
 Operator : SY/MD
 Sample : M3979-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A10

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M

Title : VOC Analysis

77	11.436	3227	3233	3239	rVV5	608	770	0.05%	0.009%
78	11.516	3256	3258	3262	rVB3	312	193	0.01%	0.002%
79	11.625	3280	3292	3316	rBV	421676	675361	42.17%	7.772%
80	11.927	3384	3386	3390	rVB2	582	294	0.02%	0.003%
81	12.040	3419	3421	3424	rBV	291	179	0.01%	0.002%
82	12.204	3468	3472	3474	rBV2	259	208	0.01%	0.002%
83	12.448	3546	3548	3551	rBV	309	181	0.01%	0.002%
84	12.516	3567	3569	3575	rVB3	365	339	0.02%	0.004%
85	12.558	3580	3582	3584	rBV2	310	188	0.01%	0.002%
86	12.702	3624	3627	3631	rBV3	369	259	0.02%	0.003%
87	13.120	3755	3757	3760	rVB	445	190	0.01%	0.002%
88	13.198	3779	3781	3784	rVB	404	193	0.01%	0.002%
89	13.310	3812	3816	3817	rBV2	273	210	0.01%	0.002%
90	13.339	3821	3825	3827	rBV2	273	178	0.01%	0.002%
91	13.439	3852	3856	3860	rVB3	335	237	0.01%	0.003%
92	13.529	3881	3884	3888	rBV	280	222	0.01%	0.003%
93	13.763	3953	3957	3959	rBV	302	200	0.01%	0.002%
94	13.866	3987	3989	3991	rBV	393	179	0.01%	0.002%
95	13.921	4001	4006	4008	rBV3	295	285	0.02%	0.003%
96	14.056	4045	4048	4054	rBV2	293	305	0.02%	0.004%
97	14.233	4101	4103	4106	rBV2	356	206	0.01%	0.002%
98	14.493	4181	4184	4186	rBV	381	191	0.01%	0.002%
99	14.554	4200	4203	4205	rBV3	423	211	0.01%	0.002%
100	14.770	4269	4270	4275	rBV2	311	261	0.02%	0.003%




Sum of corrected areas: 8689182

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022409.D
Acq On : 30 Sep 2021 04:09
Operator : SY/MD
Sample : M3979-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A10

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

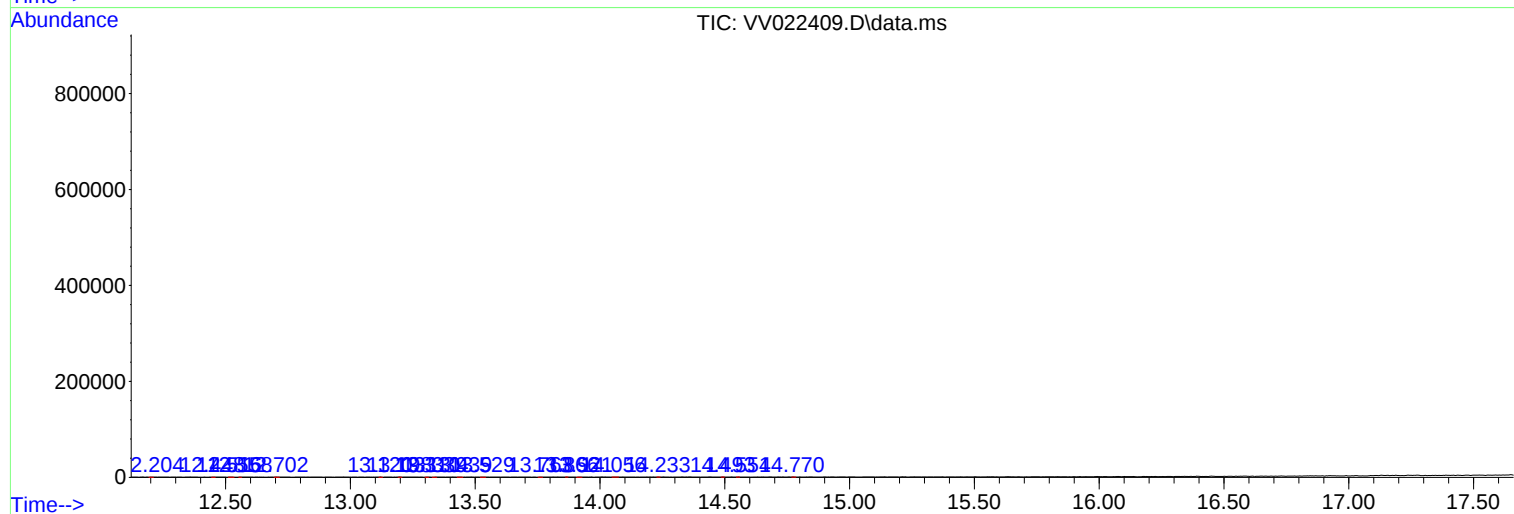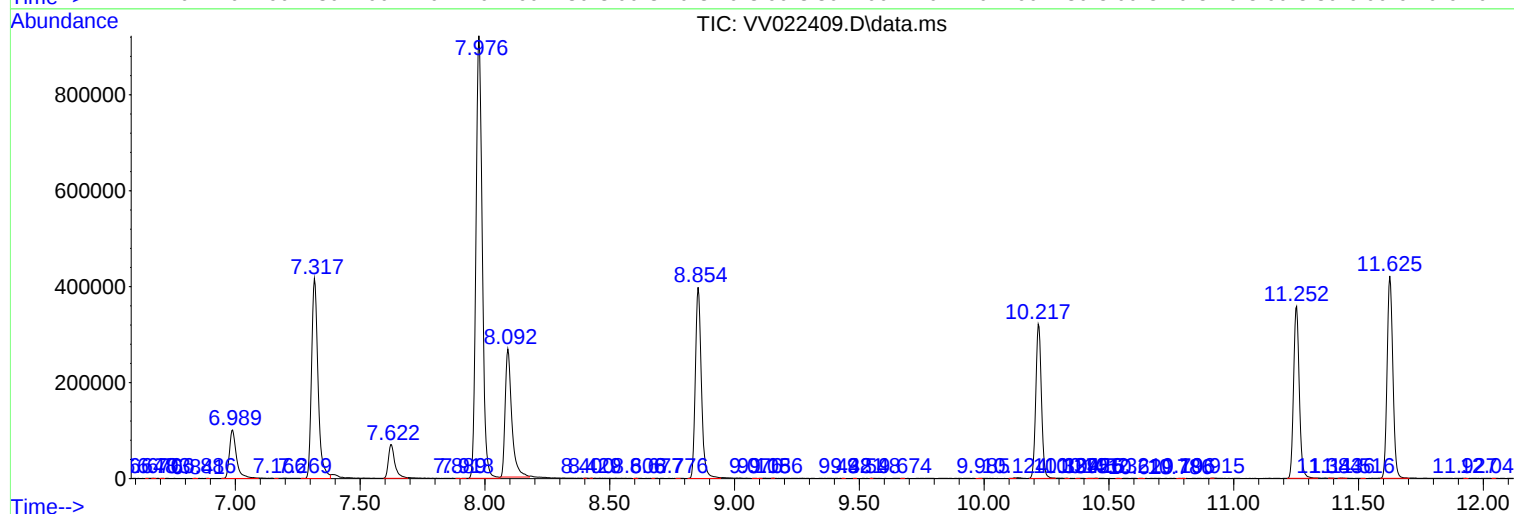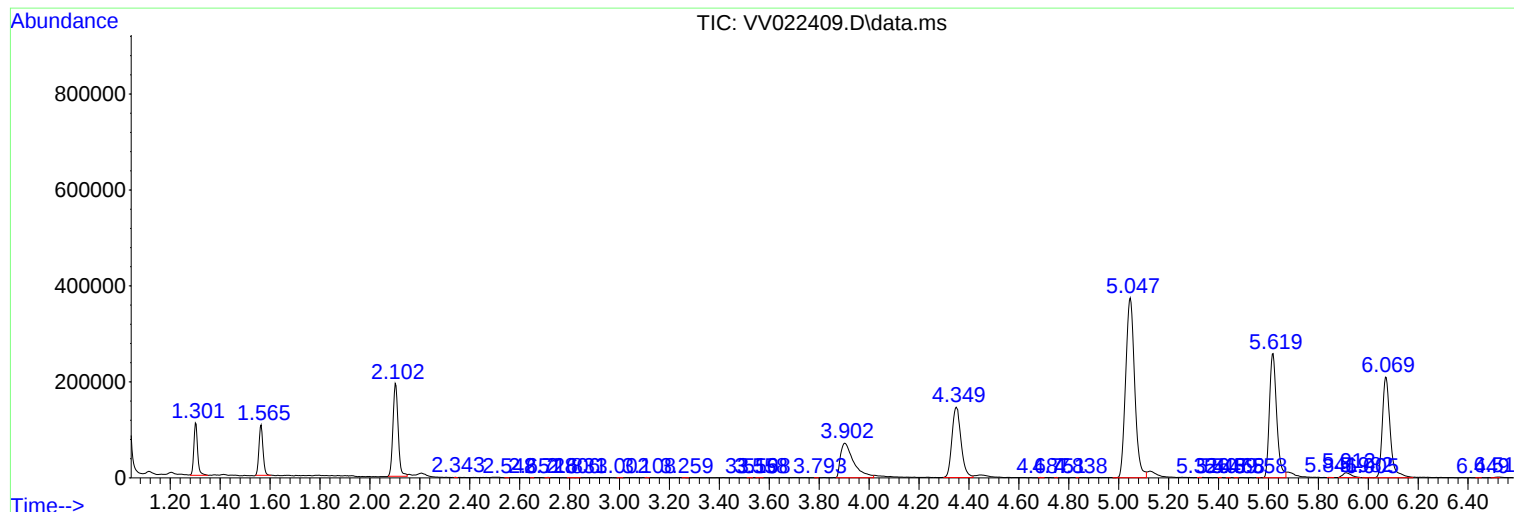

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022409.D
Acq On : 30 Sep 2021 04:09
Operator : SY/MD
Sample : M3979-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A10

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022409.D
Acq On : 30 Sep 2021 04:09
Operator : SY/MD
Sample : M3979-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A10

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------