

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022410.D
 Acq On : 30 Sep 2021 04:33
 Operator : SY/MD
 Sample : M3979-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A11

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M

Title : VOC Analysis

Signal : TIC: VV022410.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	93	rVB	106358	108263	2.07%	0.884%
2	1.561	156	162	173	rVB	99847	111779	2.13%	0.913%
3	2.101	321	330	343	rBV	194390	278988	5.32%	2.279%
4	2.661	502	504	505	rBV	366	129	0.00%	0.001%
5	2.706	515	518	520	rBV3	334	227	0.00%	0.002%
6	2.757	530	534	538	rBV3	362	352	0.01%	0.003%
7	3.063	626	629	632	rBV	297	206	0.00%	0.002%
8	3.233	679	682	684	rBV2	398	203	0.00%	0.002%
9	3.388	728	730	733	rBV3	372	194	0.00%	0.002%
10	3.404	733	735	737	rBV3	266	144	0.00%	0.001%
11	3.442	743	747	749	rBV2	243	165	0.00%	0.001%
12	3.468	751	755	759	rVB2	367	273	0.01%	0.002%
13	3.490	759	762	763	rBV2	261	133	0.00%	0.001%
14	3.622	801	803	804	rBV2	336	141	0.00%	0.001%
15	3.648	810	811	813	rVB2	193	46	0.00%	0.000%
16	3.664	813	816	820	rBV2	388	386	0.01%	0.003%
17	3.741	839	840	843	rVB2	252	60	0.00%	0.000%
18	3.754	843	844	846	rBV2	220	91	0.00%	0.001%
19	3.767	846	848	850	rVB2	208	60	0.00%	0.000%
20	3.841	868	871	873	rBV	308	204	0.00%	0.002%
21	3.902	877	890	919	rBV	76012	273222	5.21%	2.231%
22	4.349	1014	1029	1052	rBV	147063	368256	7.02%	3.008%
23	4.670	1127	1129	1130	rBV	461	163	0.00%	0.001%
24	4.802	1166	1170	1174	rBV3	246	255	0.00%	0.002%
25	4.892	1196	1198	1199	rBV2	229	83	0.00%	0.001%
26	4.957	1215	1218	1223	rVB2	461	425	0.01%	0.003%
27	4.976	1223	1224	1225	rBV2	108	30	0.00%	0.000%
28	5.047	1228	1246	1270	rBV2	367899	937487	17.88%	7.657%
29	5.397	1352	1355	1356	rBV	321	169	0.00%	0.001%
30	5.481	1378	1381	1382	rBV2	359	187	0.00%	0.002%
31	5.510	1388	1390	1392	rBV	549	324	0.01%	0.003%
32	5.551	1401	1403	1405	rBV2	306	169	0.00%	0.001%
33	5.616	1410	1423	1441	rBV	256687	517054	9.86%	4.223%
34	5.851	1493	1496	1499	rVB4	315	164	0.00%	0.001%
35	5.912	1504	1515	1530	rBV7	15591	37428	0.71%	0.306%
36	6.021	1545	1549	1551	rBV2	653	371	0.01%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022410.D
 Acq On : 30 Sep 2021 04:33
 Operator : SY/MD
 Sample : M3979-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A11

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

37	6.069	1551	1564	1595	rBV	211158	440320	8.40%	3.596%
38	6.352	1650	1652	1655	rBV2	423	229	0.00%	0.002%
39	6.400	1664	1667	1670	rBV2	351	209	0.00%	0.002%
40	6.426	1673	1675	1678	rBV2	245	148	0.00%	0.001%
41	6.471	1686	1689	1690	rBV2	202	102	0.00%	0.001%
42	6.481	1690	1692	1694	rVV	237	116	0.00%	0.001%
43	6.587	1723	1725	1728	rBV2	188	103	0.00%	0.001%
44	6.603	1728	1730	1732	rBV	255	115	0.00%	0.001%
45	6.641	1740	1742	1744	rBV2	418	233	0.00%	0.002%
46	6.754	1775	1777	1779	rBV	268	133	0.00%	0.001%
47	6.770	1779	1782	1783	rVV2	336	159	0.00%	0.001%
48	6.780	1783	1785	1787	rVB2	591	259	0.00%	0.002%
49	6.796	1787	1790	1791	rBV	425	157	0.00%	0.001%
50	6.838	1800	1803	1807	rVB2	369	194	0.00%	0.002%
51	6.860	1808	1810	1814	rBV2	355	211	0.00%	0.002%
52	6.940	1832	1835	1837	rBV	242	141	0.00%	0.001%
53	6.989	1839	1850	1877	rVV	100336	188708	3.60%	1.541%
54	7.191	1909	1913	1914	rBV3	576	385	0.01%	0.003%
55	7.317	1941	1952	1973	rBV	419964	739922	14.11%	6.043%
56	7.574	2030	2032	2034	rVB	346	117	0.00%	0.001%
57	7.590	2034	2037	2038	rBV	434	207	0.00%	0.002%
58	7.622	2038	2047	2075	rVV	69500	127527	2.43%	1.042%
59	7.818	2106	2108	2111	rVB	528	216	0.00%	0.002%
60	7.876	2125	2126	2131	rBV2	339	289	0.01%	0.002%
61	7.912	2135	2137	2139	rVB2	375	135	0.00%	0.001%
62	7.976	2142	2157	2183	rBV	3098574	5242374	100.00%	42.816%
63	8.092	2184	2193	2228	rVB	265199	502030	9.58%	4.100%
64	8.854	2419	2430	2455	rBV	386960	643407	12.27%	5.255%
65	9.053	2490	2492	2496	rBV3	510	289	0.01%	0.002%
66	9.124	2512	2514	2516	rBV2	353	153	0.00%	0.001%
67	9.223	2543	2545	2549	rVB2	656	280	0.01%	0.002%
68	9.349	2582	2584	2587	rBV	283	151	0.00%	0.001%
69	9.384	2592	2595	2598	rBV	279	228	0.00%	0.002%
70	9.429	2604	2609	2612	rBV3	602	577	0.01%	0.005%
71	9.532	2638	2641	2643	rBV	278	181	0.00%	0.001%
72	9.818	2728	2730	2732	rBV	283	109	0.00%	0.001%
73	9.969	2772	2777	2778	rBV	217	207	0.00%	0.002%
74	10.082	2810	2812	2815	rBV2	424	308	0.01%	0.003%
75	10.217	2841	2854	2872	rBV	312465	487889	9.31%	3.985%
76	10.407	2912	2913	2915	rBV2	344	115	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022410.D
 Acq On : 30 Sep 2021 04:33
 Operator : SY/MD
 Sample : M3979-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A11

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

77	10.529	2950	2951	2952	rBV2	240	89	0.00%	0.001%
78	10.577	2963	2966	2970	rVB3	310	289	0.01%	0.002%
79	10.635	2981	2984	2986	rBV	310	198	0.00%	0.002%
80	10.783	3026	3030	3033	rBV2	220	138	0.00%	0.001%
81	10.834	3044	3046	3048	rBV2	272	127	0.00%	0.001%
82	11.014	3100	3102	3106	rBV3	468	309	0.01%	0.003%
83	11.140	3139	3141	3143	rBV2	370	140	0.00%	0.001%
84	11.252	3165	3176	3199	rBV	355123	560177	10.69%	4.575%
85	11.378	3213	3215	3217	rBV	534	214	0.00%	0.002%
86	11.455	3237	3239	3241	rBV2	377	174	0.00%	0.001%
87	11.522	3256	3260	3264	rVB3	553	452	0.01%	0.004%
88	11.545	3264	3267	3274	rVB4	539	466	0.01%	0.004%
89	11.625	3281	3292	3317	rBV	420955	662427	12.64%	5.410%
90	11.792	3341	3344	3347	rBV3	455	298	0.01%	0.002%
91	11.972	3395	3400	3402	rBV2	374	388	0.01%	0.003%
92	12.355	3517	3519	3523	rBV2	384	176	0.00%	0.001%
93	12.413	3535	3537	3541	rBV2	412	282	0.01%	0.002%
94	12.693	3623	3624	3627	rBV3	256	121	0.00%	0.001%
95	12.734	3635	3637	3638	rBV	292	124	0.00%	0.001%
96	12.808	3658	3660	3666	rVB2	449	392	0.01%	0.003%
97	13.050	3733	3735	3737	rBV2	284	119	0.00%	0.001%
98	13.265	3800	3802	3804	rBV	282	121	0.00%	0.001%
99	13.619	3910	3912	3915	rBV	351	198	0.00%	0.002%
100	14.667	4237	4238	4242	rBV2	361	113	0.00%	0.001%




Sum of corrected areas: 12243996

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022410.D
Acq On : 30 Sep 2021 04:33
Operator : SY/MD
Sample : M3979-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A11

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

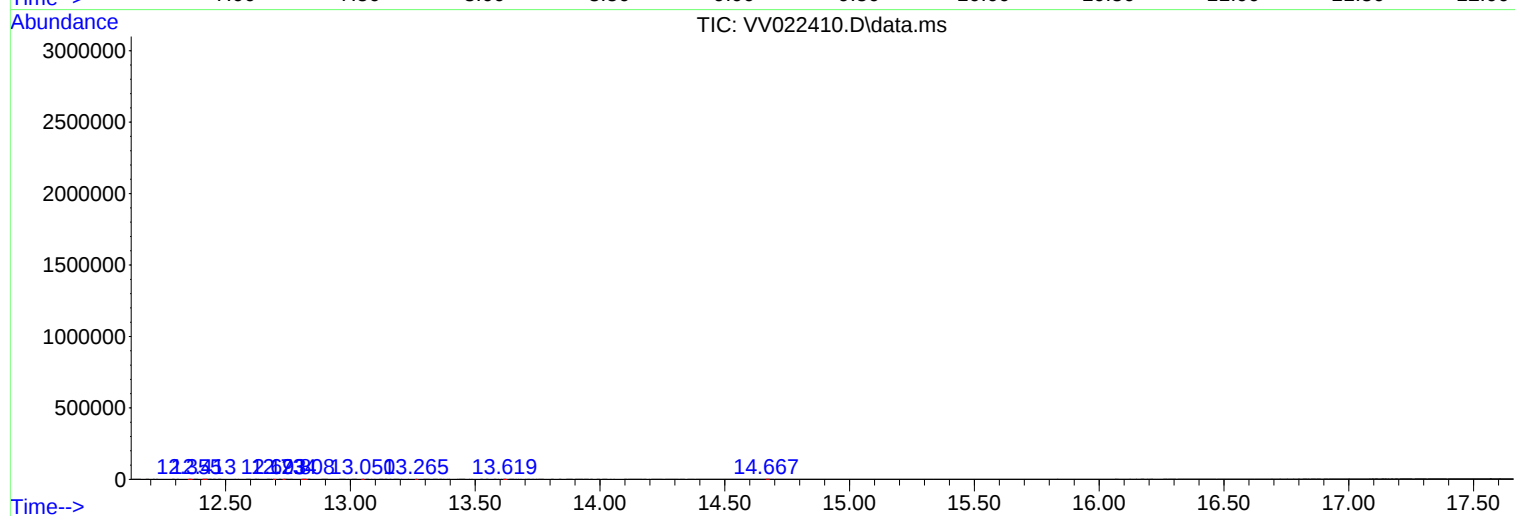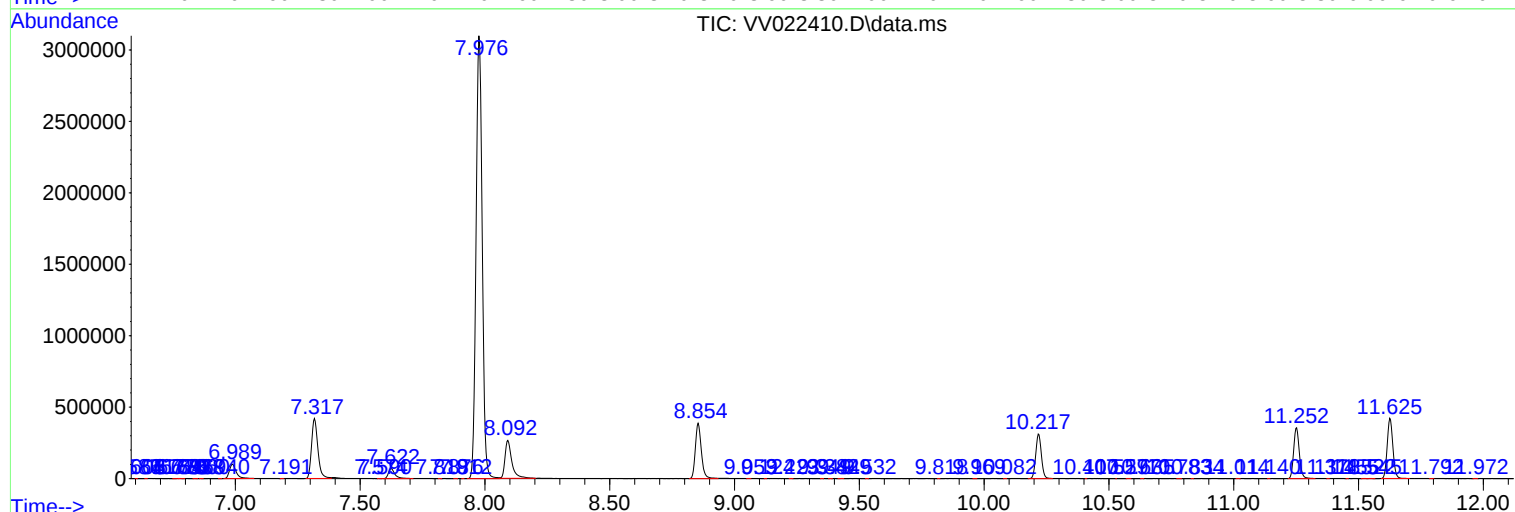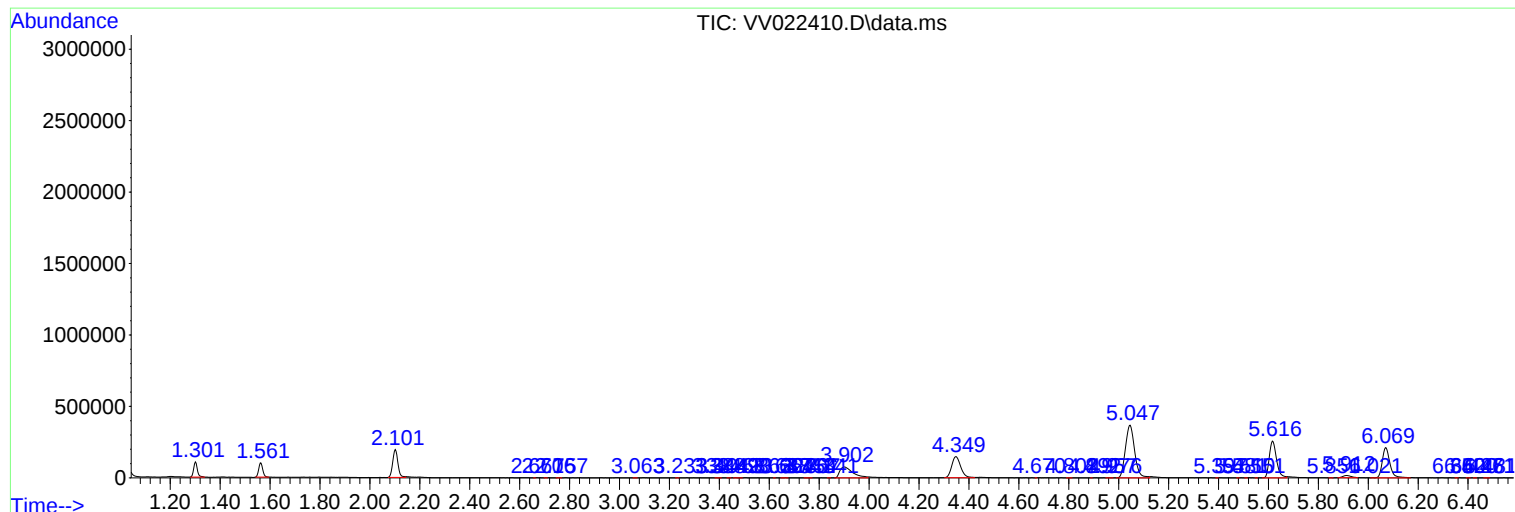

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022410.D
Acq On : 30 Sep 2021 04:33
Operator : SY/MD
Sample : M3979-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A11

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022410.D
Acq On : 30 Sep 2021 04:33
Operator : SY/MD
Sample : M3979-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A11

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------