

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022412.D
 Acq On : 30 Sep 2021 05:21
 Operator : SY/MD
 Sample : M3979-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A57

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

Signal : TIC: VV022412.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	98	rVB	109951	115842	12.23%	1.621%
2	1.565	157	163	173	rVB	105190	116151	12.26%	1.625%
3	2.105	321	331	356	rBV	195556	290669	30.68%	4.067%
4	2.622	490	492	496	rVB	465	293	0.03%	0.004%
5	2.648	497	500	503	rBV2	372	290	0.03%	0.004%
6	2.767	532	537	548	rVV5	1010	1598	0.17%	0.022%
7	2.954	589	595	596	rBV2	370	346	0.04%	0.005%
8	3.053	624	626	634	rVB2	368	328	0.03%	0.005%
9	3.291	696	700	703	rBV3	371	309	0.03%	0.004%
10	3.323	705	710	715	rVB3	354	389	0.04%	0.005%
11	3.349	715	718	722	rBV	425	282	0.03%	0.004%
12	3.407	733	736	740	rBV2	298	189	0.02%	0.003%
13	3.478	754	758	763	rVB3	258	273	0.03%	0.004%
14	3.687	819	823	827	rVB2	353	298	0.03%	0.004%
15	3.767	846	848	851	rVB2	381	211	0.02%	0.003%
16	3.899	878	889	922	rBV	72895	244710	25.83%	3.424%
17	4.349	1011	1029	1051	rBV	154760	377319	39.82%	5.279%
18	4.609	1107	1110	1116	rBV4	552	578	0.06%	0.008%
19	4.667	1124	1128	1132	rBV3	655	628	0.07%	0.009%
20	4.716	1141	1143	1145	rBV2	426	198	0.02%	0.003%
21	4.863	1186	1189	1191	rVB2	343	196	0.02%	0.003%
22	4.973	1217	1223	1225	rBV2	238	189	0.02%	0.003%
23	4.989	1225	1228	1230	rBV2	414	275	0.03%	0.004%
24	5.047	1230	1246	1265	rBV2	376246	947486	100.00%	13.256%
25	5.362	1339	1344	1346	rBV4	714	605	0.06%	0.008%
26	5.426	1361	1364	1368	rVB2	414	347	0.04%	0.005%
27	5.494	1382	1385	1387	rBV	341	229	0.02%	0.003%
28	5.513	1387	1391	1393	rBV3	472	333	0.04%	0.005%
29	5.561	1402	1406	1409	rBV	281	219	0.02%	0.003%
30	5.619	1409	1424	1441	rBV2	253003	519586	54.84%	7.269%
31	5.908	1504	1514	1530	rBV4	7287	15984	1.69%	0.224%
32	6.018	1544	1548	1550	rBV3	259	205	0.02%	0.003%
33	6.072	1550	1565	1599	rBV	218351	458885	48.43%	6.420%
34	6.400	1664	1667	1669	rVB2	555	334	0.04%	0.005%
35	6.468	1685	1688	1695	rVB3	529	490	0.05%	0.007%
36	6.587	1721	1725	1729	rVB3	366	251	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022412.D
 Acq On : 30 Sep 2021 05:21
 Operator : SY/MD
 Sample : M3979-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A57

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

37	6.677	1751	1753	1755	rBV	376	218	0.02%	0.003%
38	6.712	1761	1764	1768	rVB2	409	228	0.02%	0.003%
39	6.732	1768	1770	1776	rVB3	283	241	0.03%	0.003%
40	6.902	1820	1823	1827	rBV2	231	191	0.02%	0.003%
41	6.989	1839	1850	1877	rBV	101893	195149	20.60%	2.730%
42	7.207	1915	1918	1920	rBV	490	299	0.03%	0.004%
43	7.243	1927	1929	1933	rVB3	393	256	0.03%	0.004%
44	7.317	1939	1952	1973	rBV	427819	761174	80.34%	10.649%
45	7.625	2038	2048	2071	rBV	69413	131616	13.89%	1.841%
46	7.854	2117	2119	2123	rBV2	442	350	0.04%	0.005%
47	7.979	2148	2158	2176	rVB2	33328	57410	6.06%	0.803%
48	8.092	2183	2193	2234	rBV	269064	510391	53.87%	7.141%
49	8.458	2305	2307	2309	rVB	502	226	0.02%	0.003%
50	8.619	2355	2357	2364	rVB3	424	257	0.03%	0.004%
51	8.693	2374	2380	2382	rBV2	531	553	0.06%	0.008%
52	8.719	2385	2388	2391	rBV2	367	238	0.03%	0.003%
53	8.751	2395	2398	2402	rBV2	314	216	0.02%	0.003%
54	8.854	2418	2430	2460	rBV	388495	653900	69.01%	9.148%
55	9.124	2511	2514	2517	rBV2	384	268	0.03%	0.004%
56	9.146	2517	2521	2524	rBV3	762	665	0.07%	0.009%
57	9.191	2531	2535	2536	rVB2	406	295	0.03%	0.004%
58	9.256	2553	2555	2557	rVB2	442	202	0.02%	0.003%
59	9.294	2563	2567	2569	rBV3	406	301	0.03%	0.004%
60	9.368	2587	2590	2592	rVB	454	224	0.02%	0.003%
61	9.397	2595	2599	2603	rBV2	463	511	0.05%	0.007%
62	9.696	2687	2692	2695	rBV2	305	254	0.03%	0.004%
63	9.741	2702	2706	2708	rBV2	255	189	0.02%	0.003%
64	9.831	2730	2734	2738	rBB3	370	300	0.03%	0.004%
65	10.127	2821	2826	2828	rBV3	680	611	0.06%	0.009%
66	10.217	2842	2854	2882	rBV	322723	516127	54.47%	7.221%
67	10.358	2894	2898	2901	rBV3	575	393	0.04%	0.005%
68	10.529	2948	2951	2954	rBV3	344	230	0.02%	0.003%
69	10.712	3002	3008	3011	rBV3	358	305	0.03%	0.004%
70	10.854	3047	3052	3056	rBV3	264	201	0.02%	0.003%
71	10.879	3056	3060	3065	rBV2	323	290	0.03%	0.004%
72	10.911	3068	3070	3072	rBV2	592	370	0.04%	0.005%
73	10.998	3093	3097	3099	rBV	267	252	0.03%	0.004%
74	11.027	3101	3106	3109	rVV2	447	289	0.03%	0.004%
75	11.204	3156	3161	3163	rVB	355	258	0.03%	0.004%
76	11.252	3163	3176	3201	rBV	346546	543105	57.32%	7.598%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022412.D
 Acq On : 30 Sep 2021 05:21
 Operator : SY/MD
 Sample : M3979-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A57

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

77	11.464	3239	3242	3245	rBV2	212	189	0.02%	0.003%
78	11.493	3247	3251	3253	rBV3	432	253	0.03%	0.004%
79	11.542	3260	3266	3268	rBV2	783	804	0.08%	0.011%
80	11.625	3280	3292	3312	rBV	418614	665810	70.27%	9.315%
81	11.982	3399	3403	3408	rVB3	348	288	0.03%	0.004%
82	12.098	3437	3439	3441	rBV2	455	248	0.03%	0.003%
83	12.181	3462	3465	3470	rBV2	336	280	0.03%	0.004%
84	12.259	3488	3489	3495	rVB	492	285	0.03%	0.004%
85	12.300	3499	3502	3505	rVB	375	229	0.02%	0.003%
86	12.339	3512	3514	3518	rBV3	415	302	0.03%	0.004%
87	12.464	3551	3553	3556	rVB2	330	198	0.02%	0.003%
88	12.738	3635	3638	3642	rVV2	326	219	0.02%	0.003%
89	12.780	3649	3651	3656	rVB2	510	384	0.04%	0.005%
90	12.931	3695	3698	3703	rVB3	365	275	0.03%	0.004%
91	13.114	3751	3755	3757	rBV	549	404	0.04%	0.006%
92	13.255	3796	3799	3804	rBV	333	228	0.02%	0.003%
93	13.689	3931	3934	3936	rBV2	328	198	0.02%	0.003%
94	13.728	3944	3946	3950	rBV2	268	220	0.02%	0.003%
95	13.818	3969	3974	3979	rBV2	457	481	0.05%	0.007%
96	14.172	4082	4084	4091	rVB3	343	244	0.03%	0.003%
97	14.255	4105	4110	4113	rBV2	468	390	0.04%	0.005%
98	14.358	4139	4142	4145	rBV2	459	246	0.03%	0.003%
99	14.477	4176	4179	4184	rVB2	368	281	0.03%	0.004%
100	14.506	4184	4188	4192	rBV2	279	283	0.03%	0.004%



Sum of corrected areas: 7147807

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022412.D
Acq On : 30 Sep 2021 05:21
Operator : SY/MD
Sample : M3979-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A57

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

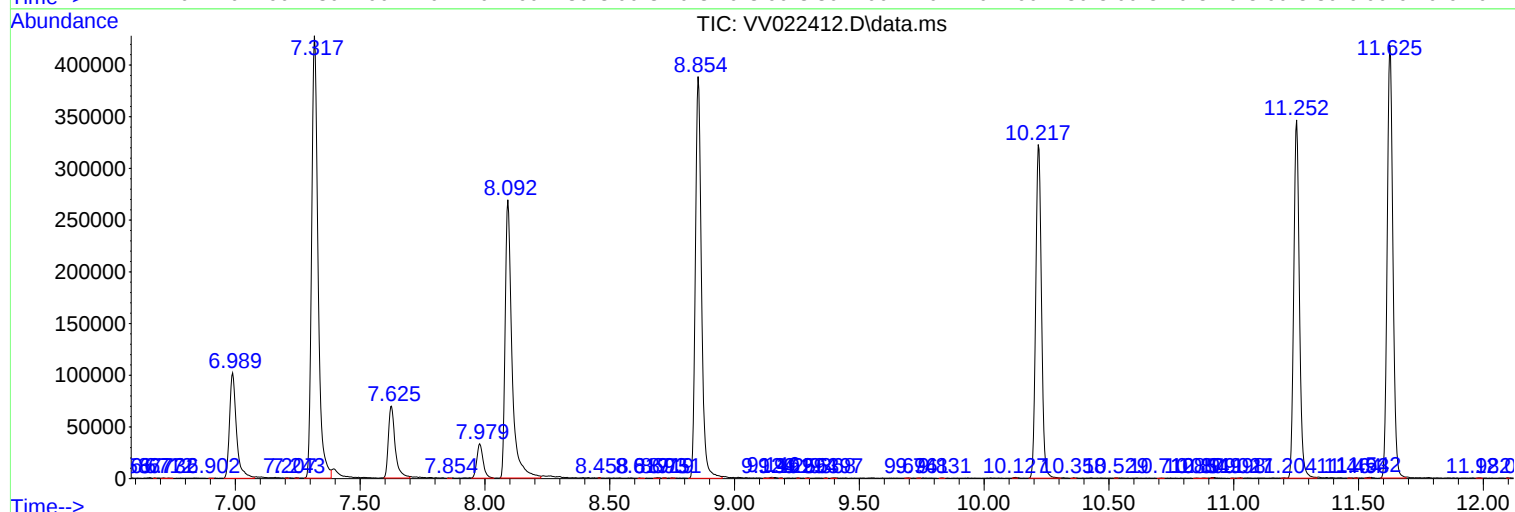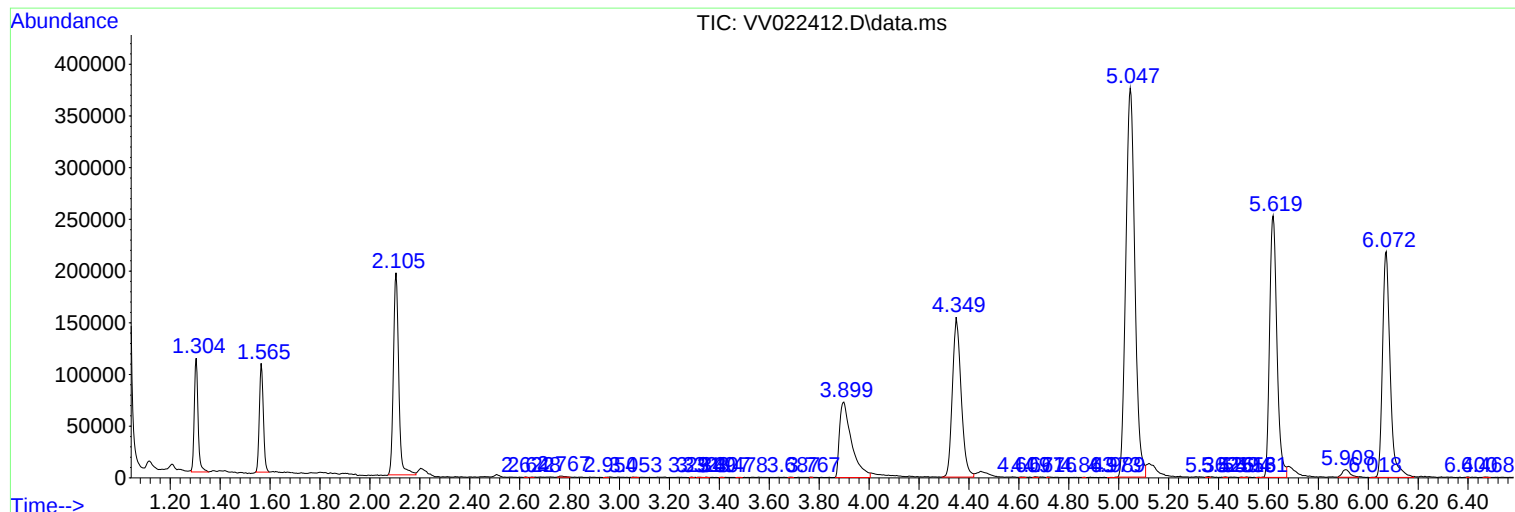

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022412.D
Acq On : 30 Sep 2021 05:21
Operator : SY/MD
Sample : M3979-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A57

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022412.D
Acq On : 30 Sep 2021 05:21
Operator : SY/MD
Sample : M3979-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A57

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
