

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022413.D
 Acq On : 30 Sep 2021 05:45
 Operator : SY/MD
 Sample : M3978-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A49

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M

Title : VOC Analysis

Signal : TIC: VV022413.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	95	rVB	105771	109393	6.06%	1.217%
2	1.564	156	163	177	rBV	104301	118260	6.55%	1.316%
3	2.105	322	331	344	rBV	189978	268386	14.87%	2.987%
4	2.764	529	536	539	rBV5	3407	4230	0.23%	0.047%
5	2.834	555	558	559	rBV2	345	147	0.01%	0.002%
6	2.979	600	603	606	rBV	412	285	0.02%	0.003%
7	3.018	611	615	619	rBV	495	387	0.02%	0.004%
8	3.069	627	631	634	rBV3	457	308	0.02%	0.003%
9	3.105	640	642	644	rVB2	433	155	0.01%	0.002%
10	3.182	660	666	667	rBV2	301	253	0.01%	0.003%
11	3.224	677	679	683	rVB	336	183	0.01%	0.002%
12	3.243	683	685	691	rVB2	348	298	0.02%	0.003%
13	3.291	698	700	704	rVV3	410	222	0.01%	0.002%
14	3.323	707	710	713	rBV2	486	315	0.02%	0.004%
15	3.381	725	728	730	rVV	233	111	0.01%	0.001%
16	3.391	730	731	733	rVV2	237	112	0.01%	0.001%
17	3.481	757	759	763	rVB	434	249	0.01%	0.003%
18	3.500	763	765	767	rBV2	400	231	0.01%	0.003%
19	3.725	833	835	839	rVB	364	221	0.01%	0.002%
20	3.857	874	876	878	rBV2	240	120	0.01%	0.001%
21	3.902	878	890	929	rBV2	84603	311841	17.28%	3.470%
22	4.349	1012	1029	1051	rBV	147409	370035	20.51%	4.118%
23	4.651	1120	1123	1127	rBV4	415	346	0.02%	0.004%
24	4.722	1143	1145	1148	rBV3	307	174	0.01%	0.002%
25	4.738	1148	1150	1154	rVB	359	238	0.01%	0.003%
26	4.831	1175	1179	1182	rVB4	372	266	0.01%	0.003%
27	4.921	1205	1207	1212	rVB2	317	264	0.01%	0.003%
28	4.969	1220	1222	1226	rVB	379	248	0.01%	0.003%
29	5.047	1226	1246	1265	rBV2	367971	935084	51.82%	10.406%
30	5.506	1387	1389	1394	rVB	507	223	0.01%	0.002%
31	5.619	1410	1424	1441	rBV	266711	542739	30.08%	6.040%
32	5.915	1504	1516	1540	rBV7	17331	42679	2.37%	0.475%
33	6.072	1551	1565	1597	rBV	212618	450731	24.98%	5.016%
34	6.349	1649	1651	1653	rVB	466	194	0.01%	0.002%
35	6.448	1680	1682	1687	rBV	307	177	0.01%	0.002%
36	6.487	1692	1694	1696	rBV2	324	111	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022413.D
 Acq On : 30 Sep 2021 05:45
 Operator : SY/MD
 Sample : M3978-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A49

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

37	6.516	1700	1703	1706	rVV2	400	202	0.01%	0.002%
38	6.535	1706	1709	1714	rVB3	322	203	0.01%	0.002%
39	6.603	1727	1730	1733	rVB2	219	127	0.01%	0.001%
40	6.641	1736	1742	1743	rBV2	636	399	0.02%	0.004%
41	6.670	1749	1751	1753	rVB	348	137	0.01%	0.002%
42	6.847	1802	1806	1809	rBV2	285	242	0.01%	0.003%
43	6.870	1809	1813	1816	rBV2	367	203	0.01%	0.002%
44	6.889	1816	1819	1821	rBV	308	135	0.01%	0.002%
45	6.921	1827	1829	1833	rBV2	329	207	0.01%	0.002%
46	6.989	1839	1850	1878	rBV	99452	190604	10.56%	2.121%
47	7.317	1941	1952	1973	rBV	417835	747313	41.42%	8.316%
48	7.622	2035	2047	2072	rBV	69127	128162	7.10%	1.426%
49	7.876	2124	2126	2129	rBV	323	226	0.01%	0.003%
50	7.976	2143	2157	2183	rBV	1045997	1804437	100.00%	20.080%
51	8.091	2184	2193	2230	rVB	261578	499437	27.68%	5.558%
52	8.493	2315	2318	2319	rBV2	373	201	0.01%	0.002%
53	8.699	2379	2382	2386	rBV2	651	398	0.02%	0.004%
54	8.773	2402	2405	2410	rVB2	418	269	0.01%	0.003%
55	8.854	2418	2430	2461	rBV	406144	685702	38.00%	7.631%
56	9.014	2479	2480	2482	rBV	416	178	0.01%	0.002%
57	9.079	2498	2500	2503	rBV2	489	195	0.01%	0.002%
58	9.156	2522	2524	2527	rVB3	671	295	0.02%	0.003%
59	9.194	2534	2536	2538	rBV2	284	175	0.01%	0.002%
60	9.214	2540	2542	2544	rVB	329	126	0.01%	0.001%
61	9.407	2596	2602	2605	rBV2	418	361	0.02%	0.004%
62	9.554	2644	2648	2650	rBV	459	304	0.02%	0.003%
63	9.638	2672	2674	2678	rVB2	318	135	0.01%	0.002%
64	9.664	2680	2682	2687	rVB3	303	176	0.01%	0.002%
65	9.747	2706	2708	2713	rBV3	208	109	0.01%	0.001%
66	9.799	2718	2724	2726	rBV2	321	267	0.01%	0.003%
67	9.979	2776	2780	2783	rBV	248	209	0.01%	0.002%
68	10.046	2798	2801	2802	rBV2	242	139	0.01%	0.002%
69	10.075	2807	2810	2812	rVB	314	130	0.01%	0.001%
70	10.217	2841	2854	2881	rBV	319352	507670	28.13%	5.649%
71	10.358	2895	2898	2902	rBV2	358	196	0.01%	0.002%
72	10.461	2928	2930	2932	rBV	395	119	0.01%	0.001%
73	10.538	2951	2954	2958	rVB	378	173	0.01%	0.002%
74	10.570	2961	2964	2965	rBV	403	206	0.01%	0.002%
75	10.680	2992	2998	3001	rBV3	303	285	0.02%	0.003%
76	10.831	3043	3045	3046	rBV3	308	117	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022413.D
 Acq On : 30 Sep 2021 05:45
 Operator : SY/MD
 Sample : M3978-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A49

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

77	10.911	3068	3070	3072	rBV2	759	494	0.03%	0.005%
78	10.956	3082	3084	3088	rBV3	317	243	0.01%	0.003%
79	11.024	3103	3105	3108	rVB2	250	137	0.01%	0.002%
80	11.075	3118	3121	3122	rBV2	244	126	0.01%	0.001%
81	11.111	3130	3132	3134	rBV	329	125	0.01%	0.001%
82	11.207	3160	3162	3164	rBV	245	120	0.01%	0.001%
83	11.252	3164	3176	3196	rBV	368066	579377	32.11%	6.447%
84	11.522	3259	3260	3265	rBV2	246	187	0.01%	0.002%
85	11.564	3271	3273	3275	rBV3	211	116	0.01%	0.001%
86	11.625	3280	3292	3312	rVV	420160	672889	37.29%	7.488%
87	11.792	3340	3344	3345	rBV2	530	309	0.02%	0.003%
88	11.914	3380	3382	3383	rBV	291	120	0.01%	0.001%
89	11.959	3392	3396	3398	rBV	386	250	0.01%	0.003%
90	12.715	3629	3631	3635	rVB2	295	169	0.01%	0.002%
91	12.738	3635	3638	3642	rBV3	357	343	0.02%	0.004%
92	12.821	3661	3664	3667	rBV2	281	235	0.01%	0.003%
93	13.185	3774	3777	3778	rBV	282	118	0.01%	0.001%
94	13.394	3840	3842	3845	rVB	360	160	0.01%	0.002%
95	13.419	3845	3850	3856	rBV3	390	443	0.02%	0.005%
96	13.583	3898	3901	3904	rBV3	354	219	0.01%	0.002%
97	13.808	3969	3971	3974	rBV	282	159	0.01%	0.002%
98	13.882	3993	3994	3999	rVB2	554	177	0.01%	0.002%
99	14.037	4040	4042	4045	rBV2	322	182	0.01%	0.002%
100	14.091	4057	4059	4064	rVB3	323	244	0.01%	0.003%




Sum of corrected areas: 8986327

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022413.D
Acq On : 30 Sep 2021 05:45
Operator : SY/MD
Sample : M3978-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A49

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

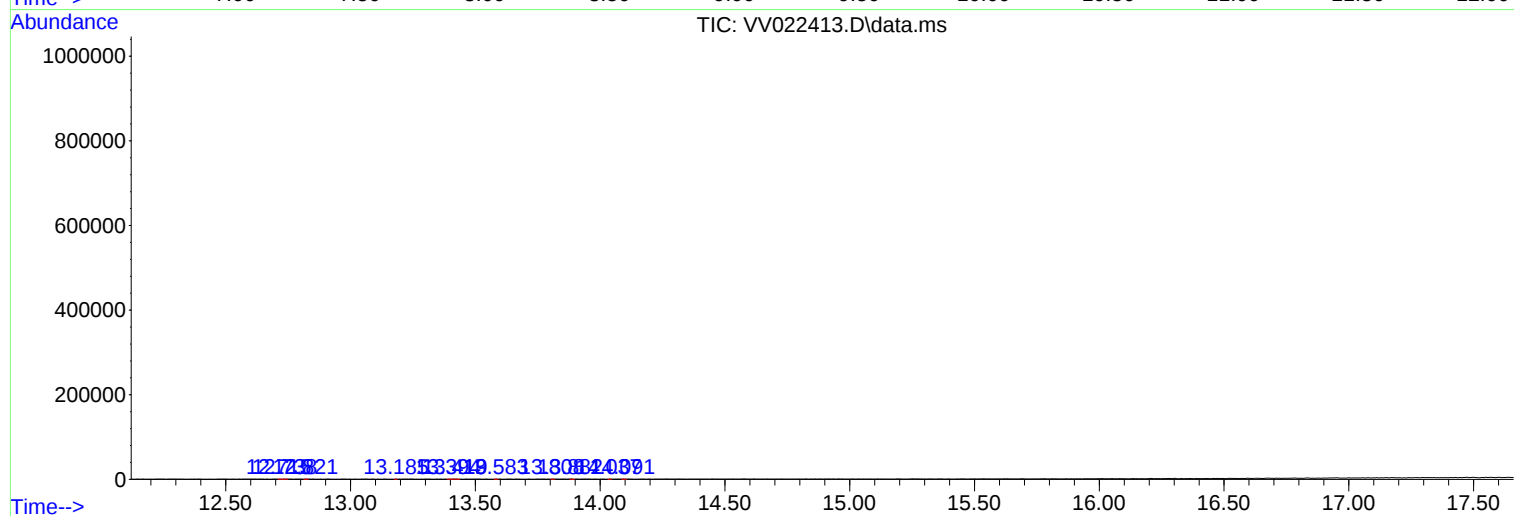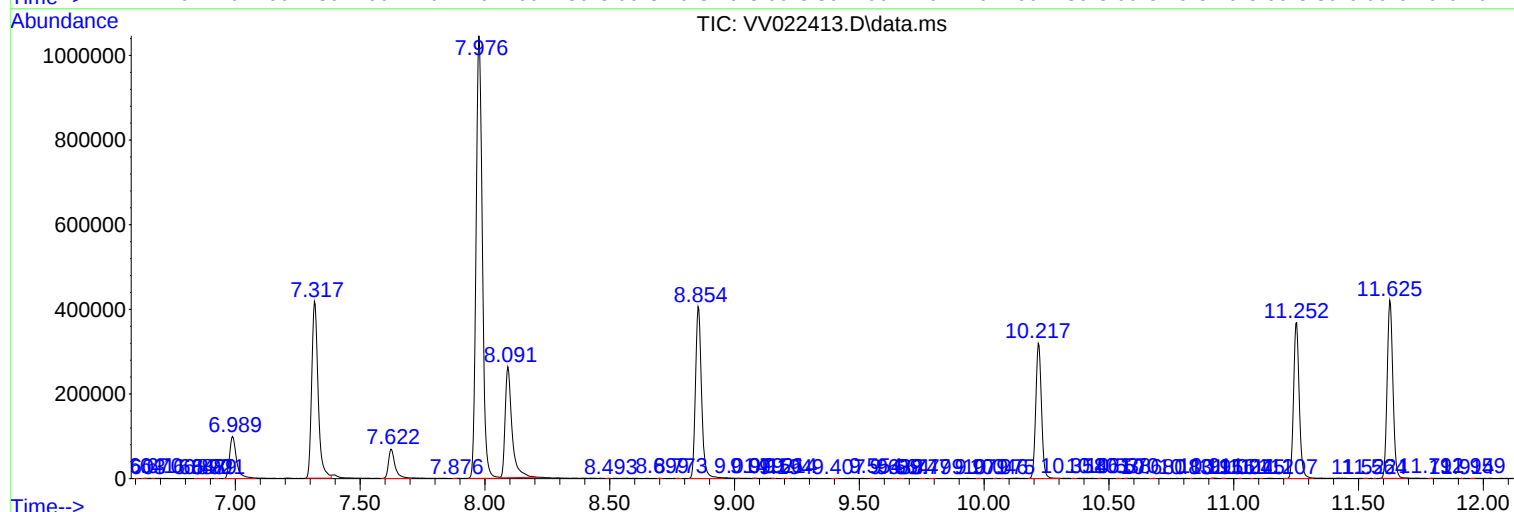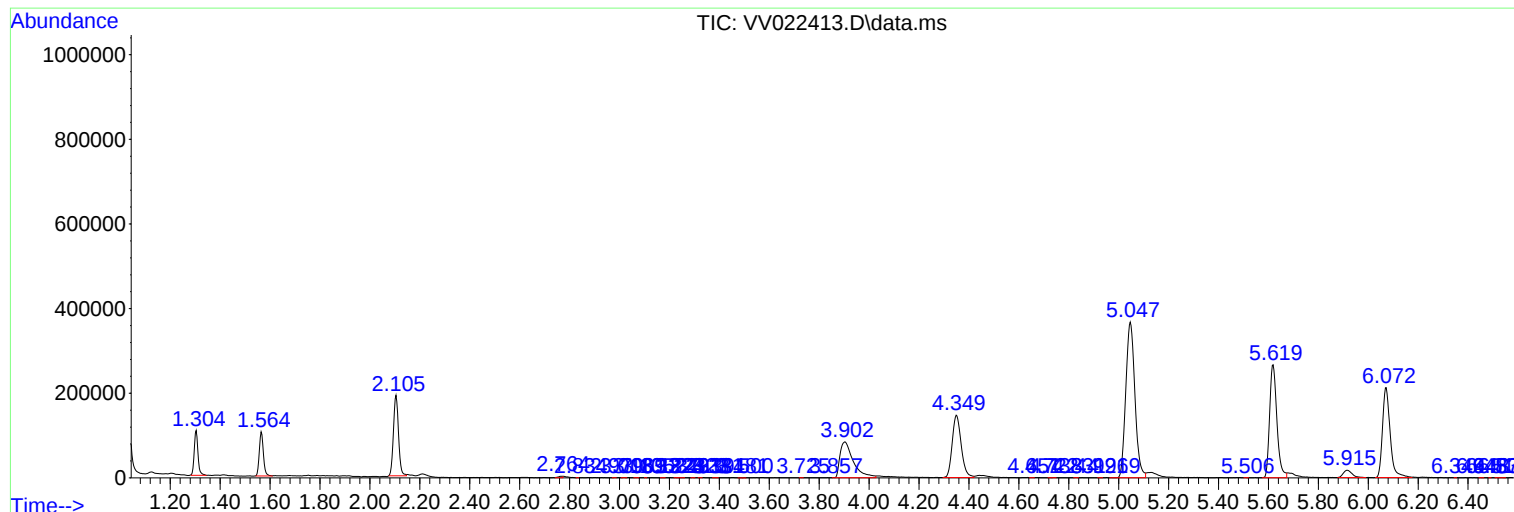

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022413.D
Acq On : 30 Sep 2021 05:45
Operator : SY/MD
Sample : M3978-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A49

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022413.D
Acq On : 30 Sep 2021 05:45
Operator : SY/MD
Sample : M3978-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A49

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
