

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022414.D
 Acq On : 30 Sep 2021 06:09
 Operator : SY/MD
 Sample : M3978-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A50

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M

Title : VOC Analysis

Signal : TIC: VV022414.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	98	rVB	105400	109921	6.04%	1.221%
2	1.565	156	163	180	rBV	100355	116227	6.39%	1.291%
3	2.105	321	331	343	rBV	192412	277511	15.26%	3.082%
4	2.603	483	486	487	rBV	507	286	0.02%	0.003%
5	2.690	511	513	517	rBV	415	239	0.01%	0.003%
6	2.841	557	560	563	rBV	375	247	0.01%	0.003%
7	2.902	575	579	583	rBV3	334	263	0.01%	0.003%
8	2.960	592	597	600	rBV2	307	317	0.02%	0.004%
9	3.092	632	638	640	rBV3	286	240	0.01%	0.003%
10	3.166	659	661	665	rBV	289	166	0.01%	0.002%
11	3.346	714	717	721	rBV2	250	194	0.01%	0.002%
12	3.420	734	740	744	rBV3	446	545	0.03%	0.006%
13	3.478	756	758	760	rBV	321	162	0.01%	0.002%
14	3.503	764	766	769	rBV3	270	153	0.01%	0.002%
15	3.629	802	805	808	rBV2	270	206	0.01%	0.002%
16	3.693	822	825	828	rBV3	264	184	0.01%	0.002%
17	3.722	832	834	838	rBV2	203	181	0.01%	0.002%
18	3.799	856	858	862	rVB2	342	143	0.01%	0.002%
19	3.828	865	867	873	rVB3	288	238	0.01%	0.003%
20	3.902	878	890	935	rBV	76358	289025	15.89%	3.210%
21	4.349	1015	1029	1053	rBV	148846	365810	20.11%	4.063%
22	4.597	1104	1106	1110	rBV3	586	462	0.03%	0.005%
23	4.725	1144	1146	1151	rVB4	357	223	0.01%	0.002%
24	4.873	1189	1192	1193	rBV	248	129	0.01%	0.001%
25	4.912	1202	1204	1206	rVB2	346	155	0.01%	0.002%
26	4.928	1206	1209	1211	rBV2	249	195	0.01%	0.002%
27	4.979	1221	1225	1229	rBV3	434	406	0.02%	0.005%
28	5.047	1229	1246	1291	rBV2	370466	976619	53.69%	10.847%
29	5.314	1327	1329	1330	rBV	346	140	0.01%	0.002%
30	5.381	1344	1350	1352	rBV2	611	563	0.03%	0.006%
31	5.417	1359	1361	1362	rBV	282	144	0.01%	0.002%
32	5.542	1396	1400	1402	rVB2	428	256	0.01%	0.003%
33	5.555	1402	1404	1407	rBV	302	209	0.01%	0.002%
34	5.619	1410	1424	1449	rBV	266900	555266	30.53%	6.167%
35	5.908	1505	1514	1532	rBV6	10954	27058	1.49%	0.301%
36	6.072	1551	1565	1592	rBV	211388	446431	24.54%	4.958%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022414.D
 Acq On : 30 Sep 2021 06:09
 Operator : SY/MD
 Sample : M3978-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A50

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

37	6.336	1646	1647	1651	rVB	277	128	0.01%	0.001%
38	6.420	1671	1673	1675	rBV	306	130	0.01%	0.001%
39	6.523	1702	1705	1708	rVB2	665	323	0.02%	0.004%
40	6.552	1708	1714	1717	rBV3	319	382	0.02%	0.004%
41	6.590	1724	1726	1731	rVB3	354	304	0.02%	0.003%
42	6.642	1740	1742	1744	rVV	452	233	0.01%	0.003%
43	6.667	1748	1750	1757	rVB4	453	459	0.03%	0.005%
44	6.712	1761	1764	1767	rBV3	459	257	0.01%	0.003%
45	6.799	1786	1791	1793	rBV2	286	238	0.01%	0.003%
46	6.851	1805	1807	1809	rBV	259	143	0.01%	0.002%
47	6.873	1812	1814	1817	rVB	172	114	0.01%	0.001%
48	6.889	1817	1819	1821	rBV	258	124	0.01%	0.001%
49	6.989	1838	1850	1872	rBV	100806	190663	10.48%	2.118%
50	7.214	1918	1920	1921	rBV2	490	180	0.01%	0.002%
51	7.262	1932	1935	1938	rVB2	334	228	0.01%	0.003%
52	7.317	1940	1952	1972	rBV	423086	752575	41.37%	8.358%
53	7.625	2037	2048	2073	rBV	69073	127794	7.03%	1.419%
54	7.863	2119	2122	2124	rBV2	342	174	0.01%	0.002%
55	7.905	2132	2135	2136	rBV2	230	125	0.01%	0.001%
56	7.976	2143	2157	2183	rBV	1066527	1818991	100.00%	20.203%
57	8.092	2184	2193	2227	rVB	265107	498339	27.40%	5.535%
58	8.410	2290	2292	2294	rBV2	425	200	0.01%	0.002%
59	8.426	2294	2297	2301	rBV4	705	469	0.03%	0.005%
60	8.487	2315	2316	2320	rBV2	257	112	0.01%	0.001%
61	8.709	2383	2385	2391	rVB5	622	518	0.03%	0.006%
62	8.738	2391	2394	2395	rBV	237	138	0.01%	0.002%
63	8.854	2416	2430	2459	rBV	397549	678470	37.30%	7.535%
64	9.092	2502	2504	2506	rBV2	299	122	0.01%	0.001%
65	9.124	2512	2514	2516	rBV	221	138	0.01%	0.002%
66	9.185	2529	2533	2536	rBV2	503	358	0.02%	0.004%
67	9.207	2537	2540	2542	rBV3	532	361	0.02%	0.004%
68	9.391	2595	2597	2600	rBV2	315	169	0.01%	0.002%
69	9.487	2624	2627	2629	rBV2	330	180	0.01%	0.002%
70	9.513	2629	2635	2639	rBV2	404	418	0.02%	0.005%
71	9.670	2682	2684	2685	rBV2	306	132	0.01%	0.001%
72	9.821	2729	2731	2732	rBV	338	106	0.01%	0.001%
73	10.079	2809	2811	2813	rBV	405	201	0.01%	0.002%
74	10.124	2823	2825	2832	rVB3	575	473	0.03%	0.005%
75	10.217	2842	2854	2874	rBV	317928	503616	27.69%	5.593%
76	10.593	2969	2971	2974	rBV	199	137	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022414.D
 Acq On : 30 Sep 2021 06:09
 Operator : SY/MD
 Sample : M3978-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A50

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

77	10.609	2974	2976	2979	rBV2	271	168	0.01%	0.002%
78	10.657	2989	2991	2993	rBV	267	141	0.01%	0.002%
79	10.712	3006	3008	3012	rVB2	267	142	0.01%	0.002%
80	10.767	3023	3025	3026	rBV	333	171	0.01%	0.002%
81	10.802	3035	3036	3039	rVB2	271	124	0.01%	0.001%
82	10.921	3069	3073	3078	rBV3	875	853	0.05%	0.009%
83	11.018	3101	3103	3107	rBV2	238	168	0.01%	0.002%
84	11.059	3113	3116	3119	rBV	337	232	0.01%	0.003%
85	11.201	3158	3160	3162	rBV2	288	189	0.01%	0.002%
86	11.252	3164	3176	3199	rVV	368082	575648	31.65%	6.393%
87	11.461	3238	3241	3242	rBV	251	169	0.01%	0.002%
88	11.500	3251	3253	3255	rVB2	458	162	0.01%	0.002%
89	11.625	3280	3292	3315	rBV	424948	674560	37.08%	7.492%
90	12.603	3594	3596	3600	rBV2	256	241	0.01%	0.003%
91	12.828	3664	3666	3670	rBV	240	149	0.01%	0.002%
92	12.860	3673	3676	3677	rBV	300	144	0.01%	0.002%
93	12.905	3688	3690	3693	rVB2	339	174	0.01%	0.002%
94	13.117	3753	3756	3761	rBB3	402	320	0.02%	0.004%
95	13.156	3767	3768	3770	rBV3	216	106	0.01%	0.001%
96	13.706	3937	3939	3942	rVB2	333	135	0.01%	0.001%
97	13.911	4001	4003	4004	rBV	388	115	0.01%	0.001%
98	14.149	4075	4077	4082	rVB	424	240	0.01%	0.003%
99	14.210	4094	4096	4101	rBV	322	236	0.01%	0.003%
100	14.294	4119	4122	4128	rVB2	615	394	0.02%	0.004%




Sum of corrected areas: 9003717

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022414.D
Acq On : 30 Sep 2021 06:09
Operator : SY/MD
Sample : M3978-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A50

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

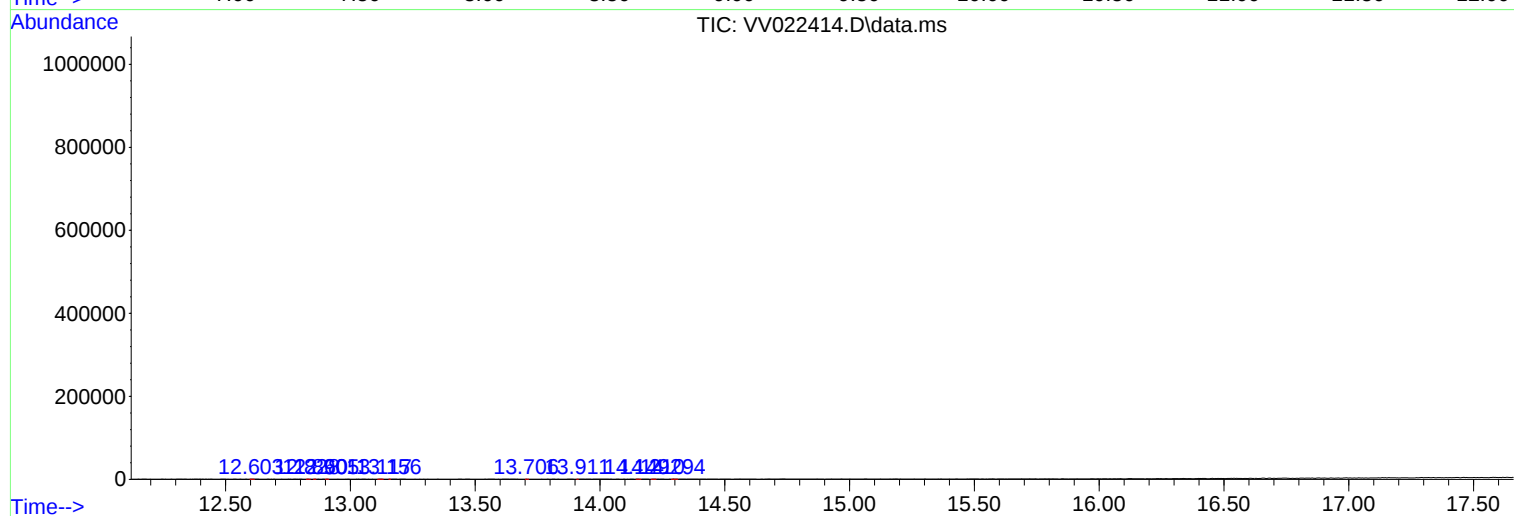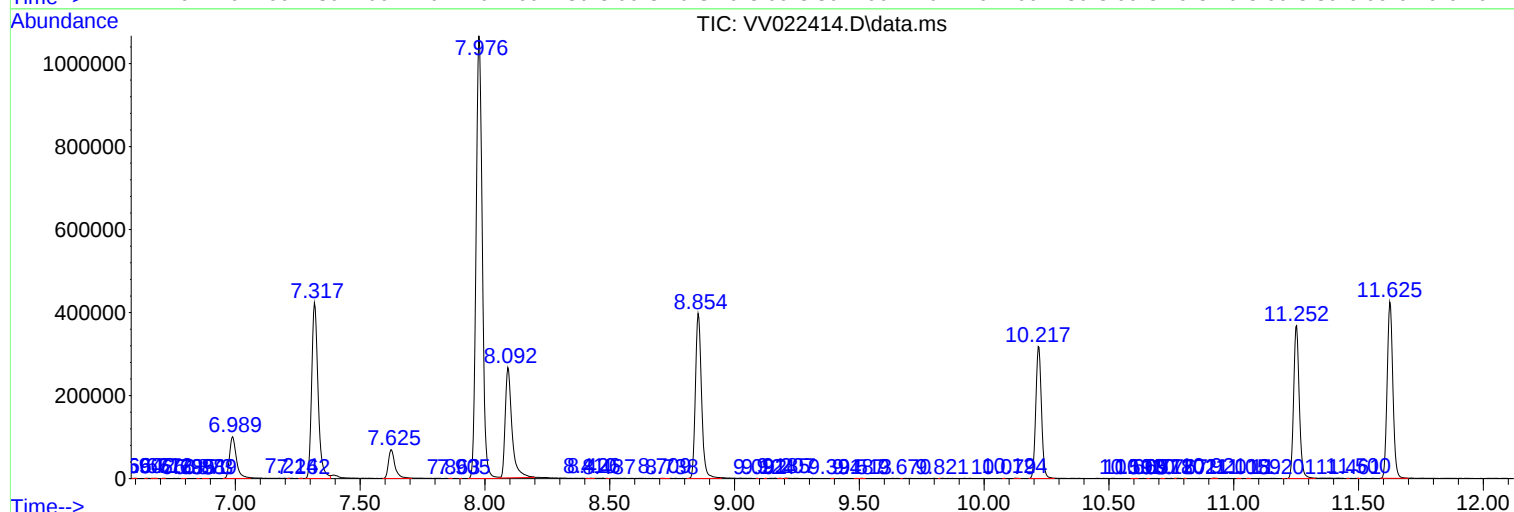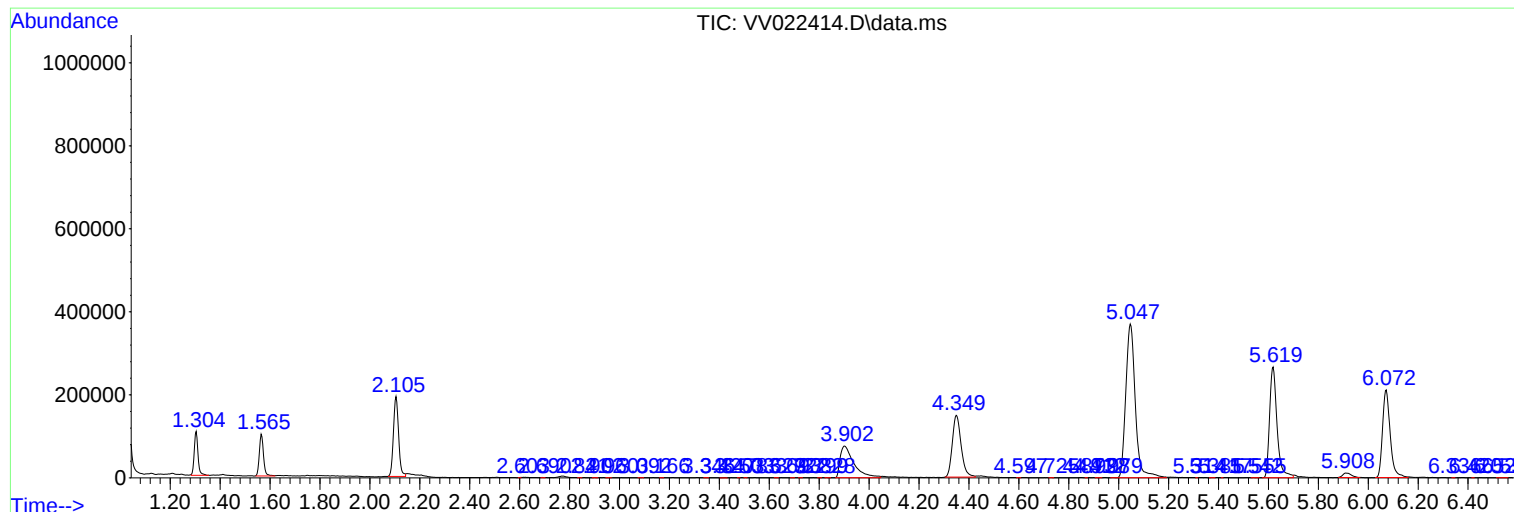

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022414.D
Acq On : 30 Sep 2021 06:09
Operator : SY/MD
Sample : M3978-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A50

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022414.D
Acq On : 30 Sep 2021 06:09
Operator : SY/MD
Sample : M3978-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A50

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
