

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022416.D
 Acq On : 30 Sep 2021 06:57
 Operator : SY/MD
 Sample : M3978-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A56

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

Signal : TIC: VV022416.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	101	rVB	113165	116893	12.25%	1.520%
2	1.564	157	163	174	rVB	104951	116015	12.16%	1.509%
3	2.105	322	331	360	rVB	197264	296748	31.10%	3.859%
4	2.580	476	479	481	rBV2	378	200	0.02%	0.003%
5	2.619	486	491	493	rBV3	313	260	0.03%	0.003%
6	2.728	521	525	528	rBV2	577	412	0.04%	0.005%
7	2.770	528	538	547	rVV7	2409	4156	0.44%	0.054%
8	2.879	571	572	578	rVB	434	354	0.04%	0.005%
9	3.008	609	612	615	rBV3	371	347	0.04%	0.005%
10	3.024	615	617	620	rVB3	522	237	0.02%	0.003%
11	3.117	644	646	651	rBV2	251	190	0.02%	0.002%
12	3.214	672	676	679	rBV2	375	243	0.03%	0.003%
13	3.317	702	708	709	rBV	285	218	0.02%	0.003%
14	3.375	724	726	730	rBV2	275	216	0.02%	0.003%
15	3.510	765	768	770	rBV3	305	165	0.02%	0.002%
16	3.680	816	821	823	rBV2	567	317	0.03%	0.004%
17	3.754	839	844	847	rVB2	307	249	0.03%	0.003%
18	3.783	847	853	856	rBV2	312	336	0.04%	0.004%
19	3.799	856	858	862	rVB	403	178	0.02%	0.002%
20	3.892	876	887	926	rBV2	73415	240641	25.22%	3.129%
21	4.349	1014	1029	1054	rBV	154142	378073	39.62%	4.916%
22	4.635	1117	1118	1122	rVB2	395	255	0.03%	0.003%
23	4.658	1122	1125	1128	rVB2	357	229	0.02%	0.003%
24	4.905	1198	1202	1204	rBV3	490	363	0.04%	0.005%
25	4.947	1208	1215	1217	rBV2	487	481	0.05%	0.006%
26	4.982	1224	1226	1229	rBV2	421	248	0.03%	0.003%
27	5.047	1229	1246	1268	rBV2	375216	954322	100.00%	12.409%
28	5.404	1355	1357	1358	rBV2	370	164	0.02%	0.002%
29	5.449	1369	1371	1375	rVB2	481	253	0.03%	0.003%
30	5.471	1375	1378	1380	rBV2	301	186	0.02%	0.002%
31	5.548	1397	1402	1404	rBV2	427	211	0.02%	0.003%
32	5.619	1410	1424	1441	rBV	271528	553974	58.05%	7.203%
33	5.915	1504	1516	1536	rBV7	18748	46138	4.83%	0.600%
34	6.072	1549	1565	1603	rBV	216335	460481	48.25%	5.987%
35	6.294	1630	1634	1637	rBV3	371	334	0.03%	0.004%
36	6.362	1652	1655	1658	rBV3	395	229	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022416.D
 Acq On : 30 Sep 2021 06:57
 Operator : SY/MD
 Sample : M3978-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A56

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

37	6.426	1673	1675	1677	rBV	354	181	0.02%	0.002%
38	6.596	1727	1728	1734	rVB2	242	211	0.02%	0.003%
39	6.622	1734	1736	1737	rBV	414	178	0.02%	0.002%
40	6.706	1760	1762	1765	rVV2	389	169	0.02%	0.002%
41	6.731	1767	1770	1772	rBV2	260	169	0.02%	0.002%
42	6.899	1816	1822	1825	rBV3	234	242	0.03%	0.003%
43	6.924	1826	1830	1831	rVV	331	202	0.02%	0.003%
44	6.989	1839	1850	1875	rBV	101161	192745	20.20%	2.506%
45	7.227	1919	1924	1927	rBV4	537	445	0.05%	0.006%
46	7.317	1940	1952	1974	rBV	422938	764194	80.08%	9.937%
47	7.625	2035	2048	2071	rBV	68796	128715	13.49%	1.674%
48	7.792	2098	2100	2104	rVB3	416	221	0.02%	0.003%
49	7.976	2138	2157	2179	rBV	257750	454494	47.62%	5.910%
50	8.091	2183	2193	2225	rBV	259634	484194	50.74%	6.296%
51	8.397	2285	2288	2294	rVB4	445	486	0.05%	0.006%
52	8.616	2354	2356	2360	rVB2	532	332	0.03%	0.004%
53	8.645	2360	2365	2369	rBV3	369	398	0.04%	0.005%
54	8.683	2374	2377	2385	rBV5	460	586	0.06%	0.008%
55	8.744	2391	2396	2401	rBV4	408	461	0.05%	0.006%
56	8.854	2419	2430	2459	rBV	410271	694841	72.81%	9.035%
57	9.037	2485	2487	2492	rVB3	530	285	0.03%	0.004%
58	9.185	2530	2533	2537	rBV3	403	279	0.03%	0.004%
59	9.339	2577	2581	2583	rVB3	285	190	0.02%	0.002%
60	9.368	2587	2590	2592	rVV2	297	181	0.02%	0.002%
61	9.390	2595	2597	2601	rBV2	391	207	0.02%	0.003%
62	9.455	2614	2617	2620	rBV2	324	239	0.03%	0.003%
63	9.477	2620	2624	2626	rBV3	220	184	0.02%	0.002%
64	9.731	2696	2703	2705	rBV3	231	208	0.02%	0.003%
65	9.802	2722	2725	2727	rVB2	350	177	0.02%	0.002%
66	9.899	2751	2755	2758	rBV2	241	208	0.02%	0.003%
67	9.998	2782	2786	2788	rVB2	337	201	0.02%	0.003%
68	10.124	2821	2825	2827	rBV4	767	600	0.06%	0.008%
69	10.217	2843	2854	2876	rBV	319974	505838	53.00%	6.577%
70	10.583	2966	2968	2970	rBV	461	199	0.02%	0.003%
71	10.625	2976	2981	2982	rBV3	277	205	0.02%	0.003%
72	10.677	2994	2997	2999	rBV	306	183	0.02%	0.002%
73	10.860	3051	3054	3062	rBV3	289	319	0.03%	0.004%
74	10.892	3062	3064	3066	rBV	397	182	0.02%	0.002%
75	10.918	3070	3072	3078	rVV4	830	642	0.07%	0.008%
76	11.027	3104	3106	3109	rBV3	320	175	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022416.D
 Acq On : 30 Sep 2021 06:57
 Operator : SY/MD
 Sample : M3978-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A56

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M

Title : VOC Analysis

77	11.252	3163	3176	3195	rBV	376219	591377	61.97%	7.689%
78	11.397	3218	3221	3223	rVB4	808	334	0.03%	0.004%
79	11.542	3259	3266	3273	rBV5	1548	2513	0.26%	0.033%
80	11.625	3281	3292	3316	rBV	426257	682687	71.54%	8.877%
81	11.850	3358	3362	3363	rBV2	477	314	0.03%	0.004%
82	11.908	3376	3380	3384	rBV3	348	357	0.04%	0.005%
83	11.947	3386	3392	3394	rBV3	376	420	0.04%	0.005%
84	12.123	3445	3447	3450	rVB	335	184	0.02%	0.002%
85	12.265	3489	3491	3496	rBV2	315	256	0.03%	0.003%
86	12.291	3497	3499	3503	rBV2	256	209	0.02%	0.003%
87	12.332	3509	3512	3517	rBV2	523	460	0.05%	0.006%
88	12.455	3545	3550	3555	rBV2	321	309	0.03%	0.004%
89	12.490	3558	3561	3563	rBV	344	188	0.02%	0.002%
90	12.892	3683	3686	3688	rBV2	242	182	0.02%	0.002%
91	13.001	3716	3720	3722	rBV2	304	206	0.02%	0.003%
92	13.146	3761	3765	3768	rBV2	203	178	0.02%	0.002%
93	13.381	3832	3838	3840	rBV3	371	392	0.04%	0.005%
94	13.606	3906	3908	3912	rBV2	393	279	0.03%	0.004%
95	13.693	3931	3935	3936	rVB	362	190	0.02%	0.002%
96	13.889	3993	3996	4002	rVB2	588	333	0.03%	0.004%
97	13.921	4004	4006	4011	rVB2	255	174	0.02%	0.002%
98	14.046	4042	4045	4048	rBV3	356	250	0.03%	0.003%
99	14.172	4082	4084	4087	rBV2	359	235	0.02%	0.003%
100	14.590	4211	4214	4215	rBV	425	203	0.02%	0.003%




Sum of corrected areas: 7690712

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022416.D
Acq On : 30 Sep 2021 06:57
Operator : SY/MD
Sample : M3978-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A56

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

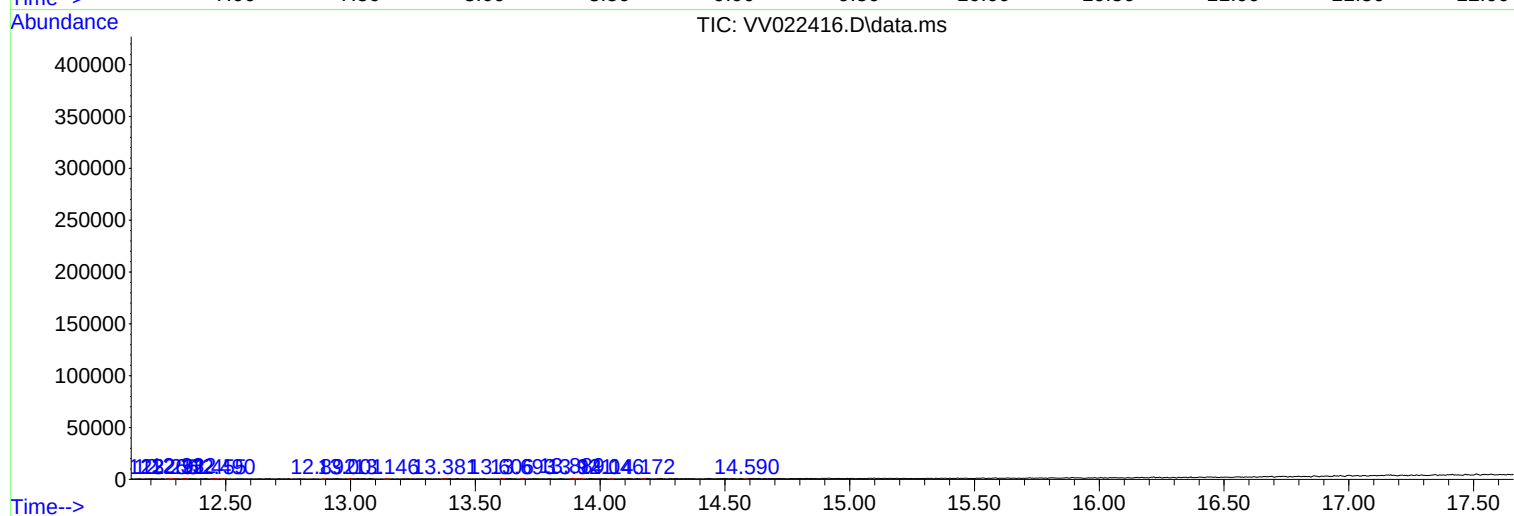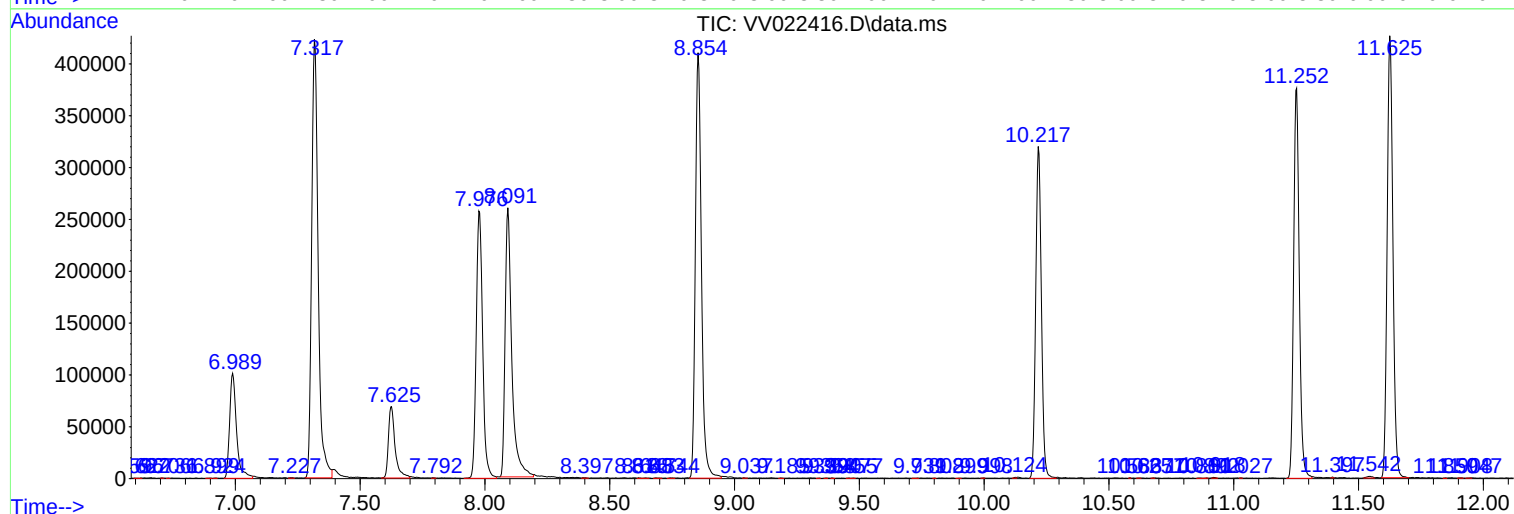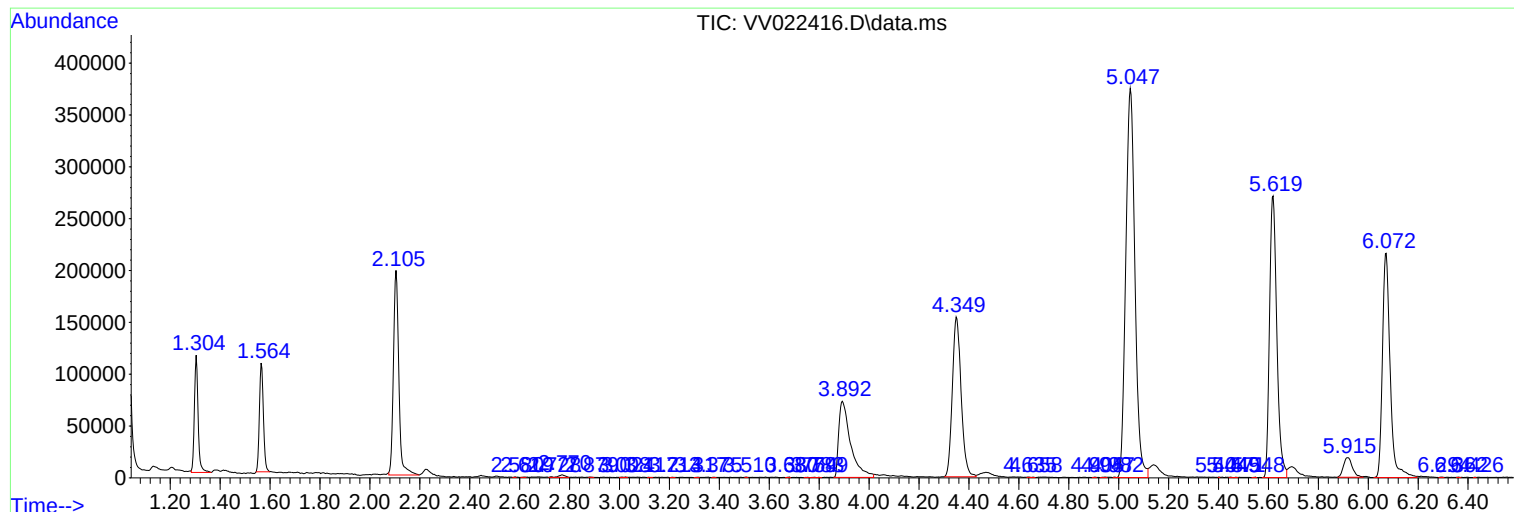

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022416.D
Acq On : 30 Sep 2021 06:57
Operator : SY/MD
Sample : M3978-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A56

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
Data File : VV022416.D
Acq On : 30 Sep 2021 06:57
Operator : SY/MD
Sample : M3978-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A56

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
