


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092921\
 Data File : VV022370.D
 Acq On : 29 Sep 2021 11:41
 Operator : SY/MD
 Sample : BFB237
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB237

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis
 Last Update : Thu Sep 30 06:55:59 2021

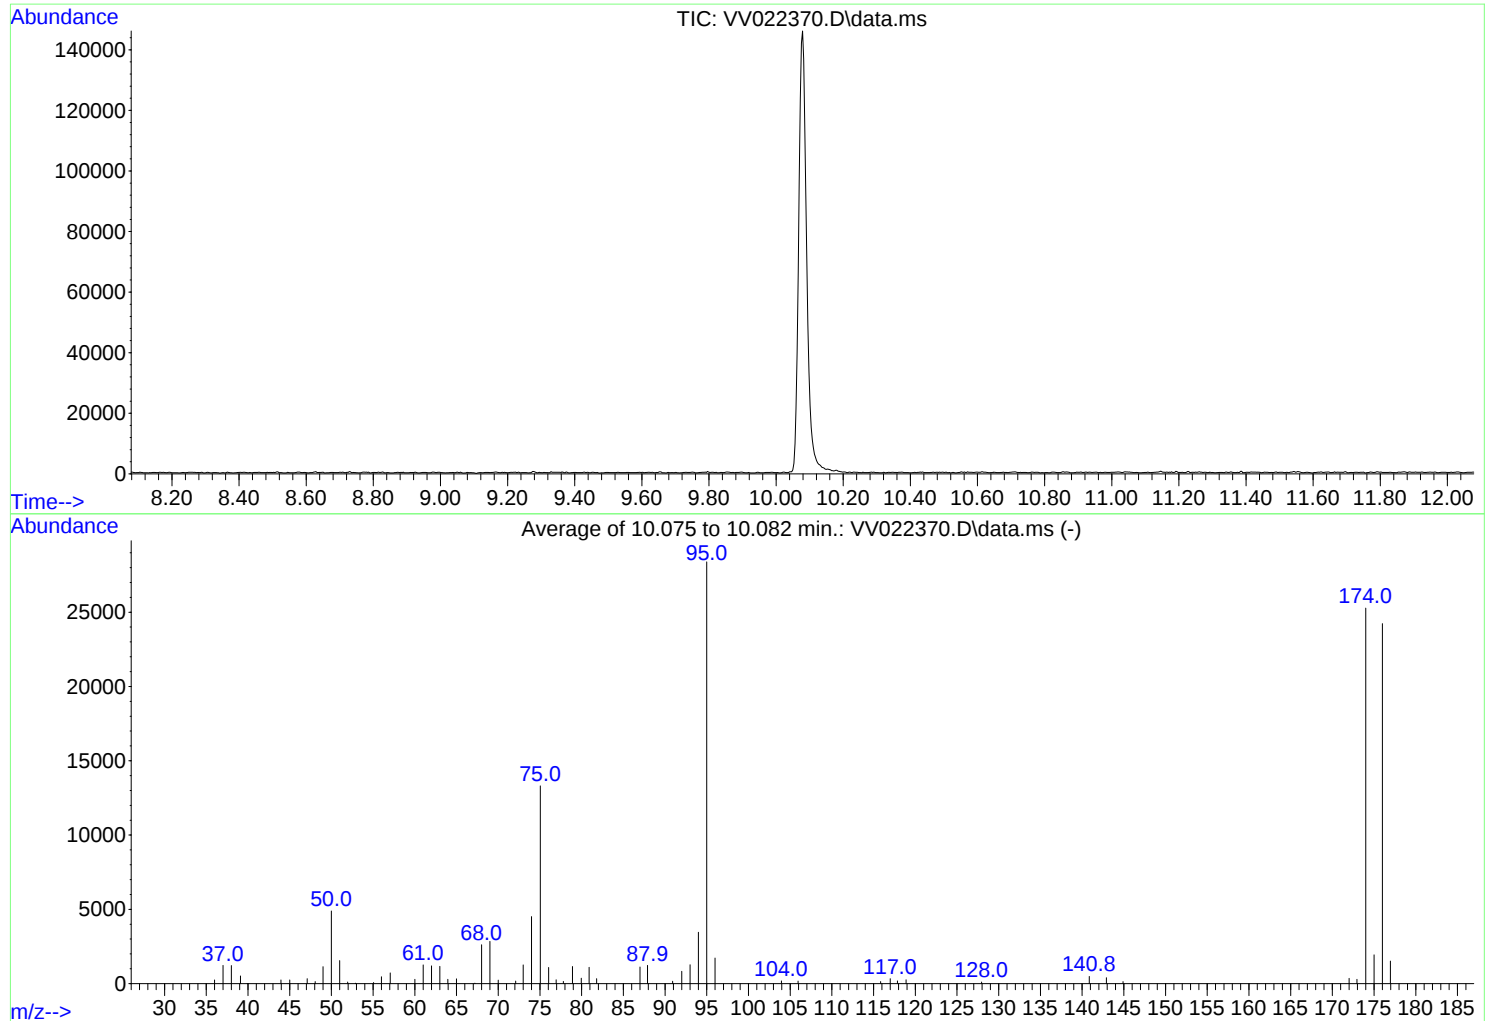

AutoFind: Scans 2810, 2811, 2812; Background Corrected with Scan 2799

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	4884	PASS
75	95	30	80	46.9	13313	PASS
95	95	100	100	100.0	28389	PASS
96	95	5	9	6.1	1723	PASS
173	174	0.00	2	1.1	288	PASS
174	95	50	120	89.0	25280	PASS
175	174	5	9	7.7	1941	PASS
176	174	95	105	95.9	24232	PASS
177	176	5	10	6.3	1522	PASS

m/z	Abundance
36.60	110.0
39.90	172.0
44.00	284.0
57.60	107.0

Instrument :
MSVOA_V
ClientSampleId :
BFB237

m/z	Abundance
36.00	219.0
37.00	1317.0
38.00	1183.0
39.10	535.0
39.90	161.0
43.90	547.0
45.00	256.0
47.10	311.0
48.00	134.0
49.00	1276.0
50.00	5224.0
51.00	1562.0
52.00	106.0
52.90	100.0
55.00	125.0
56.00	505.0
57.10	728.0
60.00	281.0
61.00	1237.0
62.00	1318.0
63.00	1297.0
63.90	289.0
65.00	338.0
67.20	115.0
68.00	2595.0
69.00	2943.0
70.00	231.0
72.10	215.0
73.00	1275.0
74.00	4420.0
75.00	13633.0
76.00	1177.0
76.90	281.0
77.80	182.0
78.90	1141.0
80.00	349.0
80.90	1031.0
81.80	350.0
87.00	1181.0
87.90	1124.0
90.90	169.0
92.00	793.0
93.00	1307.0
94.00	3453.0
95.00	28920.0
96.00	1751.0
103.90	159.0
105.90	147.0
116.00	126.0
117.00	383.0
117.80	162.0
118.90	250.0
128.00	107.0
140.90	438.0
142.90	368.0
144.90	130.0
172.00	322.0
173.00	269.0
174.00	24472.0
175.00	1916.0
176.00	23696.0
177.00	1539.0

Instrument :
MSVOA_V
ClientSampleId :
BFB237

m/z	Abundance
36.00	247.0
37.00	1269.0
38.00	1252.0
39.10	532.0
39.90	168.0
44.00	555.0
45.00	250.0
47.10	328.0
48.10	143.0
49.00	1186.0
50.00	4983.0
51.00	1611.0
52.00	108.0
55.10	110.0
56.00	467.0
57.10	762.0
60.00	312.0
61.00	1273.0
62.00	1223.0
63.00	1175.0
64.00	323.0
65.00	316.0
68.00	2728.0
69.00	2928.0
70.00	249.0
72.10	183.0
73.00	1258.0
74.00	4729.0
75.00	13677.0
76.10	1095.0
77.00	264.0
77.80	151.0
78.90	1179.0
79.90	386.0
80.90	1124.0
81.80	353.0
87.00	1161.0
87.90	1247.0
90.90	151.0
92.00	855.0
93.00	1297.0
94.00	3575.0
95.00	29248.0
96.00	1786.0
104.00	182.0
106.00	173.0
115.80	147.0
117.00	346.0
117.80	190.0
118.90	271.0
128.00	113.0
140.80	520.0
142.90	396.0
144.90	149.0
172.00	373.0
172.90	300.0
174.00	26160.0
175.00	1991.0
176.00	25112.0
177.00	1562.0

Instrument :
MSVOA_V
ClientSampleId :
BFB237

m/z	Abundance
36.00	263.0
37.00	1095.0
38.00	1211.0
39.10	493.0
39.90	190.0
44.00	494.0
45.00	245.0
47.10	368.0
48.00	145.0
49.00	970.0
50.00	4445.0
51.00	1466.0
51.90	103.0
56.00	404.0
57.00	691.0
60.00	296.0
61.00	1257.0
62.00	1057.0
63.00	1011.0
64.00	256.0
65.00	306.0
68.00	2539.0
69.00	2659.0
70.00	228.0
72.00	131.0
73.00	1232.0
74.00	4388.0
75.10	12630.0
76.10	987.0
77.00	232.0
77.80	134.0
78.90	1125.0
79.90	354.0
80.90	1153.0
81.80	297.0
87.00	1017.0
87.90	1310.0
90.90	174.0
92.00	843.0
93.00	1217.0
94.00	3356.0
95.00	27000.0
96.00	1632.0
104.00	195.0
106.00	194.0
115.80	143.0
117.00	269.0
117.90	184.0
118.90	255.0
127.90	119.0
140.80	504.0
142.90	437.0
144.90	139.0
172.00	357.0
172.90	295.0
174.00	25208.0
175.00	1917.0
176.00	23888.0
176.90	1466.0

Instrument :
MSVOA_V
ClientSampleId :
BFB237