
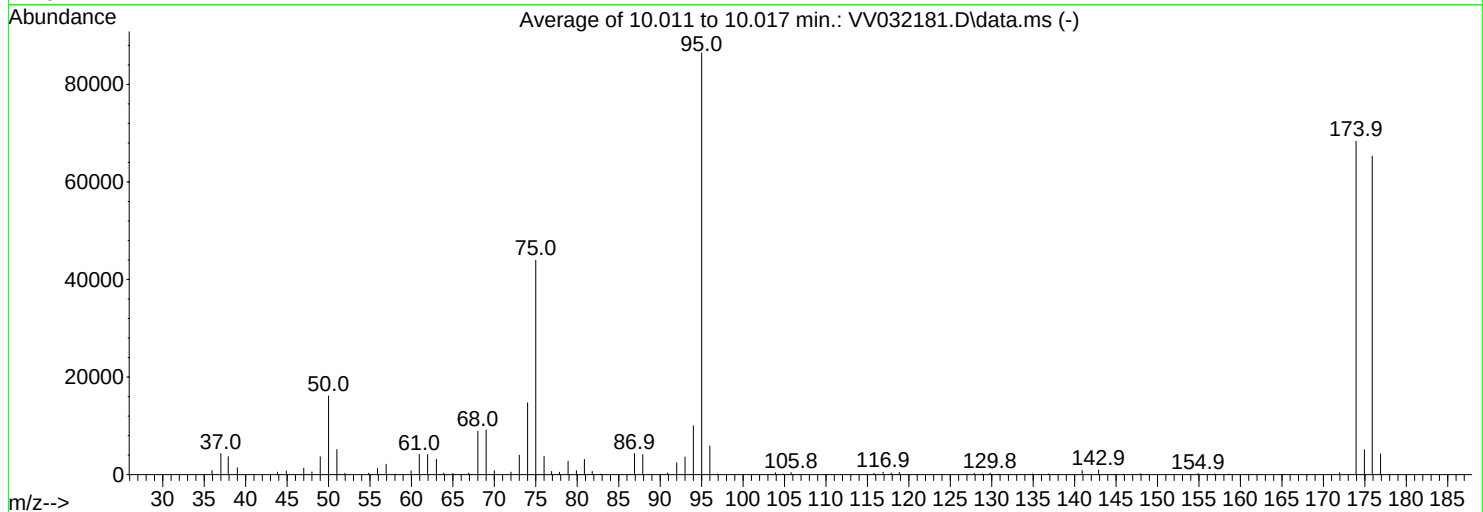


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092923\
 Data File : VV032181.D
 Acq On : 29 Sep 2023 08:54
 Operator : SY/MD
 Sample : BFB213
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB213

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Sat Sep 30 04:24:05 2023

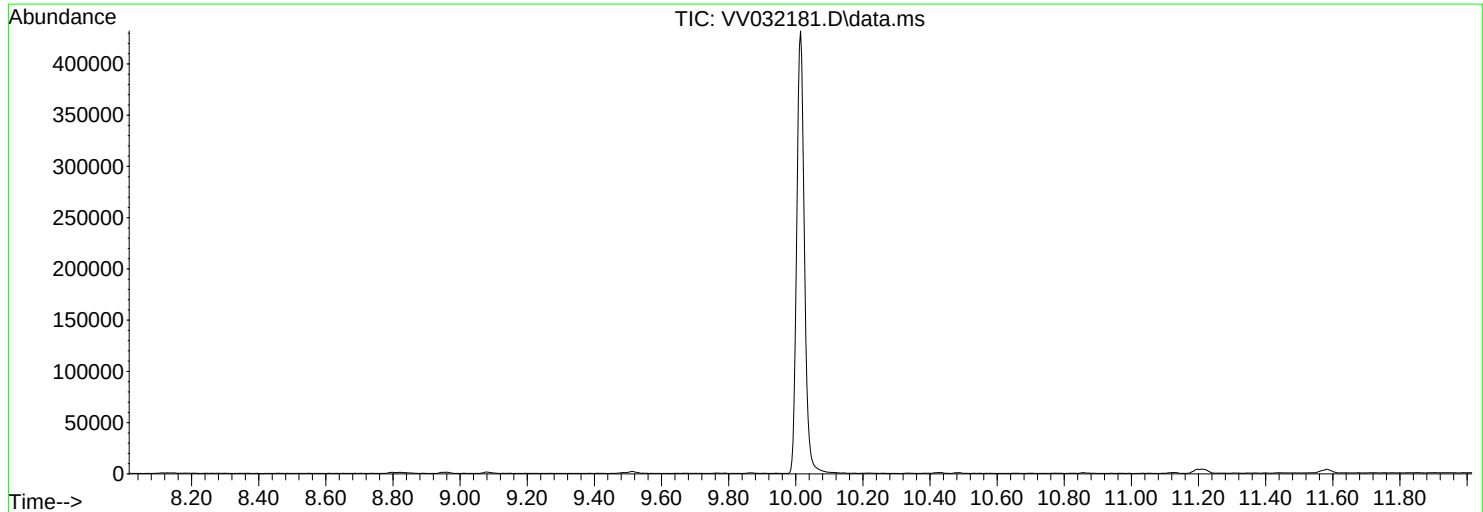

AutoFind: Scans 2790, 2791, 2792; Background Corrected with Scan 2778

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.7	16136	PASS
75	95	30	80	50.8	43939	PASS
95	95	100	100	100.0	86461	PASS
96	95	5	9	6.8	5875	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	79.1	68355	PASS
175	174	5	9	7.5	5119	PASS
176	174	95	105	95.5	65301	PASS
177	176	5	10	6.5	4236	PASS

m/z	Abundance
40.00	166.0
43.80	314.0

Instrument :
MSVOA_V
ClientSampleId :
BFB213

m/z	Abundance
36.00	894.0
37.00	4424.0
37.90	3758.0
39.00	1386.0
39.90	211.0
43.90	803.0
44.90	759.0
47.00	1377.0
48.00	542.0
49.00	3829.0
50.00	16672.0
51.00	5374.0
52.00	261.0
54.90	314.0
55.90	1351.0
56.90	2114.0
58.00	146.0
60.00	844.0
60.90	4316.0
61.90	4065.0
63.00	3198.0
63.90	323.0
65.00	294.0
66.90	335.0
68.00	8858.0
69.00	9199.0
70.00	800.0
72.00	515.0
73.00	4092.0
74.00	14727.0
75.00	44488.0
76.00	3837.0
76.90	631.0
77.80	526.0
78.90	2874.0
79.90	849.0
80.90	3114.0
81.80	641.0
82.90	124.0
86.90	4440.0
87.90	4180.0
90.90	376.0
92.00	2406.0
93.00	3481.0
94.00	10194.0
95.00	86152.0
96.00	5875.0
96.90	163.0
103.90	386.0
104.80	143.0
105.80	389.0
106.80	102.0
115.80	291.0
116.90	541.0
117.90	351.0
118.90	459.0
127.90	298.0
128.90	138.0
129.80	334.0
130.80	128.0
134.90	176.0
136.90	190.0
140.90	869.0
142.90	964.0
144.90	134.0
145.90	155.0
147.90	206.0
148.80	113.0
154.90	287.0
156.90	165.0
158.60	124.0
160.90	101.0
171.90	411.0
174.00	66432.0
174.90	5084.0
175.90	63568.0
176.90	4203.0
177.90	141.0

Instrument :
MSVOA_V
ClientSampleId :
BFB213

m/z	Abundance
36.00	902.0
37.00	4446.0
37.90	3822.0
39.00	1454.0
39.90	195.0
43.90	851.0
44.90	788.0
45.90	108.0
47.00	1412.0
48.00	587.0
49.00	3827.0
50.00	16616.0
51.00	5305.0
51.90	244.0
54.90	287.0
55.90	1369.0
56.90	2204.0
58.10	142.0
60.00	806.0
61.00	4265.0
62.00	4202.0
63.00	3245.0
63.90	328.0
65.00	284.0
66.90	342.0
68.00	9221.0
69.00	9517.0
70.00	842.0
72.00	531.0
73.00	4124.0
74.00	15210.0
75.00	45224.0
76.00	3849.0
76.90	706.0
77.80	513.0
78.90	2851.0
79.90	820.0
80.90	3219.0
81.80	679.0
82.80	129.0
86.90	4486.0
87.90	4271.0
90.90	379.0
92.00	2495.0
93.00	3725.0
94.00	10255.0
95.00	89384.0
96.00	6074.0
96.90	174.0
103.90	398.0
104.80	152.0
105.80	437.0
115.80	317.0
116.90	509.0
117.80	327.0
118.80	476.0
127.90	315.0
128.80	151.0
129.80	346.0
130.90	129.0
134.90	171.0
136.90	168.0
140.90	885.0
142.00	106.0
142.90	989.0
144.80	112.0
145.90	154.0
147.90	213.0
154.90	259.0
156.90	165.0
158.60	128.0
161.00	109.0
171.90	402.0
174.00	70712.0
174.90	5254.0
175.90	67560.0
176.90	4366.0
177.90	117.0

Instrument :
MSVOA_V
ClientSampleId :
BFB213

m/z	Abundance
35.90	816.0
37.00	4098.0
37.90	3498.0
39.00	1399.0
39.90	189.0
43.90	857.0
44.90	750.0
46.00	111.0
47.00	1276.0
48.00	536.0
49.00	3390.0
50.00	15121.0
51.00	4818.0
51.90	217.0
54.80	249.0
55.90	1255.0
57.00	2111.0
58.10	128.0
59.90	695.0
61.00	3805.0
62.00	3997.0
63.00	2980.0
63.90	309.0
65.00	257.0
66.90	297.0
68.00	8625.0
69.00	8822.0
70.00	811.0
72.00	519.0
73.00	3791.0
74.00	14276.0
75.00	42104.0
76.00	3541.0
76.90	655.0
77.90	413.0
78.90	2539.0
79.90	782.0
80.80	2986.0
81.80	669.0
82.90	116.0
86.90	4069.0
87.90	3823.0
90.90	338.0
92.00	2357.0
93.00	3640.0
94.00	9572.0
95.00	83848.0
96.00	5677.0
96.90	162.0
103.90	397.0
104.90	144.0
105.80	423.0
110.70	103.0
111.80	102.0
114.90	104.0
115.80	327.0
116.90	469.0
117.80	305.0
118.80	447.0
127.90	301.0
128.80	133.0
129.80	327.0
130.90	132.0
134.90	144.0
136.80	132.0
140.90	794.0
142.00	105.0
142.90	954.0
145.90	125.0
147.90	178.0
154.90	227.0
156.90	143.0
158.60	107.0
160.90	107.0
172.00	368.0
173.90	67920.0
175.00	5019.0
175.90	64776.0
176.90	4139.0

Instrument :
MSVOA_V
ClientSampleId :
BFB213