


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093019\
Data File : VV013009.D
Acq On : 30 Sep 2019 09:25
Operator : SY/MD
Sample : BFB62
Misc : 5.00G/10ML/MSVOA_V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB62

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SFAMVLM093019SMA.M
Title : VOC Analysis
Last Update : Mon Sep 30 13:17:58 2019

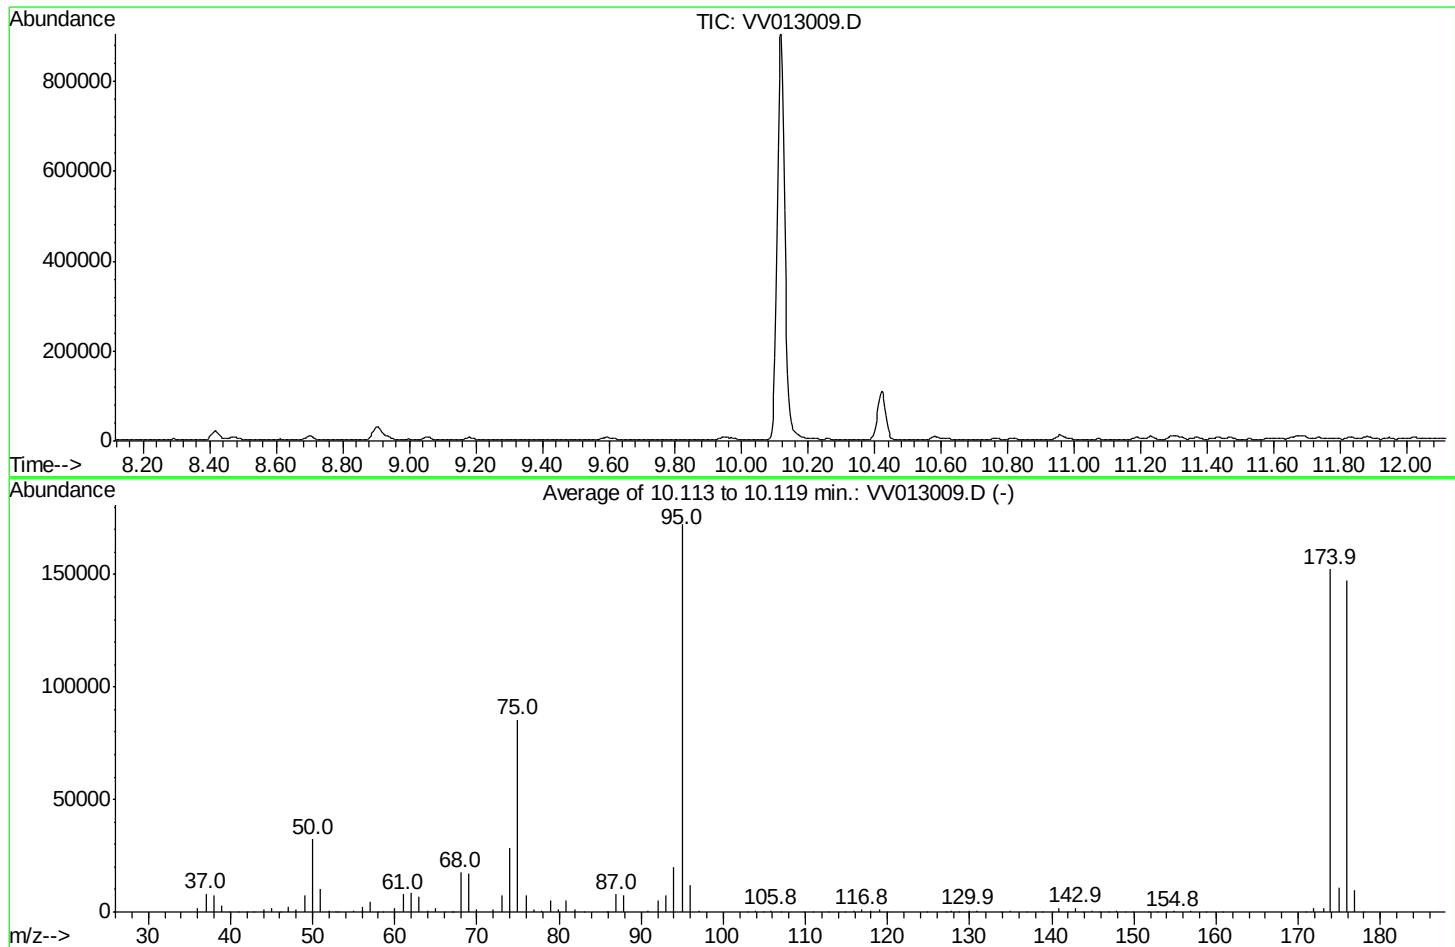

AutoFind: Scans 2806, 2807, 2808; Background Corrected with Scan 2794

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.8	32357	PASS
75	95	30	80	49.6	85536	PASS
95	95	100	100	100.0	172288	PASS
96	95	5	9	6.9	11819	PASS
173	174	0.00	2	1.2	1868	PASS
174	95	50	120	88.4	152320	PASS
175	174	5	9	7.1	10886	PASS
176	174	95	101	96.9	147605	PASS
177	176	5	9	6.4	9448	PASS

m/z	Abundance
36.00	1545.0
37.00	7897.0
38.00	7189.0
39.00	3015.0
39.90	1362.0
41.10	117.0
42.00	129.0
42.90	191.0
44.00	2008.0
45.00	1363.0
46.00	252.0
47.00	2510.0
48.00	1057.0
49.00	6562.0
50.00	30584.0
51.00	9971.0
52.00	469.0
53.10	190.0
55.00	552.0
56.00	2342.0
57.00	4396.0
58.00	229.0
60.00	1544.0
61.00	7758.0
62.00	7838.0
63.00	6342.0
64.00	821.0
65.00	1494.0
66.00	186.0
66.90	309.0
68.00	16608.0
69.00	15816.0
70.00	1284.0
72.00	944.0
73.00	7395.0
74.00	26248.0
75.00	79744.0
76.00	7247.0
77.00	896.0
78.00	880.0
78.90	4961.0
80.00	1310.0
80.90	4663.0
81.90	1157.0
83.00	107.0
85.80	163.0
87.00	7358.0
87.90	6831.0
90.80	531.0
92.00	4634.0
93.00	6865.0
94.00	17864.0
95.00	161856.0
96.00	11183.0
97.00	387.0
103.00	113.0
103.90	626.0
104.90	178.0
105.90	674.0
107.00	231.0
109.90	107.0
110.90	193.0
112.80	157.0
114.70	147.0
116.00	705.0
116.90	1061.0
117.90	596.0
119.00	885.0
127.10	106.0
127.80	451.0
128.70	189.0
129.90	537.0
130.80	259.0
133.80	113.0
134.90	396.0
136.90	285.0
138.80	121.0
140.00	119.0
140.90	1382.0
142.00	282.0
142.90	1801.0
143.80	205.0
144.90	463.0
145.80	170.0
146.80	166.0
147.80	484.0
149.90	167.0
151.80	165.0
154.00	171.0
154.90	367.0
156.90	332.0
158.80	216.0

Instrument :
MSVOA_V
ClientSampleId :
BFB62

160.80	177.0
170.80	259.0
171.90	1834.0
173.10	1659.0
173.90	137600.0
174.90	10158.0
175.90	133440.0
176.90	8575.0
177.90	227.0

Instrument :
MSVOA_V
ClientSampleId :
BFB62

m/z	Abundance
36.00	1643.0
37.00	8173.0
38.00	7801.0
39.00	3200.0
39.90	1349.0
41.00	170.0
42.00	167.0
42.90	172.0
44.00	2033.0
45.00	1617.0
46.10	253.0
47.00	2559.0
48.00	1061.0
49.00	7554.0
50.00	33472.0
51.00	10847.0
52.00	448.0
52.80	139.0
53.10	168.0
55.00	610.0
56.00	2554.0
57.00	4627.0
58.00	230.0
60.00	1767.0
61.00	8064.0
62.00	8611.0
63.00	6986.0
64.00	878.0
65.00	1572.0
66.00	222.0
67.10	323.0
68.00	18272.0
69.00	17616.0
70.00	1404.0
71.90	930.0
73.00	7766.0
74.00	29408.0
75.00	88504.0
76.00	7827.0
77.00	1044.0
78.00	836.0
78.90	5609.0
79.90	1381.0
80.90	5157.0
81.90	1331.0
82.90	149.0
85.80	192.0
86.10	189.0
87.00	8208.0
87.90	7476.0
90.90	625.0
92.00	5377.0
93.00	7687.0
94.00	20592.0
95.00	178112.0
96.00	12425.0
97.00	485.0
103.00	143.0
103.90	723.0
104.90	219.0
105.80	720.0
107.00	230.0
110.90	205.0
112.80	155.0
114.80	219.0
116.00	755.0
116.90	1155.0
118.00	625.0
118.90	1104.0
124.80	132.0
127.10	132.0
127.80	506.0
128.70	221.0
129.90	569.0
130.80	337.0
133.70	113.0
134.90	377.0
136.90	294.0
138.80	121.0
140.00	164.0
140.80	1704.0
142.00	298.0
142.90	2061.0
143.80	158.0
144.90	505.0
145.70	204.0
146.90	182.0
147.80	492.0
148.90	187.0
149.90	196.0
151.80	191.0
152.80	101.0

Instrument :
MSVOA_V
ClientSampleId :
BFB62

154.00	171.0
154.80	433.0
156.90	443.0
158.80	199.0
160.80	205.0
170.80	245.0
171.90	2016.0
173.10	1933.0
173.90	157056.0
174.90	11153.0
175.90	152320.0
176.90	9736.0
177.90	304.0

Instrument :
MSVOA_V
ClientSampleId :
BFB62

m/z	Abundance
36.00	1684.0
37.00	7858.0
38.00	7562.0
39.00	3103.0
39.90	1279.0
40.90	221.0
42.10	165.0
42.90	112.0
44.00	1912.0
45.00	1629.0
46.10	244.0
47.00	2443.0
48.00	1002.0
49.00	7463.0
50.00	33016.0
51.00	10696.0
52.00	382.0
52.80	160.0
55.00	640.0
56.00	2586.0
57.00	4354.0
58.00	224.0
58.60	124.0
60.00	1642.0
61.00	7666.0
62.00	8651.0
63.00	7007.0
64.10	878.0
65.00	1480.0
66.00	215.0
67.10	362.0
68.00	18000.0
69.00	17456.0
70.00	1420.0
71.90	942.0
73.00	7593.0
74.00	29376.0
75.00	88360.0
76.00	7599.0
77.00	1040.0
77.90	739.0
78.90	5611.0
79.90	1372.0
80.90	5297.0
81.90	1294.0
82.90	159.0
86.00	255.0
86.90	8188.0
87.90	7233.0
90.90	715.0
92.00	5357.0
93.00	7827.0
94.00	21152.0
95.00	176896.0
96.00	11851.0
97.00	489.0
102.90	149.0
103.90	790.0
104.90	248.0
105.80	817.0
106.90	192.0
110.90	183.0
112.90	123.0
114.80	240.0
115.90	671.0
116.80	1101.0
118.00	580.0
118.90	1172.0
119.90	104.0
124.80	134.0
127.00	126.0
127.80	533.0
128.70	256.0
129.90	657.0
130.80	328.0
134.90	365.0
136.90	287.0
140.00	189.0
140.90	1865.0
142.00	276.0
142.90	2082.0
144.90	572.0
145.70	234.0
147.00	183.0
147.80	413.0
148.90	233.0
149.80	209.0
151.80	183.0
154.00	126.0
154.80	463.0
156.90	467.0
158.80	179.0

Instrument :
MSVOA_V
ClientSampleId :
BFB62

160.80	231.0
170.90	230.0
171.90	1938.0
173.00	2014.0
173.90	162304.0
174.90	11349.0
175.90	157056.0
176.90	10034.0
177.90	337.0

Instrument :
MSVOA_V
ClientSampleId :
BFB62

Scan 2794 (10.074 min): VV013009.D
BFB62

m/z	Abundance
40.00	1170.0
41.00	160.0
44.00	883.0
206.90	123.0

Instrument :
MSVOA_V
ClientSampleId :
BFB62