

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV093020\
 Data File : VV018578.D
 Acq On : 30 Sep 2020 19:01
 Operator : SY/MD
 Sample : L4117-21
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AD0

Quant Time: Oct 01 09:23:43 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Oct 01 07:39:17 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	372431	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	362666	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	183982	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	76815	35.17	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	70.34%
7) Chloroethane-d5	1.58	69	78034	43.21	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	86.42%
11) 1,1-Dichloroethene-d2	2.12	63	132033	29.67	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	59.34%#
21) 2-Butanone-d5	3.92	46	154355	94.74	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	94.74%
24) Chloroform-d	4.38	84	191002	40.44	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	80.88%
26) 1,2-Dichloroethane-d4	5.06	65	129560	43.21	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	86.42%
32) Benzene-d6	5.07	84	379095	41.27	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	82.54%
36) 1,2-Dichloropropane-d6	6.09	67	123144	44.37	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	88.74%
41) Toluene-d8	7.34	98	339419	39.27	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	78.54%#
43) trans-1,3-Dichloropropene-	7.64	79	58891	39.28	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	78.56%
47) 2-Hexanone-d5	8.11	63	81758	77.55	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	77.55%
57) 1,1,2,2-Tetrachloroethane-	10.24	84	140414	38.16	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	76.32%
64) 1,2-Dichlorobenzene-d4	11.65	152	158826	44.89	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	89.78%


Target Compounds					Ovalue
13) Acetone	2.20	43	18877	13.411 ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV093020\
Data File : VV018578.D
Acq On : 30 Sep 2020 19:01
Operator : SY/MD
Sample : L4117-21
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AD0

Quant Time: Oct 01 09:23:43 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Oct 01 07:39:17 2020
Response via : Initial Calibration

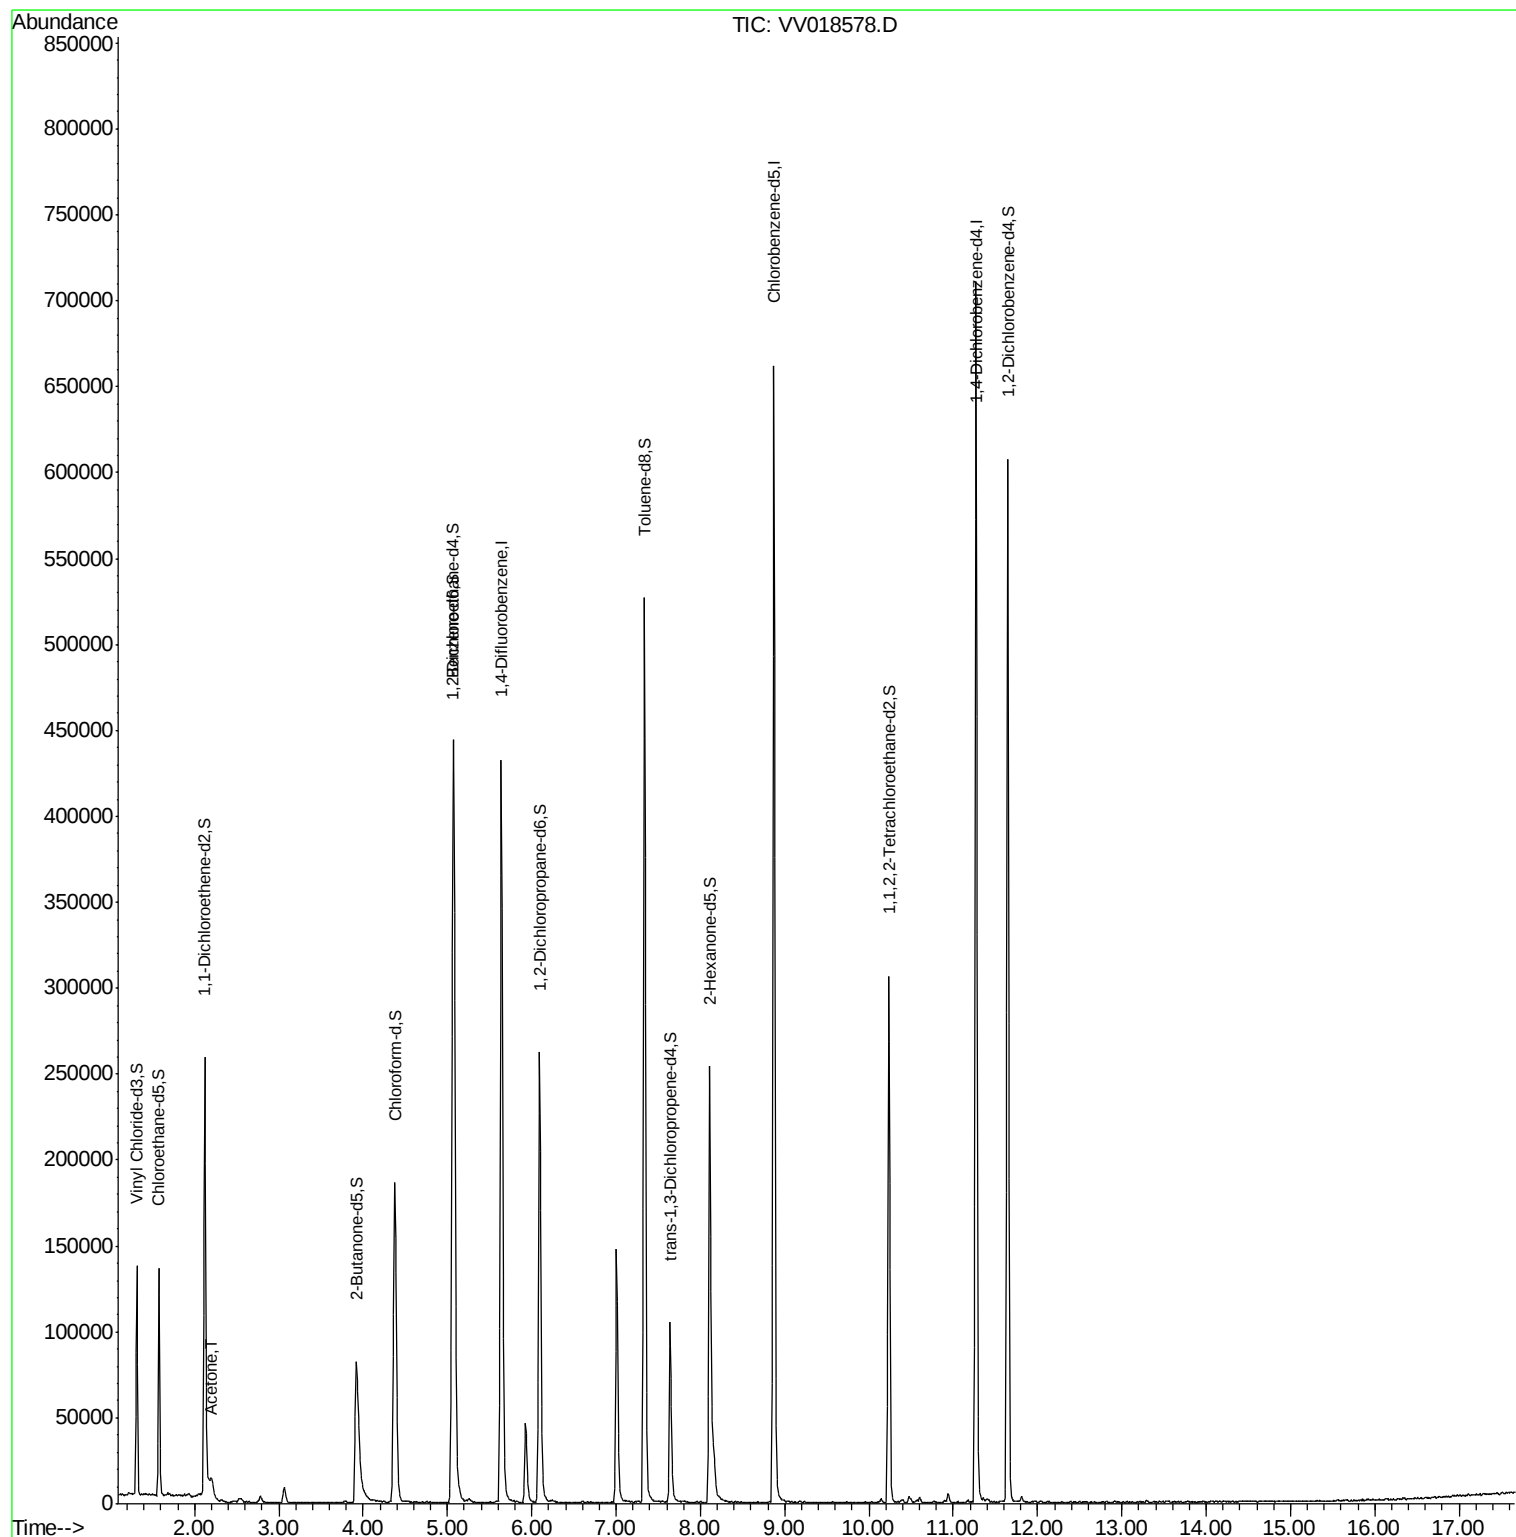

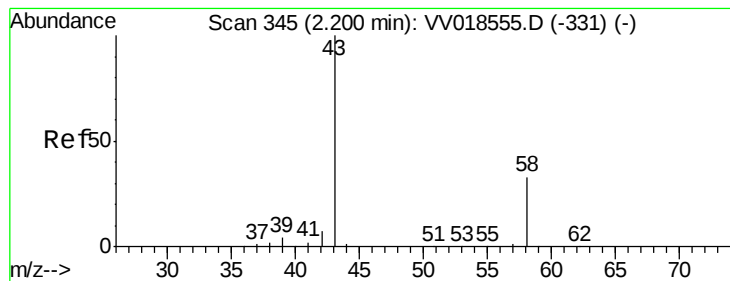

#13
 Acetone
 Concen: 13.411 ug/L
 RT: 2.20 min Scan# 346
 Delta R.T. 0.00 min
 Lab File: VV018578.D
 Acq: 30 Sep 2020 19:01

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AD0

Tot Ion: 43 Resp: 18877
 Ion Ratio Lower Upper
 43 100
 58 31.5 0.0 64.0

