

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV093020\
 Data File : VV018575.D
 Acq On : 30 Sep 2020 17:50
 Operator : SY/MD
 Sample : L4117-19DL 5X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AB4DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	79	rVB	139978	134453	11.09%	1.220%
2	1.579	145	152	165	rVB	131564	151931	12.53%	1.378%
3	2.123	312	321	353	rVB	273856	430355	35.50%	3.904%
4	2.618	473	475	476	rBV	405	175	0.01%	0.002%
5	2.782	515	526	541	rVB4	8889	17624	1.45%	0.160%
6	2.865	550	552	555	rVB2	437	230	0.02%	0.002%
7	2.881	555	557	560	rBV3	367	232	0.02%	0.002%
8	3.013	595	598	600	rBV3	485	379	0.03%	0.003%
9	3.065	604	614	630	rVB2	17132	34961	2.88%	0.317%
10	3.286	679	683	686	rVB4	431	349	0.03%	0.003%
11	3.515	752	754	757	rBV2	326	230	0.02%	0.002%
12	3.630	787	790	792	rBV2	262	174	0.01%	0.002%
13	3.675	802	804	808	rBV2	403	224	0.02%	0.002%
14	3.759	826	830	831	rBV	702	508	0.04%	0.005%
15	3.839	853	855	859	rVB2	512	245	0.02%	0.002%
16	3.920	868	880	916	rBV	98432	322521	26.60%	2.926%
17	4.261	982	986	990	rBV3	544	570	0.05%	0.005%
18	4.376	1005	1022	1046	rBV2	196637	481941	39.75%	4.372%
19	4.630	1098	1101	1104	rBV2	354	262	0.02%	0.002%
20	4.775	1142	1146	1148	rVV2	308	189	0.02%	0.002%
21	4.852	1165	1170	1173	rBV3	307	287	0.02%	0.003%
22	4.878	1177	1178	1182	rBV	307	193	0.02%	0.002%
23	5.071	1221	1238	1271	rBV2	466849	1212293	100.00%	10.998%
24	5.415	1342	1345	1346	rBV	364	152	0.01%	0.001%
25	5.550	1385	1387	1391	rBV	233	153	0.01%	0.001%
26	5.640	1402	1415	1444	rBV	451732	896495	73.95%	8.133%
27	5.875	1484	1488	1491	rBV2	676	447	0.04%	0.004%
28	5.939	1493	1508	1540	rVV2	376496	769915	63.51%	6.985%
29	6.093	1544	1556	1585	rVB	276267	560436	46.23%	5.084%
30	6.293	1616	1618	1620	rBV2	367	194	0.02%	0.002%
31	6.392	1645	1649	1650	rBV	441	221	0.02%	0.002%
32	6.454	1666	1668	1672	rBV3	267	190	0.02%	0.002%
33	6.508	1681	1685	1689	rVB2	345	286	0.02%	0.003%
34	6.646	1723	1728	1731	rBV2	376	405	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV093020\
 Data File : VV018575.D
 Acq On : 30 Sep 2020 17:50
 Operator : SY/MD
 Sample : L4117-19DL 5X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AB4DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
 Title : VOC Analysis

35	6.685	1738	1740	1747	rBV2	362	325	0.03%	0.003%
36	6.753	1758	1761	1763	rBV2	263	164	0.01%	0.001%
37	6.804	1773	1777	1782	rVB3	398	367	0.03%	0.003%
38	6.830	1782	1785	1787	rBV	243	188	0.02%	0.002%
39	6.875	1795	1799	1803	rBV2	232	265	0.02%	0.002%
40	6.894	1803	1805	1808	rVB2	297	169	0.01%	0.002%
41	6.942	1813	1820	1827	rBV4	877	1455	0.12%	0.013%
42	7.007	1829	1840	1867	rBV	160156	292528	24.13%	2.654%
43	7.187	1894	1896	1897	rBV	613	221	0.02%	0.002%
44	7.225	1906	1908	1911	rBV2	373	284	0.02%	0.003%
45	7.338	1931	1943	1967	rBV	566365	978147	80.69%	8.874%
46	7.589	2017	2021	2028	rVB7	1920	1942	0.16%	0.018%
47	7.643	2028	2038	2064	rBV	113731	198949	16.41%	1.805%
48	7.855	2102	2104	2108	rVB	376	162	0.01%	0.001%
49	7.878	2108	2111	2113	rBV2	756	300	0.02%	0.003%
50	7.894	2113	2116	2119	rBV3	473	301	0.02%	0.003%
51	8.003	2144	2150	2156	rVV6	2486	3192	0.26%	0.029%
52	8.029	2156	2158	2162	rVB2	421	257	0.02%	0.002%
53	8.109	2172	2183	2221	rBV2	282853	568010	46.85%	5.153%
54	8.508	2305	2307	2309	rVB2	538	206	0.02%	0.002%
55	8.527	2309	2313	2315	rBV2	694	566	0.05%	0.005%
56	8.627	2341	2344	2346	rBV2	445	211	0.02%	0.002%
57	8.650	2349	2351	2354	rBV2	282	184	0.02%	0.002%
58	8.678	2358	2360	2362	rBV2	484	205	0.02%	0.002%
59	8.871	2407	2420	2444	rBV	688457	1115251	92.00%	10.118%
60	9.093	2487	2489	2492	rBV3	304	186	0.02%	0.002%
61	9.125	2497	2499	2502	rBV	407	228	0.02%	0.002%
62	9.170	2507	2513	2520	rVV3	1885	2200	0.18%	0.020%
63	9.225	2526	2530	2531	rBV3	896	654	0.05%	0.006%
64	9.305	2551	2555	2557	rBV2	360	186	0.02%	0.002%
65	9.334	2562	2564	2568	rBV	248	185	0.02%	0.002%
66	9.498	2613	2615	2620	rVB2	603	340	0.03%	0.003%
67	9.572	2634	2638	2640	rBV3	815	602	0.05%	0.005%
68	9.650	2660	2662	2666	rVB	342	163	0.01%	0.001%
69	9.701	2674	2678	2682	rBV2	386	282	0.02%	0.003%
70	9.736	2682	2689	2693	rBV5	1000	1229	0.10%	0.011%
71	9.788	2702	2705	2710	rBV2	348	309	0.03%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV093020\
 Data File : VV018575.D
 Acq On : 30 Sep 2020 17:50
 Operator : SY/MD
 Sample : L4117-19DL 5X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AB4DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
 Title : VOC Analysis

72	9.817	2712	2714	2718	rVB2	732	458	0.04%	0.004%
73	9.865	2726	2729	2732	rBV2	421	339	0.03%	0.003%
74	9.936	2749	2751	2752	rBV	495	204	0.02%	0.002%
75	10.042	2776	2784	2788	rBV3	846	1276	0.11%	0.012%
76	10.080	2794	2796	2798	rBV	283	163	0.01%	0.001%
77	10.096	2798	2801	2803	rBV2	530	360	0.03%	0.003%
78	10.238	2833	2845	2866	rBV	354139	557036	45.95%	5.054%
79	10.473	2911	2918	2925	rBV2	6690	11352	0.94%	0.103%
80	10.563	2940	2946	2951	rBV5	5177	6218	0.51%	0.056%
81	10.897	3047	3050	3054	rVB5	1040	770	0.06%	0.007%
82	10.939	3056	3063	3073	rVB	12416	18164	1.50%	0.165%
83	11.051	3094	3098	3100	rBV3	525	496	0.04%	0.004%
84	11.170	3129	3135	3139	rBV6	1714	2347	0.19%	0.021%
85	11.270	3154	3166	3189	rBV	736606	1148246	94.72%	10.417%
86	11.646	3271	3283	3305	rVB	643359	1018533	84.02%	9.240%
87	11.810	3327	3334	3341	rBV7	4354	6234	0.51%	0.057%
88	12.138	3433	3436	3439	rBV3	544	355	0.03%	0.003%
89	12.383	3508	3512	3513	rBV2	916	629	0.05%	0.006%
90	12.437	3526	3529	3533	rBV2	649	618	0.05%	0.006%
91	12.563	3566	3568	3571	rBV	360	167	0.01%	0.002%
92	12.614	3581	3584	3585	rVB2	432	191	0.02%	0.002%
93	12.643	3585	3593	3594	rBV3	954	822	0.07%	0.007%
94	12.672	3594	3602	3615	rVB3	9765	15490	1.28%	0.141%
95	12.804	3638	3643	3645	rBV2	468	334	0.03%	0.003%
96	13.061	3720	3723	3726	rBV2	629	453	0.04%	0.004%
97	13.289	3786	3794	3805	rVB4	10193	15732	1.30%	0.143%
98	13.460	3845	3847	3850	rBV	400	232	0.02%	0.002%
99	13.534	3863	3870	3882	rVB	7830	12175	1.00%	0.110%
100	13.768	3937	3943	3956	rVB3	8505	13565	1.12%	0.123%


Sum of corrected areas: 11022592

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV093020\
Data File : VV018575.D
Acq On : 30 Sep 2020 17:50
Operator : SY/MD
Sample : L4117-19DL 5X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AB4DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

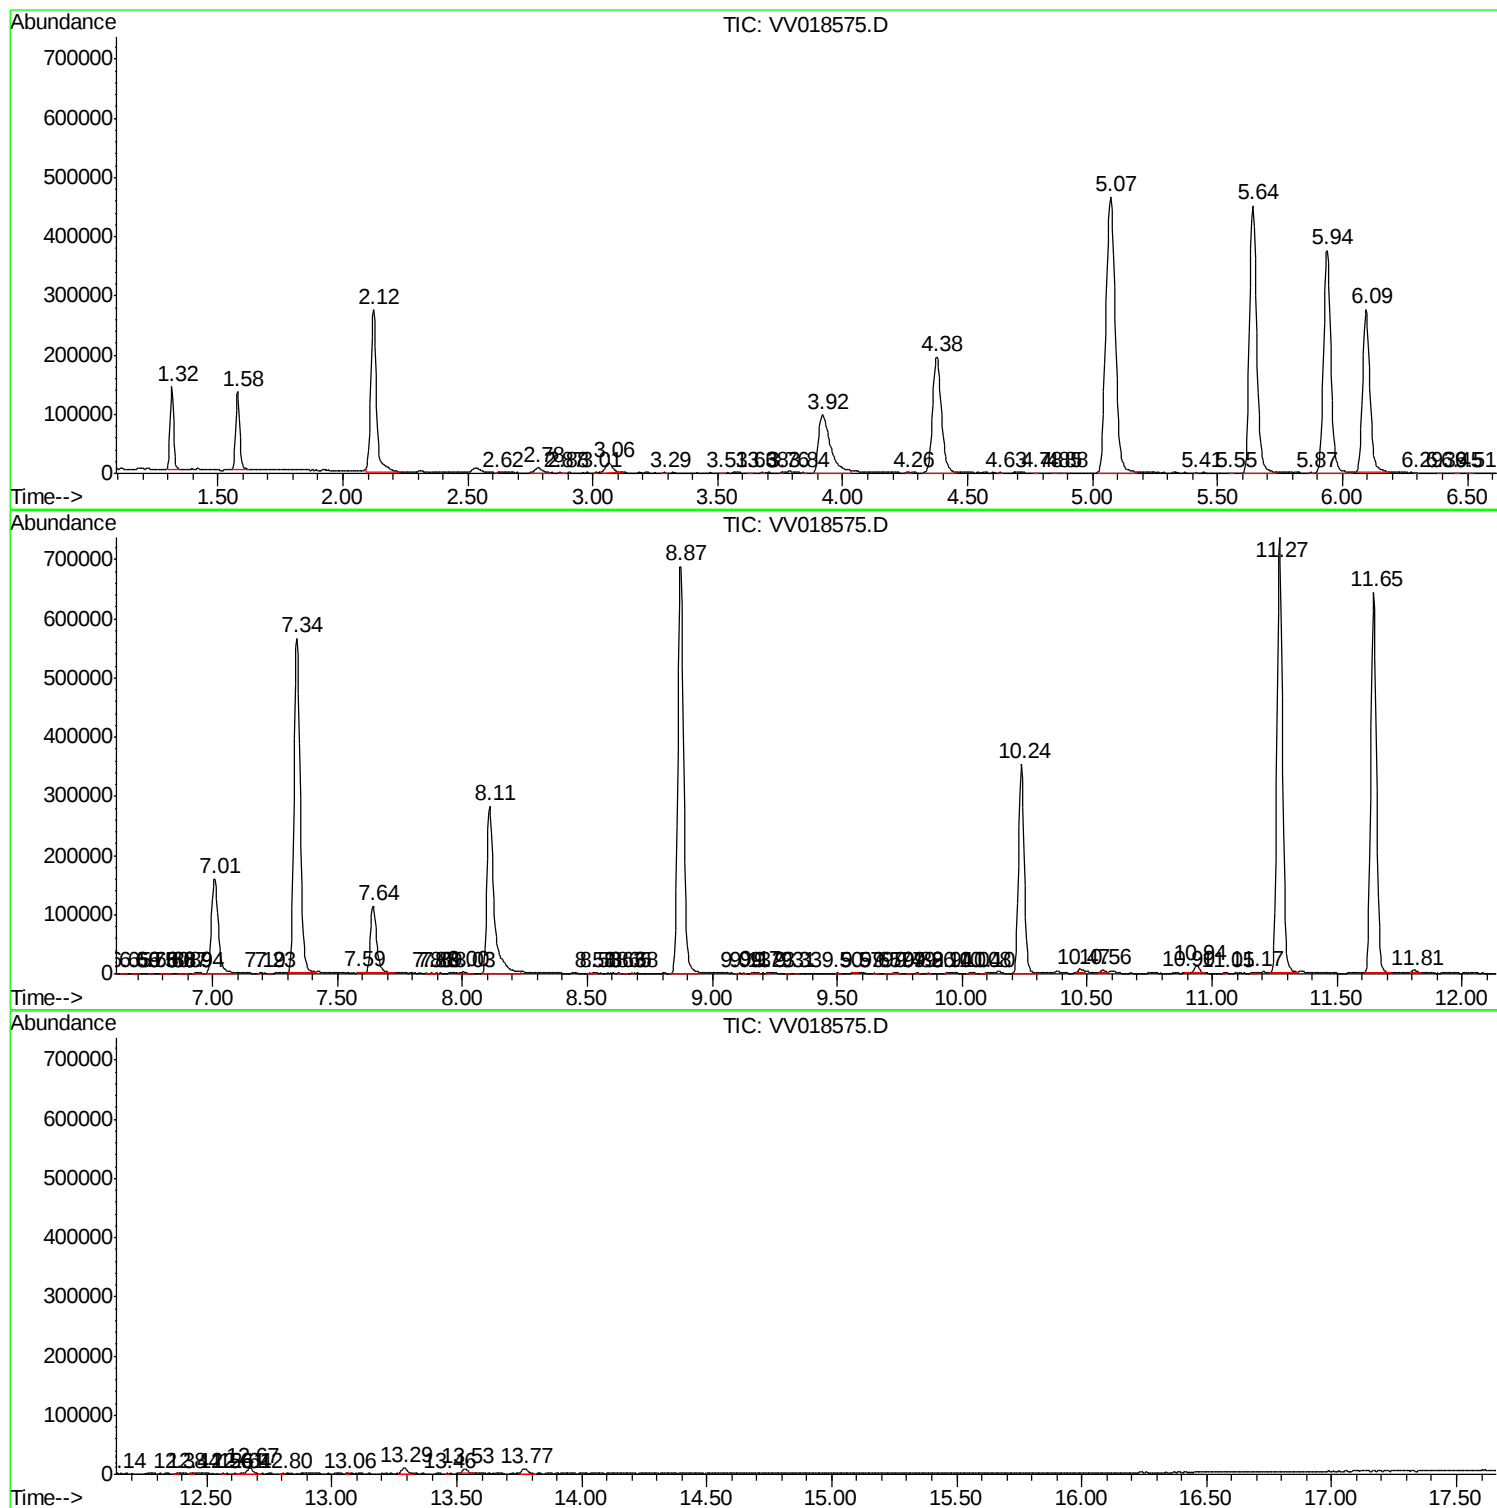

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV093020\
Data File : VV018575.D
Acq On : 30 Sep 2020 17:50
Operator : SY/MD
Sample : L4117-19DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AB4DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV093020\
Data File : VV018575.D
Acq On : 30 Sep 2020 17:50
Operator : SY/MD
Sample : L4117-19DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AB4DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc