


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV093020\
 Data File : VV018554.D
 Acq On : 30 Sep 2020 08:49
 Operator : SY/MD
 Sample : BFB63
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB63

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
 Title : VOC Analysis
 Last Update : Thu Oct 01 07:39:17 2020

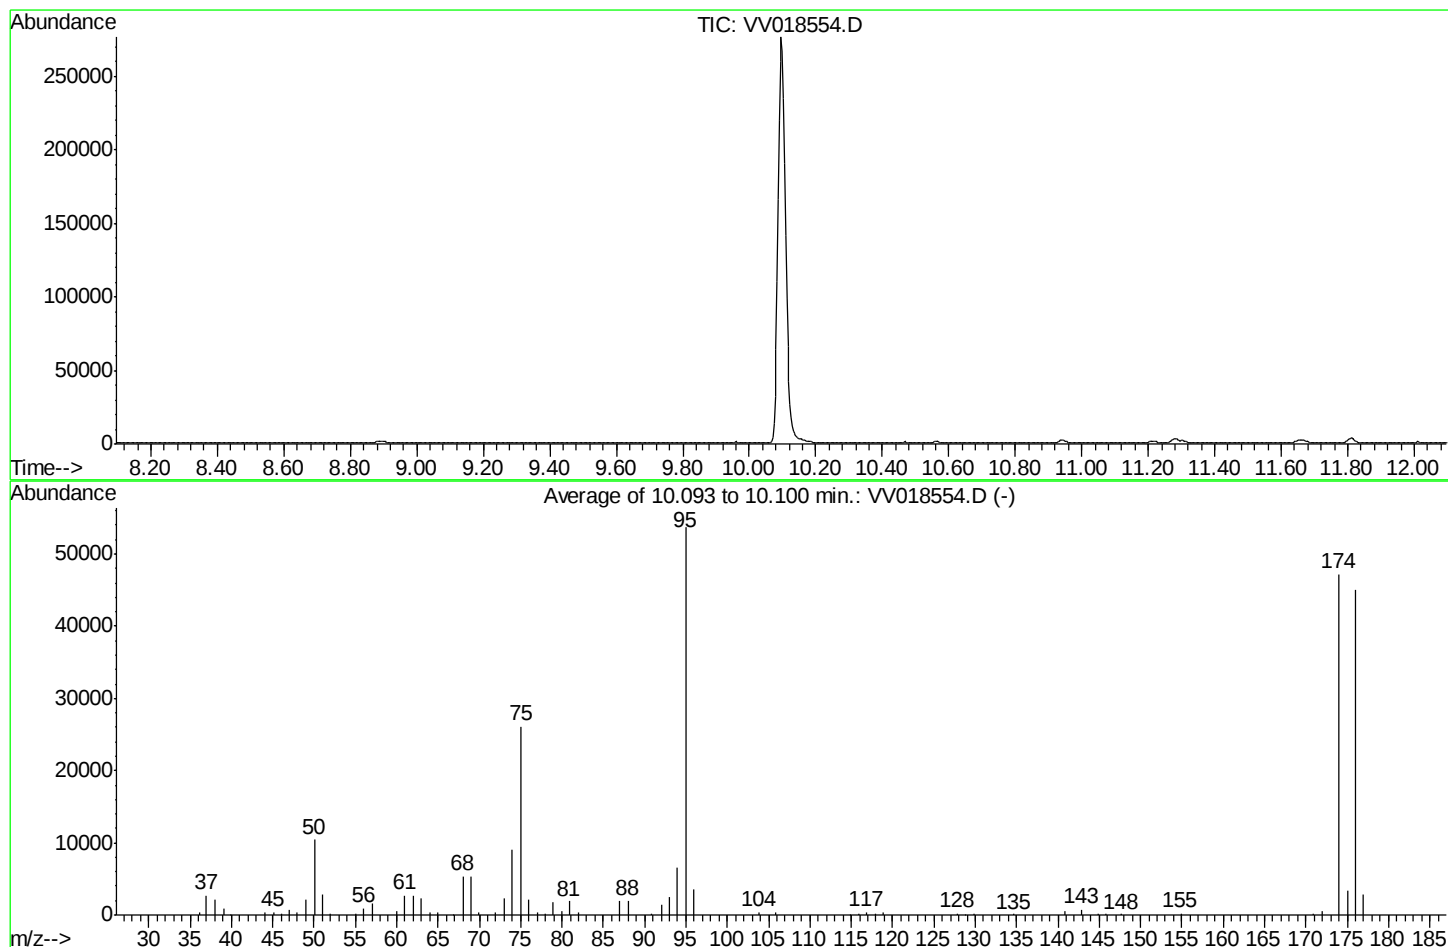

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2790

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.4	10436	PASS
75	95	30	80	48.6	26117	PASS
95	95	100	100	100.0	53693	PASS
96	95	5	9	6.6	3537	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	87.9	47178	PASS
175	174	5	9	7.1	3340	PASS
176	174	95	101	95.5	45045	PASS
177	176	5	9	6.5	2929	PASS

m/z	Abundance
36.10	471.0
37.00	2633.0
38.00	2312.0
39.00	856.0
40.00	250.0
44.00	800.0
45.10	438.0
46.10	190.0
47.00	696.0
48.00	335.0
49.00	2178.0
50.10	10384.0
51.00	3011.0
52.00	171.0
55.00	157.0
56.00	888.0
57.00	1614.0
60.00	581.0
61.00	2655.0
62.00	2645.0
63.00	2286.0
64.10	266.0
65.00	477.0
68.00	5308.0
69.00	5161.0
70.00	475.0
72.00	324.0
73.00	2297.0
74.00	8996.0
75.10	26032.0
76.00	2211.0
77.00	316.0
77.90	216.0
78.90	1675.0
80.00	594.0
80.90	1767.0
82.00	334.0
87.00	1834.0
88.00	1989.0
90.90	256.0
92.00	1447.0
93.00	2449.0
94.00	6126.0
95.00	52352.0
96.00	3442.0
103.90	335.0
105.80	336.0
115.90	226.0
116.80	392.0
118.00	217.0
118.80	263.0
127.90	271.0
128.80	131.0
129.90	205.0
134.70	109.0
140.80	559.0
142.90	732.0
144.80	160.0
145.90	110.0
147.70	170.0
154.90	195.0
170.90	125.0
171.90	571.0
174.00	44768.0
175.00	3241.0
176.00	42624.0
177.00	2661.0

Instrument :
MSVOA_V
ClientSampleId :
BFB63

m/z	Abundance
36.10	429.0
37.00	2796.0
38.00	2239.0
39.10	909.0
40.00	257.0
44.00	811.0
45.10	454.0
46.10	168.0
47.00	683.0
48.00	331.0
49.00	2290.0
50.00	10871.0
51.00	3011.0
52.00	142.0
55.10	168.0
56.00	968.0
57.00	1574.0
60.00	555.0
61.00	2810.0
62.00	2849.0
63.00	2393.0
64.10	336.0
65.00	412.0
66.70	101.0
68.00	5562.0
69.00	5473.0
70.00	431.0
72.00	308.0
73.00	2348.0
74.00	9308.0
75.10	26856.0
76.00	2277.0
77.00	366.0
77.90	254.0
78.90	1748.0
79.90	609.0
80.90	1923.0
82.00	349.0
86.90	1946.0
88.00	2090.0
90.90	208.0
92.00	1462.0
93.00	2550.0
94.00	6798.0
95.00	55328.0
96.00	3656.0
103.90	433.0
105.80	388.0
114.80	104.0
115.90	257.0
116.90	445.0
117.90	238.0
118.80	294.0
127.90	259.0
128.80	119.0
129.80	234.0
134.70	121.0
140.90	576.0
142.90	745.0
144.80	171.0
145.80	141.0
147.70	184.0
154.90	179.0
170.90	129.0
171.90	624.0
174.00	48624.0
175.00	3460.0
176.00	46728.0
177.00	3007.0

Instrument :
MSVOA_V
ClientSampleId :
BFB63

m/z	Abundance
36.10	419.0
37.00	2563.0
38.00	2046.0
39.10	886.0
39.90	263.0
44.00	722.0
45.10	431.0
47.00	684.0
48.00	302.0
49.00	2180.0
50.00	10053.0
51.10	2725.0
52.00	114.0
55.10	171.0
56.00	920.0
57.00	1354.0
60.00	496.0
61.00	2731.0
62.00	2630.0
63.00	2274.0
64.00	357.0
64.90	312.0
66.80	138.0
68.00	5341.0
69.00	5313.0
69.90	416.0
72.00	268.0
73.00	2293.0
74.00	8807.0
75.10	25464.0
76.00	2153.0
77.00	344.0
77.90	266.0
78.90	1727.0
79.90	534.0
80.90	1933.0
82.00	377.0
87.00	1870.0
88.00	2044.0
90.90	160.0
92.00	1388.0
93.00	2363.0
94.00	6640.0
95.00	53400.0
96.00	3515.0
103.90	408.0
105.80	343.0
115.90	262.0
116.80	460.0
117.80	225.0
118.80	291.0
127.80	204.0
129.90	239.0
134.70	110.0
140.90	611.0
142.90	741.0
144.90	181.0
145.80	119.0
147.70	160.0
154.90	163.0
170.90	107.0
171.90	645.0
174.00	48144.0
175.00	3321.0
176.00	45784.0
177.00	3119.0

Instrument :
MSVOA_V
ClientSampleId :
BFB63

Scan 2790 (10.061 min): VV018554.D
BFB63

m/z	Abundance
40.00	174.0
44.00	464.0

Instrument :
MSVOA_V
ClientSampleId :
BFB63