

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
 Data File : VV022454.D
 Acq On : 01 Oct 2021 00:30
 Operator : SY/MD
 Sample : M3979-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A62

Quant Time: Oct 01 04:47:06 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Oct 01 04:27:45 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	234466	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	222188	50.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	96918	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	88190	44.32	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	88.64%
7) Chloroethane-d5	1.564	69	71032	45.13	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	90.26%
11) 1,1-Dichloroethene-d2	2.105	63	121770	35.20	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	70.40%
21) 2-Butanone-d5	3.905	46	124878	88.93	ug/L	0.03
Spiked Amount	100.000	Range	40 - 130	Recovery	=	88.93%
24) Chloroform-d	4.349	84	147797	41.13	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	82.26%
26) 1,2-Dichloroethane-d4	5.034	65	94269	42.78	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	85.56%
32) Benzene-d6	5.050	84	320872	45.91	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.82%
36) 1,2-Dichloropropane-d6	6.069	67	100165	44.79	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	89.58%
41) Toluene-d8	7.317	98	275929	43.13	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	86.26%
43) trans-1,3-Dichloroprop...	7.625	79	39671	38.85	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	77.70%
47) 2-Hexanone-d5	8.092	63	74957	82.49	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	82.49%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	122914	37.87	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	75.74%
66) 1,2-Dichlorobenzene-d4	11.625	152	105426	48.92	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	97.84%
Target Compounds						
13) Acetone	2.191	43	28636	25.98	ug/L	Qvalue 70


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
Data File : VV022454.D
Acq On : 01 Oct 2021 00:30
Operator : SY/MD
Sample : M3979-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A62

Quant Time: Oct 01 04:47:06 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Oct 01 04:27:45 2021
Response via : Initial Calibration

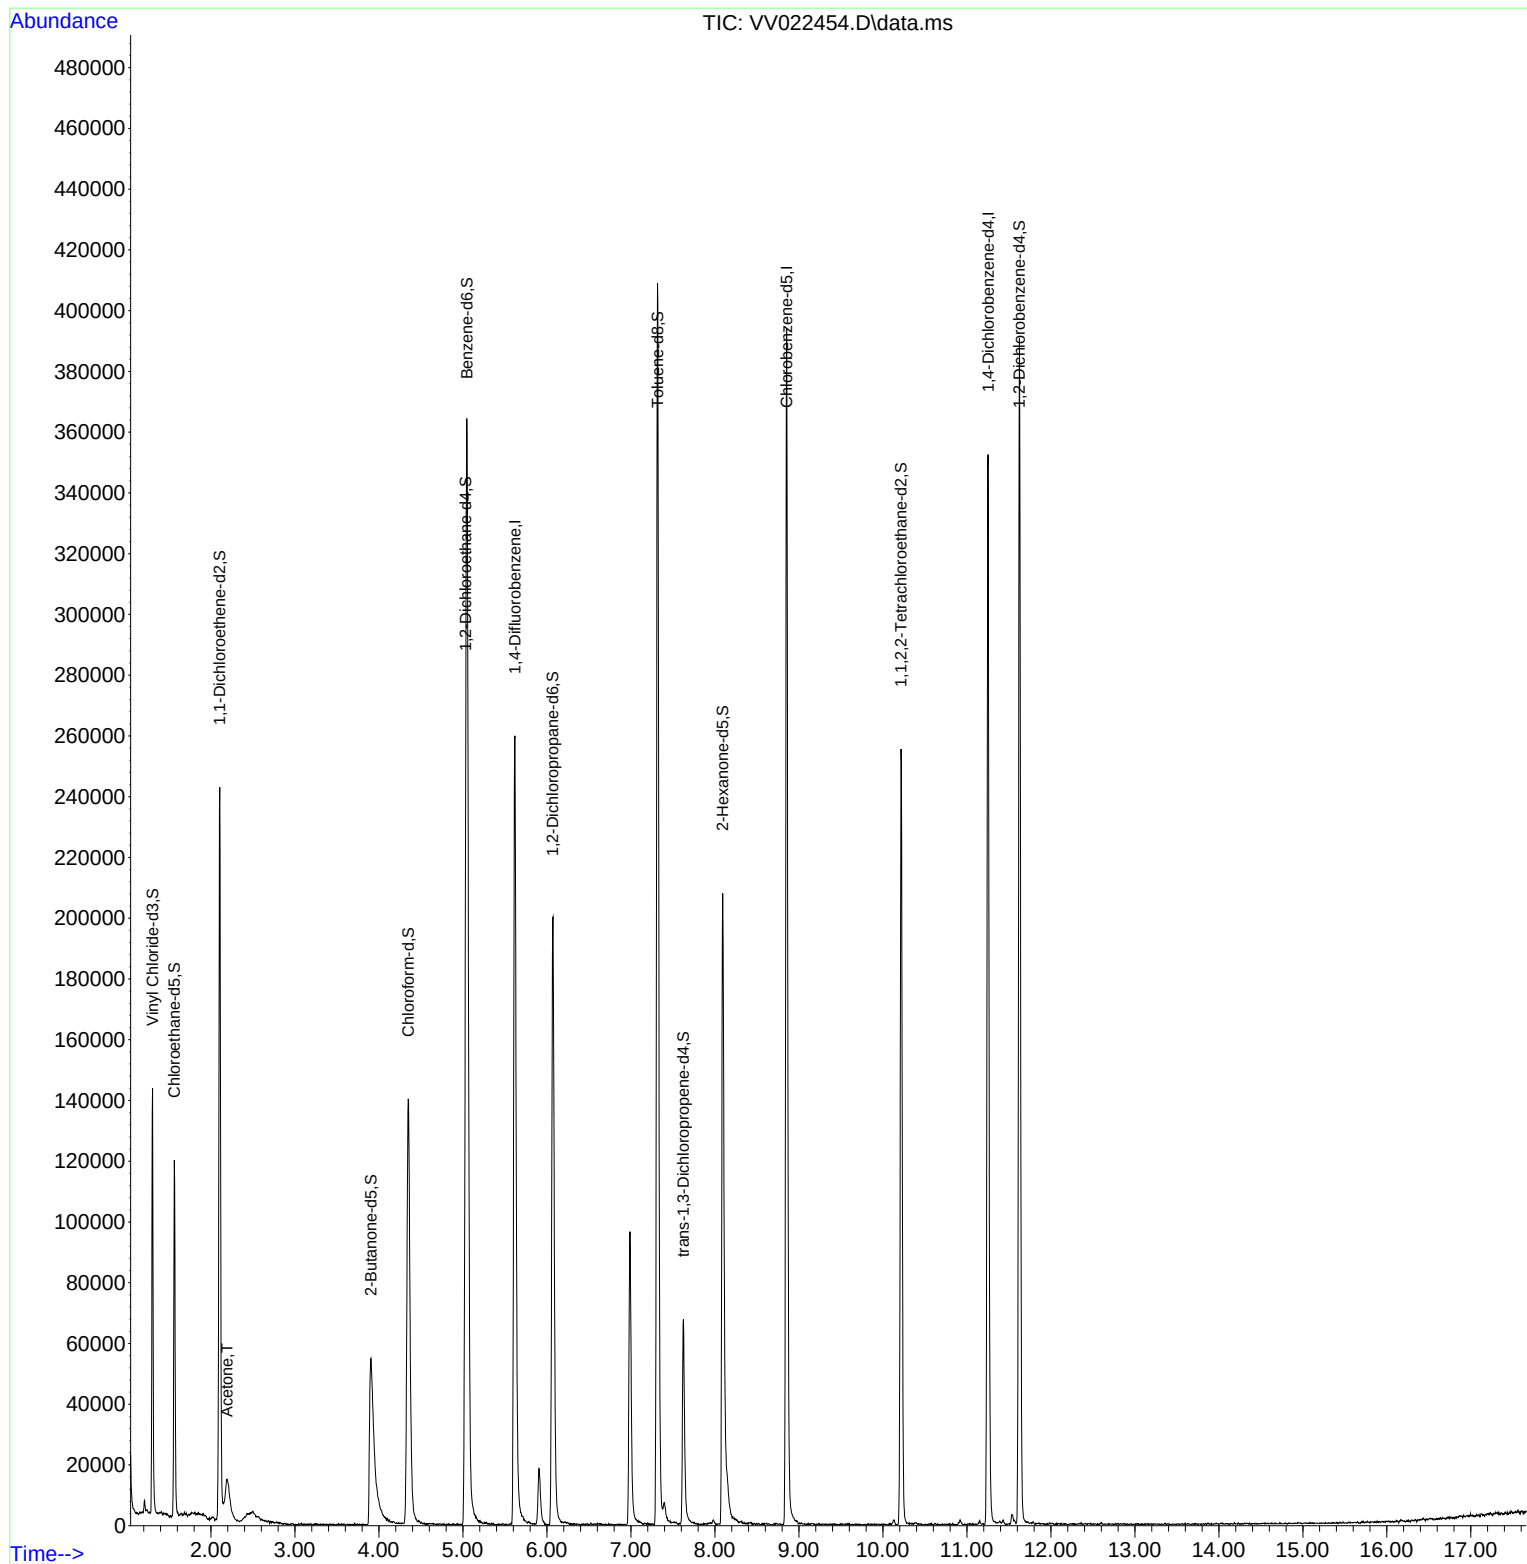

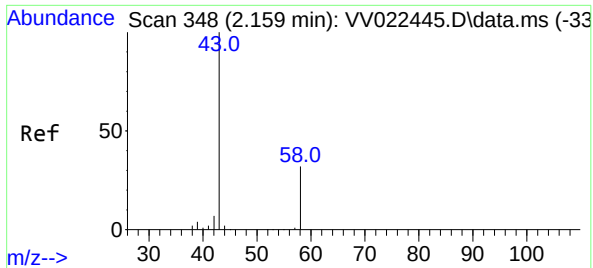

#13
 Acetone
 Concen: 25.98 ug/L
 RT: 2.191 min Scan# 358
 Delta R.T. 0.032 min
 Lab File: VV022454.D
 Acq: 01 Oct 2021 00:30

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A62

Tgt Ion:	43	Resp:	28636
Ion	Ratio	Lower	Upper
43	100		
58	16.4	0.0	67.2

