

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
 Data File : VV022420.D
 Acq On : 30 Sep 2021 10:30
 Operator : SY/MD
 Sample : VV0930MBL01
 Misc : 5.0g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK266

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M

Title : VOC Analysis

Signal : TIC: VV022420.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	98	rVB	165306	165262	16.45%	2.197%
2	1.561	156	162	177	rVB	128086	147349	14.66%	1.959%
3	2.105	321	331	351	rVB	260997	381165	37.93%	5.067%
4	2.751	529	532	533	rBV2	469	280	0.03%	0.004%
5	2.790	541	544	549	rBV2	559	365	0.04%	0.005%
6	3.159	657	659	664	rVV3	178	154	0.02%	0.002%
7	3.320	706	709	714	rBV3	281	313	0.03%	0.004%
8	3.384	726	729	736	rVB	368	501	0.05%	0.007%
9	3.417	736	739	742	rBV2	352	281	0.03%	0.004%
10	3.439	742	746	749	rVV2	302	197	0.02%	0.003%
11	3.629	801	805	809	rVV2	381	380	0.04%	0.005%
12	3.751	841	843	847	rVB	430	262	0.03%	0.003%
13	3.780	847	852	853	rBV	343	336	0.03%	0.004%
14	3.870	871	880	917	rBV	78470	212707	21.17%	2.828%
15	4.346	1013	1028	1054	rBV2	158432	392139	39.03%	5.213%
16	4.645	1115	1121	1124	rBV2	451	583	0.06%	0.008%
17	4.703	1137	1139	1141	rVB	333	140	0.01%	0.002%
18	4.799	1166	1169	1170	rBV	304	195	0.02%	0.003%
19	4.835	1176	1180	1182	rBV3	288	199	0.02%	0.003%
20	5.043	1228	1245	1271	rBV2	391215	1004799	100.00%	13.358%
21	5.481	1379	1381	1383	rBV	380	148	0.01%	0.002%
22	5.616	1410	1423	1457	rBV	278322	577936	57.52%	7.683%
23	5.912	1504	1515	1528	rBV6	5925	13392	1.33%	0.178%
24	6.069	1551	1564	1590	rBV	220886	451190	44.90%	5.998%
25	6.256	1620	1622	1628	rBV4	364	370	0.04%	0.005%
26	6.281	1628	1630	1634	rVB3	652	396	0.04%	0.005%
27	6.304	1634	1637	1639	rBV2	339	183	0.02%	0.002%
28	6.320	1639	1642	1644	rBV3	392	253	0.03%	0.003%
29	6.371	1656	1658	1661	rBV	346	221	0.02%	0.003%
30	6.416	1667	1672	1673	rBV	216	189	0.02%	0.003%
31	6.474	1688	1690	1696	rVB2	318	183	0.02%	0.002%
32	6.510	1697	1701	1706	rVB3	488	399	0.04%	0.005%
33	6.561	1714	1717	1722	rVB2	534	452	0.04%	0.006%
34	6.590	1724	1726	1732	rBV2	324	254	0.03%	0.003%
35	6.664	1747	1749	1753	rBV2	370	301	0.03%	0.004%
36	6.918	1827	1828	1832	rVB2	273	143	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
 Data File : VV022420.D
 Acq On : 30 Sep 2021 10:30
 Operator : SY/MD
 Sample : VV0930MBL01
 Misc : 5.0g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK266

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

37	6.986	1838	1849	1879	rBV	112612	213745	21.27%	2.842%
38	7.233	1924	1926	1931	rVB2	682	605	0.06%	0.008%
39	7.256	1931	1933	1938	rBV2	353	269	0.03%	0.004%
40	7.317	1938	1952	1970	rBV	468112	814730	81.08%	10.831%
41	7.622	2037	2047	2068	rBV	80091	142805	14.21%	1.898%
42	7.921	2134	2140	2143	rBV2	449	380	0.04%	0.005%
43	7.982	2152	2159	2166	rVB4	1372	1691	0.17%	0.022%
44	8.088	2182	2192	2225	rBV	229395	427301	42.53%	5.680%
45	8.423	2294	2296	2299	rVB2	500	214	0.02%	0.003%
46	8.468	2309	2310	2313	rVB2	317	160	0.02%	0.002%
47	8.484	2313	2315	2319	rBV3	374	224	0.02%	0.003%
48	8.503	2319	2321	2323	rBV	329	154	0.02%	0.002%
49	8.539	2331	2332	2334	rBV	330	150	0.01%	0.002%
50	8.606	2349	2353	2357	rBV3	475	475	0.05%	0.006%
51	8.751	2396	2398	2400	rBV2	307	153	0.02%	0.002%
52	8.854	2418	2430	2463	rBV	417590	700790	69.74%	9.316%
53	9.095	2504	2505	2508	rBV2	355	187	0.02%	0.002%
54	9.194	2533	2536	2540	rBV2	400	194	0.02%	0.003%
55	9.252	2550	2554	2559	rBV2	235	254	0.03%	0.003%
56	9.297	2565	2568	2571	rBV2	262	185	0.02%	0.002%
57	9.551	2641	2647	2651	rBV4	785	922	0.09%	0.012%
58	9.625	2668	2670	2673	rVB	250	150	0.01%	0.002%
59	9.674	2682	2685	2691	rVB3	355	318	0.03%	0.004%
60	9.719	2697	2699	2702	rVB	363	192	0.02%	0.003%
61	9.776	2714	2717	2720	rBV2	170	151	0.02%	0.002%
62	9.793	2720	2722	2727	rVV4	287	252	0.03%	0.003%
63	10.127	2819	2826	2834	rBV4	2566	3898	0.39%	0.052%
64	10.217	2842	2854	2876	rBV	298220	477432	47.52%	6.347%
65	10.493	2935	2940	2942	rBV3	406	303	0.03%	0.004%
66	10.719	3006	3010	3013	rBV3	369	229	0.02%	0.003%
67	10.757	3018	3022	3025	rVB4	428	342	0.03%	0.005%
68	10.918	3062	3072	3079	rBV4	2735	4102	0.41%	0.055%
69	11.027	3101	3106	3107	rBV	253	184	0.02%	0.002%
70	11.153	3138	3145	3149	rBV7	1095	1541	0.15%	0.020%
71	11.182	3151	3154	3155	rBV	1190	774	0.08%	0.010%
72	11.249	3164	3175	3195	rBV	394781	634036	63.10%	8.429%
73	11.493	3247	3251	3253	rBV	317	234	0.02%	0.003%
74	11.625	3279	3292	3310	rBV	447172	712693	70.93%	9.474%
75	11.905	3377	3379	3382	rBV2	336	199	0.02%	0.003%
76	12.021	3412	3415	3422	rBV2	421	390	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
 Data File : VV022420.D
 Acq On : 30 Sep 2021 10:30
 Operator : SY/MD
 Sample : VV0930MBL01
 Misc : 5.0g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK266

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

77	12.207	3467	3473	3476	rBV2	315	333	0.03%	0.004%
78	12.310	3502	3505	3507	rBV2	369	221	0.02%	0.003%
79	12.435	3542	3544	3546	rBV	408	206	0.02%	0.003%
80	12.519	3569	3570	3574	rBV2	318	143	0.01%	0.002%
81	12.545	3576	3578	3581	rBV2	273	153	0.02%	0.002%
82	12.606	3596	3597	3603	rVB	347	260	0.03%	0.003%
83	12.651	3605	3611	3617	rBV3	2864	3688	0.37%	0.049%
84	12.731	3634	3636	3640	rBV	254	148	0.01%	0.002%
85	12.944	3699	3702	3707	rVB3	239	219	0.02%	0.003%
86	13.201	3779	3782	3785	rBV2	304	287	0.03%	0.004%
87	13.268	3797	3803	3810	rBV4	2734	3931	0.39%	0.052%
88	13.419	3847	3850	3853	rBV2	350	253	0.03%	0.003%
89	13.513	3871	3879	3891	rBV3	4230	6690	0.67%	0.089%
90	13.673	3926	3929	3932	rVB3	543	390	0.04%	0.005%
91	13.709	3936	3940	3942	rVV	545	426	0.04%	0.006%
92	13.751	3946	3953	3964	rVB6	3944	6022	0.60%	0.080%
93	13.976	4021	4023	4026	rBV2	333	202	0.02%	0.003%
94	14.024	4033	4038	4039	rBV2	410	335	0.03%	0.004%
95	14.056	4047	4048	4054	rVB3	372	162	0.02%	0.002%
96	14.082	4054	4056	4061	rVB2	434	317	0.03%	0.004%
97	14.107	4061	4064	4067	rBV3	282	201	0.02%	0.003%
98	14.554	4198	4203	4208	rBV3	497	583	0.06%	0.008%
99	14.680	4239	4242	4244	rBV2	411	247	0.02%	0.003%
100	14.789	4274	4276	4279	rBV	468	201	0.02%	0.003%




Sum of corrected areas: 7522243

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
Data File : VV022420.D
Acq On : 30 Sep 2021 10:30
Operator : SY/MD
Sample : VV0930MBL01
Misc : 5.0g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK266

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

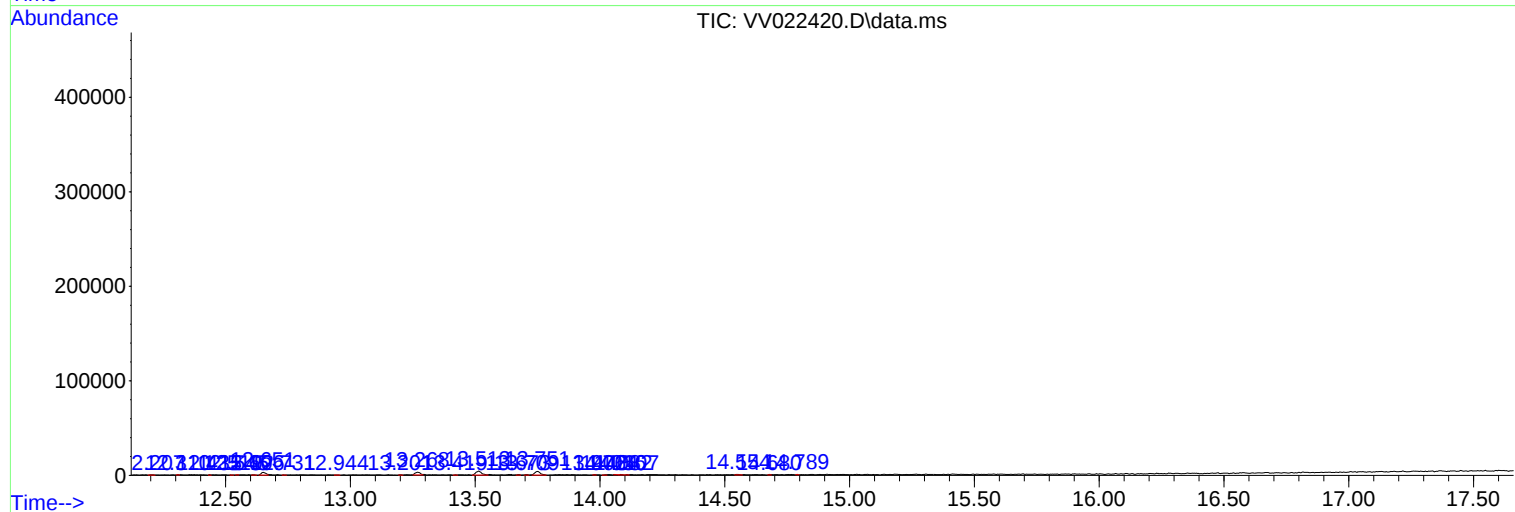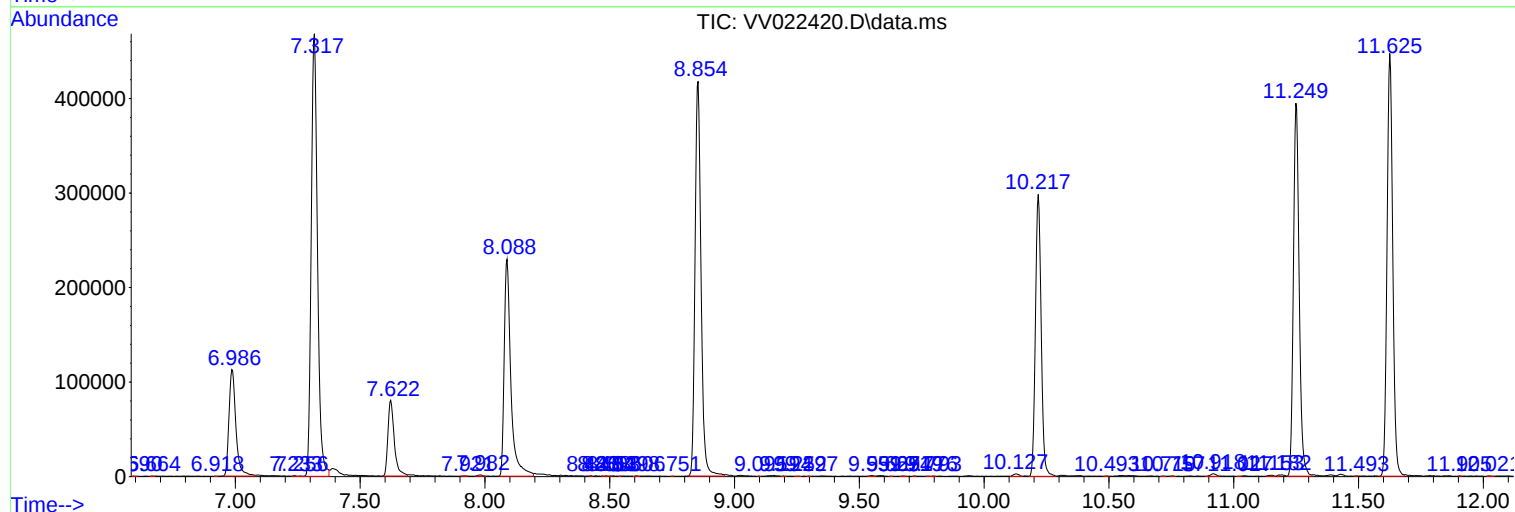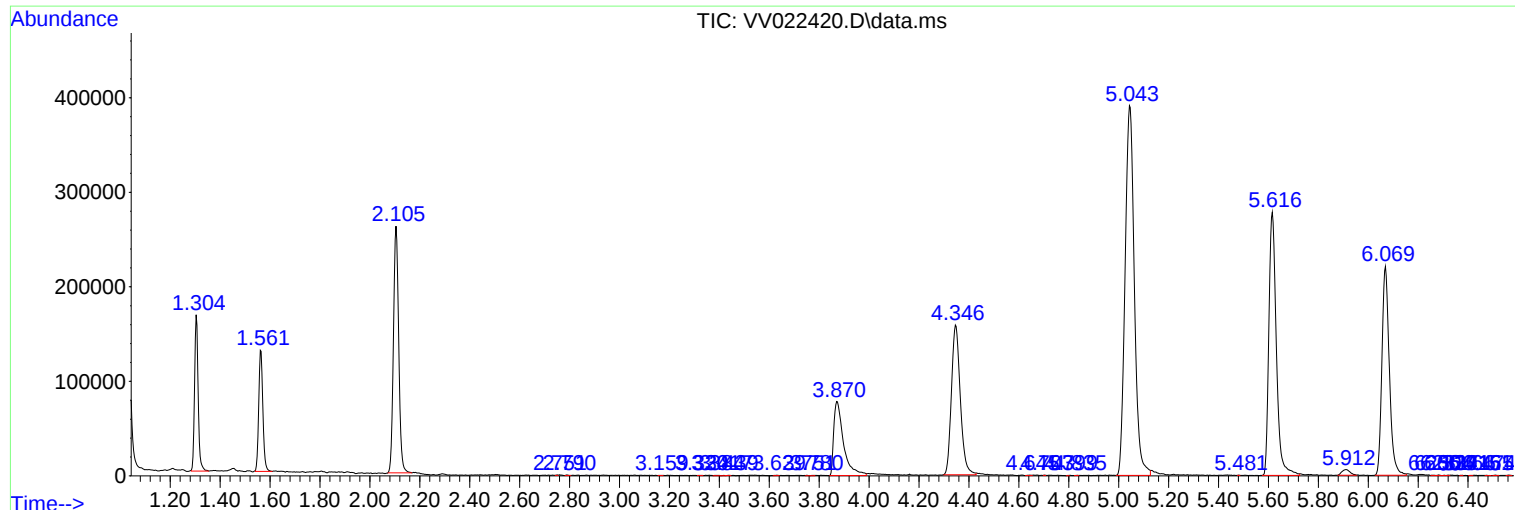

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
Data File : VV022420.D
Acq On : 30 Sep 2021 10:30
Operator : SY/MD
Sample : VV0930MBL01
Misc : 5.0g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK266

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
Data File : VV022420.D
Acq On : 30 Sep 2021 10:30
Operator : SY/MD
Sample : VV0930MBL01
Misc : 5.0g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK266

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
