

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
 Data File : VV022421.D
 Acq On : 30 Sep 2021 10:54
 Operator : SY/MD
 Sample : VV0930WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK267

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M

Title : VOC Analysis

Signal : TIC: VV022421.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	98	rVB	150635	154084	15.88%	2.142%
2	1.561	155	162	176	rVB	119487	138093	14.24%	1.920%
3	2.104	321	331	348	rBV	249111	363539	37.48%	5.054%
4	2.503	451	455	457	rBV3	882	670	0.07%	0.009%
5	2.712	517	520	523	rBB3	414	218	0.02%	0.003%
6	2.728	523	525	528	rBV	301	165	0.02%	0.002%
7	2.760	533	535	537	rVB	333	167	0.02%	0.002%
8	2.776	537	540	545	rVB2	504	395	0.04%	0.005%
9	2.831	555	557	561	rBV2	383	279	0.03%	0.004%
10	2.947	588	593	594	rBV2	336	322	0.03%	0.004%
11	3.066	627	630	633	rVB	357	187	0.02%	0.003%
12	3.095	636	639	642	rVB2	533	294	0.03%	0.004%
13	3.262	689	691	693	rVB	358	154	0.02%	0.002%
14	3.336	709	714	717	rBV3	238	276	0.03%	0.004%
15	3.484	757	760	761	rBV	293	159	0.02%	0.002%
16	3.545	775	779	781	rBV	294	221	0.02%	0.003%
17	3.603	793	797	800	rBV2	437	237	0.02%	0.003%
18	3.699	823	827	830	rBV2	326	206	0.02%	0.003%
19	3.735	835	838	839	rBV2	302	200	0.02%	0.003%
20	3.789	852	855	858	rBV	332	214	0.02%	0.003%
21	3.876	872	882	917	rBV	80488	213533	22.01%	2.968%
22	4.349	1013	1029	1056	rBV	153955	378477	39.02%	5.261%
23	4.603	1103	1108	1112	rBV4	575	632	0.07%	0.009%
24	4.715	1141	1143	1146	rVB	610	275	0.03%	0.004%
25	4.770	1156	1160	1161	rBV2	375	252	0.03%	0.004%
26	4.821	1173	1176	1178	rBV3	361	260	0.03%	0.004%
27	4.918	1203	1206	1207	rBV	285	167	0.02%	0.002%
28	5.046	1229	1246	1275	rBV2	381419	970049	100.00%	13.485%
29	5.426	1362	1364	1368	rVB2	287	174	0.02%	0.002%
30	5.445	1368	1370	1372	rBV	356	186	0.02%	0.003%
31	5.619	1411	1424	1460	rBV	266164	546663	56.35%	7.599%
32	5.908	1504	1514	1532	rVB5	4868	11061	1.14%	0.154%
33	5.972	1532	1534	1536	rBV	706	300	0.03%	0.004%
34	6.008	1540	1545	1549	rBV3	238	307	0.03%	0.004%
35	6.069	1549	1564	1595	rBV	210567	438853	45.24%	6.101%
36	6.313	1638	1640	1644	rVB	265	163	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
 Data File : VV022421.D
 Acq On : 30 Sep 2021 10:54
 Operator : SY/MD
 Sample : VV0930WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK267

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

37	6.374	1653	1659	1661	rVV2	175	179	0.02%	0.002%
38	6.387	1661	1663	1667	rVV	231	168	0.02%	0.002%
39	6.651	1742	1745	1747	rBV	255	163	0.02%	0.002%
40	6.792	1784	1789	1794	rBV3	371	374	0.04%	0.005%
41	6.921	1827	1829	1832	rBV	252	181	0.02%	0.003%
42	6.989	1839	1850	1870	rBV	109474	202417	20.87%	2.814%
43	7.130	1892	1894	1899	rBV5	629	447	0.05%	0.006%
44	7.226	1921	1924	1925	rBV2	609	325	0.03%	0.005%
45	7.316	1941	1952	1971	rBV	443329	769678	79.34%	10.700%
46	7.622	2036	2047	2065	rBV	76111	135588	13.98%	1.885%
47	7.915	2136	2138	2142	rVB2	414	277	0.03%	0.004%
48	7.982	2153	2159	2169	rVB7	2176	3169	0.33%	0.044%
49	8.024	2169	2172	2175	rBV2	379	264	0.03%	0.004%
50	8.043	2175	2178	2180	rVB	312	160	0.02%	0.002%
51	8.088	2181	2192	2224	rBV	239070	434106	44.75%	6.035%
52	8.326	2264	2266	2268	rBV2	521	165	0.02%	0.002%
53	8.545	2332	2334	2336	rVV3	387	175	0.02%	0.002%
54	8.574	2340	2343	2346	rVB2	538	329	0.03%	0.005%
55	8.590	2346	2348	2351	rBV	267	151	0.02%	0.002%
56	8.632	2358	2361	2363	rBV2	282	206	0.02%	0.003%
57	8.725	2386	2390	2393	rBV	352	298	0.03%	0.004%
58	8.799	2410	2413	2415	rBV2	392	279	0.03%	0.004%
59	8.853	2418	2430	2454	rBV	396843	661770	68.22%	9.200%
60	9.111	2508	2510	2513	rVB2	366	160	0.02%	0.002%
61	9.130	2513	2516	2518	rBV2	307	181	0.02%	0.003%
62	9.143	2518	2520	2521	rBV2	542	267	0.03%	0.004%
63	9.175	2528	2530	2535	rVB2	401	227	0.02%	0.003%
64	9.397	2596	2599	2602	rBV2	246	189	0.02%	0.003%
65	9.445	2612	2614	2616	rBV	241	147	0.02%	0.002%
66	9.474	2620	2623	2626	rBV	215	148	0.02%	0.002%
67	9.525	2636	2639	2641	rBV	297	186	0.02%	0.003%
68	9.583	2654	2657	2662	rBV2	379	313	0.03%	0.004%
69	9.738	2701	2705	2707	rBV	248	154	0.02%	0.002%
70	10.040	2797	2799	2803	rVB	493	266	0.03%	0.004%
71	10.130	2819	2827	2833	rVB4	2257	3059	0.32%	0.043%
72	10.217	2841	2854	2876	rBV	302512	478443	49.32%	6.651%
73	10.583	2966	2968	2972	rVB4	573	297	0.03%	0.004%
74	10.648	2986	2988	2990	rBV	440	258	0.03%	0.004%
75	10.750	3015	3020	3024	rBV3	367	393	0.04%	0.005%
76	10.828	3041	3044	3045	rBV	457	242	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
 Data File : VV022421.D
 Acq On : 30 Sep 2021 10:54
 Operator : SY/MD
 Sample : VV0930WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK267

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

77	10.860	3053	3054	3058	rVB	306	161	0.02%	0.002%
78	10.889	3058	3063	3064	rBV	415	262	0.03%	0.004%
79	10.918	3065	3072	3082	rVB8	2344	3899	0.40%	0.054%
80	11.040	3106	3110	3112	rBV	457	390	0.04%	0.005%
81	11.146	3139	3143	3144	rBV2	837	594	0.06%	0.008%
82	11.252	3164	3176	3205	rBV	370667	594377	61.27%	8.263%
83	11.474	3242	3245	3247	rBV2	392	282	0.03%	0.004%
84	11.522	3258	3260	3262	rBV	382	175	0.02%	0.002%
85	11.625	3280	3292	3314	rBV	421337	671198	69.19%	9.331%
86	11.779	3335	3340	3344	rBV4	867	884	0.09%	0.012%
87	11.866	3365	3367	3370	rBV2	413	279	0.03%	0.004%
88	12.014	3407	3413	3415	rVV2	249	253	0.03%	0.004%
89	12.416	3535	3538	3539	rBV	264	146	0.02%	0.002%
90	12.641	3605	3608	3609	rBV	494	245	0.03%	0.003%
91	12.873	3677	3680	3684	rVB2	391	247	0.03%	0.003%
92	13.094	3747	3749	3752	rBV2	334	208	0.02%	0.003%
93	13.233	3788	3792	3794	rBV2	355	191	0.02%	0.003%
94	13.265	3798	3802	3806	rBV3	623	653	0.07%	0.009%
95	13.503	3874	3876	3877	rBV	314	158	0.02%	0.002%
96	13.602	3904	3907	3910	rBV3	354	259	0.03%	0.004%
97	13.676	3927	3930	3932	rBV2	318	207	0.02%	0.003%
98	13.750	3949	3953	3957	rBV2	770	719	0.07%	0.010%
99	13.927	4005	4008	4011	rBV2	329	197	0.02%	0.003%
100	14.496	4183	4185	4189	rBV	315	277	0.03%	0.004%




Sum of corrected areas: 7193492

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
Data File : VV022421.D
Acq On : 30 Sep 2021 10:54
Operator : SY/MD
Sample : VV0930WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK267

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

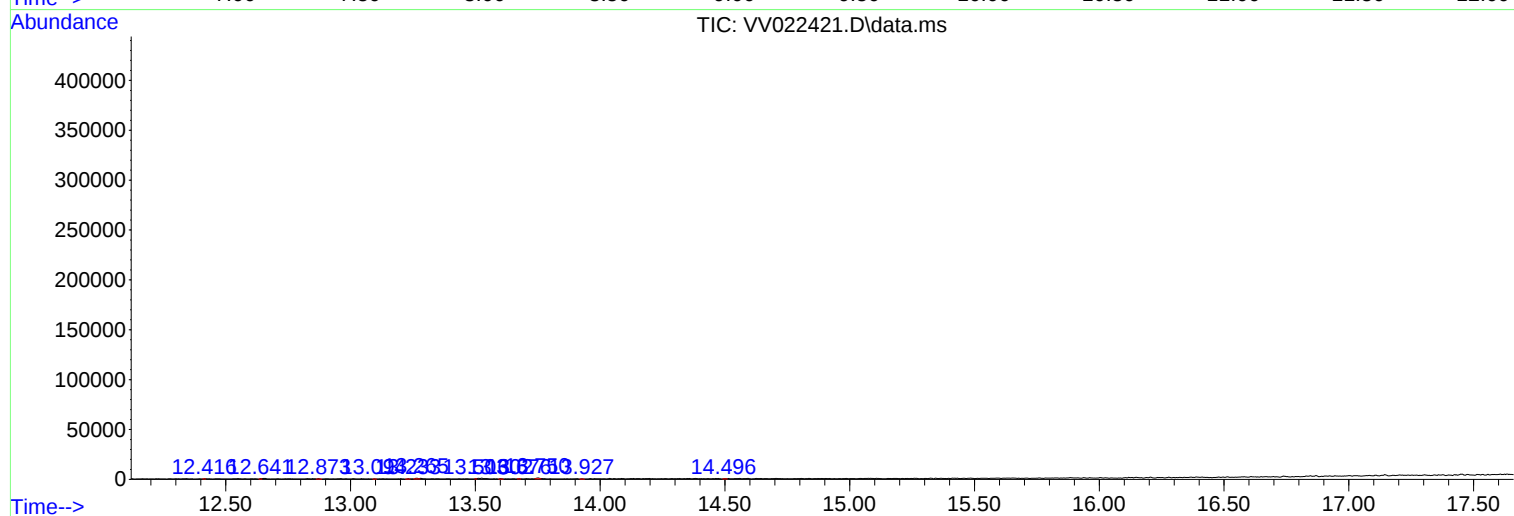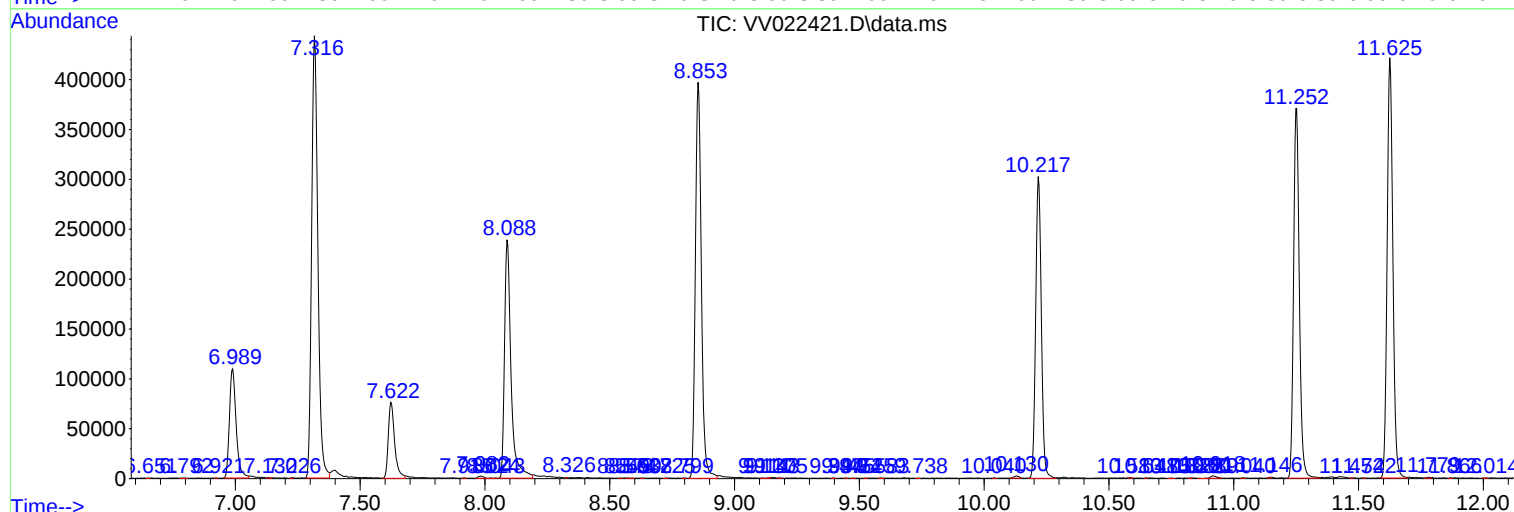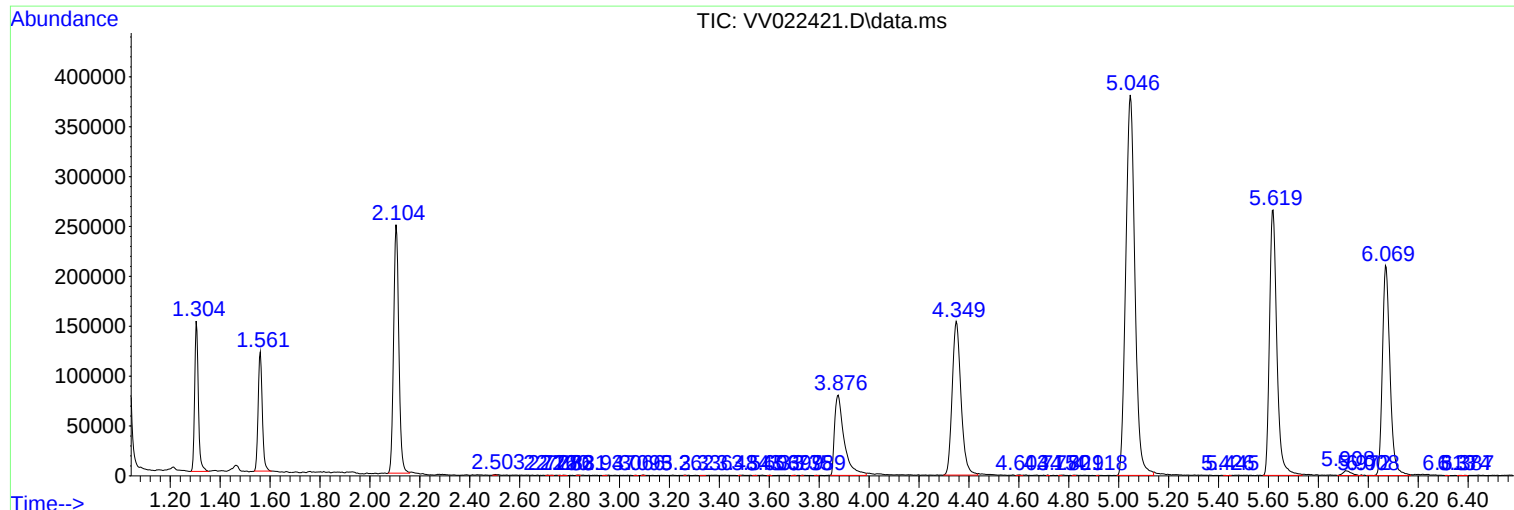

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
Data File : VV022421.D
Acq On : 30 Sep 2021 10:54
Operator : SY/MD
Sample : VV0930WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK267

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
Data File : VV022421.D
Acq On : 30 Sep 2021 10:54
Operator : SY/MD
Sample : VV0930WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK267

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
