

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
 Data File : VV022422.D
 Acq On : 30 Sep 2021 11:18
 Operator : SY/MD
 Sample : M3978-03DL 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A15DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M

Title : VOC Analysis

Signal : TIC: VV022422.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	103	rVB	149305	155982	15.95%	2.016%
2	1.565	156	163	175	rBV	120946	135497	13.86%	1.752%
3	2.105	321	331	344	rBV	247358	355471	36.36%	4.595%
4	2.590	479	482	487	rVB	485	367	0.04%	0.005%
5	2.638	494	497	499	rBV2	492	289	0.03%	0.004%
6	2.703	513	517	518	rBV	339	239	0.02%	0.003%
7	2.825	553	555	558	rBV3	372	234	0.02%	0.003%
8	2.992	604	607	610	rBV3	397	276	0.03%	0.004%
9	3.163	657	660	664	rVB2	268	187	0.02%	0.002%
10	3.375	724	726	729	rVB	323	129	0.01%	0.002%
11	3.397	729	733	735	rBV3	401	334	0.03%	0.004%
12	3.439	744	746	751	rVB2	338	229	0.02%	0.003%
13	3.468	751	755	759	rBV	199	185	0.02%	0.002%
14	3.645	806	810	811	rBV	361	245	0.03%	0.003%
15	3.761	842	846	849	rBV2	306	294	0.03%	0.004%
16	3.815	861	863	866	rVB	385	191	0.02%	0.002%
17	3.844	866	872	874	rBV2	504	304	0.03%	0.004%
18	3.905	880	891	936	rBV	55676	216942	22.19%	2.804%
19	4.349	1013	1029	1050	rBV	152182	380538	38.92%	4.919%
20	4.744	1148	1152	1159	rBV3	387	395	0.04%	0.005%
21	4.937	1209	1212	1214	rBV2	328	197	0.02%	0.003%
22	4.986	1225	1227	1230	rBV3	285	137	0.01%	0.002%
23	5.047	1230	1246	1276	rBV2	388424	977677	100.00%	12.638%
24	5.436	1365	1367	1372	rVB2	386	214	0.02%	0.003%
25	5.465	1374	1376	1379	rVV2	371	196	0.02%	0.003%
26	5.481	1379	1381	1387	rVB	237	195	0.02%	0.003%
27	5.539	1398	1399	1403	rVB3	328	135	0.01%	0.002%
28	5.619	1412	1424	1457	rBV	279167	575022	58.82%	7.433%
29	5.912	1504	1515	1529	rBV8	7260	16274	1.66%	0.210%
30	6.024	1546	1550	1551	rBV3	397	239	0.02%	0.003%
31	6.072	1551	1565	1592	rVV	209241	434631	44.46%	5.618%
32	6.336	1644	1647	1650	rBV4	460	257	0.03%	0.003%
33	6.416	1669	1672	1676	rBV2	292	223	0.02%	0.003%
34	6.674	1750	1752	1756	rBV	249	143	0.01%	0.002%
35	6.699	1758	1760	1766	rBV2	283	171	0.02%	0.002%
36	6.767	1777	1781	1783	rBV2	295	200	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
 Data File : VV022422.D
 Acq On : 30 Sep 2021 11:18
 Operator : SY/MD
 Sample : M3978-03DL 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A15DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

37	6.989	1838	1850	1880	rBV	109206	208002	21.28%	2.689%
38	7.223	1919	1923	1924	rBV2	252	164	0.02%	0.002%
39	7.243	1928	1929	1933	rVV	340	172	0.02%	0.002%
40	7.317	1940	1952	1971	rBV	446032	783575	80.15%	10.129%
41	7.587	2032	2036	2037	rBV2	339	243	0.02%	0.003%
42	7.622	2038	2047	2073	rVV	72530	134203	13.73%	1.735%
43	7.831	2105	2112	2114	rBV3	554	609	0.06%	0.008%
44	7.976	2145	2157	2182	rBV	263346	453085	46.34%	5.857%
45	8.092	2184	2193	2227	rBV	221578	428434	43.82%	5.538%
46	8.465	2306	2309	2313	rBV2	530	285	0.03%	0.004%
47	8.481	2313	2314	2320	rVB2	476	329	0.03%	0.004%
48	8.510	2320	2323	2327	rBV3	390	303	0.03%	0.004%
49	8.674	2371	2374	2380	rVB2	367	249	0.03%	0.003%
50	8.725	2387	2390	2393	rBV2	293	215	0.02%	0.003%
51	8.854	2419	2430	2457	rBV	415374	693512	70.93%	8.965%
52	9.072	2494	2498	2503	rVB5	419	377	0.04%	0.005%
53	9.095	2503	2505	2508	rBV	341	159	0.02%	0.002%
54	9.153	2519	2523	2528	rBV4	776	765	0.08%	0.010%
55	9.313	2569	2573	2576	rBV	345	246	0.03%	0.003%
56	9.374	2590	2592	2594	rVB2	495	175	0.02%	0.002%
57	9.587	2655	2658	2661	rBV	184	139	0.01%	0.002%
58	9.696	2690	2692	2699	rBV3	220	166	0.02%	0.002%
59	9.751	2706	2709	2714	rVB	371	251	0.03%	0.003%
60	9.773	2714	2716	2718	rBV2	398	166	0.02%	0.002%
61	9.879	2747	2749	2755	rVB2	294	166	0.02%	0.002%
62	9.921	2760	2762	2769	rVB2	365	411	0.04%	0.005%
63	9.966	2773	2776	2777	rVV2	243	138	0.01%	0.002%
64	9.973	2777	2778	2784	rVB2	479	246	0.03%	0.003%
65	10.127	2818	2826	2836	rVB4	3175	4722	0.48%	0.061%
66	10.217	2842	2854	2872	rBV	287545	455293	46.57%	5.885%
67	10.323	2882	2887	2892	rVB4	1011	877	0.09%	0.011%
68	10.474	2932	2934	2937	rVB	473	220	0.02%	0.003%
69	10.545	2953	2956	2959	rBV2	232	211	0.02%	0.003%
70	10.577	2960	2966	2968	rBV2	573	566	0.06%	0.007%
71	10.603	2972	2974	2975	rBV	579	223	0.02%	0.003%
72	10.686	2997	3000	3004	rBV	364	298	0.03%	0.004%
73	10.892	3059	3064	3066	rBV4	781	687	0.07%	0.009%
74	10.915	3067	3071	3073	rBV3	1509	1241	0.13%	0.016%
75	10.985	3088	3093	3095	rBV	420	336	0.03%	0.004%
76	11.030	3104	3107	3109	rBV2	518	328	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW093021\
 Data File : VW022422.D
 Acq On : 30 Sep 2021 11:18
 Operator : SY/MD
 Sample : M3978-03DL 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A15DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M

Title : VOC Analysis

77	11.149	3135	3144	3150	rBV3	1656	1875	0.19%	0.024%
78	11.252	3163	3176	3198	rBV	398791	628867	64.32%	8.129%
79	11.487	3247	3249	3252	rVB2	548	262	0.03%	0.003%
80	11.558	3267	3271	3274	rBV2	405	356	0.04%	0.005%
81	11.625	3280	3292	3317	rBV	438617	674241	68.96%	8.716%
82	11.757	3330	3333	3336	rBV3	472	300	0.03%	0.004%
83	12.101	3439	3440	3444	rVB2	859	376	0.04%	0.005%
84	12.297	3498	3501	3507	rVB2	277	262	0.03%	0.003%
85	12.342	3514	3515	3517	rBV	357	153	0.02%	0.002%
86	12.397	3530	3532	3537	rVB2	256	169	0.02%	0.002%
87	12.590	3590	3592	3595	rBV2	392	191	0.02%	0.002%
88	12.677	3616	3619	3622	rBV2	340	237	0.02%	0.003%
89	12.728	3631	3635	3636	rBV2	294	196	0.02%	0.003%
90	12.776	3647	3650	3652	rBV2	398	265	0.03%	0.003%
91	12.879	3678	3682	3684	rBV	241	205	0.02%	0.003%
92	12.982	3712	3714	3716	rBV3	352	168	0.02%	0.002%
93	13.403	3843	3845	3847	rVB	358	154	0.02%	0.002%
94	13.583	3896	3901	3904	rVB2	324	307	0.03%	0.004%
95	13.837	3977	3980	3983	rBV3	316	214	0.02%	0.003%
96	13.992	4026	4028	4031	rBV3	460	214	0.02%	0.003%
97	14.050	4043	4046	4049	rBV2	351	288	0.03%	0.004%
98	14.117	4064	4067	4069	rBV2	417	250	0.03%	0.003%
99	14.149	4075	4077	4081	rVB4	332	139	0.01%	0.002%
100	14.284	4117	4119	4122	rBV2	474	272	0.03%	0.004%




Sum of corrected areas: 7735987

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
Data File : VV022422.D
Acq On : 30 Sep 2021 11:18
Operator : SY/MD
Sample : M3978-03DL 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A15DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

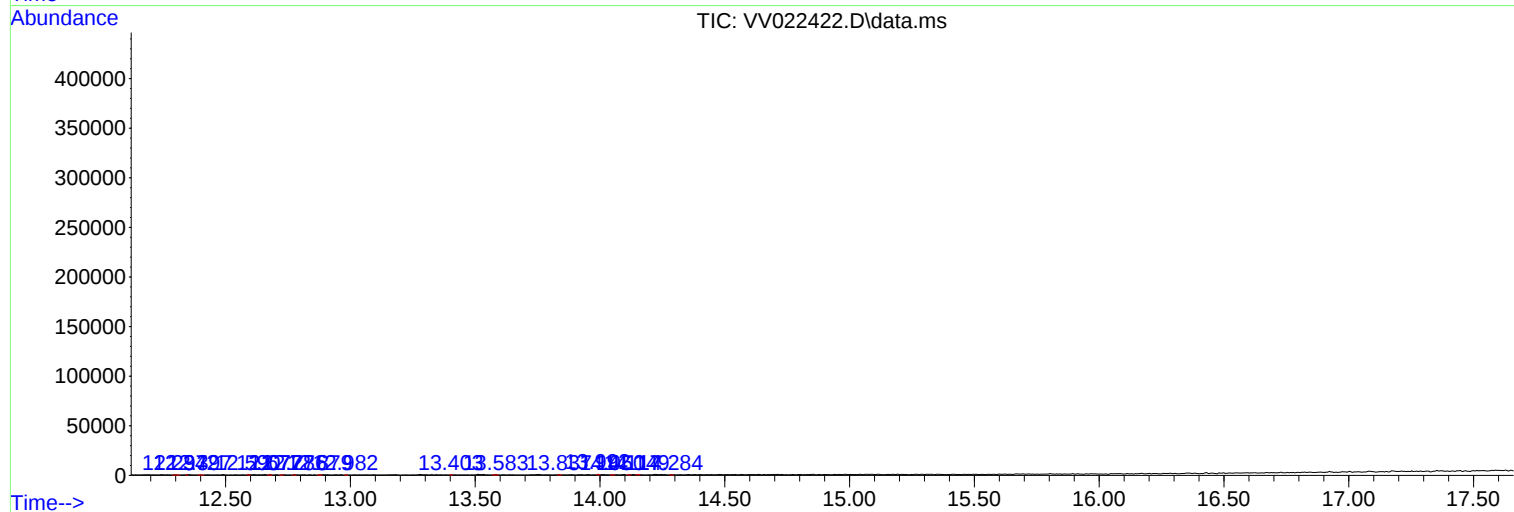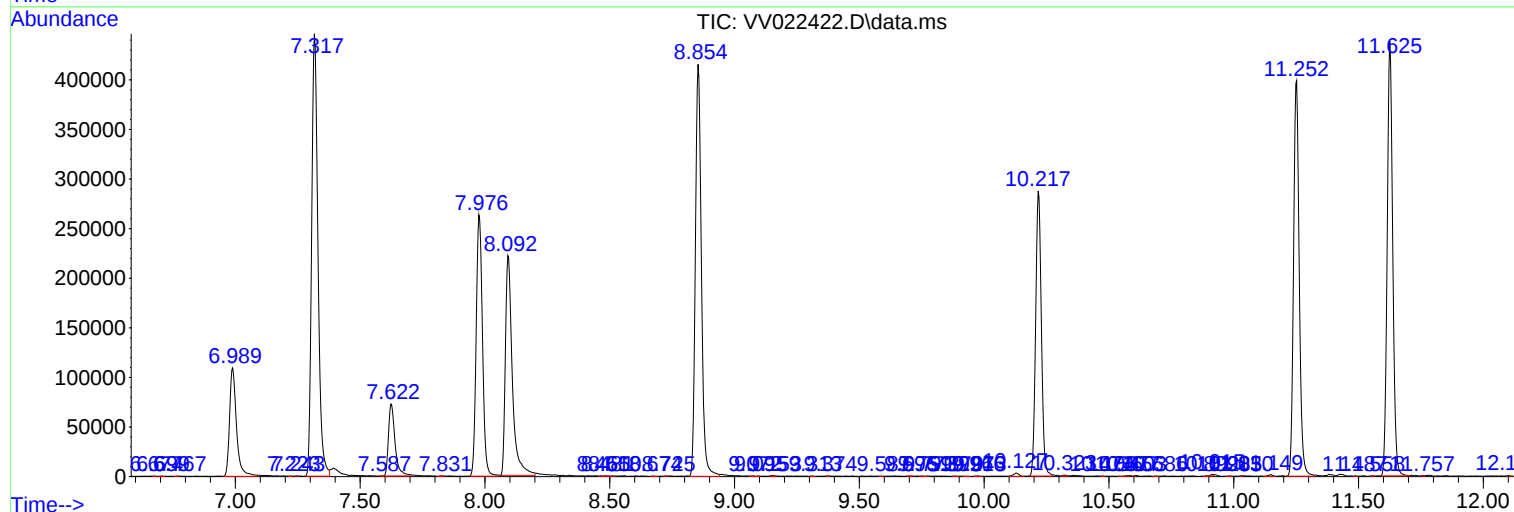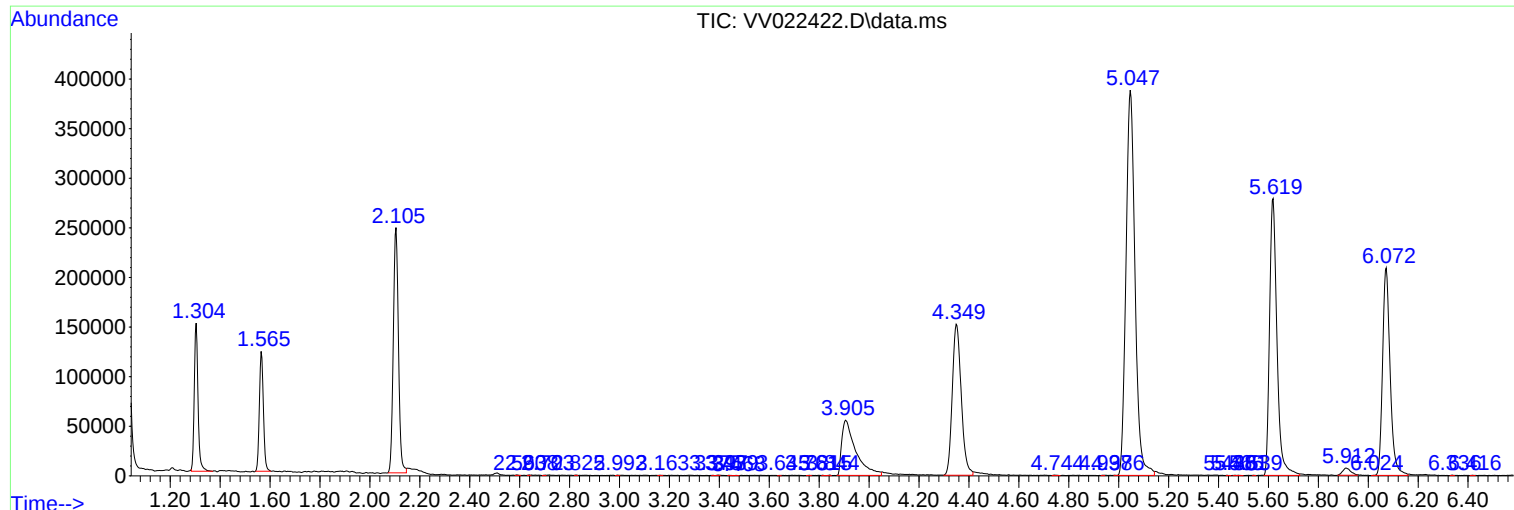

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
Data File : VV022422.D
Acq On : 30 Sep 2021 11:18
Operator : SY/MD
Sample : M3978-03DL 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A15DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
Data File : VV022422.D
Acq On : 30 Sep 2021 11:18
Operator : SY/MD
Sample : M3978-03DL 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A15DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc