

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
 Data File : VV022426.D
 Acq On : 30 Sep 2021 12:54
 Operator : SY/MD
 Sample : M3978-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A19

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

Signal : TIC: VV022426.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	97	rVB	151970	154981	16.05%	1.966%
2	1.561	156	162	176	rVB	119040	137629	14.25%	1.746%
3	2.105	321	331	356	rVB	247847	366065	37.91%	4.644%
4	2.278	383	385	387	rBV2	652	412	0.04%	0.005%
5	2.593	481	483	484	rBV	403	187	0.02%	0.002%
6	2.770	527	538	545	rBV3	2607	5346	0.55%	0.068%
7	2.947	590	593	596	rBV	366	229	0.02%	0.003%
8	3.256	686	689	690	rBV	292	137	0.01%	0.002%
9	3.355	718	720	724	rBV	288	264	0.03%	0.003%
10	3.507	758	767	769	rBV	514	536	0.06%	0.007%
11	3.664	813	816	820	rBV	244	197	0.02%	0.002%
12	3.696	824	826	831	rBV2	197	154	0.02%	0.002%
13	3.806	858	860	864	rBV2	403	293	0.03%	0.004%
14	3.876	872	882	916	rBV	77172	212822	22.04%	2.700%
15	4.349	1015	1029	1063	rVB	141596	374349	38.77%	4.749%
16	4.571	1096	1098	1099	rBV2	366	166	0.02%	0.002%
17	4.642	1118	1120	1123	rBV2	274	202	0.02%	0.003%
18	4.696	1134	1137	1138	rBV	379	168	0.02%	0.002%
19	4.735	1147	1149	1150	rBV	410	156	0.02%	0.002%
20	4.767	1157	1159	1161	rBV2	288	150	0.02%	0.002%
21	4.847	1181	1184	1188	rVB3	527	330	0.03%	0.004%
22	4.905	1200	1202	1206	rVB2	415	299	0.03%	0.004%
23	4.931	1206	1210	1213	rBV3	292	234	0.02%	0.003%
24	4.966	1217	1221	1224	rVB2	321	219	0.02%	0.003%
25	5.047	1230	1246	1268	rBV2	379413	965674	100.00%	12.252%
26	5.371	1343	1347	1353	rBV2	464	395	0.04%	0.005%
27	5.397	1353	1355	1357	rVB	352	151	0.02%	0.002%
28	5.420	1359	1362	1364	rBV2	370	231	0.02%	0.003%
29	5.619	1412	1424	1449	rBV	264007	533724	55.27%	6.772%
30	5.921	1506	1518	1533	rVB	6803	16518	1.71%	0.210%
31	6.011	1543	1546	1549	rVB	555	349	0.04%	0.004%
32	6.069	1551	1564	1589	rBV	208427	435644	45.11%	5.527%
33	6.333	1644	1646	1652	rVB2	318	222	0.02%	0.003%
34	6.375	1656	1659	1663	rVB2	303	203	0.02%	0.003%
35	6.439	1677	1679	1682	rVB2	367	195	0.02%	0.002%
36	6.465	1684	1687	1690	rVV	282	179	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
 Data File : VV022426.D
 Acq On : 30 Sep 2021 12:54
 Operator : SY/MD
 Sample : M3978-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A19

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

37	6.564	1714	1718	1719	rBV3	358	256	0.03%	0.003%
38	6.629	1734	1738	1741	rBV3	364	255	0.03%	0.003%
39	6.918	1826	1828	1830	rBV2	377	154	0.02%	0.002%
40	6.989	1838	1850	1871	rBV	108388	200998	20.81%	2.550%
41	7.204	1914	1917	1921	rBV3	502	396	0.04%	0.005%
42	7.317	1939	1952	1972	rBV	440624	773882	80.14%	9.819%
43	7.622	2038	2047	2076	rBV	76650	137215	14.21%	1.741%
44	7.889	2128	2130	2135	rBV3	269	231	0.02%	0.003%
45	7.918	2135	2139	2142	rBV3	511	448	0.05%	0.006%
46	7.976	2143	2157	2181	rBV	442073	754718	78.15%	9.575%
47	8.088	2183	2192	2227	rVV	231955	420811	43.58%	5.339%
48	8.416	2292	2294	2296	rBV	358	171	0.02%	0.002%
49	8.436	2297	2300	2301	rBV2	605	312	0.03%	0.004%
50	8.535	2329	2331	2333	rBV	424	284	0.03%	0.004%
51	8.587	2344	2347	2351	rBV3	414	276	0.03%	0.004%
52	8.767	2401	2403	2407	rBV3	308	191	0.02%	0.002%
53	8.802	2410	2414	2416	rBV	310	167	0.02%	0.002%
54	8.854	2419	2430	2457	rBV	401806	656240	67.96%	8.326%
55	9.217	2540	2543	2546	rBV3	330	215	0.02%	0.003%
56	9.291	2563	2566	2567	rBV	320	158	0.02%	0.002%
57	9.336	2576	2580	2583	rBV2	558	402	0.04%	0.005%
58	9.352	2583	2585	2587	rBV2	188	135	0.01%	0.002%
59	9.429	2606	2609	2611	rBV2	319	237	0.02%	0.003%
60	9.503	2630	2632	2637	rVB	302	161	0.02%	0.002%
61	9.538	2641	2643	2646	rBV2	505	250	0.03%	0.003%
62	9.883	2746	2750	2755	rBV3	165	161	0.02%	0.002%
63	10.011	2786	2790	2793	rBV3	460	325	0.03%	0.004%
64	10.130	2820	2827	2835	rVB6	2867	4232	0.44%	0.054%
65	10.217	2841	2854	2870	rBV	298349	470500	48.72%	5.969%
66	10.426	2914	2919	2924	rVB3	244	273	0.03%	0.003%
67	10.452	2925	2927	2931	rVV3	396	301	0.03%	0.004%
68	10.487	2934	2938	2942	rVB3	196	184	0.02%	0.002%
69	10.542	2953	2955	2961	rVB3	313	189	0.02%	0.002%
70	10.574	2961	2965	2966	rBV2	442	301	0.03%	0.004%
71	10.635	2982	2984	2986	rBV	324	141	0.01%	0.002%
72	10.651	2986	2989	2997	rVB3	549	546	0.06%	0.007%
73	10.709	3003	3007	3011	rBV2	316	243	0.03%	0.003%
74	10.831	3037	3045	3046	rBV3	504	480	0.05%	0.006%
75	10.918	3064	3072	3079	rBV4	2061	2709	0.28%	0.034%
76	11.030	3103	3107	3108	rBV2	472	284	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
 Data File : VV022426.D
 Acq On : 30 Sep 2021 12:54
 Operator : SY/MD
 Sample : M3978-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A19

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

77	11.146	3136	3143	3149	rBV6	1249	1726	0.18%	0.022%
78	11.252	3164	3176	3196	rBV	358388	574005	59.44%	7.283%
79	11.371	3208	3213	3214	rBV4	696	603	0.06%	0.008%
80	11.554	3267	3270	3271	rBV	423	207	0.02%	0.003%
81	11.625	3280	3292	3312	rBV	419195	661439	68.50%	8.392%
82	11.796	3339	3345	3348	rBV5	644	709	0.07%	0.009%
83	11.921	3380	3384	3386	rBV2	470	349	0.04%	0.004%
84	12.120	3442	3446	3448	rBV2	516	305	0.03%	0.004%
85	12.304	3501	3503	3506	rBV2	413	203	0.02%	0.003%
86	12.686	3620	3622	3626	rVB3	419	238	0.02%	0.003%
87	12.734	3633	3637	3638	rBV	358	243	0.03%	0.003%
88	12.789	3649	3654	3655	rBV	272	224	0.02%	0.003%
89	13.059	3735	3738	3743	rBV2	333	286	0.03%	0.004%
90	13.114	3752	3755	3757	rBV	258	158	0.02%	0.002%
91	13.159	3766	3769	3771	rBV	436	241	0.02%	0.003%
92	13.236	3791	3793	3794	rBV	463	224	0.02%	0.003%
93	13.291	3807	3810	3816	rBV2	418	440	0.05%	0.006%
94	13.497	3872	3874	3877	rBV2	395	200	0.02%	0.003%
95	13.664	3924	3926	3933	rVB2	499	299	0.03%	0.004%
96	13.738	3945	3949	3951	rBV	372	334	0.03%	0.004%
97	13.751	3951	3953	3958	rVB2	388	223	0.02%	0.003%
98	13.937	4009	4011	4014	rVB2	355	144	0.01%	0.002%
99	14.265	4109	4113	4114	rBV	350	240	0.02%	0.003%
100	14.316	4124	4129	4132	rBV3	370	383	0.04%	0.005%




Sum of corrected areas: 7881865

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
Data File : VV022426.D
Acq On : 30 Sep 2021 12:54
Operator : SY/MD
Sample : M3978-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
F4A19

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

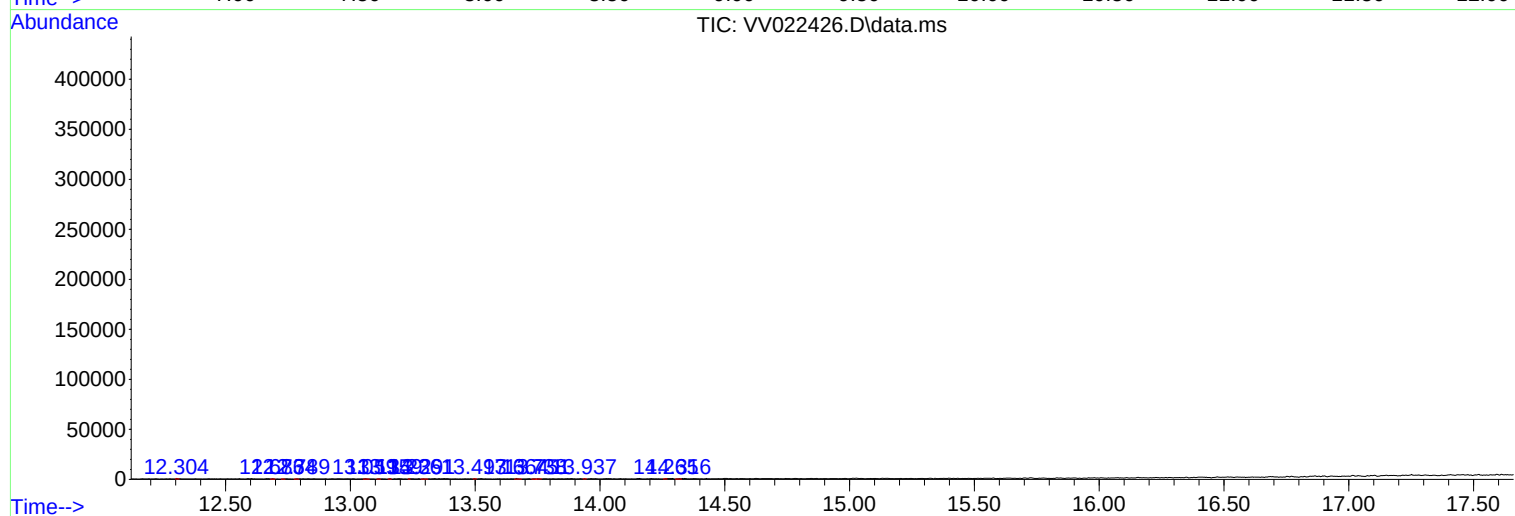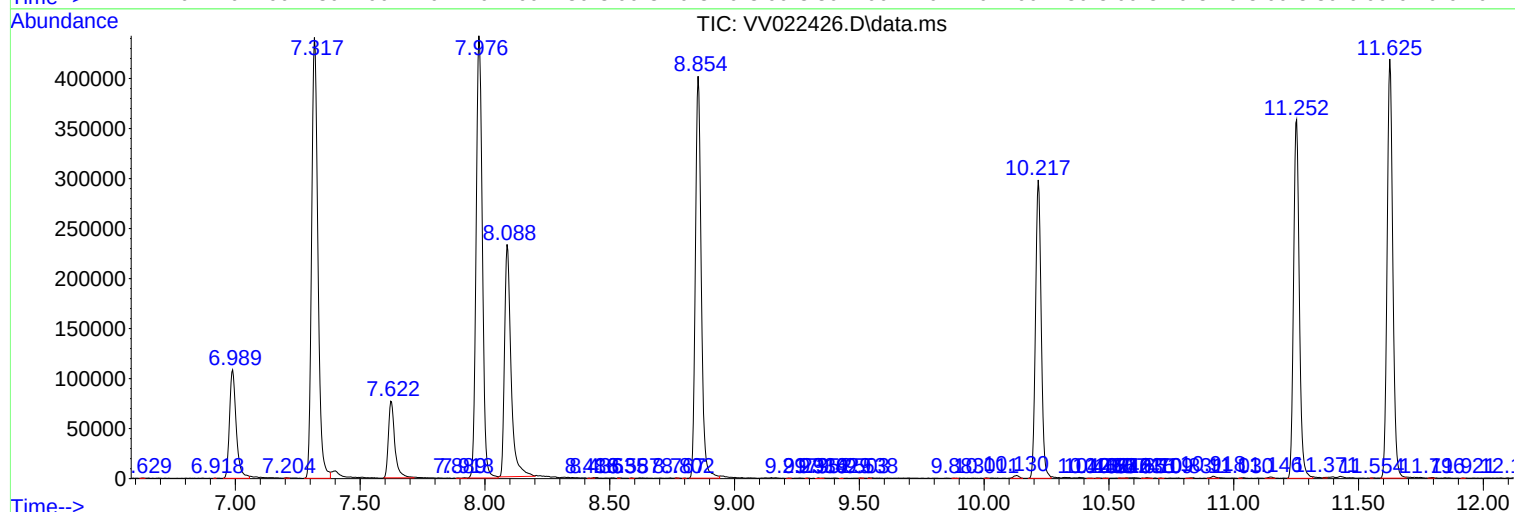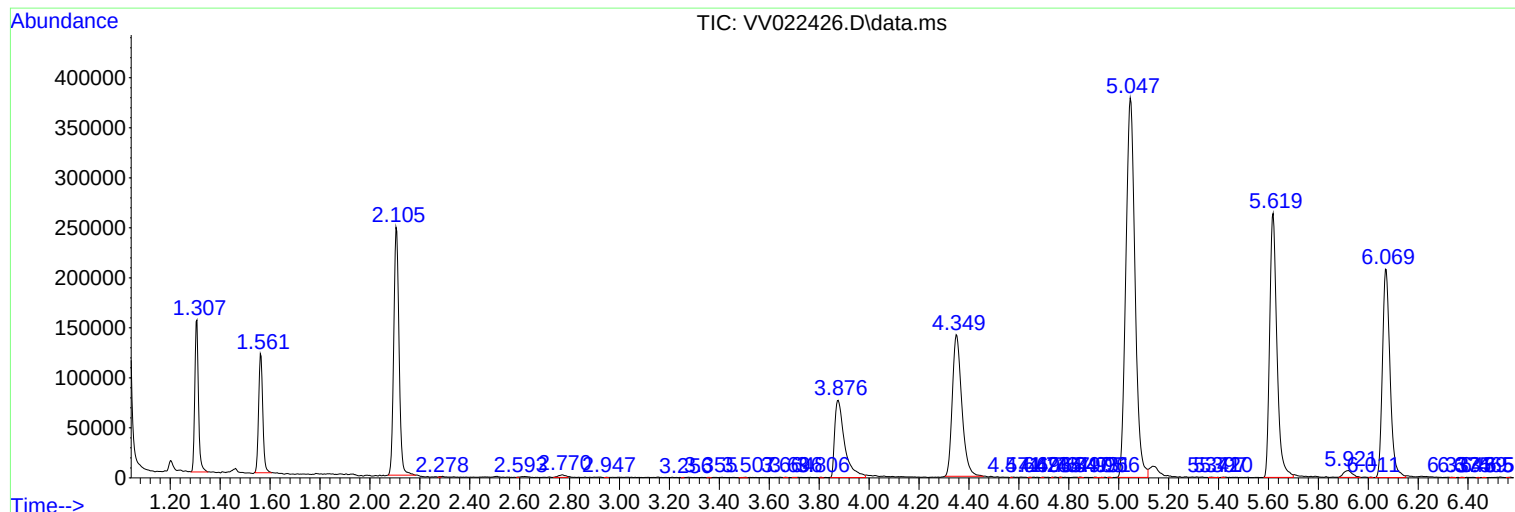

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
Data File : VV022426.D
Acq On : 30 Sep 2021 12:54
Operator : SY/MD
Sample : M3978-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A19

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
Data File : VV022426.D
Acq On : 30 Sep 2021 12:54
Operator : SY/MD
Sample : M3978-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A19

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
