

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
 Data File : VV022427.D
 Acq On : 30 Sep 2021 13:18
 Operator : SY/MD
 Sample : M3978-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A20

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

Signal : TIC: VV022427.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	96	rBV	150519	150939	15.99%	1.889%
2	1.561	155	162	176	rVB	116664	140791	14.92%	1.762%
3	2.105	321	331	359	rVB	242036	362365	38.40%	4.534%
4	2.371	411	414	416	rBV2	309	185	0.02%	0.002%
5	2.683	509	511	513	rBV2	350	183	0.02%	0.002%
6	2.722	521	523	527	rVB	414	182	0.02%	0.002%
7	2.767	527	537	547	rBV5	2464	5405	0.57%	0.068%
8	2.847	559	562	563	rBV	342	178	0.02%	0.002%
9	2.957	594	596	599	rVB	319	185	0.02%	0.002%
10	2.976	599	602	604	rBV2	481	267	0.03%	0.003%
11	2.995	604	608	613	rVB2	349	345	0.04%	0.004%
12	3.037	619	621	624	rVB3	473	200	0.02%	0.003%
13	3.143	649	654	657	rBV2	443	346	0.04%	0.004%
14	3.240	680	684	689	rBV3	363	348	0.04%	0.004%
15	3.268	689	693	694	rBV	296	197	0.02%	0.002%
16	3.442	743	747	753	rVB2	412	304	0.03%	0.004%
17	3.468	753	755	757	rBV2	293	194	0.02%	0.002%
18	3.561	780	784	786	rBV2	354	227	0.02%	0.003%
19	3.693	820	825	828	rVB3	427	345	0.04%	0.004%
20	3.715	828	832	836	rBV3	259	247	0.03%	0.003%
21	3.876	872	882	919	rBV	76383	224090	23.75%	2.804%
22	4.272	1002	1005	1008	rBV4	553	378	0.04%	0.005%
23	4.349	1014	1029	1057	rBV	141437	371610	39.38%	4.650%
24	4.664	1123	1127	1128	rBV	400	249	0.03%	0.003%
25	4.805	1168	1171	1173	rBV3	241	199	0.02%	0.002%
26	4.953	1214	1217	1220	rVB3	378	215	0.02%	0.003%
27	5.047	1229	1246	1267	rBV2	369503	943682	100.00%	11.807%
28	5.413	1359	1360	1363	rBV2	277	170	0.02%	0.002%
29	5.497	1384	1386	1390	rVB	453	243	0.03%	0.003%
30	5.619	1411	1424	1462	rBV	270287	557254	59.05%	6.972%
31	5.915	1505	1516	1535	rVB8	7851	18684	1.98%	0.234%
32	6.069	1551	1564	1601	rBV	206930	431849	45.76%	5.403%
33	6.278	1627	1629	1632	rVB4	424	223	0.02%	0.003%
34	6.384	1658	1662	1664	rBV3	290	201	0.02%	0.003%
35	6.529	1704	1707	1711	rVV4	354	259	0.03%	0.003%
36	6.747	1774	1775	1778	rVB	487	231	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
 Data File : VV022427.D
 Acq On : 30 Sep 2021 13:18
 Operator : SY/MD
 Sample : M3978-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A20

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

37	6.857	1806	1809	1813	rVV2	318	226	0.02%	0.003%
38	6.892	1816	1820	1823	rBV	227	169	0.02%	0.002%
39	6.989	1839	1850	1872	rBV	106055	198241	21.01%	2.480%
40	7.156	1900	1902	1909	rVB4	656	657	0.07%	0.008%
41	7.204	1915	1917	1918	rBV	394	167	0.02%	0.002%
42	7.317	1939	1952	1971	rBV	433687	755259	80.03%	9.450%
43	7.622	2037	2047	2072	rBV	72027	131525	13.94%	1.646%
44	7.866	2120	2123	2125	rBV	298	177	0.02%	0.002%
45	7.976	2144	2157	2183	rBV	515189	874776	92.70%	10.945%
46	8.088	2183	2192	2229	rVV	223378	411714	43.63%	5.151%
47	8.439	2299	2301	2304	rVB3	595	364	0.04%	0.005%
48	8.458	2304	2307	2309	rBV	556	395	0.04%	0.005%
49	8.516	2322	2325	2329	rBV4	372	262	0.03%	0.003%
50	8.609	2352	2354	2357	rVB2	314	164	0.02%	0.002%
51	8.628	2357	2360	2363	rBV2	422	314	0.03%	0.004%
52	8.670	2369	2373	2374	rBV	317	217	0.02%	0.003%
53	8.741	2390	2395	2396	rBV2	272	196	0.02%	0.002%
54	8.853	2419	2430	2457	rBV	412621	679798	72.04%	8.505%
55	9.188	2530	2534	2540	rVB2	322	336	0.04%	0.004%
56	9.220	2540	2544	2547	rBV2	376	267	0.03%	0.003%
57	9.509	2632	2634	2635	rBV	353	171	0.02%	0.002%
58	9.522	2635	2638	2640	rVV2	233	181	0.02%	0.002%
59	9.561	2648	2650	2654	rVB2	409	197	0.02%	0.002%
60	9.625	2667	2670	2671	rBV	399	237	0.03%	0.003%
61	9.654	2676	2679	2681	rVV2	267	173	0.02%	0.002%
62	9.667	2681	2683	2685	rVV	324	192	0.02%	0.002%
63	9.802	2723	2725	2730	rBB2	194	169	0.02%	0.002%
64	10.127	2819	2826	2835	rVB3	2366	3273	0.35%	0.041%
65	10.217	2842	2854	2874	rBV	299112	465691	49.35%	5.827%
66	10.413	2911	2915	2917	rBV3	285	218	0.02%	0.003%
67	10.506	2940	2944	2945	rBV2	231	167	0.02%	0.002%
68	10.561	2959	2961	2965	rVB2	475	317	0.03%	0.004%
69	10.583	2965	2968	2977	rVB5	749	931	0.10%	0.012%
70	10.657	2989	2991	2994	rVB2	369	189	0.02%	0.002%
71	10.763	3022	3024	3027	rBV	344	176	0.02%	0.002%
72	10.844	3047	3049	3054	rVB2	480	245	0.03%	0.003%
73	10.924	3067	3074	3081	rBV5	1720	2638	0.28%	0.033%
74	11.033	3105	3108	3109	rBV	486	244	0.03%	0.003%
75	11.143	3139	3142	3151	rVB4	736	876	0.09%	0.011%
76	11.252	3165	3176	3200	rBV	368173	593108	62.85%	7.421%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
 Data File : VV022427.D
 Acq On : 30 Sep 2021 13:18
 Operator : SY/MD
 Sample : M3978-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A20

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

77	11.429	3225	3231	3236	rBV6	1332	1531	0.16%	0.019%
78	11.484	3245	3248	3251	rBV3	256	170	0.02%	0.002%
79	11.625	3280	3292	3314	rBV	407492	647987	68.67%	8.107%
80	11.895	3374	3376	3379	rBV2	359	176	0.02%	0.002%
81	12.011	3409	3412	3415	rBV	359	349	0.04%	0.004%
82	12.046	3421	3423	3427	rBV2	331	269	0.03%	0.003%
83	12.149	3452	3455	3456	rBV	319	177	0.02%	0.002%
84	12.371	3519	3524	3527	rVB2	288	200	0.02%	0.003%
85	12.561	3581	3583	3585	rBV2	334	180	0.02%	0.002%
86	12.631	3602	3605	3609	rVB3	493	303	0.03%	0.004%
87	12.664	3611	3615	3618	rVB3	386	293	0.03%	0.004%
88	12.828	3664	3666	3670	rVB2	298	176	0.02%	0.002%
89	12.860	3673	3676	3680	rVB	467	383	0.04%	0.005%
90	12.882	3680	3683	3686	rBV3	385	249	0.03%	0.003%
91	13.303	3812	3814	3817	rBV2	220	165	0.02%	0.002%
92	13.438	3853	3856	3860	rBV	392	204	0.02%	0.003%
93	13.959	4014	4018	4019	rBV2	355	222	0.02%	0.003%
94	13.988	4025	4027	4030	rBV3	265	188	0.02%	0.002%
95	14.024	4036	4038	4040	rBV2	355	169	0.02%	0.002%
96	14.085	4055	4057	4061	rVB4	381	256	0.03%	0.003%
97	14.107	4061	4064	4068	rBV3	274	247	0.03%	0.003%
98	14.609	4218	4220	4224	rBV	408	270	0.03%	0.003%
99	15.088	4367	4369	4374	rBV2	481	340	0.04%	0.004%
100	15.728	4566	4568	4573	rBV3	615	373	0.04%	0.005%




Sum of corrected areas: 7992464

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
Data File : VV022427.D
Acq On : 30 Sep 2021 13:18
Operator : SY/MD
Sample : M3978-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A20

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

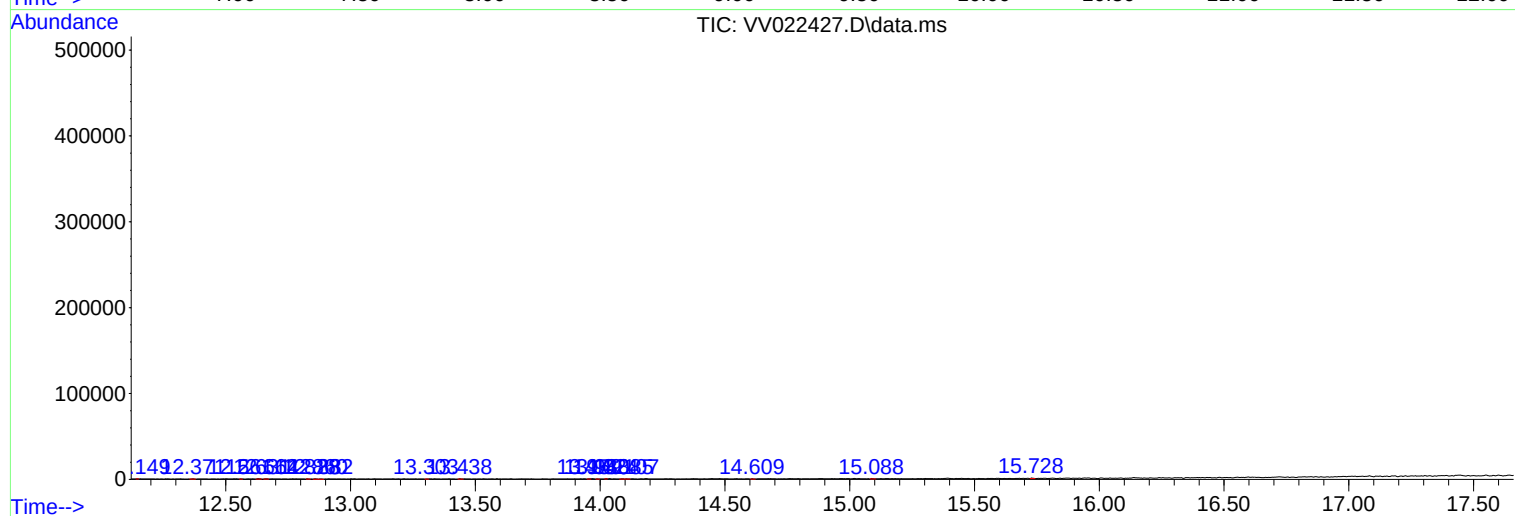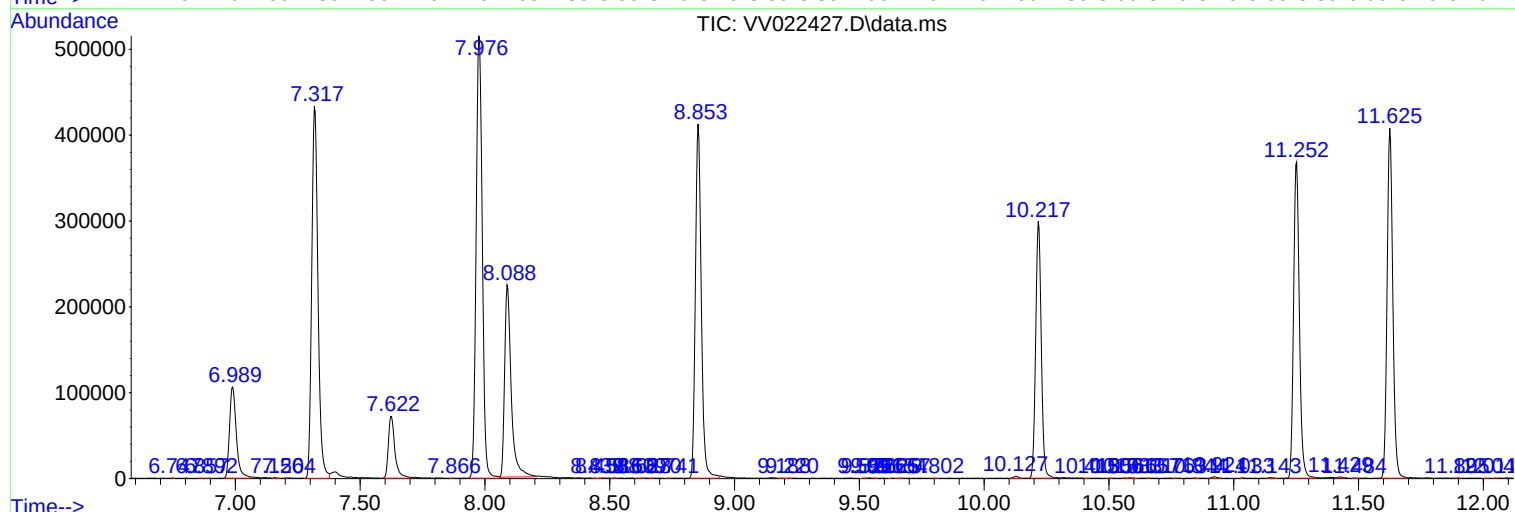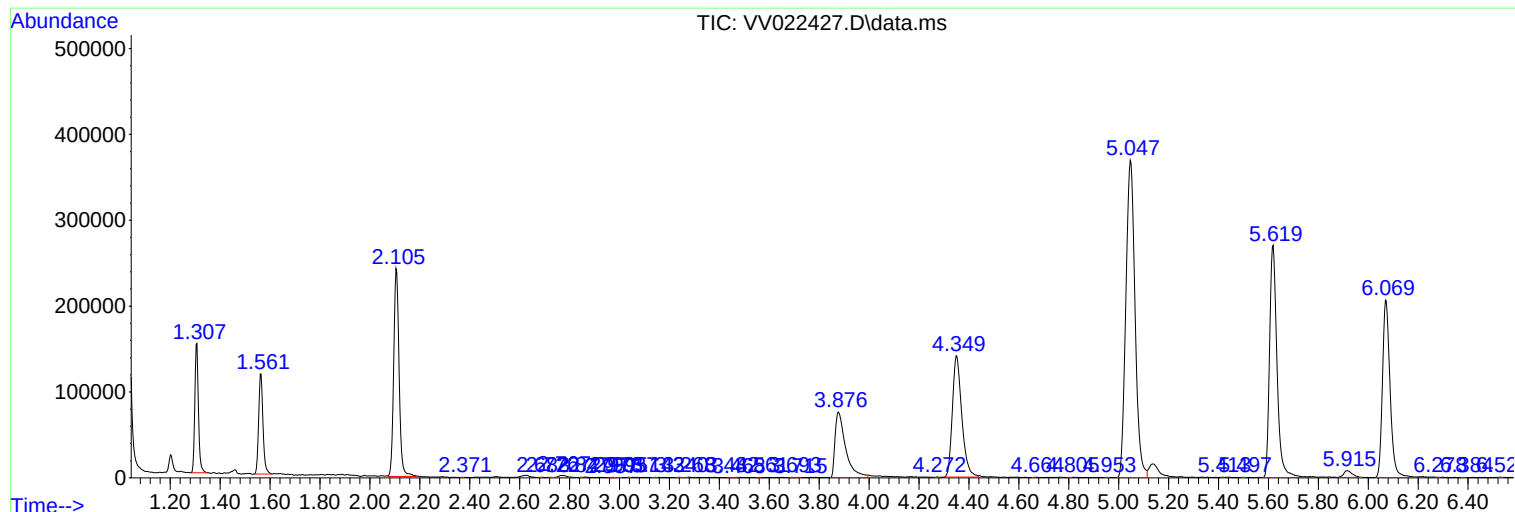

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
Data File : VV022427.D
Acq On : 30 Sep 2021 13:18
Operator : SY/MD
Sample : M3978-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A20

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
Data File : VV022427.D
Acq On : 30 Sep 2021 13:18
Operator : SY/MD
Sample : M3978-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A20

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
