

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
 Data File : VV022429.D
 Acq On : 30 Sep 2021 14:06
 Operator : SY/MD
 Sample : M3978-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A33

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M

Title : VOC Analysis

Signal : TIC: VV022429.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	99	rVB	151982	154084	8.74%	1.703%
2	1.564	156	163	176	rBV	123148	136342	7.73%	1.507%
3	2.105	321	331	350	rBV	244016	356516	20.21%	3.941%
4	2.436	432	434	437	rBV2	390	232	0.01%	0.003%
5	2.712	515	520	521	rBV	276	228	0.01%	0.003%
6	2.777	526	540	552	rBV3	4711	11061	0.63%	0.122%
7	2.918	581	584	588	rBV	405	362	0.02%	0.004%
8	2.995	605	608	610	rBV	272	216	0.01%	0.002%
9	3.153	655	657	662	rBV	252	268	0.02%	0.003%
10	3.179	662	665	668	rVB2	518	264	0.01%	0.003%
11	3.275	691	695	698	rBV	273	230	0.01%	0.003%
12	3.320	706	709	711	rBV2	223	142	0.01%	0.002%
13	3.590	791	793	795	rVB2	439	170	0.01%	0.002%
14	3.902	879	890	922	rBV2	59524	209772	11.89%	2.319%
15	4.349	1013	1029	1054	rBV	146472	380157	21.55%	4.202%
16	4.600	1106	1107	1111	rBV3	346	214	0.01%	0.002%
17	4.625	1111	1115	1116	rBV3	398	261	0.01%	0.003%
18	4.654	1123	1124	1127	rBV	260	174	0.01%	0.002%
19	4.937	1208	1212	1216	rVB2	484	376	0.02%	0.004%
20	5.047	1229	1246	1289	rBV2	382382	989377	56.09%	10.937%
21	5.288	1318	1321	1322	rBV2	499	260	0.01%	0.003%
22	5.358	1340	1343	1344	rBV2	398	187	0.01%	0.002%
23	5.413	1358	1360	1363	rBV2	585	359	0.02%	0.004%
24	5.432	1363	1366	1370	rVB3	497	391	0.02%	0.004%
25	5.490	1381	1384	1386	rBV3	621	333	0.02%	0.004%
26	5.545	1399	1401	1404	rBV2	273	180	0.01%	0.002%
27	5.619	1412	1424	1461	rBV	266793	556305	31.54%	6.150%
28	5.838	1490	1492	1496	rBV3	573	338	0.02%	0.004%
29	5.918	1504	1517	1535	rBV3	18448	42573	2.41%	0.471%
30	6.072	1550	1565	1599	rBV2	208488	442212	25.07%	4.888%
31	6.278	1627	1629	1634	rVB2	360	223	0.01%	0.002%
32	6.358	1652	1654	1658	rVB2	316	148	0.01%	0.002%
33	6.397	1664	1666	1668	rBV2	456	196	0.01%	0.002%
34	6.452	1681	1683	1685	rVB	535	180	0.01%	0.002%
35	6.580	1719	1723	1725	rVB2	293	203	0.01%	0.002%
36	6.625	1735	1737	1740	rBV	352	283	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
 Data File : VV022429.D
 Acq On : 30 Sep 2021 14:06
 Operator : SY/MD
 Sample : M3978-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A33

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

37	6.664	1744	1749	1752	rVV3	505	446	0.03%	0.005%
38	6.677	1752	1753	1757	rVV	341	178	0.01%	0.002%
39	6.696	1757	1759	1763	rVV2	228	165	0.01%	0.002%
40	6.947	1834	1837	1839	rBV2	287	163	0.01%	0.002%
41	6.989	1839	1850	1877	rBV	105414	204780	11.61%	2.264%
42	7.317	1941	1952	1973	rBV	445128	782321	44.35%	8.648%
43	7.567	2028	2030	2032	rBV	489	268	0.02%	0.003%
44	7.622	2038	2047	2071	rBV	76782	135715	7.69%	1.500%
45	7.873	2122	2125	2127	rBV	313	230	0.01%	0.003%
46	7.931	2139	2143	2144	rBV3	518	394	0.02%	0.004%
47	7.976	2144	2157	2183	rVV	1045900	1763910	100.00%	19.499%
48	8.091	2184	2193	2232	rVB	236955	440792	24.99%	4.873%
49	8.509	2320	2323	2325	rBV2	219	182	0.01%	0.002%
50	8.526	2326	2328	2331	rVV	471	309	0.02%	0.003%
51	8.555	2335	2337	2341	rBV2	317	196	0.01%	0.002%
52	8.619	2353	2357	2359	rBV	423	284	0.02%	0.003%
53	8.670	2371	2373	2377	rBV3	561	366	0.02%	0.004%
54	8.702	2380	2383	2386	rBV2	291	234	0.01%	0.003%
55	8.741	2392	2395	2396	rBV2	399	167	0.01%	0.002%
56	8.776	2402	2406	2409	rVB	445	302	0.02%	0.003%
57	8.854	2418	2430	2453	rBV	412999	678326	38.46%	7.498%
58	9.075	2495	2499	2501	rBV	506	333	0.02%	0.004%
59	9.143	2517	2520	2522	rBV	492	340	0.02%	0.004%
60	9.368	2586	2590	2597	rBV4	647	618	0.04%	0.007%
61	9.407	2598	2602	2608	rVV3	393	407	0.02%	0.004%
62	9.497	2626	2630	2634	rVB2	349	364	0.02%	0.004%
63	9.519	2634	2637	2642	rBV3	314	269	0.02%	0.003%
64	9.542	2642	2644	2650	rBV	354	302	0.02%	0.003%
65	9.680	2686	2687	2690	rVB2	340	154	0.01%	0.002%
66	9.709	2693	2696	2700	rVB2	601	369	0.02%	0.004%
67	9.780	2714	2718	2721	rBV2	380	288	0.02%	0.003%
68	9.837	2733	2736	2740	rVB3	350	246	0.01%	0.003%
69	10.043	2797	2800	2802	rBV2	292	179	0.01%	0.002%
70	10.091	2813	2815	2817	rBV2	401	184	0.01%	0.002%
71	10.127	2820	2826	2835	rVB4	1718	2982	0.17%	0.033%
72	10.217	2842	2854	2875	rBV	291861	468362	26.55%	5.177%
73	10.352	2894	2896	2897	rBV3	357	159	0.01%	0.002%
74	10.464	2926	2931	2932	rBV	290	177	0.01%	0.002%
75	10.567	2962	2963	2964	rBV	491	151	0.01%	0.002%
76	10.606	2973	2975	2982	rVB4	661	457	0.03%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
 Data File : VV022429.D
 Acq On : 30 Sep 2021 14:06
 Operator : SY/MD
 Sample : M3978-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A33

Integration Parameters: LSCINT.P

Integrator: RTE

Smoother: OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

77	10.661	2990	2992	2994	rVB2	521	202	0.01%	0.002%
78	10.889	3060	3063	3065	rBV2	402	201	0.01%	0.002%
79	10.918	3067	3072	3079	rVB5	1669	2206	0.13%	0.024%
80	11.014	3099	3102	3103	rBV2	322	199	0.01%	0.002%
81	11.066	3116	3118	3121	rVB3	505	208	0.01%	0.002%
82	11.085	3121	3124	3128	rBV2	450	298	0.02%	0.003%
83	11.149	3138	3144	3153	rVB6	1231	1546	0.09%	0.017%
84	11.191	3153	3157	3159	rVB3	355	195	0.01%	0.002%
85	11.207	3160	3162	3164	rBV2	355	166	0.01%	0.002%
86	11.252	3164	3176	3201	rBV	385431	595268	33.75%	6.580%
87	11.509	3252	3256	3259	rBV2	367	269	0.02%	0.003%
88	11.545	3265	3267	3269	rBV2	562	283	0.02%	0.003%
89	11.625	3280	3292	3309	rBV	423455	671387	38.06%	7.422%
90	11.837	3355	3358	3360	rBV2	688	404	0.02%	0.004%
91	11.963	3394	3397	3400	rBV2	261	177	0.01%	0.002%
92	12.162	3454	3459	3463	rBV3	338	427	0.02%	0.005%
93	12.300	3499	3502	3503	rBV	336	163	0.01%	0.002%
94	12.468	3552	3554	3558	rVB3	288	156	0.01%	0.002%
95	12.583	3586	3590	3591	rBV	313	233	0.01%	0.003%
96	12.857	3673	3675	3678	rBV2	433	295	0.02%	0.003%
97	12.898	3687	3688	3694	rVV2	314	244	0.01%	0.003%
98	13.181	3774	3776	3779	rBV	470	248	0.01%	0.003%
99	13.496	3873	3874	3878	rBV	221	149	0.01%	0.002%
100	15.583	4520	4523	4526	rBV	545	455	0.03%	0.005%




Sum of corrected areas: 9046265

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
Data File : VV022429.D
Acq On : 30 Sep 2021 14:06
Operator : SY/MD
Sample : M3978-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A33

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

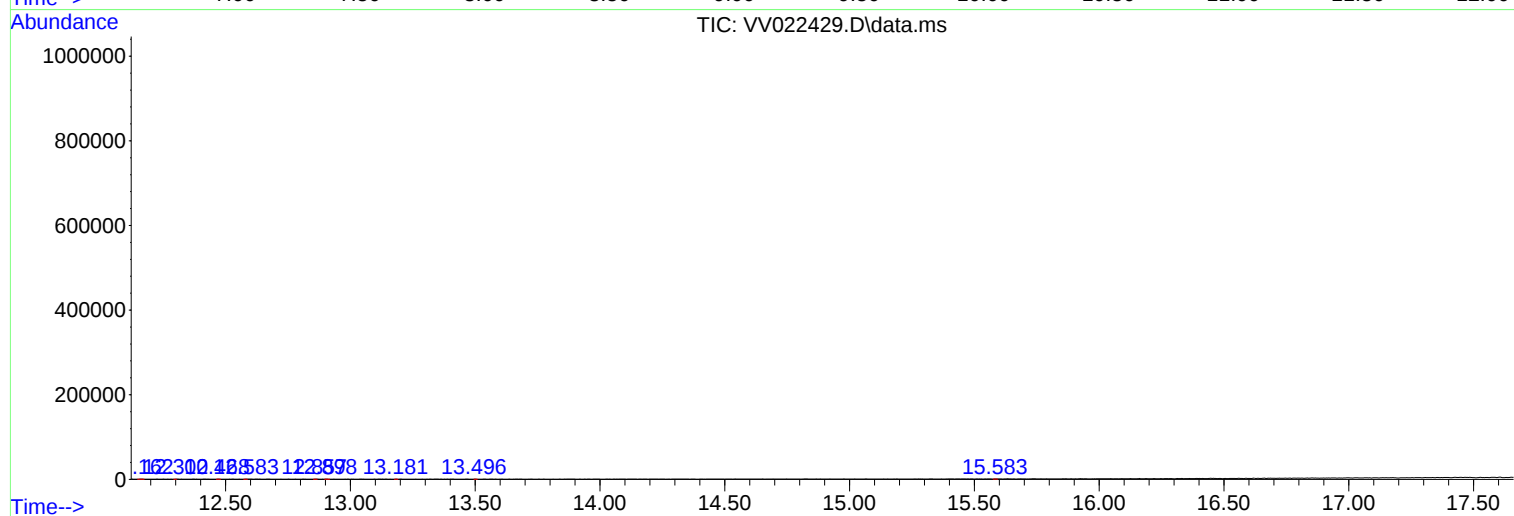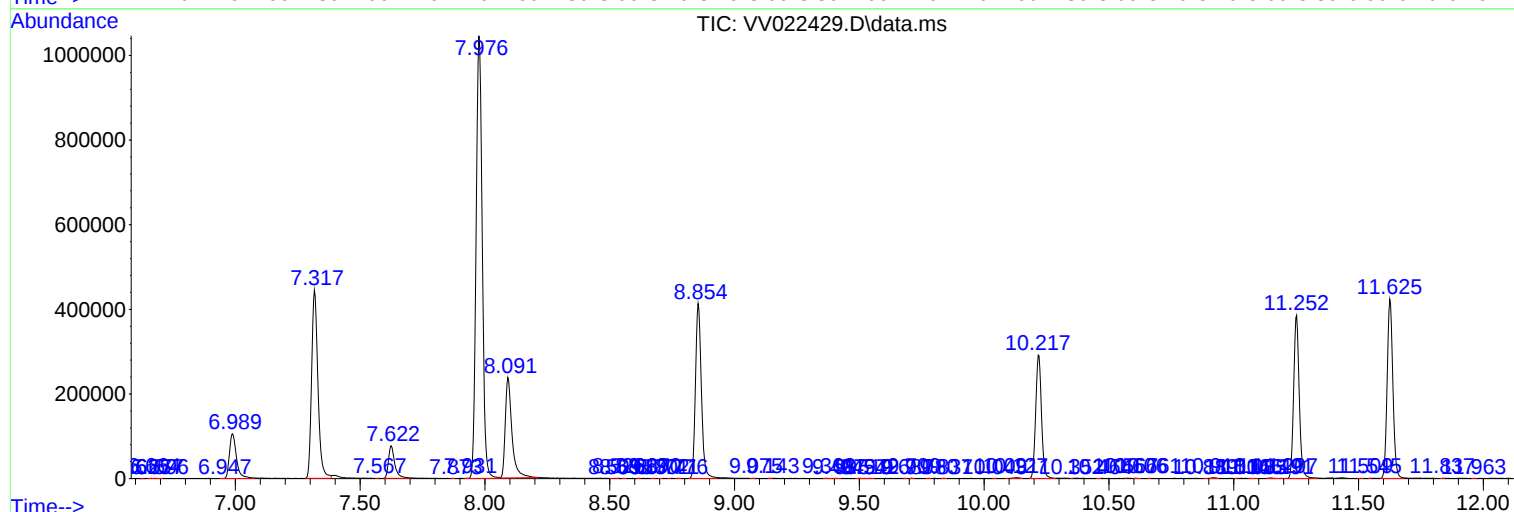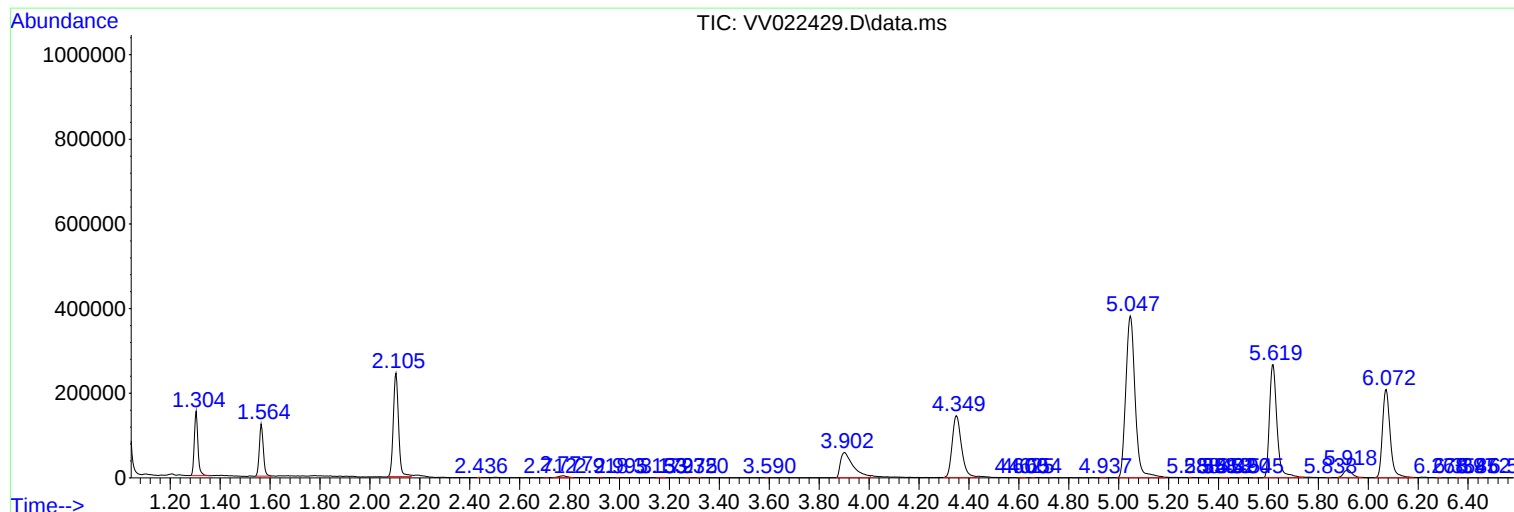

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
Data File : VV022429.D
Acq On : 30 Sep 2021 14:06
Operator : SY/MD
Sample : M3978-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A33

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
Data File : VV022429.D
Acq On : 30 Sep 2021 14:06
Operator : SY/MD
Sample : M3978-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A33

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
