

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
 Data File : VV022430.D
 Acq On : 30 Sep 2021 14:30
 Operator : SY/MD
 Sample : M3978-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A34

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

Signal : TIC: VV022430.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	98	rVB	149765	152781	8.25%	1.704%
2	1.564	156	163	175	rVB	121019	136080	7.35%	1.518%
3	2.105	321	331	354	rBV	238488	348498	18.82%	3.887%
4	2.542	466	467	471	rBV	407	265	0.01%	0.003%
5	2.619	488	491	492	rBV2	386	174	0.01%	0.002%
6	2.674	506	508	510	rVB	382	148	0.01%	0.002%
7	2.690	510	513	516	rBV3	370	299	0.02%	0.003%
8	2.767	528	537	550	rVV4	5011	10664	0.58%	0.119%
9	2.851	561	563	565	rBV	249	115	0.01%	0.001%
10	3.050	622	625	631	rBV2	416	285	0.02%	0.003%
11	3.153	654	657	660	rBV	313	185	0.01%	0.002%
12	3.307	703	705	708	rBV	279	133	0.01%	0.001%
13	3.481	756	759	764	rBV3	321	346	0.02%	0.004%
14	3.561	780	784	785	rBV2	270	146	0.01%	0.002%
15	3.600	791	796	797	rBV2	249	158	0.01%	0.002%
16	3.706	826	829	832	rVB	451	295	0.02%	0.003%
17	3.728	832	836	838	rBV2	254	208	0.01%	0.002%
18	3.857	873	876	877	rBV	290	152	0.01%	0.002%
19	3.902	879	890	921	rBV	57185	201964	10.91%	2.253%
20	4.349	1014	1029	1054	rVV	148180	371670	20.07%	4.146%
21	4.767	1158	1159	1163	rBV2	254	147	0.01%	0.002%
22	4.844	1180	1183	1185	rBV	456	241	0.01%	0.003%
23	4.876	1190	1193	1194	rBV	347	195	0.01%	0.002%
24	4.908	1201	1203	1207	rVB3	417	203	0.01%	0.002%
25	4.947	1210	1215	1216	rBV	321	209	0.01%	0.002%
26	4.989	1225	1228	1229	rBV2	263	116	0.01%	0.001%
27	5.047	1229	1246	1269	rBV2	378097	950936	51.35%	10.606%
28	5.272	1314	1316	1320	rBV3	483	285	0.02%	0.003%
29	5.516	1390	1392	1395	rBV	264	142	0.01%	0.002%
30	5.542	1398	1400	1401	rBV	286	141	0.01%	0.002%
31	5.619	1410	1424	1455	rBV	263915	548333	29.61%	6.116%
32	5.873	1501	1503	1504	rBV2	411	125	0.01%	0.001%
33	5.915	1504	1516	1535	rVV5	19787	49035	2.65%	0.547%
34	6.069	1551	1564	1588	rBV	204357	429596	23.20%	4.792%
35	6.291	1628	1633	1637	rBV3	446	325	0.02%	0.004%
36	6.313	1637	1640	1641	rVV2	315	132	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
 Data File : VV022430.D
 Acq On : 30 Sep 2021 14:30
 Operator : SY/MD
 Sample : M3978-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A34

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

37	6.323	1641	1643	1647	rVB2	400	215	0.01%	0.002%
38	6.349	1648	1651	1655	rBV2	428	396	0.02%	0.004%
39	6.378	1658	1660	1662	rBV	250	160	0.01%	0.002%
40	6.391	1662	1664	1668	rBV2	265	217	0.01%	0.002%
41	6.500	1696	1698	1703	rVB2	301	198	0.01%	0.002%
42	6.613	1731	1733	1736	rVB2	287	137	0.01%	0.002%
43	6.654	1744	1746	1752	rVB3	405	375	0.02%	0.004%
44	6.686	1752	1756	1758	rBV2	358	220	0.01%	0.002%
45	6.728	1763	1769	1770	rBV3	495	368	0.02%	0.004%
46	6.928	1829	1831	1833	rBV	313	155	0.01%	0.002%
47	6.989	1838	1850	1880	rBV	105335	201054	10.86%	2.243%
48	7.252	1930	1932	1933	rBV	339	161	0.01%	0.002%
49	7.317	1940	1952	1972	rBV	435800	767943	41.47%	8.565%
50	7.622	2038	2047	2072	rBV2	72733	135768	7.33%	1.514%
51	7.838	2110	2114	2115	rBV2	350	220	0.01%	0.002%
52	7.976	2143	2157	2182	rBV	1101834	1851939	100.00%	20.656%
53	8.092	2184	2193	2227	rVB	235642	432819	23.37%	4.828%
54	8.690	2376	2379	2381	rBV3	390	223	0.01%	0.002%
55	8.799	2410	2413	2416	rVB2	457	278	0.02%	0.003%
56	8.854	2418	2430	2447	rBV	403335	658820	35.57%	7.348%
57	9.156	2520	2524	2525	rBV2	597	395	0.02%	0.004%
58	9.301	2566	2569	2571	rBV	427	247	0.01%	0.003%
59	9.329	2575	2578	2580	rBV	284	195	0.01%	0.002%
60	9.423	2606	2607	2611	rVB3	676	308	0.02%	0.003%
61	9.452	2611	2616	2620	rBV2	384	528	0.03%	0.006%
62	9.558	2646	2649	2654	rBV5	513	451	0.02%	0.005%
63	9.696	2690	2692	2695	rVB2	387	162	0.01%	0.002%
64	9.899	2751	2755	2757	rBV2	378	271	0.01%	0.003%
65	9.927	2762	2764	2765	rBV2	249	116	0.01%	0.001%
66	9.963	2773	2775	2778	rVB2	283	134	0.01%	0.001%
67	9.998	2781	2786	2788	rBV	338	240	0.01%	0.003%
68	10.043	2797	2800	2802	rVB2	242	129	0.01%	0.001%
69	10.127	2818	2826	2833	rBV4	2733	3805	0.21%	0.042%
70	10.217	2843	2854	2873	rBV	288987	457814	24.72%	5.106%
71	10.439	2919	2923	2925	rBV2	591	416	0.02%	0.005%
72	10.461	2928	2930	2932	rBV3	369	201	0.01%	0.002%
73	10.542	2953	2955	2957	rBV2	326	164	0.01%	0.002%
74	10.603	2971	2974	2976	rBV2	592	427	0.02%	0.005%
75	10.696	3000	3003	3004	rBV2	303	131	0.01%	0.001%
76	10.706	3004	3006	3009	rVV2	244	132	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
 Data File : VV022430.D
 Acq On : 30 Sep 2021 14:30
 Operator : SY/MD
 Sample : M3978-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A34

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

77	10.747	3017	3019	3022	rVB	318	135	0.01%	0.002%
78	10.921	3064	3073	3082	rVV5	1918	2947	0.16%	0.033%
79	11.034	3105	3108	3109	rBV2	451	252	0.01%	0.003%
80	11.072	3116	3120	3123	rBV3	255	210	0.01%	0.002%
81	11.146	3136	3143	3144	rBV4	916	884	0.05%	0.010%
82	11.185	3149	3155	3157	rBV4	512	418	0.02%	0.005%
83	11.249	3164	3175	3203	rBV	370005	581119	31.38%	6.482%
84	11.625	3281	3292	3314	rVB	409306	653674	35.30%	7.291%
85	11.969	3397	3399	3400	rBV2	264	114	0.01%	0.001%
86	12.056	3424	3426	3431	rVB2	478	323	0.02%	0.004%
87	12.297	3499	3501	3503	rBV	340	173	0.01%	0.002%
88	12.554	3577	3581	3584	rBV2	339	302	0.02%	0.003%
89	12.812	3657	3661	3664	rVB2	311	256	0.01%	0.003%
90	12.940	3700	3701	3703	rBV	274	135	0.01%	0.002%
91	12.972	3709	3711	3714	rBV	348	258	0.01%	0.003%
92	13.043	3731	3733	3735	rVB	428	133	0.01%	0.001%
93	13.117	3753	3756	3759	rBV	238	186	0.01%	0.002%
94	13.484	3868	3870	3872	rBV	278	120	0.01%	0.001%
95	13.574	3896	3898	3900	rBV	256	118	0.01%	0.001%
96	14.117	4063	4067	4068	rBV	549	383	0.02%	0.004%
97	14.287	4117	4120	4122	rBV2	429	285	0.02%	0.003%
98	14.432	4163	4165	4168	rBV3	284	175	0.01%	0.002%
99	14.558	4202	4204	4207	rBV	392	223	0.01%	0.002%
100	15.037	4352	4353	4357	rVB2	356	132	0.01%	0.001%



Sum of corrected areas: 8965614

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
Data File : VV022430.D
Acq On : 30 Sep 2021 14:30
Operator : SY/MD
Sample : M3978-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A34

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

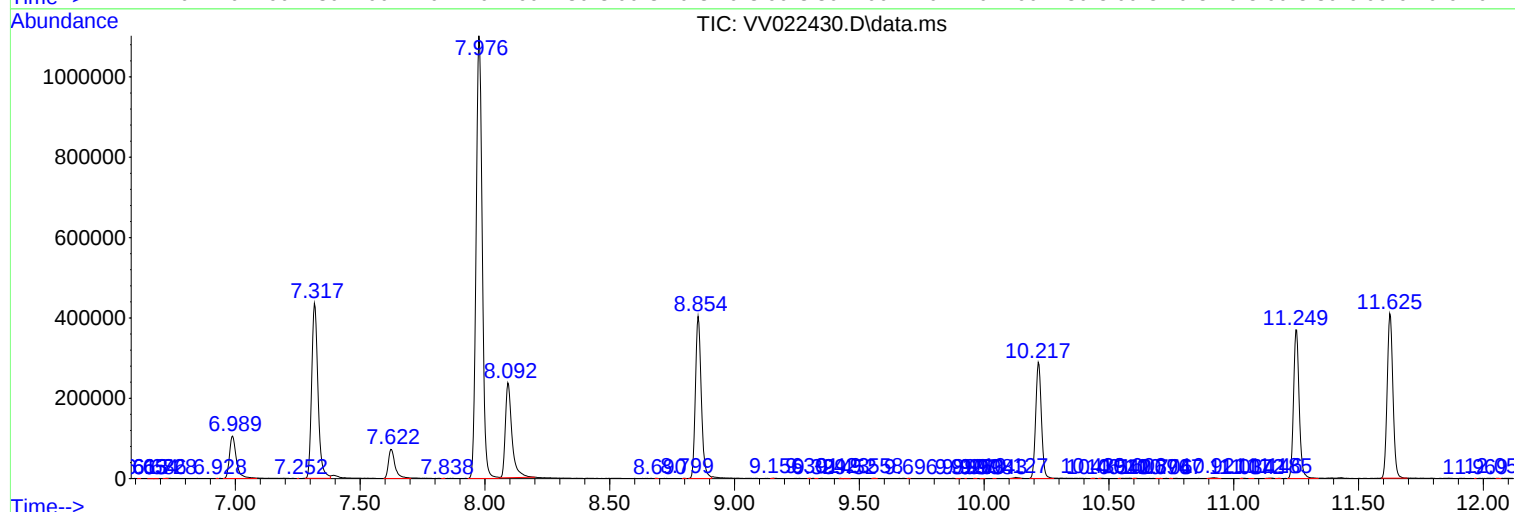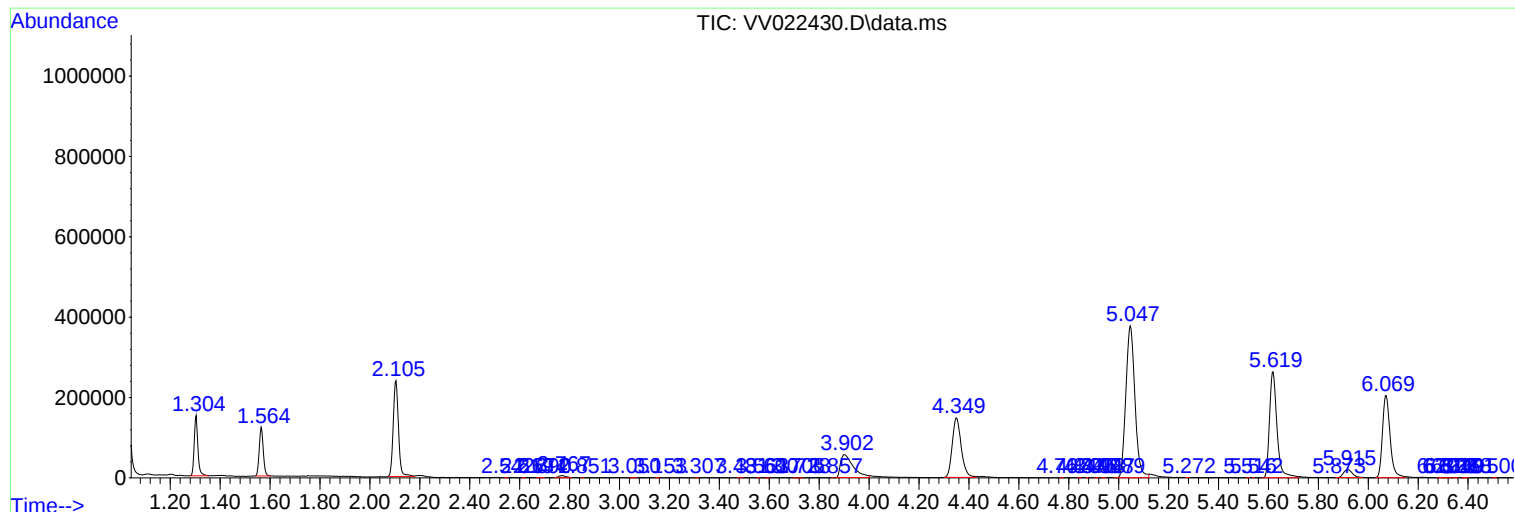

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
Data File : VV022430.D
Acq On : 30 Sep 2021 14:30
Operator : SY/MD
Sample : M3978-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A34

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
Data File : VV022430.D
Acq On : 30 Sep 2021 14:30
Operator : SY/MD
Sample : M3978-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A34

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------