

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
 Data File : VV022431.D
 Acq On : 30 Sep 2021 14:54
 Operator : SY/MD
 Sample : M3978-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A35

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M

Title : VOC Analysis

Signal : TIC: VV022431.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	99	rVB	144340	150383	8.53%	1.705%
2	1.564	157	163	179	rVB	119009	135938	7.71%	1.541%
3	2.105	321	331	352	rBV	233755	346284	19.64%	3.925%
4	2.506	451	456	457	rBV3	848	638	0.04%	0.007%
5	2.596	482	484	487	rVV2	269	165	0.01%	0.002%
6	2.632	493	495	497	rBV2	370	179	0.01%	0.002%
7	2.680	507	510	515	rBV3	488	361	0.02%	0.004%
8	2.767	530	537	551	rVB4	4756	9677	0.55%	0.110%
9	2.863	564	567	570	rBV2	512	253	0.01%	0.003%
10	3.230	678	681	684	rVB2	266	178	0.01%	0.002%
11	3.477	754	758	760	rVV2	228	168	0.01%	0.002%
12	3.506	765	767	772	rVV	275	227	0.01%	0.003%
13	3.532	772	775	778	rVV	263	184	0.01%	0.002%
14	3.558	778	783	786	rVV2	265	255	0.01%	0.003%
15	3.609	794	799	801	rBV2	335	236	0.01%	0.003%
16	3.699	825	827	831	rBV2	208	152	0.01%	0.002%
17	3.776	849	851	854	rVB	343	194	0.01%	0.002%
18	3.899	878	889	930	rBV	60670	209874	11.90%	2.379%
19	4.349	1014	1029	1050	rBV	145674	361936	20.53%	4.102%
20	4.606	1106	1109	1110	rBV	338	152	0.01%	0.002%
21	4.709	1139	1141	1147	rVB2	453	225	0.01%	0.003%
22	4.754	1147	1155	1158	rBV3	403	489	0.03%	0.006%
23	4.940	1209	1213	1217	rVB2	320	251	0.01%	0.003%
24	4.979	1222	1225	1228	rVB	422	205	0.01%	0.002%
25	5.047	1228	1246	1266	rBV2	368273	933064	52.92%	10.576%
26	5.220	1297	1300	1303	rBV3	1013	722	0.04%	0.008%
27	5.346	1336	1339	1340	rBV2	330	177	0.01%	0.002%
28	5.381	1348	1350	1354	rVB2	460	220	0.01%	0.002%
29	5.429	1362	1365	1367	rBV2	329	171	0.01%	0.002%
30	5.619	1412	1424	1442	rBV	260232	530816	30.11%	6.017%
31	5.841	1491	1493	1499	rBV3	278	223	0.01%	0.003%
32	5.918	1504	1517	1532	rBV6	18416	44095	2.50%	0.500%
33	6.027	1549	1551	1552	rBV6	402	206	0.01%	0.002%
34	6.072	1552	1565	1592	rVV	204725	433198	24.57%	4.910%
35	6.223	1610	1612	1617	rBV3	603	465	0.03%	0.005%
36	6.429	1675	1676	1679	rVB2	397	158	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
 Data File : VV022431.D
 Acq On : 30 Sep 2021 14:54
 Operator : SY/MD
 Sample : M3978-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A35

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

37	6.503	1697	1699	1706	rVB2	326	264	0.01%	0.003%
38	6.641	1737	1742	1744	rVB2	445	312	0.02%	0.004%
39	6.661	1745	1748	1749	rBV2	342	161	0.01%	0.002%
40	6.763	1777	1780	1783	rBV2	389	241	0.01%	0.003%
41	6.815	1793	1796	1800	rVB2	319	224	0.01%	0.003%
42	6.844	1802	1805	1809	rBV3	394	307	0.02%	0.003%
43	6.905	1817	1824	1825	rBV	175	162	0.01%	0.002%
44	6.918	1825	1828	1836	rBV2	234	219	0.01%	0.002%
45	6.989	1837	1850	1879	rBV	103239	200888	11.39%	2.277%
46	7.194	1909	1914	1917	rBV3	489	455	0.03%	0.005%
47	7.255	1931	1933	1935	rBV	311	165	0.01%	0.002%
48	7.317	1940	1952	1973	rBV	425966	765052	43.39%	8.672%
49	7.625	2038	2048	2072	rBV	71785	134127	7.61%	1.520%
50	7.763	2088	2091	2096	rVB3	640	444	0.03%	0.005%
51	7.976	2144	2157	2183	rBV	1038718	1763161	100.00%	19.985%
52	8.091	2184	2193	2233	rVB	227378	432335	24.52%	4.900%
53	8.738	2389	2394	2399	rVV2	423	392	0.02%	0.004%
54	8.853	2418	2430	2454	rBV	402029	665650	37.75%	7.545%
55	9.082	2497	2501	2504	rBV3	309	233	0.01%	0.003%
56	9.152	2518	2523	2528	rBV5	935	1062	0.06%	0.012%
57	9.204	2537	2539	2541	rVV	372	165	0.01%	0.002%
58	9.217	2541	2543	2546	rVV2	327	195	0.01%	0.002%
59	9.236	2547	2549	2552	rVV	342	202	0.01%	0.002%
60	9.259	2554	2556	2558	rVV3	418	194	0.01%	0.002%
61	9.275	2558	2561	2565	rVB	385	265	0.02%	0.003%
62	9.355	2580	2586	2588	rBV2	271	241	0.01%	0.003%
63	9.378	2591	2593	2594	rBV	311	163	0.01%	0.002%
64	9.503	2628	2632	2634	rVV3	277	218	0.01%	0.002%
65	9.583	2653	2657	2659	rBV	212	150	0.01%	0.002%
66	9.657	2675	2680	2682	rVB2	382	257	0.01%	0.003%
67	9.744	2704	2707	2709	rBV	270	187	0.01%	0.002%
68	9.873	2745	2747	2751	rBV2	249	201	0.01%	0.002%
69	10.078	2808	2811	2815	rBV2	289	248	0.01%	0.003%
70	10.130	2820	2827	2834	rVV4	2009	2937	0.17%	0.033%
71	10.217	2841	2854	2876	rBV	290315	457354	25.94%	5.184%
72	10.345	2892	2894	2898	rVB3	540	312	0.02%	0.004%
73	10.496	2938	2941	2943	rBV	338	155	0.01%	0.002%
74	10.574	2963	2965	2969	rBV2	404	264	0.01%	0.003%
75	10.876	3055	3059	3061	rBV	524	386	0.02%	0.004%
76	10.921	3065	3073	3080	rVB3	1869	2572	0.15%	0.029%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
 Data File : VV022431.D
 Acq On : 30 Sep 2021 14:54
 Operator : SY/MD
 Sample : M3978-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A35

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

77	10.982	3088	3092	3093	rBV2	460	319	0.02%	0.004%
78	11.033	3102	3108	3114	rBV3	857	898	0.05%	0.010%
79	11.146	3137	3143	3148	rBV4	779	1047	0.06%	0.012%
80	11.252	3164	3176	3195	rBV	361398	570493	32.36%	6.466%
81	11.371	3210	3213	3215	rBV2	807	467	0.03%	0.005%
82	11.625	3280	3292	3315	rVV	408690	650067	36.87%	7.368%
83	11.930	3386	3387	3391	rVB	448	217	0.01%	0.002%
84	11.972	3397	3400	3405	rBV4	315	351	0.02%	0.004%
85	12.229	3478	3480	3482	rBV2	400	220	0.01%	0.002%
86	12.667	3614	3616	3621	rVB	277	214	0.01%	0.002%
87	12.934	3695	3699	3703	rBV2	284	273	0.02%	0.003%
88	12.953	3703	3705	3710	rVV	230	195	0.01%	0.002%
89	13.120	3752	3757	3758	rBV3	521	326	0.02%	0.004%
90	13.130	3758	3760	3763	rVB	419	149	0.01%	0.002%
91	13.152	3765	3767	3769	rBV2	320	151	0.01%	0.002%
92	13.779	3960	3962	3965	rVB3	404	208	0.01%	0.002%
93	13.853	3982	3985	3988	rVB	413	290	0.02%	0.003%
94	13.934	4008	4010	4017	rVB3	398	308	0.02%	0.003%
95	14.001	4029	4031	4036	rVB3	424	267	0.02%	0.003%
96	14.030	4036	4040	4043	rBV	371	345	0.02%	0.004%
97	14.274	4115	4116	4120	rVB2	388	245	0.01%	0.003%
98	14.297	4120	4123	4124	rBV	354	193	0.01%	0.002%
99	14.528	4193	4195	4198	rBV2	425	322	0.02%	0.004%
100	14.789	4274	4276	4279	rBV2	424	203	0.01%	0.002%




Sum of corrected areas: 8822407

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
Data File : VV022431.D
Acq On : 30 Sep 2021 14:54
Operator : SY/MD
Sample : M3978-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A35

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

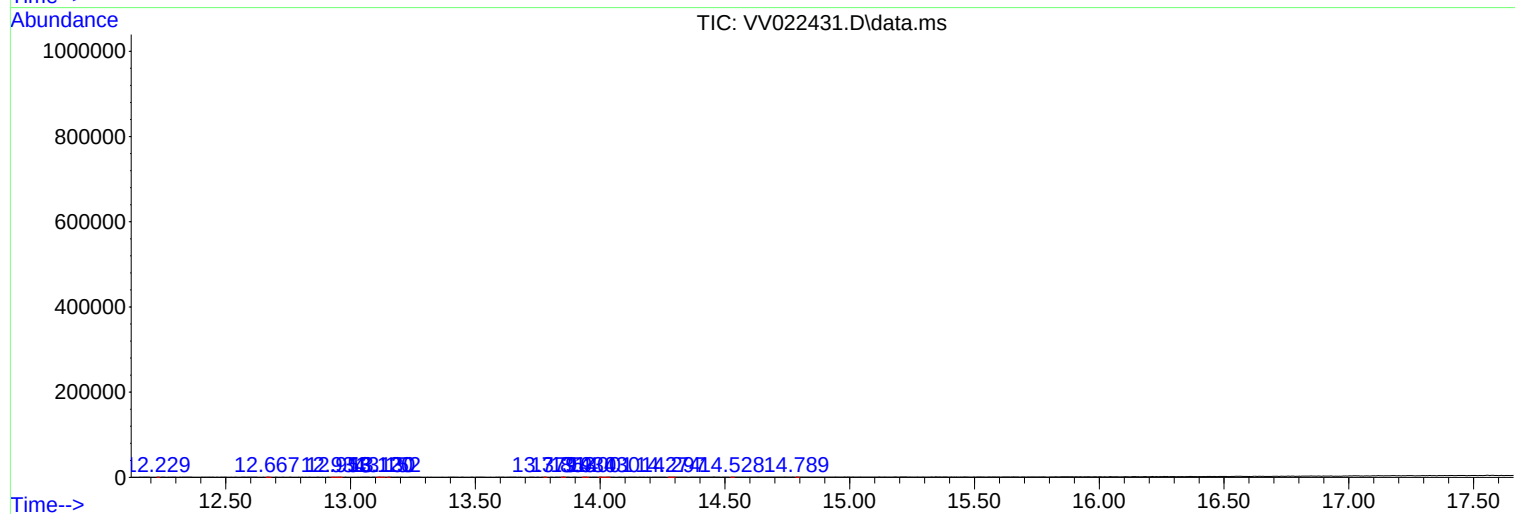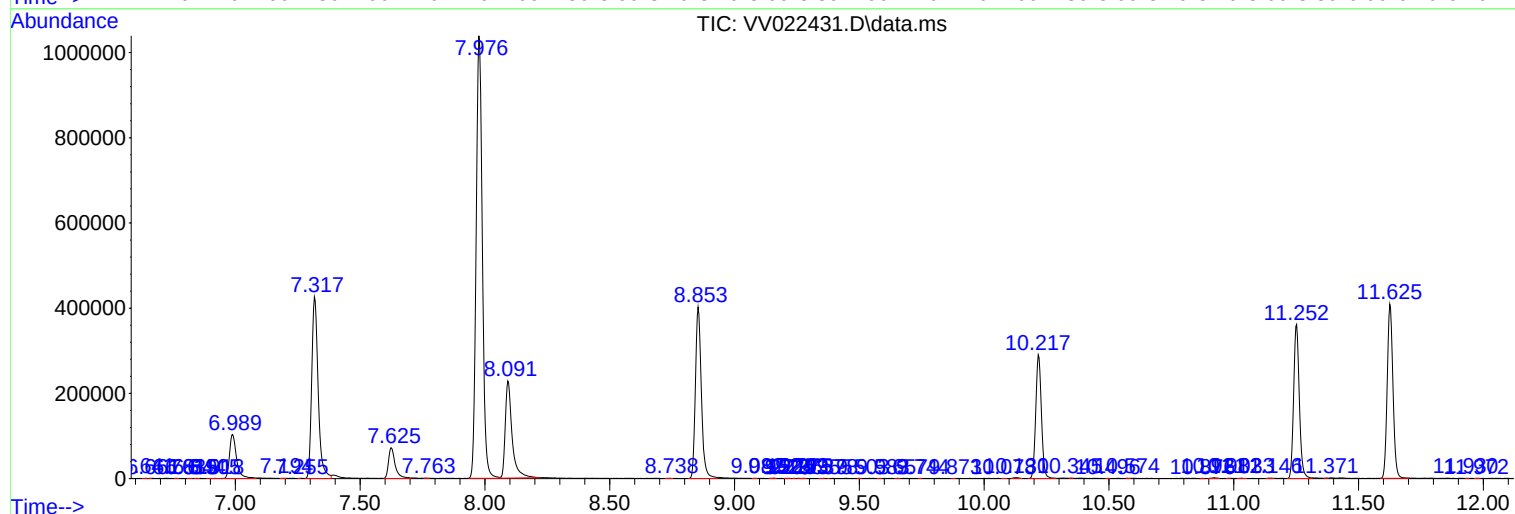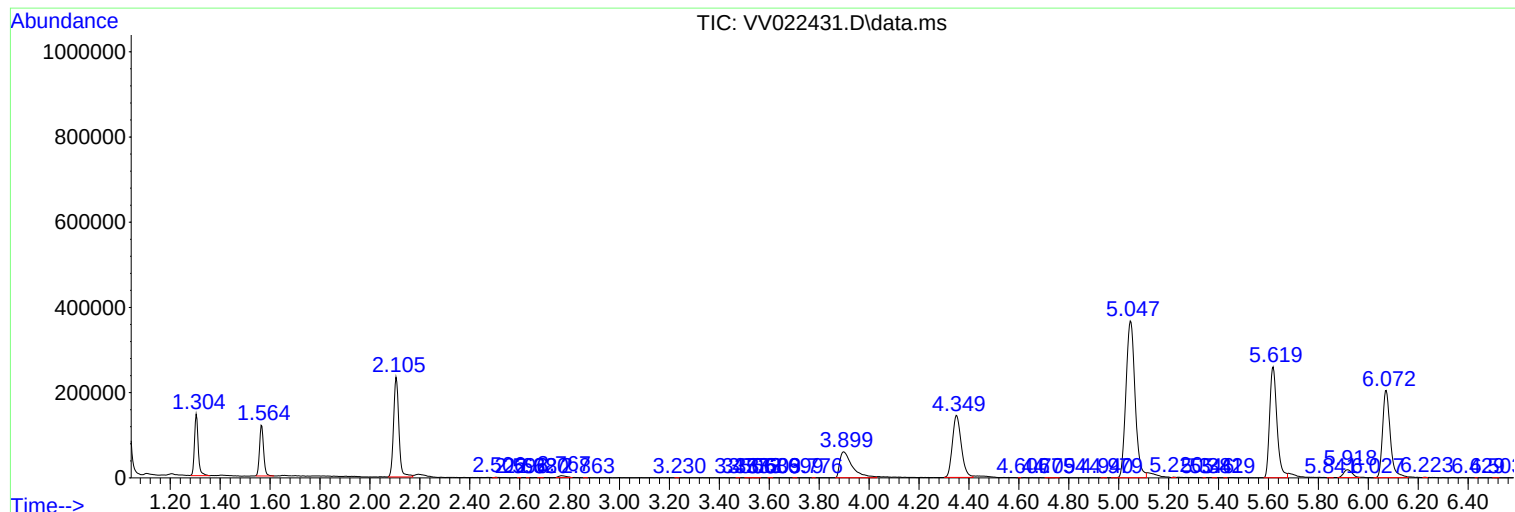

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
Data File : VV022431.D
Acq On : 30 Sep 2021 14:54
Operator : SY/MD
Sample : M3978-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A35

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
Data File : VV022431.D
Acq On : 30 Sep 2021 14:54
Operator : SY/MD
Sample : M3978-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A35

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------