

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
 Data File : VV022433.D
 Acq On : 30 Sep 2021 15:42
 Operator : SY/MD
 Sample : M3978-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A46

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

Signal : TIC: VV022433.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	101	rVB	145923	152186	15.77%	1.969%
2	1.564	156	163	177	rBV	120753	135167	14.01%	1.749%
3	2.105	321	331	345	rBV	240899	347562	36.01%	4.498%
4	2.500	449	454	456	rBV3	636	745	0.08%	0.010%
5	2.709	516	519	521	rBV2	264	189	0.02%	0.002%
6	2.773	528	539	551	rVB7	2508	5685	0.59%	0.074%
7	2.851	558	563	566	rBV2	370	270	0.03%	0.003%
8	3.092	635	638	641	rVB2	285	207	0.02%	0.003%
9	3.625	801	804	808	rVB2	367	245	0.03%	0.003%
10	3.744	839	841	846	rVB2	453	311	0.03%	0.004%
11	3.899	877	889	926	rBV	62425	220171	22.81%	2.849%
12	4.291	1009	1011	1013	rBV	444	213	0.02%	0.003%
13	4.349	1014	1029	1050	rVV	148617	370607	38.40%	4.796%
14	4.703	1133	1139	1140	rBV3	297	230	0.02%	0.003%
15	4.748	1149	1153	1156	rVB2	225	182	0.02%	0.002%
16	4.770	1156	1160	1166	rVB2	374	314	0.03%	0.004%
17	4.805	1166	1171	1173	rBV3	462	388	0.04%	0.005%
18	4.902	1198	1201	1204	rBV2	275	179	0.02%	0.002%
19	4.924	1205	1208	1210	rVB2	356	187	0.02%	0.002%
20	5.047	1230	1246	1293	rBV2	374979	965060	100.00%	12.488%
21	5.490	1382	1384	1388	rBV2	212	175	0.02%	0.002%
22	5.513	1388	1391	1394	rVB	426	180	0.02%	0.002%
23	5.619	1412	1424	1445	rBV	260026	533382	55.27%	6.902%
24	5.857	1494	1498	1500	rBV	293	258	0.03%	0.003%
25	5.870	1500	1502	1504	rBV2	441	196	0.02%	0.003%
26	5.915	1504	1516	1530	rBV5	23935	55835	5.79%	0.723%
27	6.072	1549	1565	1599	rBV	208122	437101	45.29%	5.656%
28	6.336	1644	1647	1651	rBV3	254	176	0.02%	0.002%
29	6.394	1662	1665	1670	rVB	355	309	0.03%	0.004%
30	6.449	1680	1682	1688	rVB2	301	207	0.02%	0.003%
31	6.481	1688	1692	1693	rBV2	429	192	0.02%	0.002%
32	6.519	1702	1704	1709	rVB3	440	289	0.03%	0.004%
33	6.561	1712	1717	1721	rBV2	353	424	0.04%	0.005%
34	6.596	1725	1728	1730	rBV2	398	294	0.03%	0.004%
35	6.648	1741	1744	1746	rBV3	486	286	0.03%	0.004%
36	6.667	1748	1750	1753	rVV3	667	321	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
 Data File : VV022433.D
 Acq On : 30 Sep 2021 15:42
 Operator : SY/MD
 Sample : M3978-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A46

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

37	6.696	1756	1759	1762	rVB2	375	212	0.02%	0.003%
38	6.719	1762	1766	1772	rBV3	476	390	0.04%	0.005%
39	6.751	1772	1776	1780	rBV3	385	231	0.02%	0.003%
40	6.831	1799	1801	1805	rVB2	517	250	0.03%	0.003%
41	6.870	1811	1813	1817	rBV2	359	202	0.02%	0.003%
42	6.989	1838	1850	1873	rBV	105043	197697	20.49%	2.558%
43	7.185	1907	1911	1914	rBV3	354	343	0.04%	0.004%
44	7.317	1941	1952	1971	rBV	429809	765004	79.27%	9.899%
45	7.558	2025	2027	2030	rVB2	490	177	0.02%	0.002%
46	7.625	2035	2048	2081	rBV	72814	135052	13.99%	1.748%
47	7.815	2104	2107	2109	rBV3	249	179	0.02%	0.002%
48	7.863	2120	2122	2124	rVB	552	205	0.02%	0.003%
49	7.879	2124	2127	2130	rBV3	502	312	0.03%	0.004%
50	7.931	2139	2143	2145	rBV3	415	332	0.03%	0.004%
51	7.976	2145	2157	2177	rBV	360378	616699	63.90%	7.980%
52	8.092	2184	2193	2227	rBV	233044	438104	45.40%	5.669%
53	8.529	2326	2329	2332	rBV	349	199	0.02%	0.003%
54	8.558	2336	2338	2343	rBV3	504	346	0.04%	0.004%
55	8.603	2349	2352	2356	rBV2	469	383	0.04%	0.005%
56	8.699	2380	2382	2386	rVB	302	175	0.02%	0.002%
57	8.725	2386	2390	2393	rBV3	456	409	0.04%	0.005%
58	8.757	2396	2400	2402	rBV2	216	173	0.02%	0.002%
59	8.776	2402	2406	2407	rBV2	271	198	0.02%	0.003%
60	8.854	2418	2430	2461	rBV	394648	653963	67.76%	8.462%
61	9.143	2516	2520	2522	rBV2	488	447	0.05%	0.006%
62	9.272	2557	2560	2566	rVB3	454	303	0.03%	0.004%
63	9.349	2582	2584	2586	rBV2	346	170	0.02%	0.002%
64	9.513	2632	2635	2637	rBV2	346	180	0.02%	0.002%
65	9.545	2643	2645	2647	rBV	317	184	0.02%	0.002%
66	10.108	2815	2820	2821	rBV2	459	369	0.04%	0.005%
67	10.124	2821	2825	2826	rBV3	1352	1083	0.11%	0.014%
68	10.217	2842	2854	2874	rBV	290248	458667	47.53%	5.935%
69	10.352	2893	2896	2901	rVB3	559	467	0.05%	0.006%
70	10.381	2901	2905	2906	rBV2	590	328	0.03%	0.004%
71	10.677	2995	2997	3001	rVB	453	306	0.03%	0.004%
72	10.918	3063	3072	3081	rVB6	1609	2650	0.27%	0.034%
73	11.034	3104	3108	3109	rBV	468	300	0.03%	0.004%
74	11.146	3138	3143	3150	rVB4	988	1153	0.12%	0.015%
75	11.175	3150	3152	3154	rVB	360	169	0.02%	0.002%
76	11.201	3154	3160	3164	rBV4	505	463	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
 Data File : VV022433.D
 Acq On : 30 Sep 2021 15:42
 Operator : SY/MD
 Sample : M3978-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A46

Integration Parameters: LSCINT.P

Integrator: RTE

Smoother: OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M

Title : VOC Analysis

77	11.252	3164	3176	3196	rBV	362386	565534	58.60%	7.318%
78	11.625	3280	3292	3310	rBV	406442	647891	67.13%	8.384%
79	11.754	3328	3332	3335	rBV2	262	244	0.03%	0.003%
80	11.783	3337	3341	3347	rBV5	712	899	0.09%	0.012%
81	11.873	3367	3369	3372	rBV	302	218	0.02%	0.003%
82	12.046	3418	3423	3425	rBV2	518	472	0.05%	0.006%
83	12.085	3433	3435	3438	rBV2	450	323	0.03%	0.004%
84	12.114	3442	3444	3446	rVB	496	172	0.02%	0.002%
85	12.165	3456	3460	3464	rVB2	338	308	0.03%	0.004%
86	12.406	3533	3535	3539	rBV2	279	230	0.02%	0.003%
87	12.497	3560	3563	3566	rBV2	370	238	0.02%	0.003%
88	12.529	3571	3573	3579	rVB3	329	238	0.02%	0.003%
89	12.596	3592	3594	3596	rBV2	263	185	0.02%	0.002%
90	12.873	3677	3680	3682	rBV	228	164	0.02%	0.002%
91	13.374	3833	3836	3840	rVB2	348	201	0.02%	0.003%
92	13.532	3882	3885	3887	rBV	429	227	0.02%	0.003%
93	13.612	3908	3910	3914	rBV	288	164	0.02%	0.002%
94	13.718	3940	3943	3945	rBV	300	198	0.02%	0.003%
95	13.754	3952	3954	3960	rVB	254	222	0.02%	0.003%
96	13.795	3963	3967	3969	rBV2	388	275	0.03%	0.004%
97	13.924	4004	4007	4011	rBV2	466	338	0.04%	0.004%
98	14.123	4067	4069	4076	rBV2	407	276	0.03%	0.004%
99	14.281	4115	4118	4120	rBV	452	219	0.02%	0.003%
100	14.516	4185	4191	4192	rBV3	400	347	0.04%	0.004%




Sum of corrected areas: 7727780

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
Data File : VV022433.D
Acq On : 30 Sep 2021 15:42
Operator : SY/MD
Sample : M3978-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A46

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

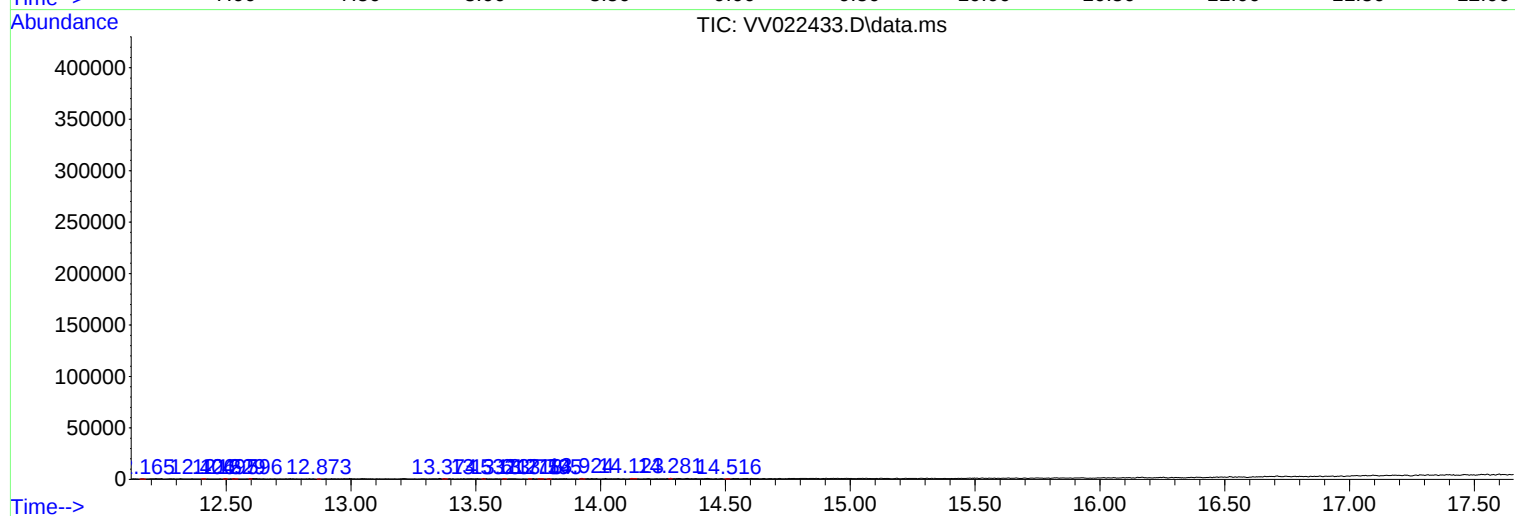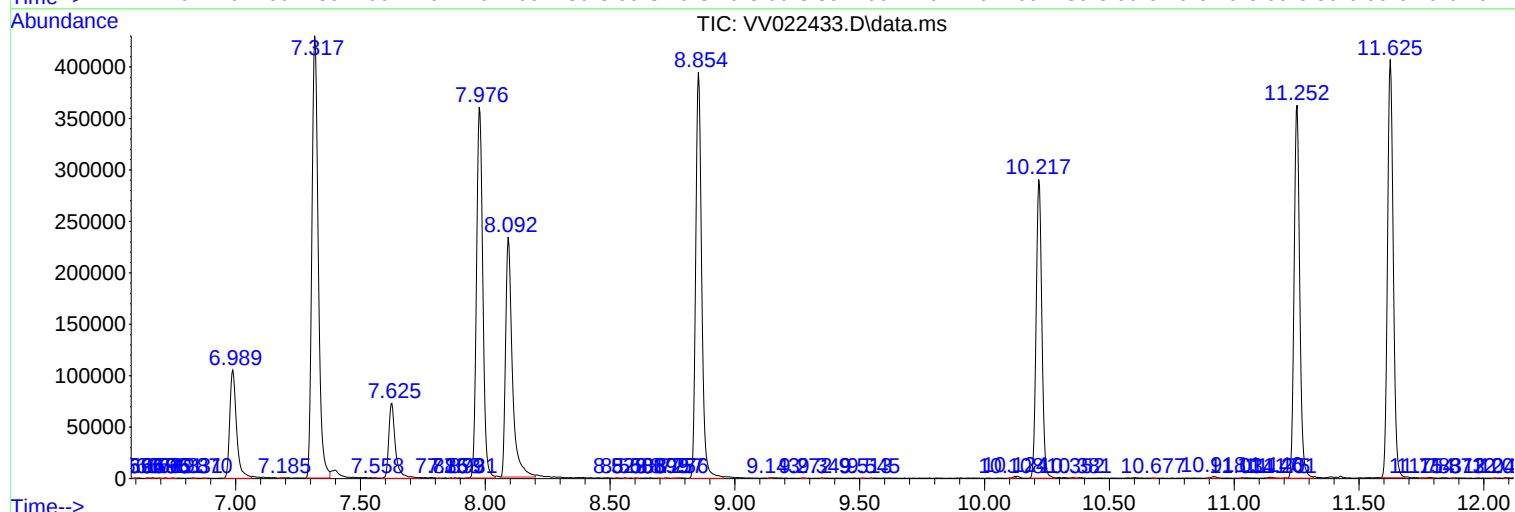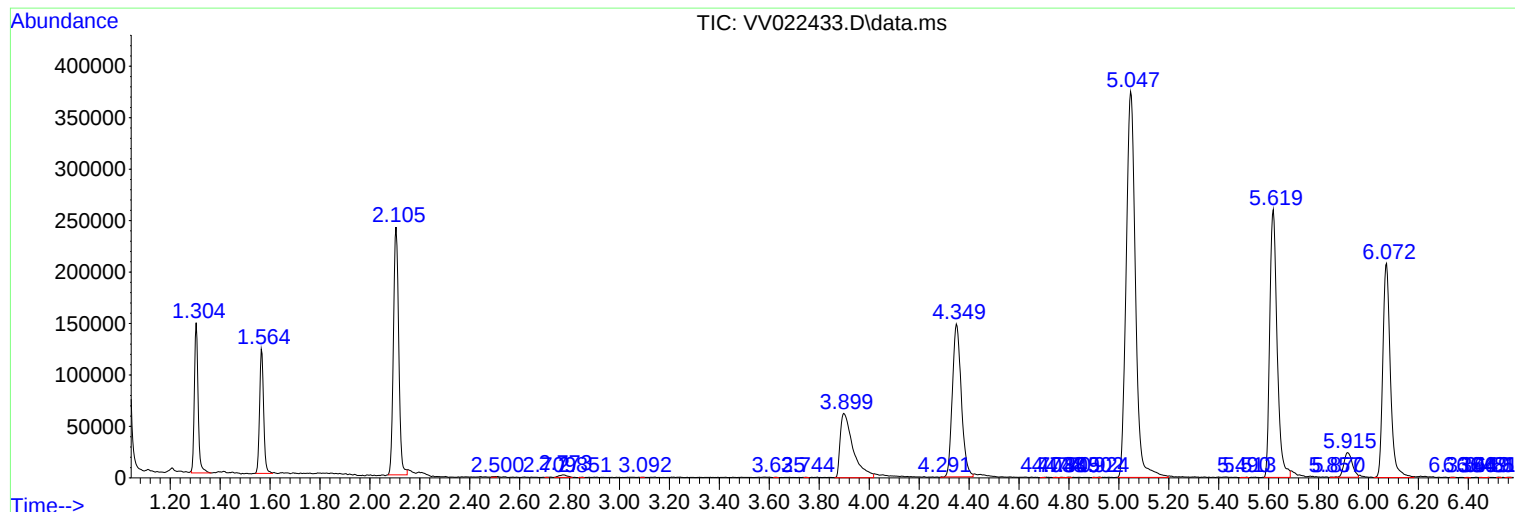

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
Data File : VV022433.D
Acq On : 30 Sep 2021 15:42
Operator : SY/MD
Sample : M3978-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A46

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
Data File : VV022433.D
Acq On : 30 Sep 2021 15:42
Operator : SY/MD
Sample : M3978-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A46

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------