

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
 Data File : VV022436.D
 Acq On : 30 Sep 2021 16:54
 Operator : SY/MD
 Sample : M3979-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A04

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M

Title : VOC Analysis

Signal : TIC: VV022436.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	98	rVB	144218	145039	15.94%	2.007%
2	1.565	156	163	177	rVB	117833	133617	14.69%	1.849%
3	2.105	321	331	362	rVB	224735	335697	36.90%	4.644%
4	2.716	519	521	524	rBV	437	225	0.02%	0.003%
5	2.770	530	538	551	rVB4	4172	8039	0.88%	0.111%
6	2.847	559	562	564	rVB	401	219	0.02%	0.003%
7	2.860	564	566	568	rBV2	387	216	0.02%	0.003%
8	3.066	627	630	634	rVB2	280	184	0.02%	0.003%
9	3.101	639	641	644	rBV	216	131	0.01%	0.002%
10	3.127	644	649	652	rBV	459	273	0.03%	0.004%
11	3.259	686	690	693	rBV	292	195	0.02%	0.003%
12	3.336	711	714	718	rBV2	301	231	0.03%	0.003%
13	3.590	787	793	797	rBV2	386	427	0.05%	0.006%
14	3.616	797	801	805	rVV	292	282	0.03%	0.004%
15	3.645	808	810	813	rBV	252	158	0.02%	0.002%
16	3.709	826	830	836	rVB3	531	368	0.04%	0.005%
17	3.802	855	859	860	rBV2	215	122	0.01%	0.002%
18	3.838	868	870	874	rVB2	274	143	0.02%	0.002%
19	3.902	878	890	933	rBV2	73217	274868	30.21%	3.803%
20	4.352	1016	1030	1058	rBV	137815	351460	38.63%	4.863%
21	5.047	1228	1246	1268	rBV2	363958	909754	100.00%	12.587%
22	5.278	1314	1318	1321	rBV4	482	358	0.04%	0.005%
23	5.349	1338	1340	1345	rVB3	426	228	0.03%	0.003%
24	5.404	1355	1357	1359	rVB3	463	168	0.02%	0.002%
25	5.484	1378	1382	1385	rBV3	305	244	0.03%	0.003%
26	5.535	1396	1398	1401	rVB	301	138	0.02%	0.002%
27	5.574	1406	1410	1412	rBV3	478	298	0.03%	0.004%
28	5.619	1412	1424	1442	rBV	257866	519808	57.14%	7.192%
29	5.844	1491	1494	1500	rVB5	656	667	0.07%	0.009%
30	5.908	1504	1514	1530	rBV6	9858	22919	2.52%	0.317%
31	6.072	1551	1565	1583	rBV	199686	414067	45.51%	5.729%
32	6.320	1639	1642	1643	rBV2	258	136	0.01%	0.002%
33	6.519	1699	1704	1706	rBV2	903	692	0.08%	0.010%
34	6.693	1756	1758	1761	rBV3	400	157	0.02%	0.002%
35	6.732	1768	1770	1772	rBV	354	181	0.02%	0.003%
36	6.773	1781	1783	1787	rBV2	215	134	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
 Data File : VV022436.D
 Acq On : 30 Sep 2021 16:54
 Operator : SY/MD
 Sample : M3979-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A04

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

37	6.854	1806	1808	1811	rBV	239	157	0.02%	0.002%
38	6.931	1829	1832	1833	rBV	206	127	0.01%	0.002%
39	6.989	1839	1850	1875	rBV	100449	193116	21.23%	2.672%
40	7.204	1914	1917	1919	rBV	417	240	0.03%	0.003%
41	7.262	1932	1935	1936	rBV	303	133	0.01%	0.002%
42	7.317	1940	1952	1995	rVV	413440	761598	83.71%	10.537%
43	7.625	2038	2048	2076	rBV2	68978	130665	14.36%	1.808%
44	7.828	2109	2111	2112	rBV	534	282	0.03%	0.004%
45	7.860	2118	2121	2123	rBV3	526	280	0.03%	0.004%
46	7.979	2147	2158	2178	rBV	151762	263949	29.01%	3.652%
47	8.092	2183	2193	2223	rBV	222890	424771	46.69%	5.877%
48	8.336	2267	2269	2273	rBV3	515	334	0.04%	0.005%
49	8.432	2296	2299	2302	rBV2	376	281	0.03%	0.004%
50	8.497	2315	2319	2321	rBV2	334	175	0.02%	0.002%
51	8.632	2357	2361	2362	rBV	266	169	0.02%	0.002%
52	8.706	2380	2384	2388	rBV2	288	148	0.02%	0.002%
53	8.741	2392	2395	2396	rBV	388	173	0.02%	0.002%
54	8.789	2404	2410	2414	rBV4	393	361	0.04%	0.005%
55	8.854	2419	2430	2454	rBV	400188	662773	72.85%	9.170%
56	9.047	2488	2490	2491	rBV	313	141	0.02%	0.002%
57	9.075	2496	2499	2503	rVV4	683	441	0.05%	0.006%
58	9.104	2506	2508	2514	rVB2	508	421	0.05%	0.006%
59	9.156	2517	2524	2526	rBV2	374	460	0.05%	0.006%
60	9.391	2594	2597	2598	rVB	465	198	0.02%	0.003%
61	9.426	2605	2608	2609	rBV3	251	131	0.01%	0.002%
62	9.529	2638	2640	2644	rBV3	360	254	0.03%	0.004%
63	9.657	2678	2680	2682	rBV	347	156	0.02%	0.002%
64	9.834	2732	2735	2740	rVB3	323	250	0.03%	0.003%
65	9.886	2748	2751	2752	rBV	282	165	0.02%	0.002%
66	10.133	2819	2828	2836	rVB7	2161	3465	0.38%	0.048%
67	10.217	2843	2854	2873	rBV	285688	449037	49.36%	6.213%
68	10.378	2902	2904	2906	rBV	328	128	0.01%	0.002%
69	10.574	2959	2965	2968	rBV3	606	594	0.07%	0.008%
70	10.677	2995	2997	3001	rVB	237	123	0.01%	0.002%
71	10.879	3057	3060	3063	rBV	418	249	0.03%	0.003%
72	11.030	3104	3107	3112	rBV3	806	717	0.08%	0.010%
73	11.104	3126	3130	3132	rBV2	344	255	0.03%	0.004%
74	11.136	3138	3140	3141	rBV	469	233	0.03%	0.003%
75	11.188	3151	3156	3158	rBV2	244	207	0.02%	0.003%
76	11.252	3164	3176	3199	rBV	356010	564941	62.10%	7.816%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
 Data File : VV022436.D
 Acq On : 30 Sep 2021 16:54
 Operator : SY/MD
 Sample : M3979-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A04

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

77	11.374	3212	3214	3215	rBV	725	304	0.03%	0.004%
78	11.625	3280	3292	3315	rBV	397258	638383	70.17%	8.832%
79	11.998	3405	3408	3411	rVB	250	165	0.02%	0.002%
80	12.014	3411	3413	3416	rBV2	324	240	0.03%	0.003%
81	12.075	3429	3432	3435	rBV2	501	311	0.03%	0.004%
82	12.194	3467	3469	3471	rBV	316	134	0.01%	0.002%
83	12.210	3471	3474	3480	rVV3	465	469	0.05%	0.006%
84	12.484	3556	3559	3560	rBV	261	135	0.01%	0.002%
85	12.606	3595	3597	3603	rVB4	433	275	0.03%	0.004%
86	12.632	3603	3605	3609	rVB2	274	175	0.02%	0.002%
87	12.664	3611	3615	3617	rBV3	462	294	0.03%	0.004%
88	12.760	3643	3645	3647	rBV2	332	149	0.02%	0.002%
89	12.857	3670	3675	3679	rBV2	236	296	0.03%	0.004%
90	13.172	3772	3773	3776	rVB	345	163	0.02%	0.002%
91	13.197	3779	3781	3782	rBV	274	131	0.01%	0.002%
92	13.513	3877	3879	3884	rVB2	489	275	0.03%	0.004%
93	13.776	3958	3961	3966	rBV	255	260	0.03%	0.004%
94	13.847	3980	3983	3985	rBV2	392	231	0.03%	0.003%
95	13.953	4012	4016	4018	rBV2	362	312	0.03%	0.004%
96	14.027	4037	4039	4042	rBV	302	157	0.02%	0.002%
97	14.162	4079	4081	4084	rBV2	304	194	0.02%	0.003%
98	14.220	4097	4099	4104	rBV2	319	267	0.03%	0.004%
99	14.358	4139	4142	4144	rBV2	268	145	0.02%	0.002%
100	14.480	4176	4180	4184	rBV2	370	313	0.03%	0.004%



Sum of corrected areas: 7227919

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
Data File : VV022436.D
Acq On : 30 Sep 2021 16:54
Operator : SY/MD
Sample : M3979-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
F4A04

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

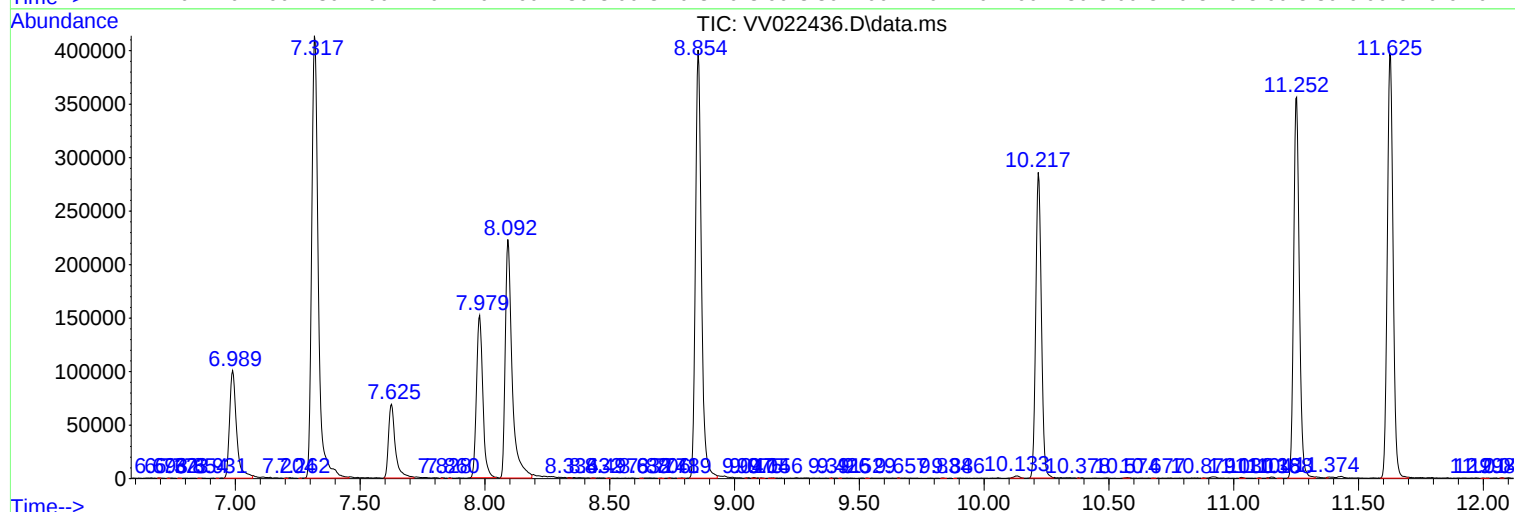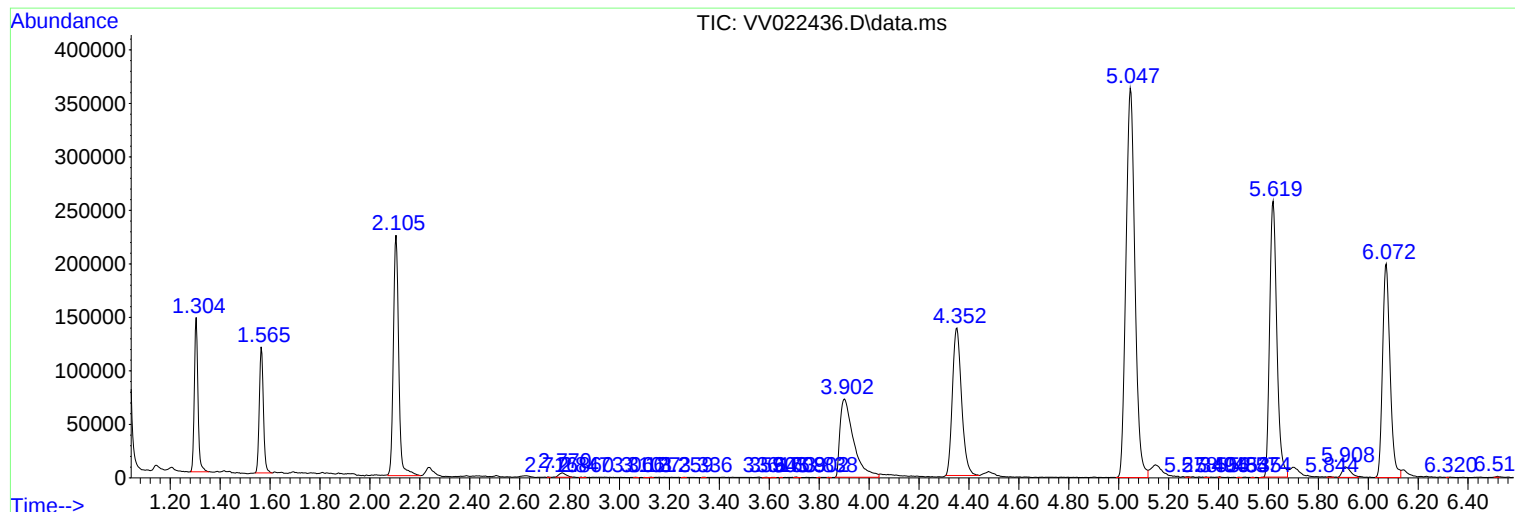

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
Data File : VV022436.D
Acq On : 30 Sep 2021 16:54
Operator : SY/MD
Sample : M3979-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A04

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
Data File : VV022436.D
Acq On : 30 Sep 2021 16:54
Operator : SY/MD
Sample : M3979-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A04

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
