

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
 Data File : VV022437.D
 Acq On : 30 Sep 2021 17:18
 Operator : SY/MD
 Sample : M3979-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A05

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M

Title : VOC Analysis

Signal : TIC: VV022437.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	101	rVB	134927	141174	13.34%	1.794%
2	1.564	156	163	176	rBV	116186	129988	12.29%	1.652%
3	2.105	321	331	344	rBV	223086	322193	30.45%	4.094%
4	2.564	471	474	480	rBV2	653	564	0.05%	0.007%
5	2.654	500	502	506	rBV2	466	286	0.03%	0.004%
6	2.770	528	538	551	rBV4	5931	12475	1.18%	0.159%
7	2.841	558	560	562	rBV	334	165	0.02%	0.002%
8	3.072	628	632	633	rBV	205	116	0.01%	0.001%
9	3.330	710	712	713	rBV	372	120	0.01%	0.002%
10	3.394	729	732	736	rBV	319	214	0.02%	0.003%
11	3.513	765	769	773	rBV2	256	204	0.02%	0.003%
12	3.619	797	802	805	rVB2	522	555	0.05%	0.007%
13	3.706	826	829	831	rBV	184	128	0.01%	0.002%
14	3.754	842	844	847	rVB2	438	240	0.02%	0.003%
15	3.770	847	849	853	rVV2	226	128	0.01%	0.002%
16	3.899	879	889	921	rBV2	57705	205531	19.43%	2.612%
17	4.217	985	988	989	rBV2	425	225	0.02%	0.003%
18	4.349	1012	1029	1056	rBV	142073	362808	34.29%	4.611%
19	4.619	1110	1113	1115	rBV2	274	164	0.02%	0.002%
20	4.683	1131	1133	1137	rBV2	454	279	0.03%	0.004%
21	4.982	1224	1226	1229	rBV	159	117	0.01%	0.001%
22	5.047	1229	1246	1266	rBV2	358942	897754	84.85%	11.409%
23	5.378	1343	1349	1352	rBV3	459	499	0.05%	0.006%
24	5.619	1411	1424	1441	rBV	259522	522641	49.40%	6.642%
25	5.912	1504	1515	1533	rBV8	9627	21869	2.07%	0.278%
26	5.992	1537	1540	1548	rBV2	336	422	0.04%	0.005%
27	6.072	1551	1565	1596	rBV	195653	416630	39.38%	5.295%
28	6.285	1628	1631	1632	rBV	290	164	0.02%	0.002%
29	6.352	1646	1652	1655	rBV2	363	362	0.03%	0.005%
30	6.404	1666	1668	1671	rBV3	309	233	0.02%	0.003%
31	6.481	1688	1692	1694	rBV	308	217	0.02%	0.003%
32	6.516	1697	1703	1704	rBV2	1177	925	0.09%	0.012%
33	6.596	1725	1728	1733	rBV3	561	480	0.05%	0.006%
34	6.625	1733	1737	1739	rVV2	396	196	0.02%	0.002%
35	6.648	1741	1744	1747	rVV2	243	170	0.02%	0.002%
36	6.690	1755	1757	1761	rVB2	223	133	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
 Data File : VV022437.D
 Acq On : 30 Sep 2021 17:18
 Operator : SY/MD
 Sample : M3979-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A05

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

37	6.783	1782	1786	1791	rBV2	274	279	0.03%	0.004%
38	6.805	1791	1793	1799	rVB2	384	291	0.03%	0.004%
39	6.915	1822	1827	1829	rBV2	384	319	0.03%	0.004%
40	6.989	1839	1850	1882	rBV	101173	190461	18.00%	2.420%
41	7.317	1940	1952	1971	rBV	409488	727558	68.77%	9.246%
42	7.622	2038	2047	2072	rBV	67981	125652	11.88%	1.597%
43	7.815	2100	2107	2113	rVB4	384	504	0.05%	0.006%
44	7.844	2114	2116	2119	rBV2	328	196	0.02%	0.002%
45	7.976	2144	2157	2183	rBV	617401	1058010	100.00%	13.445%
46	8.092	2184	2193	2230	rVV	227887	429076	40.56%	5.453%
47	8.439	2298	2301	2302	rBV2	503	223	0.02%	0.003%
48	8.606	2350	2353	2354	rBV2	235	135	0.01%	0.002%
49	8.661	2367	2370	2371	rBV2	217	132	0.01%	0.002%
50	8.706	2381	2384	2387	rBV2	409	269	0.03%	0.003%
51	8.770	2402	2404	2406	rVB2	344	111	0.01%	0.001%
52	8.854	2419	2430	2450	rBV	394127	653493	61.77%	8.305%
53	9.059	2492	2494	2497	rBV	410	179	0.02%	0.002%
54	9.108	2507	2509	2510	rBV	376	170	0.02%	0.002%
55	9.214	2540	2542	2544	rBV	338	140	0.01%	0.002%
56	9.310	2571	2572	2575	rBV2	310	137	0.01%	0.002%
57	9.490	2625	2628	2632	rBV2	210	146	0.01%	0.002%
58	9.548	2643	2646	2648	rBV3	534	277	0.03%	0.004%
59	9.654	2675	2679	2682	rBV2	278	252	0.02%	0.003%
60	9.738	2701	2705	2707	rBV2	236	212	0.02%	0.003%
61	9.776	2715	2717	2719	rBV2	209	119	0.01%	0.002%
62	9.944	2766	2769	2772	rBV2	198	134	0.01%	0.002%
63	9.979	2778	2780	2784	rVB	321	131	0.01%	0.002%
64	10.130	2819	2827	2837	rBV4	2457	3475	0.33%	0.044%
65	10.217	2843	2854	2878	rBV	283341	445957	42.15%	5.667%
66	10.320	2884	2886	2890	rBV4	601	339	0.03%	0.004%
67	10.371	2900	2902	2904	rVB2	414	155	0.01%	0.002%
68	10.471	2930	2933	2934	rBV3	577	244	0.02%	0.003%
69	10.516	2945	2947	2950	rVB2	345	196	0.02%	0.002%
70	10.606	2972	2975	2976	rBV	390	192	0.02%	0.002%
71	10.661	2988	2992	2994	rBV2	523	360	0.03%	0.005%
72	10.677	2994	2997	2998	rBV	417	157	0.01%	0.002%
73	10.747	3016	3019	3024	rBV2	310	323	0.03%	0.004%
74	10.821	3039	3042	3044	rBV2	317	220	0.02%	0.003%
75	10.844	3047	3049	3052	rVV3	294	167	0.02%	0.002%
76	10.863	3052	3055	3058	rBV2	201	167	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
 Data File : VV022437.D
 Acq On : 30 Sep 2021 17:18
 Operator : SY/MD
 Sample : M3979-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A05

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

77	10.982	3089	3092	3095	rVV3	283	199	0.02%	0.003%
78	11.117	3130	3134	3137	rVB	338	250	0.02%	0.003%
79	11.146	3139	3143	3148	rVB4	1131	1030	0.10%	0.013%
80	11.252	3164	3176	3199	rBV	352161	559226	52.86%	7.107%
81	11.506	3253	3255	3260	rVB2	382	254	0.02%	0.003%
82	11.625	3280	3292	3314	rBV	397343	623117	58.90%	7.919%
83	11.783	3338	3341	3342	rBV2	485	274	0.03%	0.003%
84	12.361	3518	3521	3527	rVB3	596	528	0.05%	0.007%
85	12.410	3533	3536	3537	rBV	261	163	0.02%	0.002%
86	12.660	3611	3614	3617	rBV2	262	193	0.02%	0.002%
87	12.760	3640	3645	3648	rVB	390	354	0.03%	0.004%
88	13.021	3723	3726	3727	rBV	214	115	0.01%	0.001%
89	13.111	3752	3754	3756	rBV	314	230	0.02%	0.003%
90	13.159	3766	3769	3772	rBV	399	262	0.02%	0.003%
91	13.352	3825	3829	3831	rBV	343	271	0.03%	0.003%
92	13.378	3835	3837	3842	rBV2	297	224	0.02%	0.003%
93	13.439	3854	3856	3860	rVB2	350	202	0.02%	0.003%
94	13.754	3952	3954	3957	rBV	446	211	0.02%	0.003%
95	13.950	4013	4015	4016	rBV	324	130	0.01%	0.002%
96	13.988	4024	4027	4028	rBV	296	125	0.01%	0.002%
97	14.104	4061	4063	4066	rBV2	283	153	0.01%	0.002%
98	14.368	4142	4145	4149	rBV2	269	174	0.02%	0.002%
99	14.554	4200	4203	4205	rBV	313	213	0.02%	0.003%
100	14.754	4262	4265	4268	rBV2	511	283	0.03%	0.004%




Sum of corrected areas: 7869108

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
Data File : VV022437.D
Acq On : 30 Sep 2021 17:18
Operator : SY/MD
Sample : M3979-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A05

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

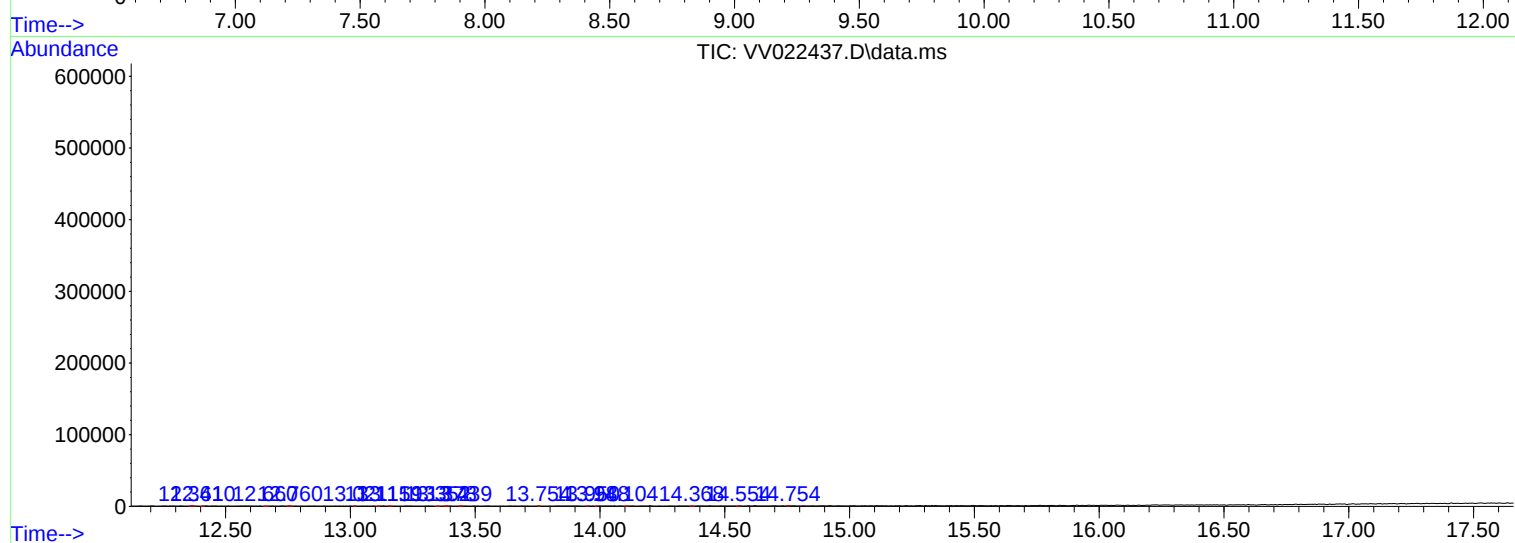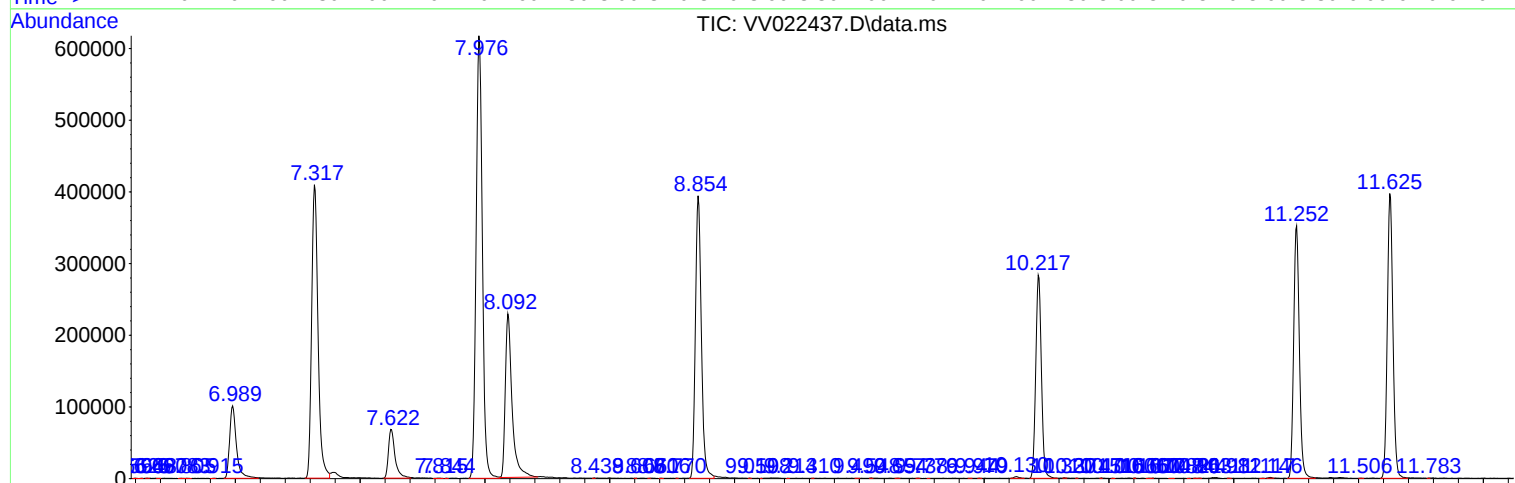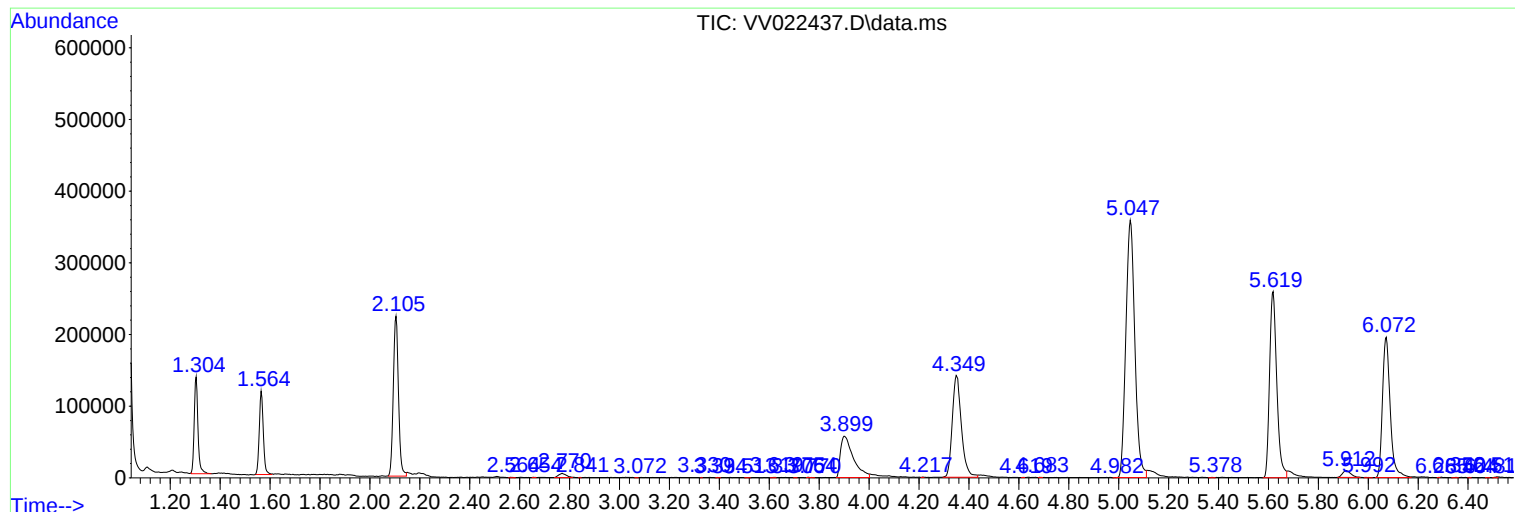

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
Data File : VV022437.D
Acq On : 30 Sep 2021 17:18
Operator : SY/MD
Sample : M3979-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A05

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
Data File : VV022437.D
Acq On : 30 Sep 2021 17:18
Operator : SY/MD
Sample : M3979-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A05

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
