

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
 Data File : VV022439.D
 Acq On : 30 Sep 2021 18:06
 Operator : SY/MD
 Sample : M3979-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A07

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

Signal : TIC: VV022439.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	102	rVB	140497	148166	13.99%	1.869%
2	1.564	156	163	178	rBV	113606	129705	12.25%	1.636%
3	2.104	322	331	344	rBV	224229	319344	30.15%	4.029%
4	2.494	449	452	453	rBV	684	375	0.04%	0.005%
5	2.580	477	479	480	rBV	328	146	0.01%	0.002%
6	2.622	490	492	493	rBV	375	130	0.01%	0.002%
7	2.680	508	510	513	rVB2	499	239	0.02%	0.003%
8	2.773	527	539	551	rBV5	5618	12182	1.15%	0.154%
9	2.854	560	564	565	rBV4	375	235	0.02%	0.003%
10	2.883	571	573	574	rBV4	267	104	0.01%	0.001%
11	2.979	601	603	604	rBV4	454	158	0.01%	0.002%
12	3.137	648	652	654	rBV3	336	242	0.02%	0.003%
13	3.342	709	716	721	rBV3	465	553	0.05%	0.007%
14	3.522	767	772	776	rBV	287	294	0.03%	0.004%
15	3.542	776	778	782	rVV2	203	136	0.01%	0.002%
16	3.564	782	785	787	rVB	206	94	0.01%	0.001%
17	3.606	796	798	800	rBV2	194	118	0.01%	0.001%
18	3.661	813	815	821	rBV2	426	278	0.03%	0.004%
19	3.693	822	825	827	rBV2	171	126	0.01%	0.002%
20	3.738	837	839	842	rBV	191	121	0.01%	0.002%
21	3.841	869	871	876	rBV2	244	227	0.02%	0.003%
22	3.895	878	888	922	rBV	63861	219532	20.73%	2.770%
23	4.349	1014	1029	1054	rBV	141531	357698	33.77%	4.513%
24	4.664	1121	1127	1131	rBV6	513	625	0.06%	0.008%
25	4.725	1144	1146	1148	rBV	245	135	0.01%	0.002%
26	4.786	1163	1165	1167	rBV2	305	182	0.02%	0.002%
27	4.837	1179	1181	1185	rVB2	349	144	0.01%	0.002%
28	4.866	1187	1190	1194	rVV2	493	265	0.03%	0.003%
29	4.886	1194	1196	1200	rVV2	228	131	0.01%	0.002%
30	4.905	1200	1202	1206	rBV2	302	176	0.02%	0.002%
31	4.953	1213	1217	1218	rBV2	355	265	0.03%	0.003%
32	5.046	1226	1246	1267	rBV2	358384	905714	85.51%	11.426%
33	5.378	1347	1349	1352	rBV3	311	206	0.02%	0.003%
34	5.432	1365	1366	1368	rBV	280	142	0.01%	0.002%
35	5.461	1373	1375	1377	rVV2	377	146	0.01%	0.002%
36	5.526	1393	1395	1396	rBV	308	106	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
 Data File : VV022439.D
 Acq On : 30 Sep 2021 18:06
 Operator : SY/MD
 Sample : M3979-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A07

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

37	5.567	1402	1408	1409	rBV2	345	300	0.03%	0.004%
38	5.619	1412	1424	1443	rBV	257670	519261	49.03%	6.551%
39	5.915	1504	1516	1527	rBV8	10191	23523	2.22%	0.297%
40	6.072	1550	1565	1581	rBV	199020	408933	38.61%	5.159%
41	6.445	1678	1681	1684	rVB2	222	136	0.01%	0.002%
42	6.474	1687	1690	1694	rBV3	256	248	0.02%	0.003%
43	6.516	1698	1703	1706	rBV3	758	861	0.08%	0.011%
44	6.844	1803	1805	1806	rBV3	331	128	0.01%	0.002%
45	6.908	1822	1825	1828	rBV2	207	163	0.02%	0.002%
46	6.924	1828	1830	1833	rVB2	363	155	0.01%	0.002%
47	6.989	1838	1850	1879	rBV	100046	191812	18.11%	2.420%
48	7.210	1917	1919	1920	rBV2	326	164	0.02%	0.002%
49	7.243	1928	1929	1932	rVB	336	164	0.02%	0.002%
50	7.316	1939	1952	1973	rBV	410424	735593	69.45%	9.280%
51	7.580	2032	2034	2038	rVB3	510	245	0.02%	0.003%
52	7.625	2038	2048	2079	rBV2	69296	131394	12.41%	1.658%
53	7.831	2110	2112	2113	rBV	242	95	0.01%	0.001%
54	7.873	2123	2125	2129	rVB3	403	234	0.02%	0.003%
55	7.924	2138	2141	2142	rBV	347	164	0.02%	0.002%
56	7.976	2144	2157	2183	rVV	611328	1059157	100.00%	13.362%
57	8.091	2184	2193	2227	rVV	236747	445077	42.02%	5.615%
58	8.577	2341	2344	2345	rBV2	391	263	0.02%	0.003%
59	8.715	2386	2387	2390	rVB	256	117	0.01%	0.001%
60	8.731	2390	2392	2395	rVB2	341	138	0.01%	0.002%
61	8.750	2395	2398	2399	rBV	272	143	0.01%	0.002%
62	8.853	2419	2430	2451	rBV	392426	650820	61.45%	8.211%
63	9.226	2544	2546	2548	rBV2	191	117	0.01%	0.001%
64	9.355	2585	2586	2588	rBV	219	95	0.01%	0.001%
65	9.442	2610	2613	2615	rBV	255	126	0.01%	0.002%
66	9.493	2627	2629	2631	rVB2	395	156	0.01%	0.002%
67	9.593	2656	2660	2661	rBV2	393	255	0.02%	0.003%
68	9.776	2713	2717	2720	rBV3	403	421	0.04%	0.005%
69	9.818	2728	2730	2735	rVB2	271	179	0.02%	0.002%
70	9.934	2764	2766	2769	rVB2	407	119	0.01%	0.002%
71	9.979	2778	2780	2784	rVB2	321	211	0.02%	0.003%
72	10.001	2784	2787	2788	rBV2	419	183	0.02%	0.002%
73	10.085	2810	2813	2815	rBV	382	191	0.02%	0.002%
74	10.127	2819	2826	2832	rBV5	2122	2859	0.27%	0.036%
75	10.217	2842	2854	2879	rBV	285682	453511	42.82%	5.721%
76	10.323	2885	2887	2893	rVB4	838	523	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
 Data File : VV022439.D
 Acq On : 30 Sep 2021 18:06
 Operator : SY/MD
 Sample : M3979-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A07

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M

Title : VOC Analysis

77	10.348	2893	2895	2898	rVB2	508	233	0.02%	0.003%
78	10.387	2904	2907	2909	rVB2	378	182	0.02%	0.002%
79	10.490	2937	2939	2940	rBV2	258	90	0.01%	0.001%
80	10.606	2973	2975	2978	rBV2	313	187	0.02%	0.002%
81	10.757	3020	3022	3025	rVB	332	146	0.01%	0.002%
82	10.805	3035	3037	3039	rBV	259	92	0.01%	0.001%
83	10.918	3067	3072	3085	rVB6	1596	2478	0.23%	0.031%
84	11.001	3096	3098	3101	rVB2	360	172	0.02%	0.002%
85	11.017	3101	3103	3104	rBV2	259	94	0.01%	0.001%
86	11.139	3138	3141	3143	rBV2	656	500	0.05%	0.006%
87	11.252	3164	3176	3192	rBV	359878	563209	53.18%	7.105%
88	11.625	3281	3292	3313	rBV	395001	630505	59.53%	7.954%
89	11.773	3335	3338	3339	rBV2	444	184	0.02%	0.002%
90	12.127	3446	3448	3450	rVB	275	106	0.01%	0.001%
91	12.207	3470	3473	3476	rVB2	503	199	0.02%	0.003%
92	12.274	3492	3494	3496	rBV2	268	153	0.01%	0.002%
93	12.307	3502	3504	3506	rBV	349	207	0.02%	0.003%
94	12.866	3677	3678	3680	rBV	298	147	0.01%	0.002%
95	13.120	3754	3757	3759	rBV2	506	320	0.03%	0.004%
96	13.419	3848	3850	3852	rBV2	242	89	0.01%	0.001%
97	13.622	3911	3913	3914	rBV2	350	122	0.01%	0.002%
98	13.789	3963	3965	3968	rVB2	402	162	0.02%	0.002%
99	14.033	4039	4041	4044	rBV2	252	126	0.01%	0.002%
100	14.233	4101	4103	4104	rBV2	359	174	0.02%	0.002%




Sum of corrected areas: 7926551

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
Data File : VV022439.D
Acq On : 30 Sep 2021 18:06
Operator : SY/MD
Sample : M3979-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
F4A07

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

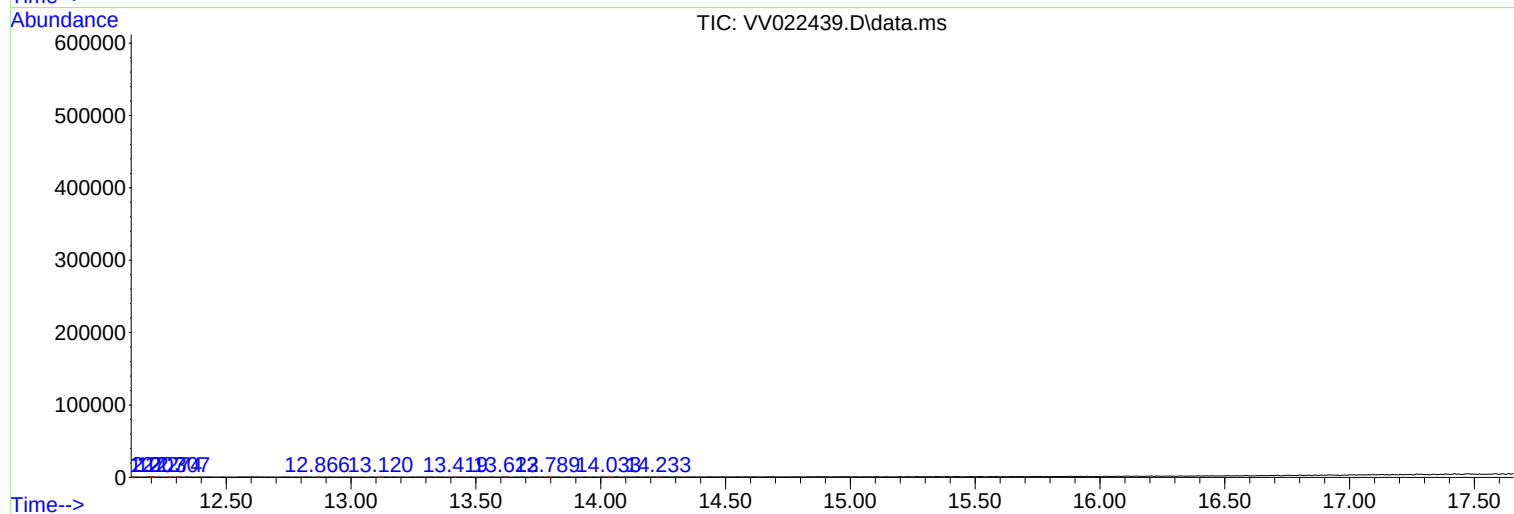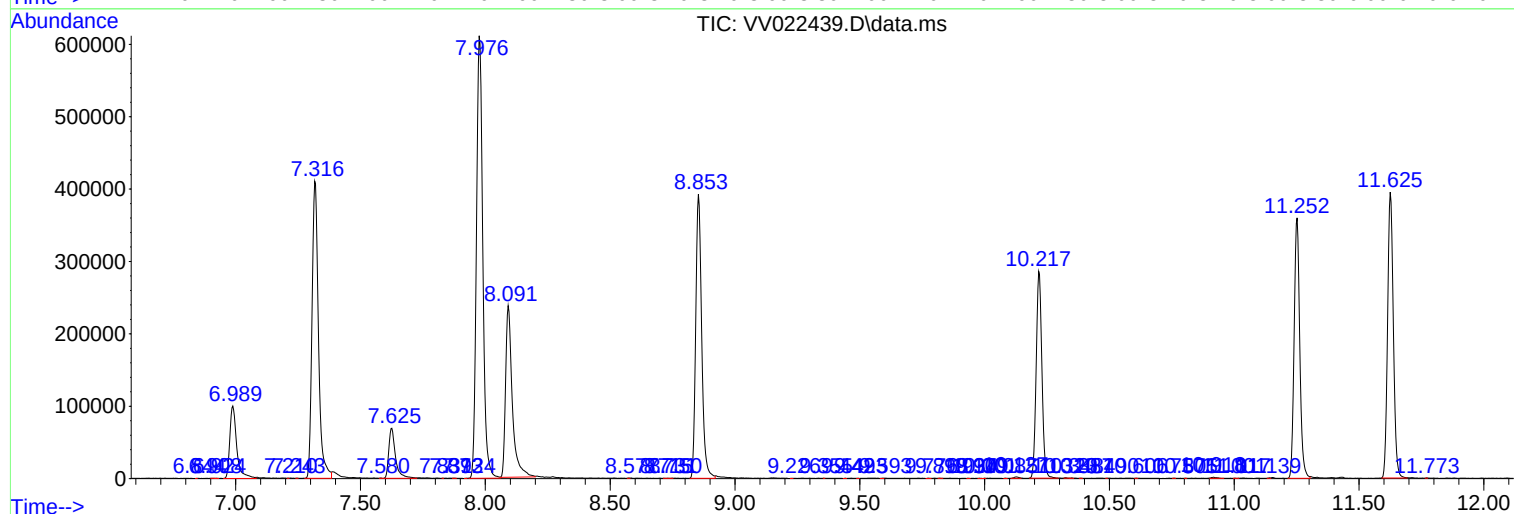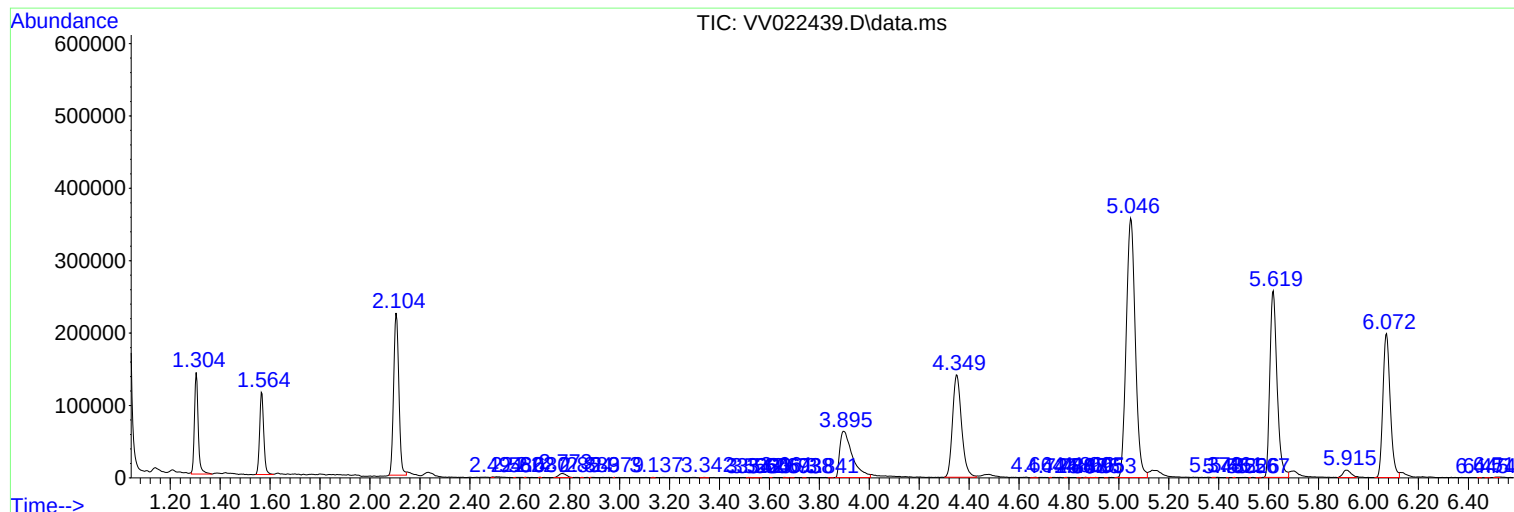

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
Data File : VV022439.D
Acq On : 30 Sep 2021 18:06
Operator : SY/MD
Sample : M3979-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A07

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
Data File : VV022439.D
Acq On : 30 Sep 2021 18:06
Operator : SY/MD
Sample : M3979-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A07

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
