

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
 Data File : VV022441.D
 Acq On : 30 Sep 2021 18:54
 Operator : SY/MD
 Sample : M3979-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A57

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

Signal : TIC: VV022441.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	101	rVB	137780	145823	16.03%	2.101%
2	1.565	157	163	180	rVB	117133	132985	14.62%	1.916%
3	2.105	322	331	347	rBV	224790	320617	35.25%	4.619%
4	2.545	465	468	471	rBV3	320	254	0.03%	0.004%
5	2.651	498	501	502	rBV	210	132	0.01%	0.002%
6	2.761	531	535	538	rBV3	1051	1021	0.11%	0.015%
7	3.146	650	655	658	rBV3	271	224	0.02%	0.003%
8	3.172	661	663	668	rBV2	298	175	0.02%	0.003%
9	3.278	693	696	698	rBV	241	150	0.02%	0.002%
10	3.513	767	769	772	rVB2	366	203	0.02%	0.003%
11	3.790	852	855	861	rVB3	271	200	0.02%	0.003%
12	3.818	861	864	867	rBV	364	176	0.02%	0.003%
13	3.899	879	889	920	rBV	58434	204125	22.44%	2.941%
14	4.349	1012	1029	1050	rBV	143509	355683	39.10%	5.124%
15	4.558	1092	1094	1096	rVB2	592	215	0.02%	0.003%
16	4.571	1096	1098	1102	rBV2	314	270	0.03%	0.004%
17	4.716	1140	1143	1144	rBV	378	203	0.02%	0.003%
18	4.764	1156	1158	1161	rBV2	271	140	0.02%	0.002%
19	4.806	1166	1171	1172	rBV	162	139	0.02%	0.002%
20	4.892	1195	1198	1199	rBV	360	160	0.02%	0.002%
21	4.963	1218	1220	1223	rBV3	338	182	0.02%	0.003%
22	5.047	1229	1246	1267	rBV2	360201	909566	100.00%	13.104%
23	5.336	1334	1336	1339	rVB3	505	212	0.02%	0.003%
24	5.352	1339	1341	1343	rBV	467	180	0.02%	0.003%
25	5.571	1406	1409	1411	rBV	355	276	0.03%	0.004%
26	5.619	1411	1424	1440	rBV	266319	536863	59.02%	7.735%
27	5.905	1505	1513	1537	rVB5	8855	20025	2.20%	0.289%
28	6.005	1541	1544	1549	rVB2	434	300	0.03%	0.004%
29	6.069	1550	1564	1601	rBV	197199	426444	46.88%	6.144%
30	6.246	1617	1619	1624	rVB4	551	293	0.03%	0.004%
31	6.272	1625	1627	1630	rVB3	437	189	0.02%	0.003%
32	6.339	1641	1648	1649	rBV	343	294	0.03%	0.004%
33	6.416	1667	1672	1675	rBV4	400	406	0.04%	0.006%
34	6.580	1721	1723	1726	rVB2	718	396	0.04%	0.006%
35	6.606	1726	1731	1732	rBV2	306	205	0.02%	0.003%
36	6.687	1754	1756	1758	rBV2	322	189	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
 Data File : VV022441.D
 Acq On : 30 Sep 2021 18:54
 Operator : SY/MD
 Sample : M3979-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A57

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

37	6.989	1836	1850	1880	rBV	100108	193632	21.29%	2.790%
38	7.201	1914	1916	1917	rBV	329	138	0.02%	0.002%
39	7.317	1941	1952	1973	rBV	410177	738909	81.24%	10.646%
40	7.625	2037	2048	2072	rBV2	67538	127220	13.99%	1.833%
41	7.815	2102	2107	2109	rBV2	522	444	0.05%	0.006%
42	7.934	2137	2144	2145	rBV3	816	739	0.08%	0.011%
43	7.979	2149	2158	2172	rVB	23190	40786	4.48%	0.588%
44	8.092	2179	2193	2229	rBV	220680	434784	47.80%	6.264%
45	8.394	2285	2287	2290	rBV2	401	259	0.03%	0.004%
46	8.423	2293	2296	2298	rBV2	527	263	0.03%	0.004%
47	8.558	2334	2338	2340	rBV2	433	320	0.04%	0.005%
48	8.603	2349	2352	2355	rVB2	428	241	0.03%	0.003%
49	8.625	2355	2359	2362	rBV5	366	312	0.03%	0.004%
50	8.854	2419	2430	2462	rBV	408208	675795	74.30%	9.736%
51	9.043	2486	2489	2490	rBV2	382	203	0.02%	0.003%
52	9.114	2505	2511	2515	rBV3	326	296	0.03%	0.004%
53	9.227	2542	2546	2547	rBV	282	145	0.02%	0.002%
54	9.249	2552	2553	2556	rBV3	360	201	0.02%	0.003%
55	9.497	2628	2630	2631	rBV	460	148	0.02%	0.002%
56	9.506	2631	2633	2635	rVV4	604	257	0.03%	0.004%
57	9.667	2681	2683	2686	rBV2	263	139	0.02%	0.002%
58	10.124	2820	2825	2826	rBV2	1630	1081	0.12%	0.016%
59	10.217	2842	2854	2876	rVV	280342	448572	49.32%	6.463%
60	10.320	2884	2886	2888	rBV2	454	296	0.03%	0.004%
61	10.358	2895	2898	2901	rBV2	374	344	0.04%	0.005%
62	10.371	2901	2902	2905	rVV2	397	217	0.02%	0.003%
63	10.471	2931	2933	2935	rBV	284	201	0.02%	0.003%
64	10.551	2953	2958	2963	rVB3	501	419	0.05%	0.006%
65	10.593	2963	2971	2972	rBV	363	393	0.04%	0.006%
66	10.603	2972	2974	2977	rVV2	295	180	0.02%	0.003%
67	10.635	2981	2984	2986	rBV	424	277	0.03%	0.004%
68	10.754	3017	3021	3024	rVB2	302	203	0.02%	0.003%
69	10.879	3058	3060	3063	rBV	317	233	0.03%	0.003%
70	10.924	3063	3074	3079	rVB6	1597	2290	0.25%	0.033%
71	10.953	3079	3083	3086	rBV	238	145	0.02%	0.002%
72	11.140	3138	3141	3144	rBV3	528	361	0.04%	0.005%
73	11.249	3164	3175	3196	rBV	363792	575537	63.28%	8.292%
74	11.468	3241	3243	3248	rBV2	409	251	0.03%	0.004%
75	11.538	3259	3265	3270	rBV6	1276	1602	0.18%	0.023%
76	11.625	3280	3292	3316	rBV	392703	628836	69.14%	9.060%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
 Data File : VV022441.D
 Acq On : 30 Sep 2021 18:54
 Operator : SY/MD
 Sample : M3979-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A57

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

77	11.950	3391	3393	3397	rBV2	274	189	0.02%	0.003%
78	11.969	3397	3399	3401	rBV	225	135	0.01%	0.002%
79	11.995	3403	3407	3408	rBV	350	191	0.02%	0.003%
80	12.355	3515	3519	3521	rBV3	423	308	0.03%	0.004%
81	12.426	3538	3541	3544	rVB2	344	197	0.02%	0.003%
82	12.452	3544	3549	3551	rBV3	453	361	0.04%	0.005%
83	12.522	3567	3571	3574	rBV2	329	291	0.03%	0.004%
84	12.718	3630	3632	3634	rBV2	361	161	0.02%	0.002%
85	12.760	3643	3645	3646	rBV2	335	140	0.02%	0.002%
86	12.815	3659	3662	3664	rBV	316	215	0.02%	0.003%
87	12.908	3687	3691	3692	rBV2	241	138	0.02%	0.002%
88	12.937	3697	3700	3702	rBV2	363	210	0.02%	0.003%
89	13.008	3718	3722	3724	rBV2	333	284	0.03%	0.004%
90	13.056	3732	3737	3740	rBV2	302	271	0.03%	0.004%
91	13.587	3900	3902	3909	rVB3	318	262	0.03%	0.004%
92	13.632	3913	3916	3917	rBV	283	156	0.02%	0.002%
93	13.792	3964	3966	3968	rBV	279	146	0.02%	0.002%
94	13.866	3986	3989	3993	rBV	259	198	0.02%	0.003%
95	13.898	3997	3999	4001	rBV	357	151	0.02%	0.002%
96	14.043	4041	4044	4045	rBV	385	197	0.02%	0.003%
97	14.432	4163	4165	4168	rBV	310	160	0.02%	0.002%
98	14.461	4172	4174	4176	rBV2	283	158	0.02%	0.002%
99	14.660	4232	4236	4239	rBV2	460	408	0.04%	0.006%
100	15.320	4438	4441	4444	rBV4	656	525	0.06%	0.008%




Sum of corrected areas: 6941036

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
Data File : VV022441.D
Acq On : 30 Sep 2021 18:54
Operator : SY/MD
Sample : M3979-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A57

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

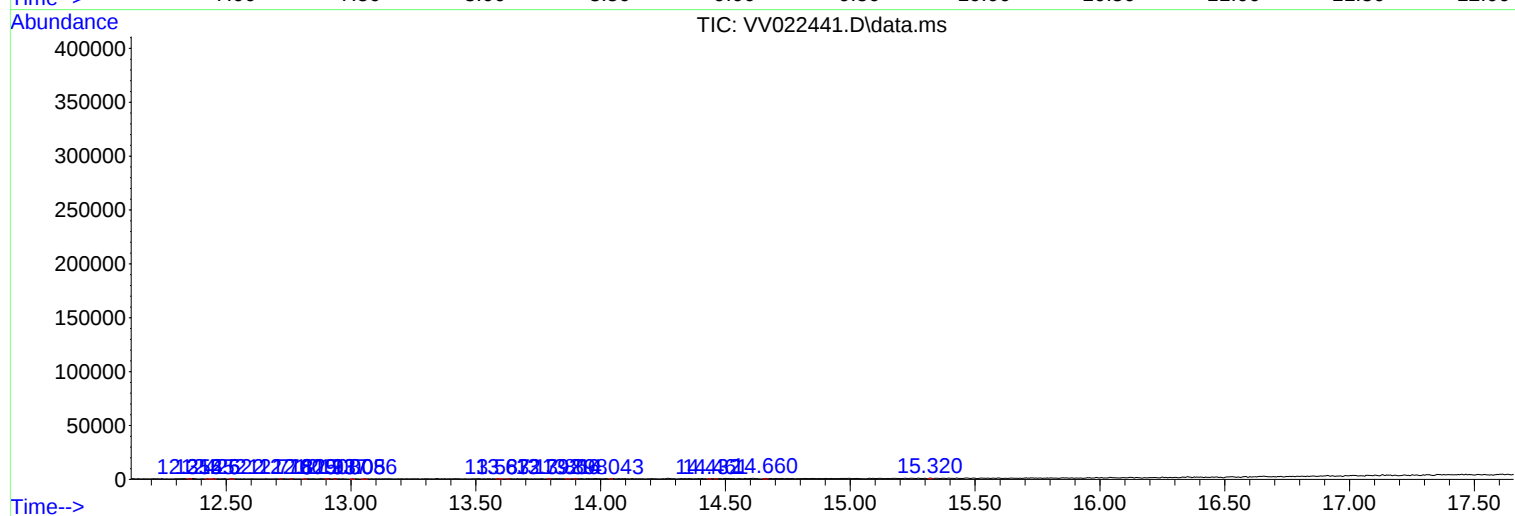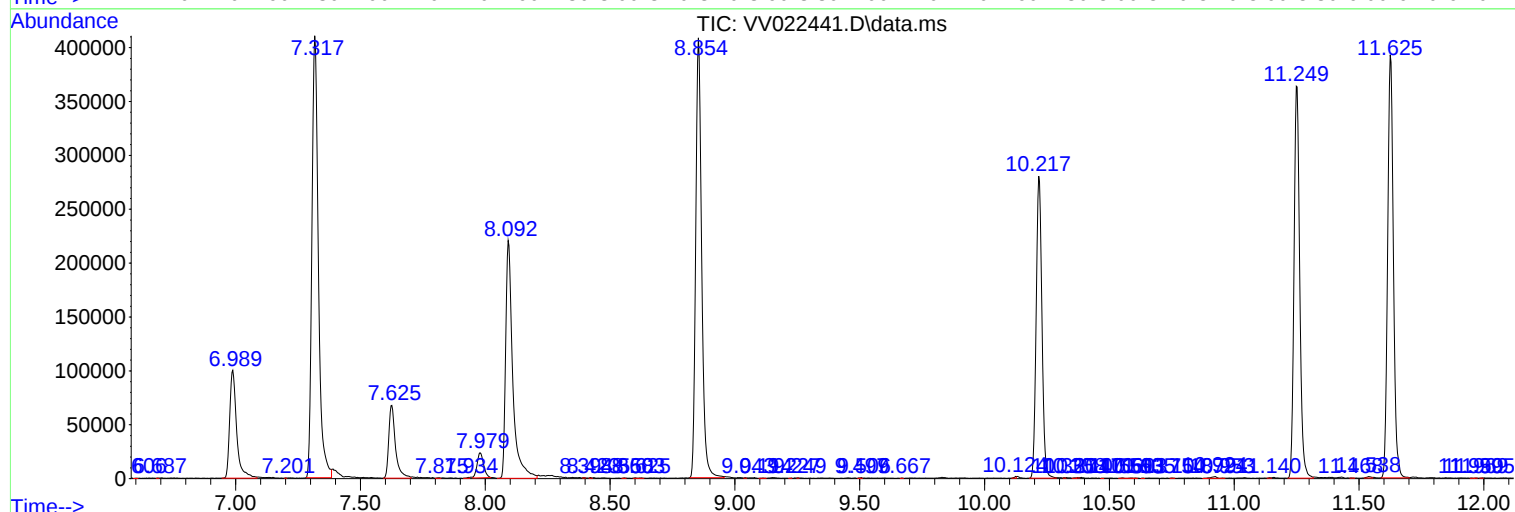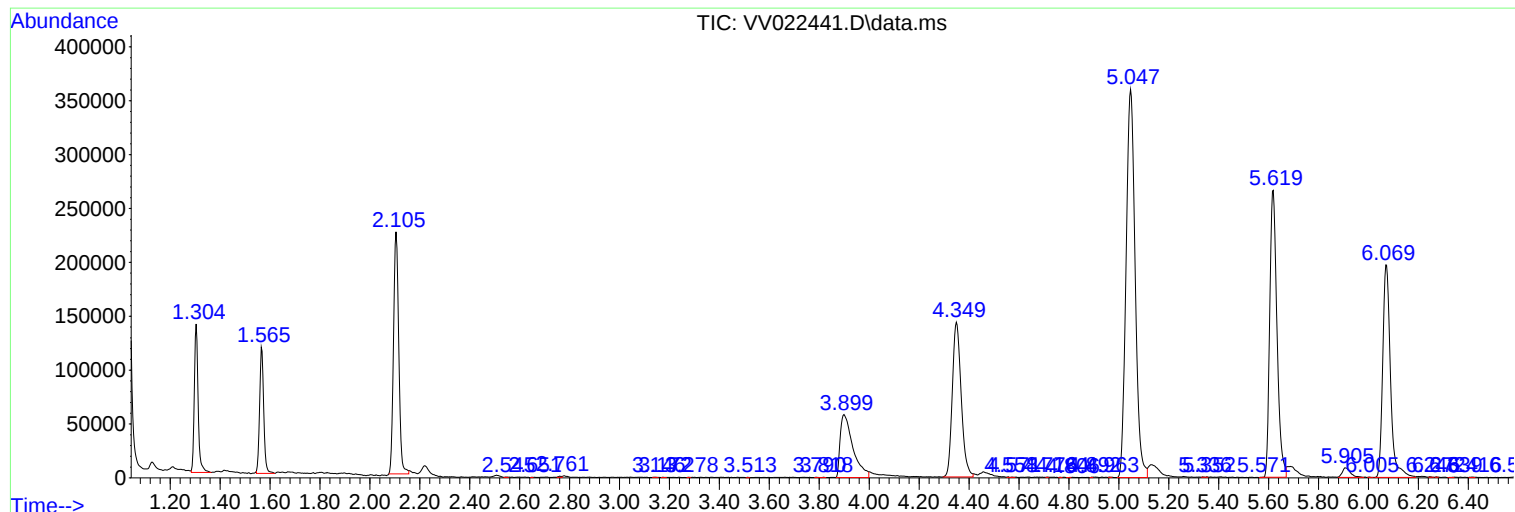

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
Data File : VV022441.D
Acq On : 30 Sep 2021 18:54
Operator : SY/MD
Sample : M3979-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A57

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
Data File : VV022441.D
Acq On : 30 Sep 2021 18:54
Operator : SY/MD
Sample : M3979-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A57

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
