

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
 Data File : VV022443.D
 Acq On : 30 Sep 2021 19:42
 Operator : SY/MD
 Sample : M3979-03DL 4X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A44DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M

Title : VOC Analysis

Signal : TIC: VV022443.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.201	45	50	58	rVB	81759	71314	7.87%	0.959%
2	1.304	76	82	100	rVB	140842	143621	15.85%	1.931%
3	1.564	156	163	178	rBV	113812	131583	14.52%	1.769%
4	2.105	321	331	355	rBV	228792	335810	37.06%	4.515%
5	2.609	483	488	489	rBV3	723	622	0.07%	0.008%
6	2.928	586	587	591	rBV	300	117	0.01%	0.002%
7	3.002	607	610	612	rBV	235	189	0.02%	0.003%
8	3.027	615	618	621	rBV2	472	320	0.04%	0.004%
9	3.146	651	655	659	rBV2	322	220	0.02%	0.003%
10	3.362	717	722	725	rBV3	285	296	0.03%	0.004%
11	3.436	740	745	750	rBV3	403	514	0.06%	0.007%
12	3.574	785	788	790	rBV	358	169	0.02%	0.002%
13	3.600	795	796	799	rVB2	435	168	0.02%	0.002%
14	3.712	829	831	834	rVB	513	248	0.03%	0.003%
15	3.738	834	839	841	rBV2	289	227	0.03%	0.003%
16	3.767	841	848	849	rBV2	370	264	0.03%	0.004%
17	3.834	866	869	872	rVB	328	128	0.01%	0.002%
18	3.857	874	876	879	rBV	238	119	0.01%	0.002%
19	3.905	879	891	930	rBV2	57263	225571	24.89%	3.033%
20	4.349	1013	1029	1053	rBV	144349	359476	39.67%	4.833%
21	4.596	1103	1106	1110	rBV3	462	427	0.05%	0.006%
22	4.677	1126	1131	1133	rBV2	294	217	0.02%	0.003%
23	4.879	1191	1194	1197	rVB	302	145	0.02%	0.002%
24	4.899	1197	1200	1202	rBV	248	112	0.01%	0.002%
25	5.047	1230	1246	1270	rBV2	360415	906126	100.00%	12.182%
26	5.323	1330	1332	1333	rBV	383	136	0.02%	0.002%
27	5.477	1378	1380	1382	rVB	599	264	0.03%	0.004%
28	5.490	1382	1384	1386	rBV	394	248	0.03%	0.003%
29	5.522	1392	1394	1397	rVB	215	117	0.01%	0.002%
30	5.558	1403	1405	1407	rVB2	430	168	0.02%	0.002%
31	5.619	1412	1424	1442	rBV	254692	514279	56.76%	6.914%
32	5.911	1504	1515	1533	rBV7	14042	34195	3.77%	0.460%
33	6.072	1550	1565	1590	rBV	199687	417517	46.08%	5.613%
34	6.288	1630	1632	1634	rBV	457	201	0.02%	0.003%
35	6.513	1700	1702	1704	rBV	485	198	0.02%	0.003%
36	6.529	1705	1707	1710	rBV	286	169	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
 Data File : VV022443.D
 Acq On : 30 Sep 2021 19:42
 Operator : SY/MD
 Sample : M3979-03DL 4X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A44DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

37	6.612	1730	1733	1735	rBV3	309	175	0.02%	0.002%
38	6.744	1772	1774	1778	rVB3	583	360	0.04%	0.005%
39	6.773	1781	1783	1785	rBV	160	104	0.01%	0.001%
40	6.792	1786	1789	1791	rBV	228	99	0.01%	0.001%
41	6.809	1791	1794	1795	rBV	404	195	0.02%	0.003%
42	6.866	1809	1812	1816	rBV2	292	163	0.02%	0.002%
43	6.989	1839	1850	1873	rBV	99878	188589	20.81%	2.535%
44	7.182	1908	1910	1913	rBV2	494	306	0.03%	0.004%
45	7.262	1930	1935	1937	rBV2	409	231	0.03%	0.003%
46	7.317	1938	1952	1972	rBV	411730	728457	80.39%	9.794%
47	7.538	2018	2021	2023	rBV3	519	289	0.03%	0.004%
48	7.625	2038	2048	2072	rBV	68000	123982	13.68%	1.667%
49	7.809	2103	2105	2108	rBV2	452	198	0.02%	0.003%
50	7.915	2135	2138	2140	rBV	237	121	0.01%	0.002%
51	7.976	2145	2157	2178	rBV	331842	566697	62.54%	7.619%
52	8.091	2183	2193	2231	rBV	214547	420087	46.36%	5.648%
53	8.455	2304	2306	2310	rBV3	309	277	0.03%	0.004%
54	8.564	2337	2340	2341	rBV	286	185	0.02%	0.002%
55	8.616	2354	2356	2361	rVB2	325	208	0.02%	0.003%
56	8.644	2363	2365	2366	rBV2	304	121	0.01%	0.002%
57	8.693	2376	2380	2382	rVB2	310	187	0.02%	0.003%
58	8.744	2393	2396	2398	rBV	245	156	0.02%	0.002%
59	8.783	2406	2408	2415	rVB4	409	367	0.04%	0.005%
60	8.815	2416	2418	2419	rBV	220	117	0.01%	0.002%
61	8.853	2419	2430	2455	rBV	384567	640369	70.67%	8.609%
62	9.104	2505	2508	2511	rBV3	421	320	0.04%	0.004%
63	9.136	2516	2518	2520	rBV	430	247	0.03%	0.003%
64	9.156	2522	2524	2528	rVB3	328	207	0.02%	0.003%
65	9.233	2546	2548	2550	rBV3	236	108	0.01%	0.001%
66	9.365	2588	2589	2592	rBV	244	140	0.02%	0.002%
67	9.455	2614	2617	2619	rBV2	209	150	0.02%	0.002%
68	9.558	2646	2649	2653	rVB3	248	146	0.02%	0.002%
69	9.696	2690	2692	2696	rBV3	346	247	0.03%	0.003%
70	9.786	2717	2720	2723	rBV2	314	255	0.03%	0.003%
71	10.079	2808	2811	2814	rBV	309	195	0.02%	0.003%
72	10.127	2821	2826	2834	rVB5	1412	2116	0.23%	0.028%
73	10.217	2842	2854	2871	rBV	272952	434120	47.91%	5.836%
74	10.657	2989	2991	2993	rBV2	260	114	0.01%	0.002%
75	10.686	2998	3000	3002	rBV	394	122	0.01%	0.002%
76	10.718	3006	3010	3014	rBV2	227	227	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
 Data File : VV022443.D
 Acq On : 30 Sep 2021 19:42
 Operator : SY/MD
 Sample : M3979-03DL 4X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A44DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M

Title : VOC Analysis

77	10.821	3038	3042	3043	rBV	507	294	0.03%	0.004%
78	10.831	3043	3045	3051	rVB4	439	383	0.04%	0.005%
79	10.921	3066	3073	3080	rVB7	1213	1751	0.19%	0.024%
80	10.992	3092	3095	3098	rBV3	248	191	0.02%	0.003%
81	11.082	3121	3123	3127	rBV2	344	195	0.02%	0.003%
82	11.146	3138	3143	3149	rVB4	789	975	0.11%	0.013%
83	11.252	3164	3176	3193	rBV	348712	550965	60.80%	7.407%
84	11.625	3280	3292	3315	rBV	384768	623367	68.79%	8.381%
85	11.844	3352	3360	3365	rBV5	468	687	0.08%	0.009%
86	11.953	3392	3394	3395	rBV	276	108	0.01%	0.001%
87	12.172	3461	3462	3464	rBV2	238	115	0.01%	0.002%
88	12.323	3507	3509	3512	rVB2	428	184	0.02%	0.002%
89	12.458	3550	3551	3554	rBV2	255	140	0.02%	0.002%
90	12.564	3581	3584	3589	rVB2	399	257	0.03%	0.003%
91	12.590	3589	3592	3593	rBV2	298	186	0.02%	0.003%
92	13.024	3725	3727	3730	rBV2	355	177	0.02%	0.002%
93	13.236	3791	3793	3795	rBV2	287	113	0.01%	0.002%
94	13.336	3822	3824	3826	rVB	300	101	0.01%	0.001%
95	13.397	3841	3843	3847	rVB2	362	201	0.02%	0.003%
96	13.474	3865	3867	3870	rBV2	258	127	0.01%	0.002%
97	13.619	3909	3912	3913	rBV	332	150	0.02%	0.002%
98	13.837	3977	3980	3986	rBV2	380	449	0.05%	0.006%
99	14.033	4038	4041	4043	rBV	338	197	0.02%	0.003%
100	14.072	4048	4053	4058	rBV2	474	534	0.06%	0.007%




Sum of corrected areas: 7438096

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
Data File : VV022443.D
Acq On : 30 Sep 2021 19:42
Operator : SY/MD
Sample : M3979-03DL 4X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A44DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

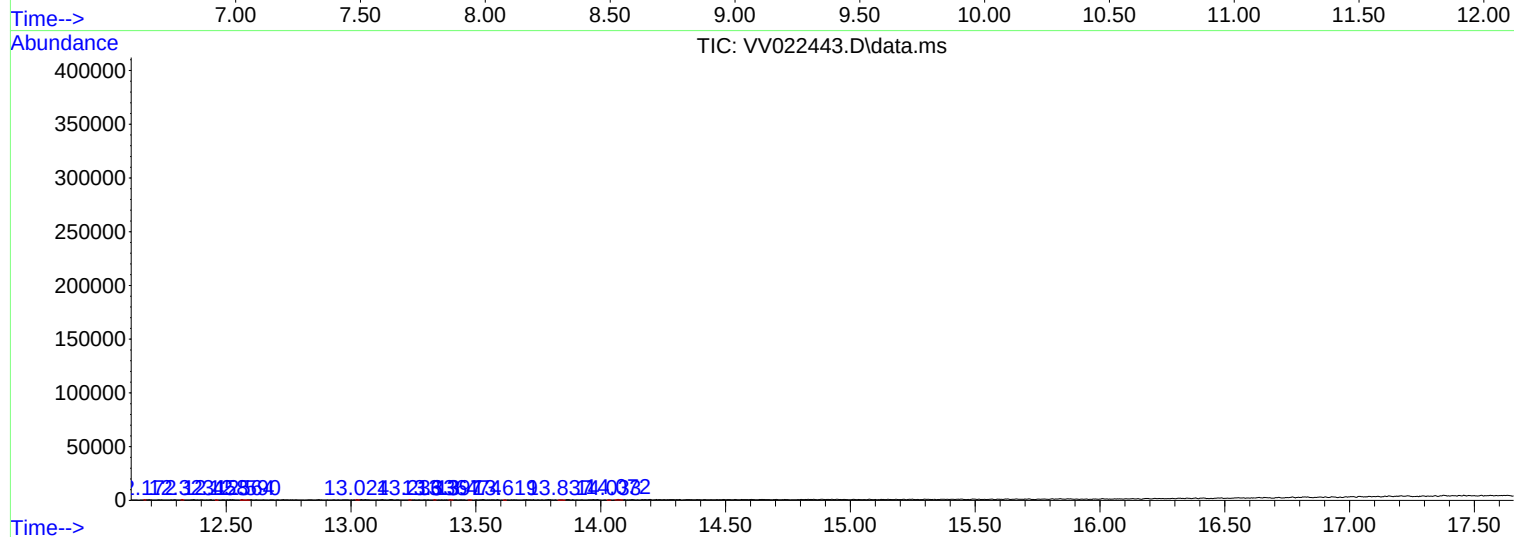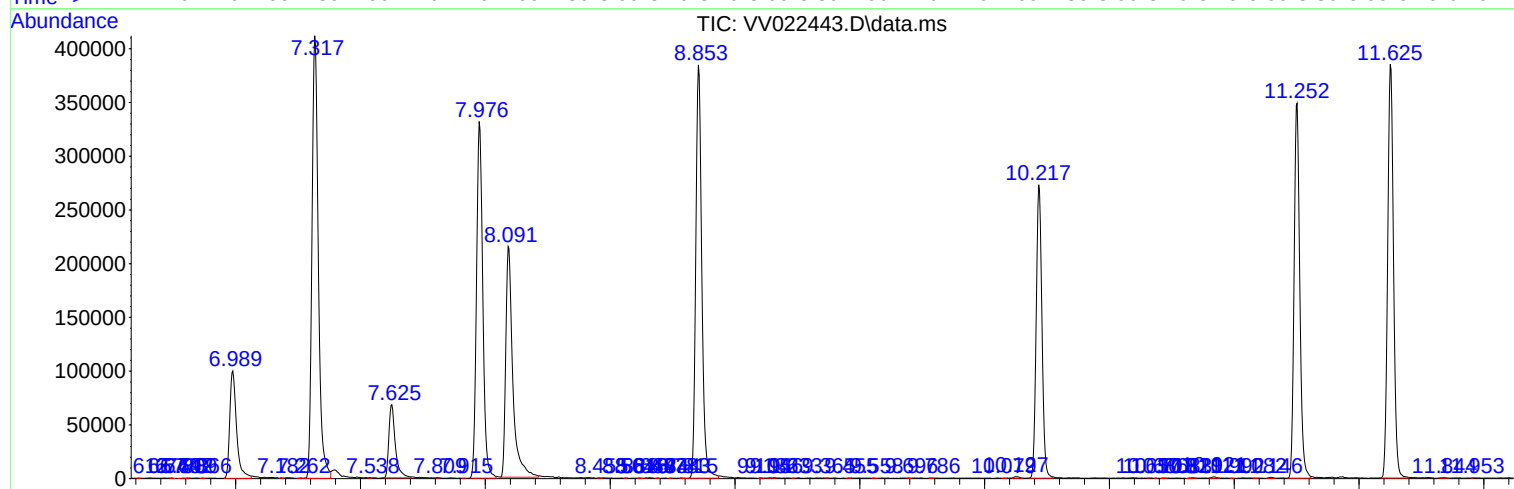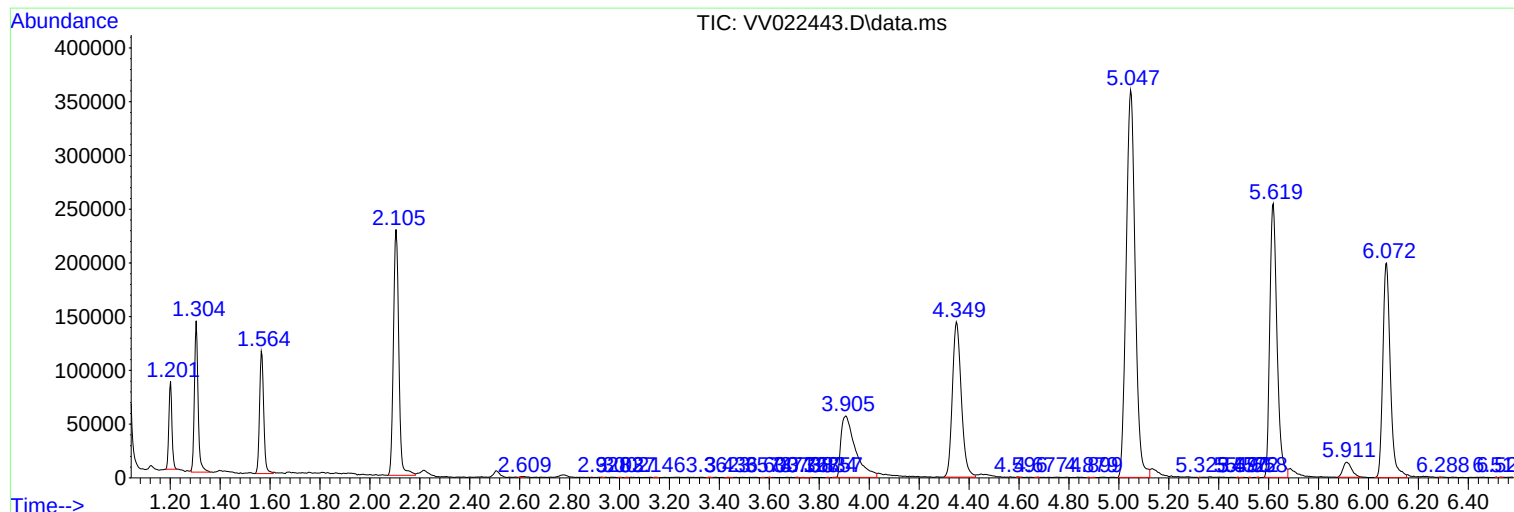

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
Data File : VV022443.D
Acq On : 30 Sep 2021 19:42
Operator : SY/MD
Sample : M3979-03DL 4X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A44DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
Data File : VV022443.D
Acq On : 30 Sep 2021 19:42
Operator : SY/MD
Sample : M3979-03DL 4X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A44DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------