

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
 Data File : VV022444.D
 Acq On : 30 Sep 2021 20:07
 Operator : SY/MD
 Sample : M3979-04DL 4X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A45DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M

Title : VOC Analysis

Signal : TIC: VV022444.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.201	46	50	58	rVB	26040	23134	2.47%	0.307%
2	1.304	76	82	99	rVB	137250	141978	15.18%	1.886%
3	1.564	156	163	180	rBV	116450	131178	14.02%	1.743%
4	2.105	322	331	345	rBV	228156	323397	34.57%	4.296%
5	2.506	449	456	467	rVV2	6463	10258	1.10%	0.136%
6	2.564	470	474	475	rBV2	237	170	0.02%	0.002%
7	2.770	531	538	550	rVB6	2221	4438	0.47%	0.059%
8	2.995	605	608	612	rBV	425	248	0.03%	0.003%
9	3.375	723	726	728	rBV2	157	140	0.01%	0.002%
10	3.391	729	731	736	rVB3	419	279	0.03%	0.004%
11	3.429	741	743	748	rBV2	300	231	0.02%	0.003%
12	3.902	879	890	934	rBV	61753	242741	25.95%	3.225%
13	4.349	1013	1029	1056	rBV	139574	362611	38.77%	4.817%
14	4.616	1109	1112	1114	rBV2	366	192	0.02%	0.003%
15	4.625	1114	1115	1119	rVB3	430	260	0.03%	0.003%
16	4.702	1136	1139	1140	rBV	359	220	0.02%	0.003%
17	4.863	1187	1189	1192	rVB2	353	190	0.02%	0.003%
18	4.937	1207	1212	1214	rBV3	398	272	0.03%	0.004%
19	5.047	1229	1246	1299	rBV2	366787	935383	100.00%	12.426%
20	5.381	1346	1350	1352	rBV	318	213	0.02%	0.003%
21	5.448	1369	1371	1374	rBV2	259	138	0.01%	0.002%
22	5.468	1374	1377	1381	rVV3	571	359	0.04%	0.005%
23	5.497	1384	1386	1388	rVV2	419	172	0.02%	0.002%
24	5.519	1390	1393	1396	rBV2	231	180	0.02%	0.002%
25	5.619	1411	1424	1456	rBV	257372	535116	57.21%	7.108%
26	5.812	1482	1484	1489	rVB3	498	378	0.04%	0.005%
27	5.915	1503	1516	1533	rBV7	13671	32612	3.49%	0.433%
28	6.072	1551	1565	1594	rBV	202345	418916	44.79%	5.565%
29	6.329	1643	1645	1649	rVB4	462	285	0.03%	0.004%
30	6.349	1649	1651	1653	rBV3	302	164	0.02%	0.002%
31	6.381	1659	1661	1664	rBV2	402	240	0.03%	0.003%
32	6.526	1703	1706	1709	rVB2	336	203	0.02%	0.003%
33	6.558	1714	1716	1720	rVV2	312	195	0.02%	0.003%
34	6.606	1729	1731	1736	rVB	241	179	0.02%	0.002%
35	6.670	1745	1751	1754	rVV	300	288	0.03%	0.004%
36	6.709	1759	1763	1768	rVB	224	195	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
 Data File : VV022444.D
 Acq On : 30 Sep 2021 20:07
 Operator : SY/MD
 Sample : M3979-04DL 4X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A45DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

37	6.751	1773	1776	1782	rBV4	325	356	0.04%	0.005%
38	6.989	1839	1850	1877	rBV	98822	187123	20.00%	2.486%
39	7.149	1896	1900	1901	rBV	412	310	0.03%	0.004%
40	7.188	1909	1912	1916	rVB3	370	274	0.03%	0.004%
41	7.217	1916	1921	1922	rBV	681	591	0.06%	0.008%
42	7.317	1940	1952	1971	rBV	406712	727898	77.82%	9.669%
43	7.625	2037	2048	2073	rBV	66620	123944	13.25%	1.646%
44	7.767	2089	2092	2095	rBV3	328	198	0.02%	0.003%
45	7.831	2109	2112	2115	rBV	360	267	0.03%	0.004%
46	7.976	2144	2157	2177	rBV	356035	607721	64.97%	8.073%
47	8.091	2184	2193	2228	rBV	224151	425281	45.47%	5.649%
48	8.361	2273	2277	2279	rBV3	311	271	0.03%	0.004%
49	8.548	2330	2335	2339	rBV3	330	334	0.04%	0.004%
50	8.616	2350	2356	2357	rBV3	391	350	0.04%	0.005%
51	8.625	2357	2359	2362	rVB2	502	238	0.03%	0.003%
52	8.641	2362	2364	2367	rBV2	365	165	0.02%	0.002%
53	8.670	2367	2373	2375	rBV2	272	271	0.03%	0.004%
54	8.757	2396	2400	2402	rBV2	248	192	0.02%	0.003%
55	8.796	2409	2412	2415	rVB2	539	229	0.02%	0.003%
56	8.853	2415	2430	2458	rBV	388697	647214	69.19%	8.598%
57	9.043	2487	2489	2490	rBV	274	153	0.02%	0.002%
58	9.120	2510	2513	2514	rBV	347	158	0.02%	0.002%
59	9.194	2534	2536	2539	rBV2	259	155	0.02%	0.002%
60	9.349	2581	2584	2587	rBV	304	174	0.02%	0.002%
61	9.394	2595	2598	2601	rVB	479	226	0.02%	0.003%
62	9.419	2601	2606	2607	rBV	295	182	0.02%	0.002%
63	9.445	2611	2614	2617	rVB2	424	222	0.02%	0.003%
64	10.014	2789	2791	2796	rVB2	250	142	0.02%	0.002%
65	10.104	2814	2819	2820	rBV	277	258	0.03%	0.003%
66	10.127	2820	2826	2833	rVB3	2070	2811	0.30%	0.037%
67	10.217	2840	2854	2872	rBV	278638	443266	47.39%	5.888%
68	10.448	2924	2926	2931	rVB2	387	272	0.03%	0.004%
69	10.484	2934	2937	2942	rBV	261	188	0.02%	0.002%
70	10.583	2963	2968	2970	rBV6	488	447	0.05%	0.006%
71	10.673	2993	2996	2998	rBV2	294	149	0.02%	0.002%
72	10.783	3027	3030	3032	rBV2	199	167	0.02%	0.002%
73	10.802	3035	3036	3041	rVB2	405	185	0.02%	0.002%
74	10.911	3067	3070	3072	rBV3	1130	716	0.08%	0.010%
75	11.249	3164	3175	3198	rBV	350189	557050	59.55%	7.400%
76	11.464	3239	3242	3245	rVB3	466	296	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
 Data File : VV022444.D
 Acq On : 30 Sep 2021 20:07
 Operator : SY/MD
 Sample : M3979-04DL 4X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A45DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M

Title : VOC Analysis

77	11.484	3246	3248	3252	rBV2	226	154	0.02%	0.002%
78	11.561	3269	3272	3275	rBV2	487	310	0.03%	0.004%
79	11.625	3280	3292	3313	rBV	389937	624330	66.75%	8.294%
80	11.747	3328	3330	3333	rVB	846	454	0.05%	0.006%
81	11.773	3336	3338	3339	rBV	503	205	0.02%	0.003%
82	11.969	3396	3399	3401	rBV	248	206	0.02%	0.003%
83	12.027	3413	3417	3421	rVB2	363	295	0.03%	0.004%
84	12.053	3421	3425	3427	rBV	442	285	0.03%	0.004%
85	12.194	3464	3469	3472	rBV2	507	500	0.05%	0.007%
86	12.387	3525	3529	3532	rVB2	360	216	0.02%	0.003%
87	12.455	3547	3550	3553	rBV	268	189	0.02%	0.003%
88	12.538	3574	3576	3582	rVB2	408	178	0.02%	0.002%
89	12.574	3583	3587	3591	rBV	369	244	0.03%	0.003%
90	12.593	3591	3593	3597	rBV	323	246	0.03%	0.003%
91	12.821	3662	3664	3667	rVB	400	150	0.02%	0.002%
92	12.975	3710	3712	3715	rVB2	466	251	0.03%	0.003%
93	12.998	3715	3719	3721	rBV2	316	227	0.02%	0.003%
94	13.024	3725	3727	3730	rVV2	277	139	0.01%	0.002%
95	13.085	3742	3746	3751	rBV2	364	325	0.03%	0.004%
96	13.747	3947	3952	3955	rBV3	401	308	0.03%	0.004%
97	14.136	4071	4073	4077	rVB3	350	191	0.02%	0.003%
98	14.242	4104	4106	4109	rBV2	396	266	0.03%	0.004%
99	14.406	4151	4157	4159	rBV2	269	285	0.03%	0.004%
100	14.802	4276	4280	4282	rBV	403	373	0.04%	0.005%




Sum of corrected areas: 7527924

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
Data File : VV022444.D
Acq On : 30 Sep 2021 20:07
Operator : SY/MD
Sample : M3979-04DL 4X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A45DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

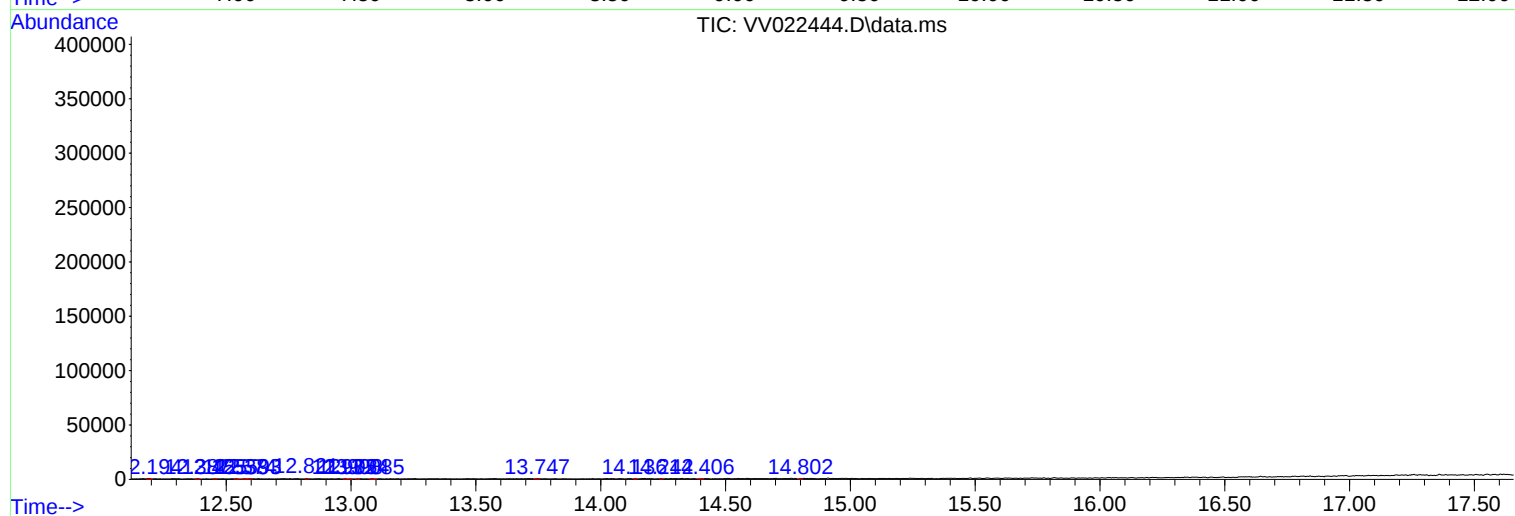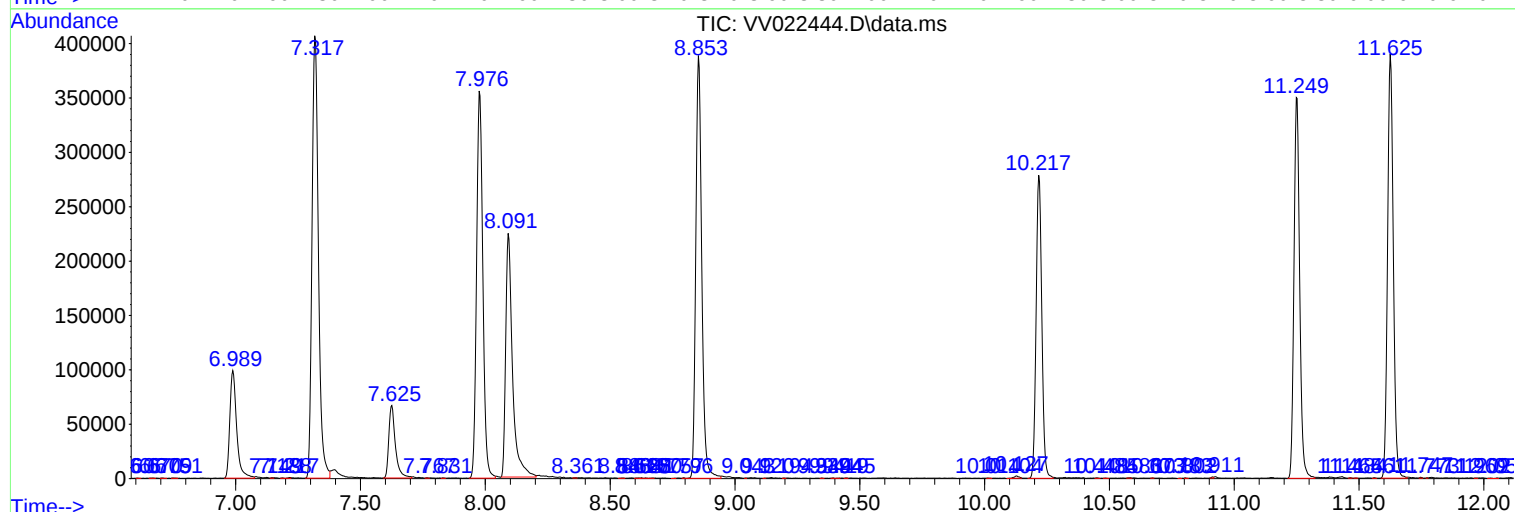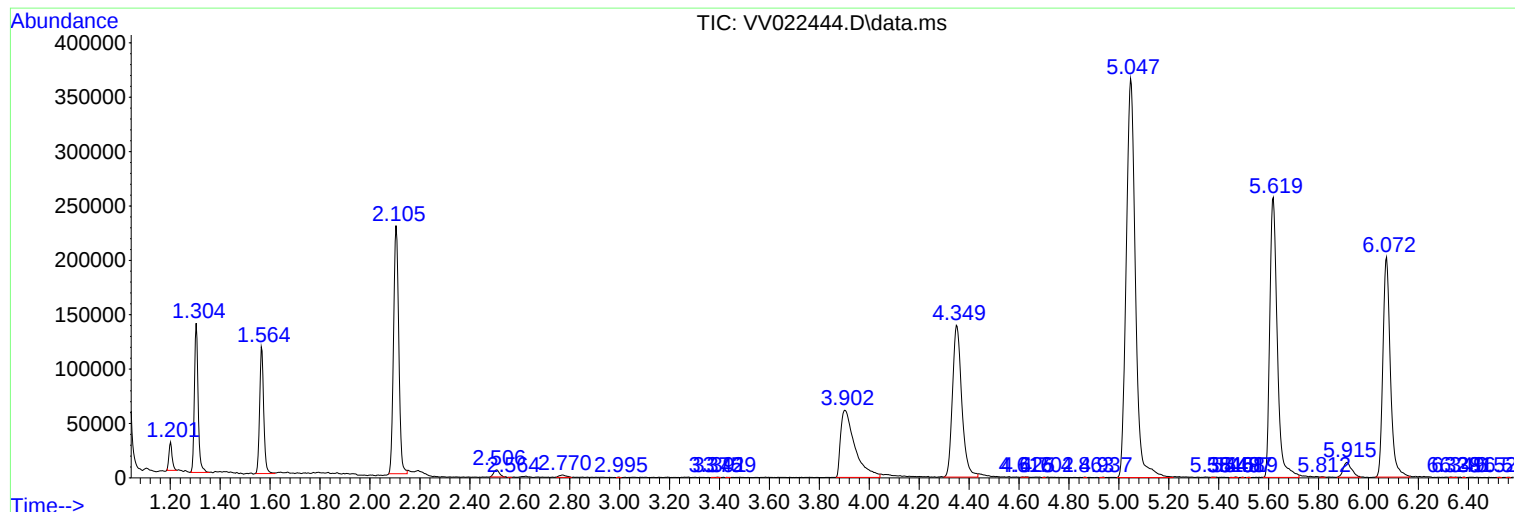

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
Data File : VV022444.D
Acq On : 30 Sep 2021 20:07
Operator : SY/MD
Sample : M3979-04DL 4X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A45DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
Data File : VV022444.D
Acq On : 30 Sep 2021 20:07
Operator : SY/MD
Sample : M3979-04DL 4X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A45DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
