

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
 Data File : VV022446.D
 Acq On : 30 Sep 2021 21:19
 Operator : SY/MD
 Sample : VV0930WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK268

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M

Title : VOC Analysis

Signal : TIC: VV022446.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	95	rBV	143185	144466	15.61%	2.105%
2	1.561	155	162	177	rVB	119981	137165	14.83%	1.999%
3	2.105	322	331	356	rVB	238682	350854	37.92%	5.113%
4	2.507	445	456	466	rBV3	4211	7413	0.80%	0.108%
5	2.683	508	511	514	rBV2	228	211	0.02%	0.003%
6	2.754	531	533	535	rBV	308	153	0.02%	0.002%
7	3.008	610	612	615	rVB2	428	225	0.02%	0.003%
8	3.050	620	625	627	rBV2	369	274	0.03%	0.004%
9	3.323	707	710	714	rBV2	297	186	0.02%	0.003%
10	3.423	735	741	745	rBV4	273	308	0.03%	0.004%
11	3.494	758	763	766	rBV2	195	210	0.02%	0.003%
12	3.545	776	779	782	rBV	297	210	0.02%	0.003%
13	3.873	872	881	911	rBV	74696	195121	21.09%	2.843%
14	4.349	1014	1029	1064	rBV	143149	364096	39.35%	5.306%
15	4.748	1149	1153	1158	rVB3	269	214	0.02%	0.003%
16	4.925	1205	1208	1211	rBV3	371	281	0.03%	0.004%
17	4.944	1212	1214	1218	rVB2	413	242	0.03%	0.004%
18	4.963	1218	1220	1223	rBV2	446	274	0.03%	0.004%
19	5.047	1229	1246	1275	rBV2	360917	925222	100.00%	13.483%
20	5.326	1330	1333	1336	rVB2	377	193	0.02%	0.003%
21	5.452	1369	1372	1373	rBV	377	166	0.02%	0.002%
22	5.555	1401	1404	1409	rBV2	335	279	0.03%	0.004%
23	5.619	1410	1424	1457	rBV	254764	528997	57.18%	7.709%
24	5.908	1504	1514	1525	rBV4	10001	20751	2.24%	0.302%
25	5.992	1537	1540	1546	rVB2	466	454	0.05%	0.007%
26	6.024	1546	1550	1551	rBV2	407	271	0.03%	0.004%
27	6.069	1551	1564	1595	rVV2	198569	417648	45.14%	6.086%
28	6.352	1650	1652	1655	rBV	363	266	0.03%	0.004%
29	6.449	1678	1682	1685	rBV	176	167	0.02%	0.002%
30	6.519	1700	1704	1705	rBV2	290	159	0.02%	0.002%
31	6.622	1733	1736	1739	rBV2	308	225	0.02%	0.003%
32	6.703	1759	1761	1765	rBV	253	206	0.02%	0.003%
33	6.760	1776	1779	1783	rBV2	288	189	0.02%	0.003%
34	6.989	1838	1850	1881	rBV	100980	188809	20.41%	2.751%
35	7.172	1905	1907	1909	rVB2	493	153	0.02%	0.002%
36	7.214	1917	1920	1922	rBV2	440	224	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
 Data File : VV022446.D
 Acq On : 30 Sep 2021 21:19
 Operator : SY/MD
 Sample : VV0930WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK268

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

37	7.317	1940	1952	1971	rBV	425779	736758	79.63%	10.737%
38	7.622	2037	2047	2074	rVV	70006	126349	13.66%	1.841%
39	7.796	2097	2101	2102	rBV2	393	243	0.03%	0.004%
40	7.876	2123	2126	2128	rBV	225	169	0.02%	0.002%
41	7.931	2139	2143	2147	rBV2	369	206	0.02%	0.003%
42	7.989	2152	2161	2167	rBV6	1622	2455	0.27%	0.036%
43	8.018	2167	2170	2173	rVB2	270	177	0.02%	0.003%
44	8.088	2180	2192	2230	rBV	215227	407826	44.08%	5.943%
45	8.381	2281	2283	2285	rBV2	295	193	0.02%	0.003%
46	8.468	2306	2310	2313	rBV2	377	349	0.04%	0.005%
47	8.510	2320	2323	2325	rVB2	384	234	0.03%	0.003%
48	8.616	2352	2356	2358	rBV2	338	287	0.03%	0.004%
49	8.651	2365	2367	2374	rBV3	388	326	0.04%	0.005%
50	8.757	2397	2400	2404	rBV2	324	233	0.03%	0.003%
51	8.854	2419	2430	2455	rBV	391266	640966	69.28%	9.341%
52	9.101	2502	2507	2510	rBV3	526	383	0.04%	0.006%
53	9.146	2516	2521	2523	rBV4	541	513	0.06%	0.007%
54	9.333	2577	2579	2582	rVB3	308	164	0.02%	0.002%
55	9.355	2582	2586	2590	rVB2	400	331	0.04%	0.005%
56	9.429	2607	2609	2613	rVB2	498	308	0.03%	0.004%
57	9.465	2613	2620	2623	rBV3	313	384	0.04%	0.006%
58	9.609	2662	2665	2668	rVB	307	154	0.02%	0.002%
59	9.641	2671	2675	2680	rVB3	187	182	0.02%	0.003%
60	9.764	2705	2713	2717	rBV	210	329	0.04%	0.005%
61	9.783	2717	2719	2721	rVV	343	156	0.02%	0.002%
62	9.963	2772	2775	2776	rBV	290	196	0.02%	0.003%
63	10.063	2802	2806	2809	rBV	283	262	0.03%	0.004%
64	10.120	2817	2824	2826	rBV3	1755	1518	0.16%	0.022%
65	10.217	2842	2854	2872	rBV	276855	439780	47.53%	6.409%
66	10.346	2892	2894	2896	rBV	562	185	0.02%	0.003%
67	10.542	2952	2955	2956	rBV	356	158	0.02%	0.002%
68	10.612	2972	2977	2978	rBV2	451	321	0.03%	0.005%
69	10.718	3007	3010	3012	rBV	285	193	0.02%	0.003%
70	10.956	3082	3084	3088	rVB2	221	162	0.02%	0.002%
71	11.079	3119	3122	3130	rVB3	520	400	0.04%	0.006%
72	11.114	3130	3133	3136	rBV	292	213	0.02%	0.003%
73	11.130	3136	3138	3141	rBV3	325	186	0.02%	0.003%
74	11.149	3141	3144	3149	rVB4	825	663	0.07%	0.010%
75	11.181	3152	3154	3156	rBV	423	266	0.03%	0.004%
76	11.249	3164	3175	3197	rBV	355161	563877	60.95%	8.217%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
 Data File : VV022446.D
 Acq On : 30 Sep 2021 21:19
 Operator : SY/MD
 Sample : VV0930WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK268

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

77	11.381	3213	3216	3217	rBV3	654	379	0.04%	0.006%
78	11.481	3245	3247	3250	rVB2	310	156	0.02%	0.002%
79	11.545	3263	3267	3272	rBV3	537	521	0.06%	0.008%
80	11.625	3281	3292	3321	rBV	406735	641389	69.32%	9.347%
81	11.780	3338	3340	3342	rBV	506	297	0.03%	0.004%
82	11.870	3362	3368	3369	rBV4	472	463	0.05%	0.007%
83	12.066	3426	3429	3431	rBV3	301	155	0.02%	0.002%
84	12.593	3591	3593	3596	rVB2	479	237	0.03%	0.003%
85	12.654	3606	3612	3613	rBV3	351	287	0.03%	0.004%
86	12.995	3716	3718	3722	rVB2	350	216	0.02%	0.003%
87	13.278	3801	3806	3811	rVB3	580	647	0.07%	0.009%
88	13.313	3811	3817	3819	rBV	194	225	0.02%	0.003%
89	13.352	3826	3829	3831	rBV	365	251	0.03%	0.004%
90	13.416	3847	3849	3851	rBV2	344	200	0.02%	0.003%
91	13.429	3851	3853	3856	rVB2	342	166	0.02%	0.002%
92	13.606	3906	3908	3911	rVB2	341	189	0.02%	0.003%
93	13.622	3911	3913	3916	rBV2	402	217	0.02%	0.003%
94	13.667	3925	3927	3932	rVB2	256	178	0.02%	0.003%
95	13.699	3932	3937	3940	rBV2	287	387	0.04%	0.006%
96	13.789	3962	3965	3966	rBV	494	178	0.02%	0.003%
97	13.976	4021	4023	4026	rVB	329	188	0.02%	0.003%
98	14.532	4192	4196	4198	rBV3	352	265	0.03%	0.004%
99	14.680	4239	4242	4245	rBV3	333	261	0.03%	0.004%
100	15.670	4548	4550	4552	rBV	705	368	0.04%	0.005%




Sum of corrected areas: 6862157

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
Data File : VV022446.D
Acq On : 30 Sep 2021 21:19
Operator : SY/MD
Sample : VV0930WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK268

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

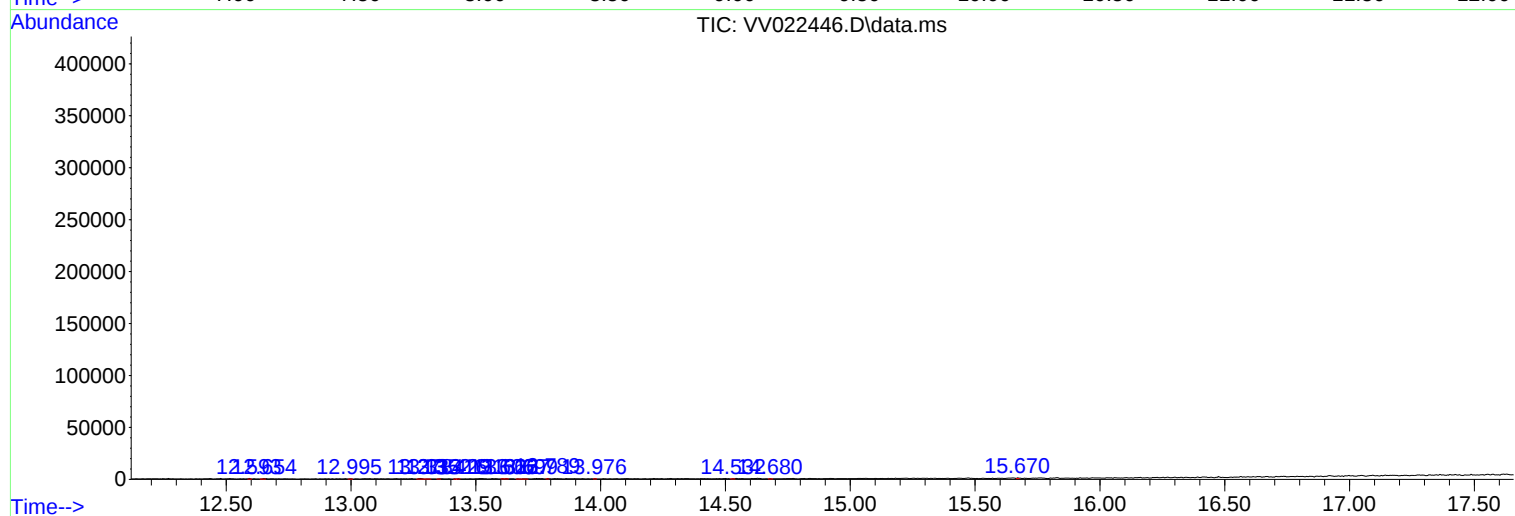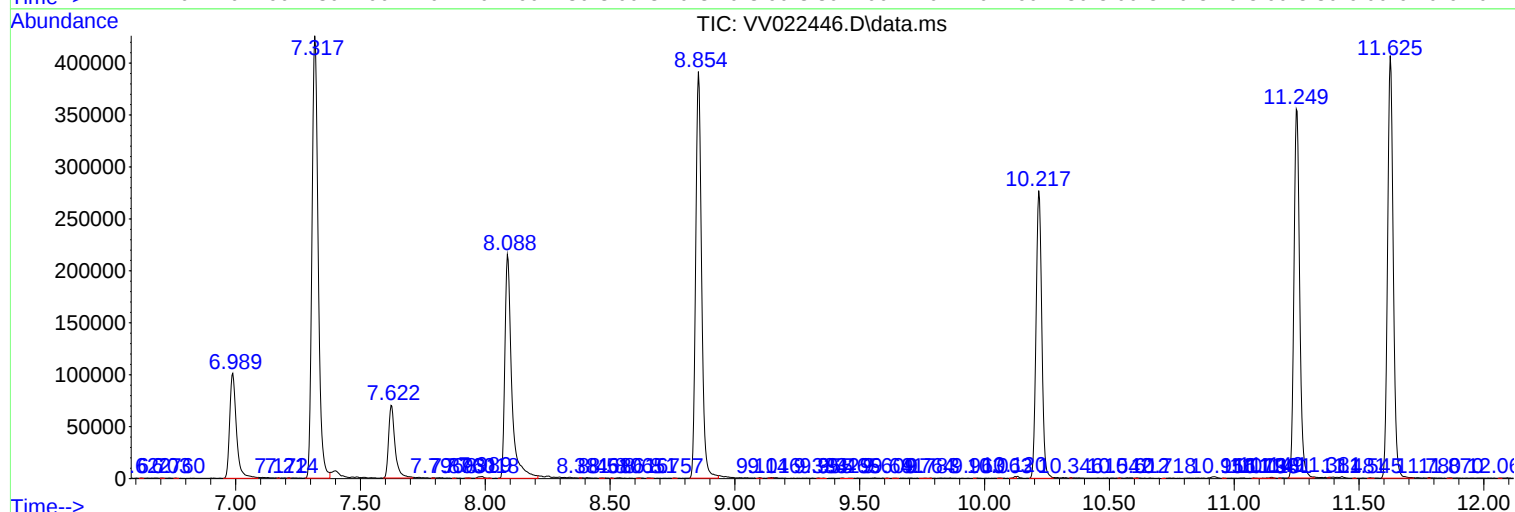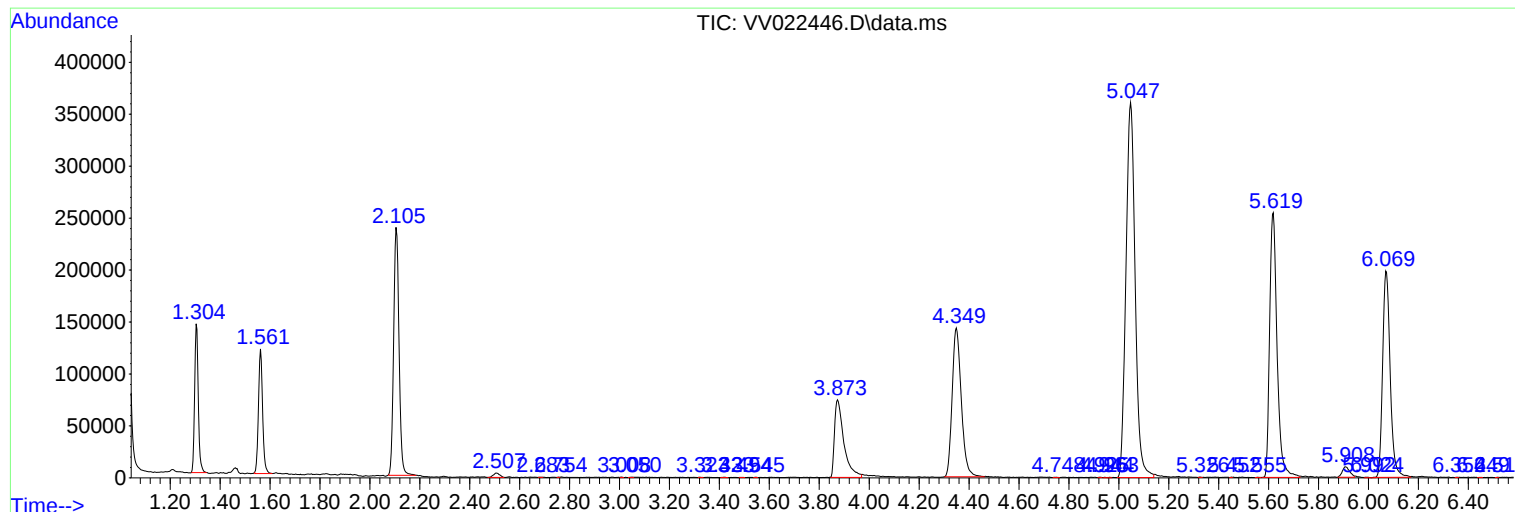

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
Data File : VV022446.D
Acq On : 30 Sep 2021 21:19
Operator : SY/MD
Sample : VV0930WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK268

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
Data File : VV022446.D
Acq On : 30 Sep 2021 21:19
Operator : SY/MD
Sample : VV0930WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK268

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
