

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
 Data File : VV022448.D
 Acq On : 30 Sep 2021 22:07
 Operator : SY/MD
 Sample : M3979-01DL 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A26DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M

Title : VOC Analysis

Signal : TIC: VV022448.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	97	rVB	142778	142720	15.25%	1.939%
2	1.564	156	163	175	rBV	116303	130132	13.91%	1.768%
3	2.105	321	331	345	rBV	232653	335435	35.84%	4.557%
4	2.510	447	457	465	rBV3	7803	12986	1.39%	0.176%
5	2.574	475	477	480	rBV	289	157	0.02%	0.002%
6	2.658	500	503	504	rBV	283	141	0.02%	0.002%
7	2.770	530	538	546	rBV7	1746	3228	0.34%	0.044%
8	2.960	592	597	599	rBV4	380	278	0.03%	0.004%
9	3.223	676	679	682	rBV	230	132	0.01%	0.002%
10	3.275	694	695	699	rBV2	258	161	0.02%	0.002%
11	3.387	728	730	734	rBV2	223	147	0.02%	0.002%
12	3.619	800	802	803	rBV2	265	127	0.01%	0.002%
13	3.661	813	815	818	rBV	206	135	0.01%	0.002%
14	3.680	818	821	831	rVB3	358	378	0.04%	0.005%
15	3.751	840	843	850	rBB	282	168	0.02%	0.002%
16	3.908	880	892	939	rBV	50771	212981	22.76%	2.893%
17	4.349	1013	1029	1069	rBV	145208	372335	39.79%	5.058%
18	4.786	1162	1165	1170	rBV2	257	275	0.03%	0.004%
19	4.831	1176	1179	1181	rBV2	249	154	0.02%	0.002%
20	4.895	1197	1199	1202	rBV	266	182	0.02%	0.002%
21	4.979	1222	1225	1230	rVB3	341	253	0.03%	0.003%
22	5.047	1230	1246	1277	rBV2	367620	935814	100.00%	12.713%
23	5.503	1386	1388	1391	rBV2	282	158	0.02%	0.002%
24	5.619	1410	1424	1454	rBV	260108	540051	57.71%	7.337%
25	5.908	1505	1514	1530	rVB6	10890	23434	2.50%	0.318%
26	5.989	1536	1539	1543	rBV2	375	290	0.03%	0.004%
27	6.072	1552	1565	1590	rBV	201238	417314	44.59%	5.669%
28	6.365	1650	1656	1657	rBV	253	215	0.02%	0.003%
29	6.538	1706	1710	1713	rVB2	272	199	0.02%	0.003%
30	6.580	1721	1723	1726	rBV2	244	130	0.01%	0.002%
31	6.628	1735	1738	1741	rBV2	345	288	0.03%	0.004%
32	6.731	1767	1770	1776	rBV3	266	242	0.03%	0.003%
33	6.780	1782	1785	1788	rBV2	410	202	0.02%	0.003%
34	6.873	1811	1814	1816	rVB2	339	176	0.02%	0.002%
35	6.915	1824	1827	1829	rBV3	260	163	0.02%	0.002%
36	6.989	1838	1850	1878	rBV	98828	189036	20.20%	2.568%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
 Data File : VV022448.D
 Acq On : 30 Sep 2021 22:07
 Operator : SY/MD
 Sample : M3979-01DL 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A26DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

37	7.317	1940	1952	1971	rBV	420337	736720	78.73%	10.009%
38	7.625	2038	2048	2066	rBV2	70687	124920	13.35%	1.697%
39	7.924	2138	2141	2143	rBV2	260	188	0.02%	0.003%
40	7.976	2145	2157	2176	rVV	263665	441815	47.21%	6.002%
41	8.095	2184	2194	2229	rBV	215821	421710	45.06%	5.729%
42	8.368	2277	2279	2282	rBV	402	156	0.02%	0.002%
43	8.410	2288	2292	2298	rBV4	456	531	0.06%	0.007%
44	8.509	2320	2323	2325	rBV2	336	187	0.02%	0.003%
45	8.587	2345	2347	2348	rBV	302	126	0.01%	0.002%
46	8.635	2358	2362	2364	rBV3	415	307	0.03%	0.004%
47	8.664	2369	2371	2373	rBV	365	215	0.02%	0.003%
48	8.783	2403	2408	2412	rBV2	443	399	0.04%	0.005%
49	8.815	2416	2418	2419	rBV3	333	169	0.02%	0.002%
50	8.853	2419	2430	2453	rBV	391996	650300	69.49%	8.835%
51	9.088	2500	2503	2504	rBV3	298	177	0.02%	0.002%
52	9.149	2518	2522	2531	rVV4	568	737	0.08%	0.010%
53	9.207	2538	2540	2544	rVB2	449	248	0.03%	0.003%
54	9.262	2556	2557	2561	rBV2	234	130	0.01%	0.002%
55	9.416	2602	2605	2609	rBV3	202	167	0.02%	0.002%
56	9.493	2625	2629	2631	rBV2	269	235	0.03%	0.003%
57	9.673	2683	2685	2690	rBV3	432	344	0.04%	0.005%
58	9.731	2701	2703	2707	rVB2	299	155	0.02%	0.002%
59	9.751	2707	2709	2713	rBV2	289	160	0.02%	0.002%
60	9.911	2757	2759	2761	rVB	289	133	0.01%	0.002%
61	9.950	2766	2771	2773	rBV3	308	265	0.03%	0.004%
62	10.072	2807	2809	2812	rVB2	385	137	0.01%	0.002%
63	10.133	2819	2828	2832	rBV4	1469	2078	0.22%	0.028%
64	10.217	2843	2854	2874	rBV	274874	438636	46.87%	5.959%
65	10.365	2895	2900	2903	rBV3	450	394	0.04%	0.005%
66	10.381	2903	2905	2909	rVV3	307	206	0.02%	0.003%
67	10.426	2914	2919	2922	rVB3	367	311	0.03%	0.004%
68	10.455	2926	2928	2930	rVB	337	123	0.01%	0.002%
69	10.468	2930	2932	2935	rBV3	411	301	0.03%	0.004%
70	10.567	2960	2963	2964	rBV	502	253	0.03%	0.003%
71	10.709	3004	3007	3008	rVV	215	126	0.01%	0.002%
72	10.776	3024	3028	3032	rBV2	402	372	0.04%	0.005%
73	10.921	3066	3073	3078	rBV4	1645	1975	0.21%	0.027%
74	11.133	3138	3139	3140	rBV4	354	132	0.01%	0.002%
75	11.181	3151	3154	3157	rVB	440	274	0.03%	0.004%
76	11.197	3157	3159	3162	rBV	410	243	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
 Data File : VV022448.D
 Acq On : 30 Sep 2021 22:07
 Operator : SY/MD
 Sample : M3979-01DL 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A26DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M

Title : VOC Analysis

77	11.252	3164	3176	3199	rBV	359312	570577	60.97%	7.752%
78	11.390	3215	3219	3222	rBV5	602	572	0.06%	0.008%
79	11.519	3256	3259	3265	rVB3	418	359	0.04%	0.005%
80	11.625	3281	3292	3310	rBV	396960	636787	68.05%	8.651%
81	11.808	3346	3349	3353	rBV2	341	248	0.03%	0.003%
82	11.860	3360	3365	3367	rBV2	587	465	0.05%	0.006%
83	11.911	3378	3381	3384	rBV	298	186	0.02%	0.003%
84	12.098	3435	3439	3447	rVB3	711	882	0.09%	0.012%
85	12.165	3456	3460	3465	rBV2	449	568	0.06%	0.008%
86	12.213	3471	3475	3477	rBV	379	274	0.03%	0.004%
87	12.255	3485	3488	3491	rVB	350	207	0.02%	0.003%
88	12.281	3495	3496	3499	rBV	237	151	0.02%	0.002%
89	12.307	3502	3504	3506	rBV	423	275	0.03%	0.004%
90	12.474	3551	3556	3560	rVB3	571	510	0.05%	0.007%
91	12.493	3560	3562	3563	rBV	371	176	0.02%	0.002%
92	12.885	3681	3684	3685	rBV	308	169	0.02%	0.002%
93	13.213	3783	3786	3789	rVB3	488	307	0.03%	0.004%
94	13.278	3804	3806	3810	rVB	295	150	0.02%	0.002%
95	13.429	3848	3853	3858	rBV3	529	539	0.06%	0.007%
96	13.506	3875	3877	3879	rBV	397	136	0.01%	0.002%
97	13.744	3946	3951	3952	rBV2	312	258	0.03%	0.004%
98	13.950	4013	4015	4017	rBV2	413	176	0.02%	0.002%
99	14.040	4040	4043	4044	rBV2	413	240	0.03%	0.003%
100	14.493	4181	4184	4188	rBV2	326	324	0.03%	0.004%




Sum of corrected areas: 7360808

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
Data File : VV022448.D
Acq On : 30 Sep 2021 22:07
Operator : SY/MD
Sample : M3979-01DL 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
F4A26DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

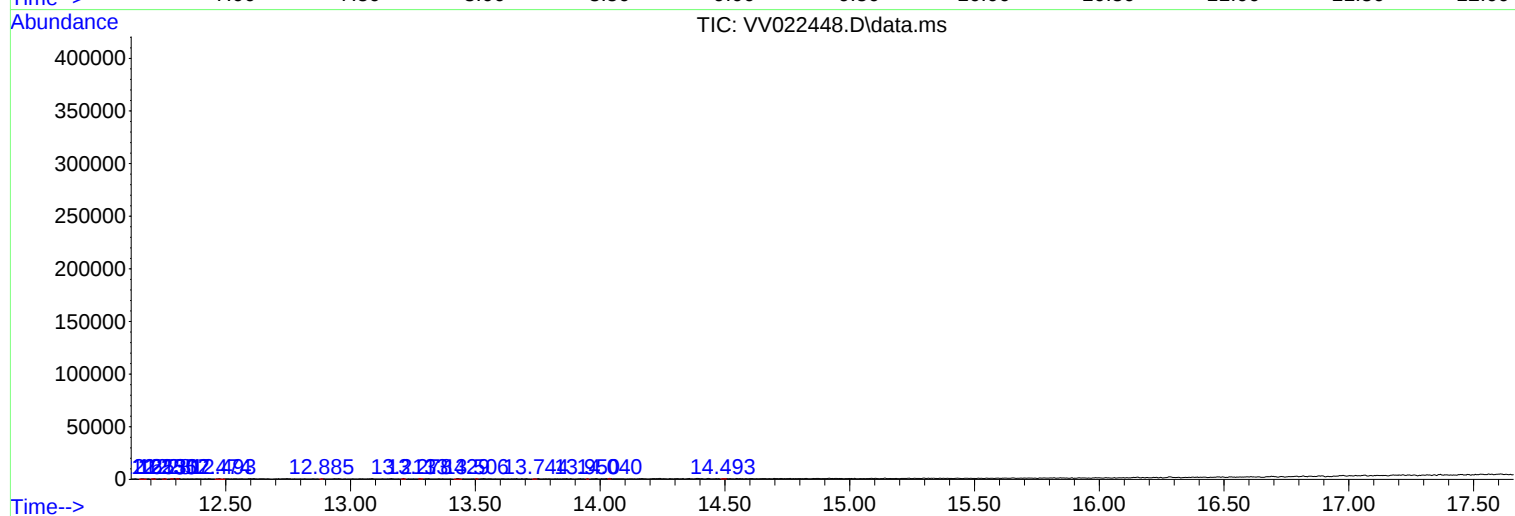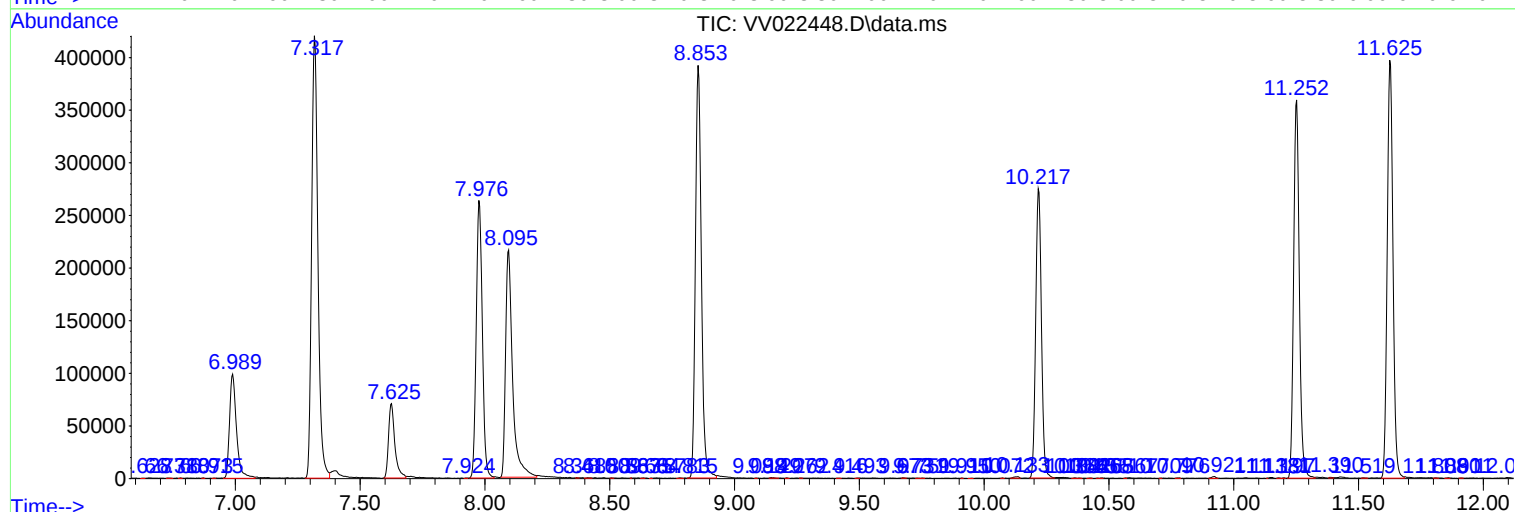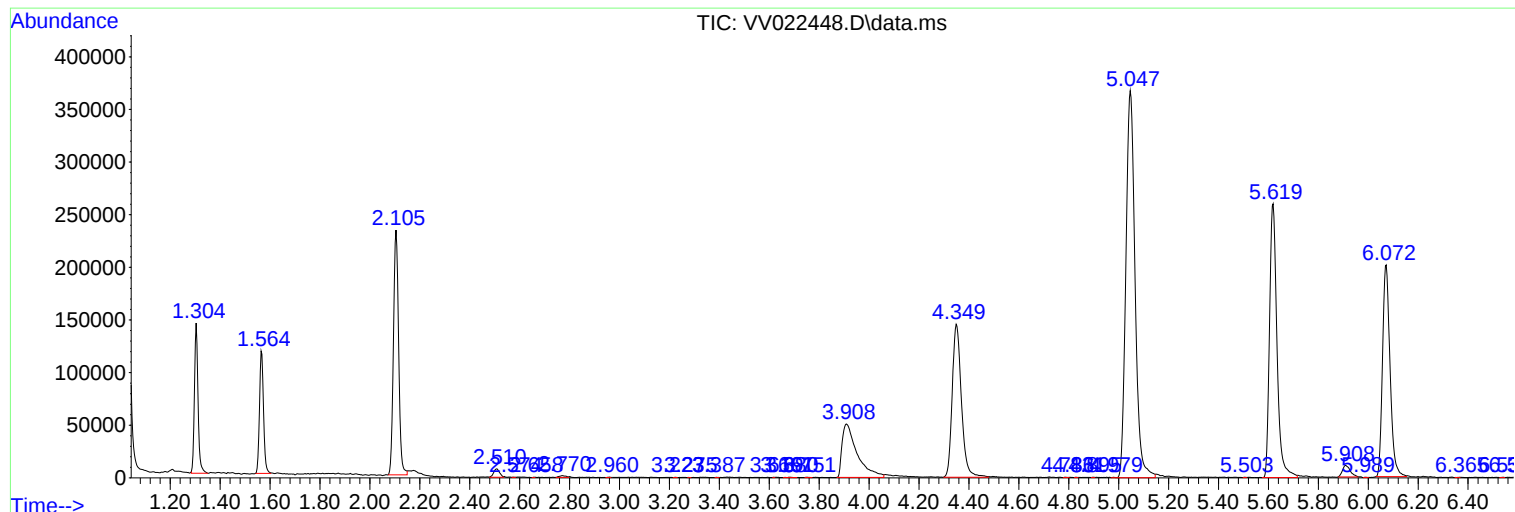

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
Data File : VV022448.D
Acq On : 30 Sep 2021 22:07
Operator : SY/MD
Sample : M3979-01DL 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A26DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
Data File : VV022448.D
Acq On : 30 Sep 2021 22:07
Operator : SY/MD
Sample : M3979-01DL 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A26DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
