

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
 Data File : VV022456.D
 Acq On : 01 Oct 2021 01:18
 Operator : SY/MD
 Sample : M3979-21
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M

Title : VOC Analysis

Signal : TIC: VV022456.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	96	rVB	142905	145841	16.03%	2.178%
2	1.561	155	162	175	rVB	119282	132698	14.58%	1.982%
3	2.105	322	331	360	rVB	236137	348377	38.29%	5.203%
4	2.510	450	457	471	rVB	4483	7322	0.80%	0.109%
5	2.629	492	494	498	rVB	425	270	0.03%	0.004%
6	2.716	519	521	523	rBV	322	141	0.02%	0.002%
7	2.767	536	537	543	rVV	386	285	0.03%	0.004%
8	3.089	632	637	640	rBV2	360	293	0.03%	0.004%
9	3.192	666	669	670	rBV3	489	237	0.03%	0.004%
10	3.417	736	739	742	rVB2	277	139	0.02%	0.002%
11	3.462	749	753	757	rVB2	269	201	0.02%	0.003%
12	3.494	760	763	766	rBV	456	235	0.03%	0.004%
13	3.786	851	854	860	rVB2	348	199	0.02%	0.003%
14	3.876	873	882	913	rBV	74121	198633	21.83%	2.967%
15	4.195	979	981	982	rBV	404	180	0.02%	0.003%
16	4.349	1014	1029	1055	rBV2	139873	357482	39.29%	5.339%
17	4.542	1087	1089	1094	rBV2	421	395	0.04%	0.006%
18	4.568	1095	1097	1100	rVB2	469	203	0.02%	0.003%
19	4.616	1110	1112	1121	rVB4	922	749	0.08%	0.011%
20	4.835	1178	1180	1183	rBV	233	146	0.02%	0.002%
21	4.976	1220	1224	1226	rBV3	387	295	0.03%	0.004%
22	5.047	1230	1246	1286	rVV2	354227	909947	100.00%	13.590%
23	5.365	1343	1345	1348	rBV2	336	214	0.02%	0.003%
24	5.404	1354	1357	1362	rBV4	462	316	0.03%	0.005%
25	5.478	1377	1380	1382	rBV3	407	214	0.02%	0.003%
26	5.542	1398	1400	1402	rBV3	317	187	0.02%	0.003%
27	5.619	1412	1424	1449	rBV	247342	510301	56.08%	7.621%
28	5.912	1504	1515	1534	rVB3	10065	23245	2.55%	0.347%
29	5.982	1534	1537	1539	rBV	437	257	0.03%	0.004%
30	6.069	1550	1564	1590	rBV	197508	412411	45.32%	6.159%
31	6.252	1619	1621	1624	rVB	445	204	0.02%	0.003%
32	6.384	1660	1662	1667	rVB	457	241	0.03%	0.004%
33	6.429	1671	1676	1677	rBV	240	220	0.02%	0.003%
34	6.497	1695	1697	1703	rVB2	298	268	0.03%	0.004%
35	6.677	1749	1753	1754	rBV2	680	317	0.03%	0.005%
36	6.989	1838	1850	1871	rBV2	96424	178239	19.59%	2.662%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
 Data File : VV022456.D
 Acq On : 01 Oct 2021 01:18
 Operator : SY/MD
 Sample : M3979-21
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

37	7.207	1915	1918	1919	rBV	504	246	0.03%	0.004%
38	7.317	1940	1952	1971	rBV	413584	720632	79.19%	10.762%
39	7.625	2035	2048	2074	rBV	67410	121503	13.35%	1.815%
40	7.828	2109	2111	2115	rVB2	518	189	0.02%	0.003%
41	7.892	2129	2131	2134	rBV2	541	293	0.03%	0.004%
42	7.918	2137	2139	2141	rVB2	394	153	0.02%	0.002%
43	7.937	2142	2145	2146	rBV2	373	194	0.02%	0.003%
44	7.982	2154	2159	2168	rVB7	1221	1682	0.18%	0.025%
45	8.092	2182	2193	2222	rBV	213525	405818	44.60%	6.061%
46	8.442	2300	2302	2304	rBV	476	199	0.02%	0.003%
47	8.519	2324	2326	2329	rBV2	334	154	0.02%	0.002%
48	8.619	2355	2357	2358	rBV	327	145	0.02%	0.002%
49	8.677	2370	2375	2379	rBV2	400	446	0.05%	0.007%
50	8.728	2388	2391	2393	rBV	439	192	0.02%	0.003%
51	8.812	2415	2417	2419	rBV	401	179	0.02%	0.003%
52	8.854	2419	2430	2451	rBV	375992	613265	67.40%	9.159%
53	9.011	2477	2479	2480	rBV	494	204	0.02%	0.003%
54	9.111	2507	2510	2511	rBV	306	163	0.02%	0.002%
55	9.140	2517	2519	2521	rBV2	507	257	0.03%	0.004%
56	9.256	2552	2555	2557	rBV2	333	159	0.02%	0.002%
57	9.281	2560	2563	2565	rBV	271	215	0.02%	0.003%
58	9.333	2577	2579	2582	rBV2	298	152	0.02%	0.002%
59	9.448	2613	2615	2618	rBV	292	197	0.02%	0.003%
60	9.555	2646	2648	2653	rVB4	549	348	0.04%	0.005%
61	9.680	2685	2687	2690	rBV	432	223	0.02%	0.003%
62	9.744	2705	2707	2711	rVB2	286	168	0.02%	0.003%
63	10.005	2786	2788	2792	rVB	355	195	0.02%	0.003%
64	10.037	2796	2798	2806	rVV3	336	343	0.04%	0.005%
65	10.098	2814	2817	2820	rVB	399	233	0.03%	0.003%
66	10.127	2820	2826	2836	rVB5	1602	2387	0.26%	0.036%
67	10.217	2839	2854	2873	rBV	268527	429306	47.18%	6.412%
68	10.439	2921	2923	2924	rBV2	245	136	0.01%	0.002%
69	10.661	2990	2992	2995	rBV2	406	229	0.03%	0.003%
70	10.812	3036	3039	3043	rVV3	188	174	0.02%	0.003%
71	10.860	3050	3054	3055	rBV	292	153	0.02%	0.002%
72	10.915	3063	3071	3081	rBV6	1412	2446	0.27%	0.037%
73	10.979	3089	3091	3093	rBV	426	183	0.02%	0.003%
74	11.146	3138	3143	3152	rVB4	735	869	0.10%	0.013%
75	11.252	3163	3176	3202	rBV	334139	534439	58.73%	7.982%
76	11.387	3213	3218	3225	rVB5	960	1282	0.14%	0.019%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
 Data File : VV022456.D
 Acq On : 01 Oct 2021 01:18
 Operator : SY/MD
 Sample : M3979-21
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

77	11.416	3225	3227	3228	rBV	564	239	0.03%	0.004%
78	11.625	3280	3292	3311	rBV	388650	619418	68.07%	9.251%
79	11.908	3377	3380	3383	rBV3	251	191	0.02%	0.003%
80	11.927	3383	3386	3392	rVV	308	304	0.03%	0.005%
81	11.956	3392	3395	3398	rBV	386	260	0.03%	0.004%
82	12.098	3435	3439	3443	rBV3	292	251	0.03%	0.004%
83	12.223	3475	3478	3481	rBV2	400	246	0.03%	0.004%
84	12.294	3496	3500	3505	rBV3	317	340	0.04%	0.005%
85	12.458	3549	3551	3552	rBV	380	156	0.02%	0.002%
86	12.590	3588	3592	3596	rBV3	283	258	0.03%	0.004%
87	12.670	3612	3617	3618	rBV	300	233	0.03%	0.003%
88	12.693	3622	3624	3626	rBV3	315	202	0.02%	0.003%
89	12.808	3656	3660	3665	rBV3	320	353	0.04%	0.005%
90	12.889	3682	3685	3690	rBV2	355	248	0.03%	0.004%
91	13.072	3740	3742	3746	rBV3	384	262	0.03%	0.004%
92	13.333	3821	3823	3825	rBV	256	170	0.02%	0.003%
93	13.442	3854	3857	3859	rBV	257	161	0.02%	0.002%
94	13.464	3861	3864	3868	rBV	453	275	0.03%	0.004%
95	13.554	3889	3892	3897	rBV2	542	451	0.05%	0.007%
96	13.911	4001	4003	4010	rVB2	261	160	0.02%	0.002%
97	14.214	4096	4097	4100	rBV2	344	239	0.03%	0.004%
98	14.387	4148	4151	4155	rBV2	302	255	0.03%	0.004%
99	14.439	4163	4167	4168	rBV	392	259	0.03%	0.004%
100	15.805	4590	4592	4593	rBV	605	273	0.03%	0.004%


Sum of corrected areas: 6695857

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
Data File : VV022456.D
Acq On : 01 Oct 2021 01:18
Operator : SY/MD
Sample : M3979-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

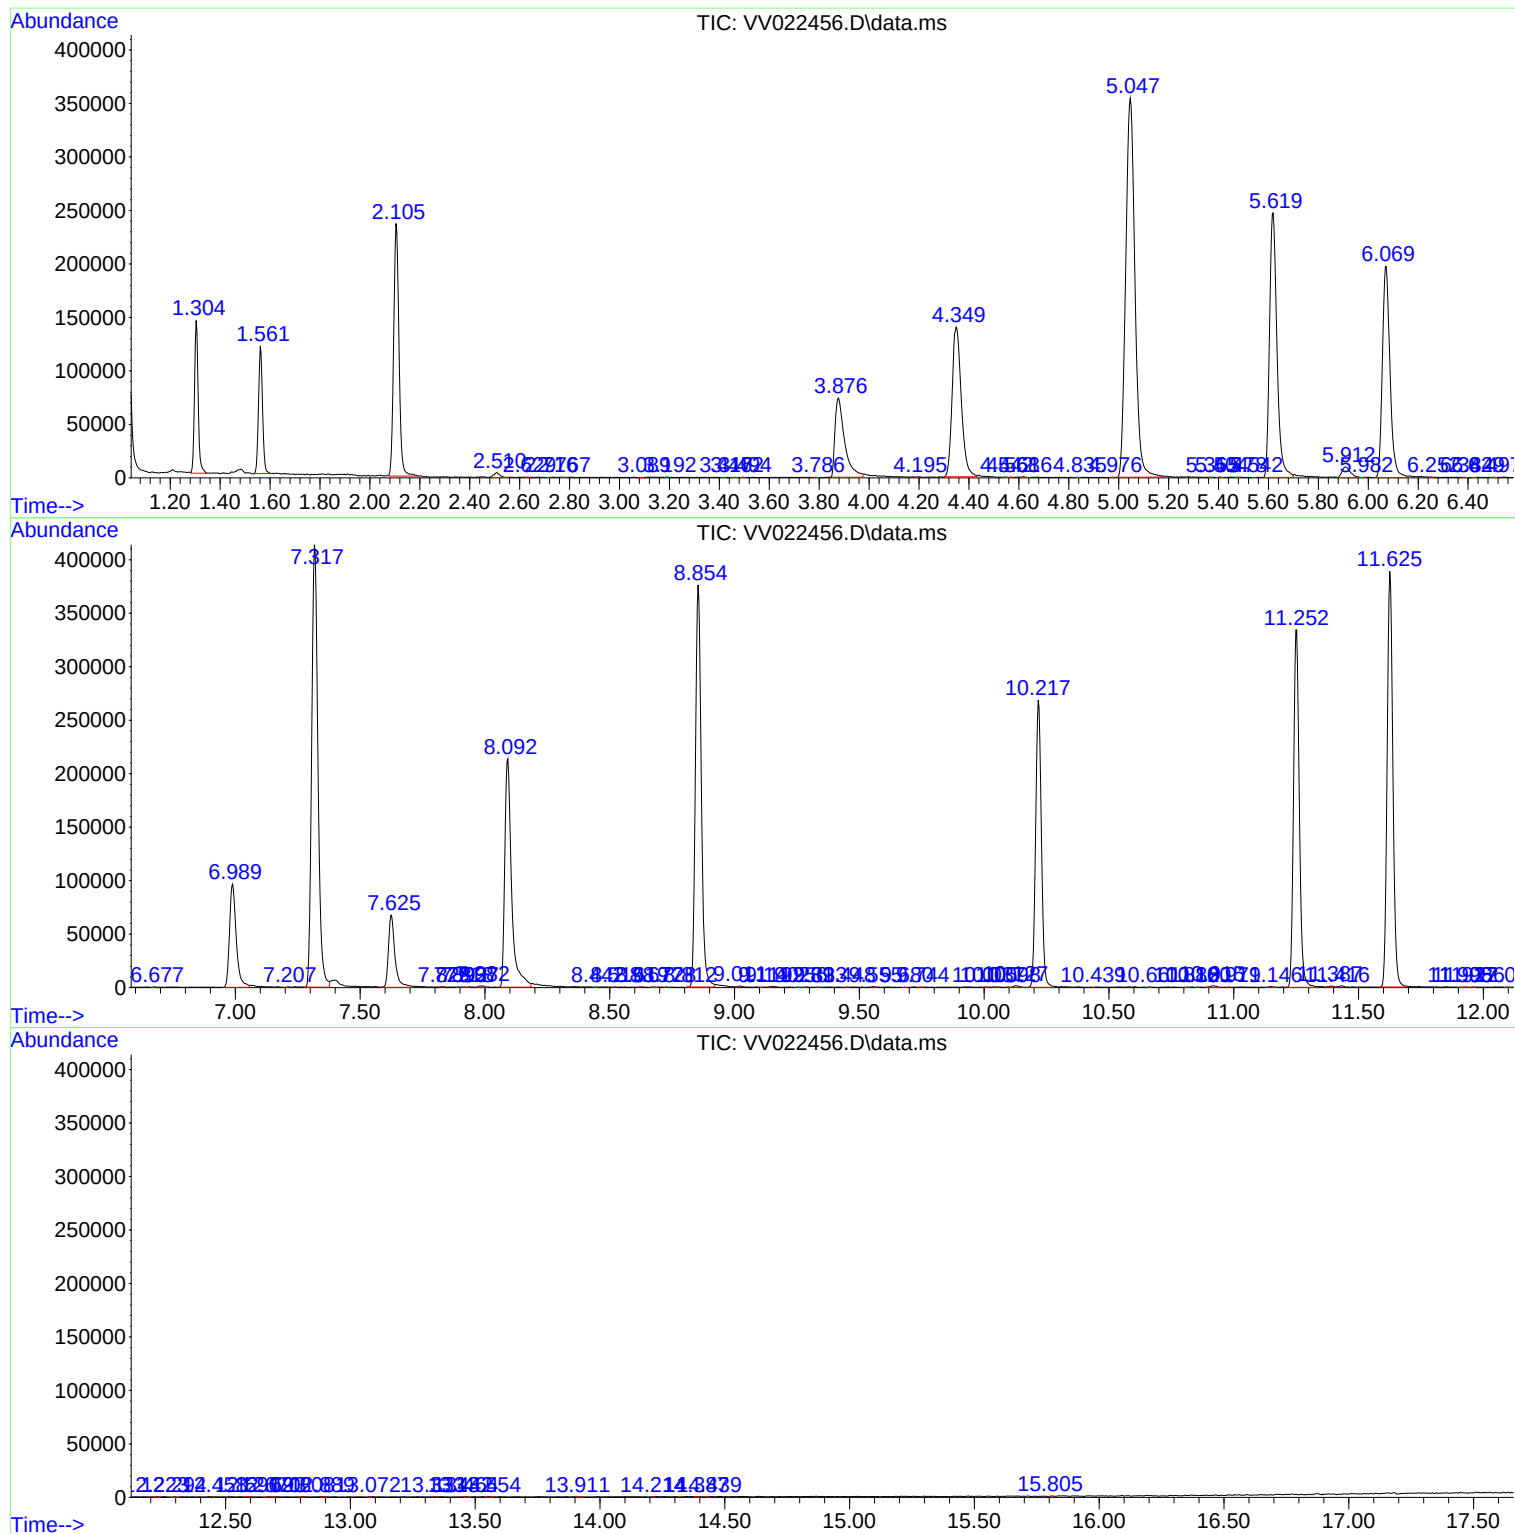

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
Data File : VV022456.D
Acq On : 01 Oct 2021 01:18
Operator : SY/MD
Sample : M3979-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
Data File : VV022456.D
Acq On : 01 Oct 2021 01:18
Operator : SY/MD
Sample : M3979-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
