

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
 Data File : VV022457.D
 Acq On : 01 Oct 2021 01:42
 Operator : SY/MD
 Sample : M3978-21
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M

Title : VOC Analysis

Signal : TIC: VV022457.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	97	rVB	137435	139300	15.63%	2.124%
2	1.561	155	162	176	rVB	114253	130002	14.59%	1.982%
3	2.105	321	331	344	rBV	226399	331894	37.24%	5.060%
4	2.378	414	416	422	rBV4	360	263	0.03%	0.004%
5	2.510	448	457	469	rVB3	4235	7626	0.86%	0.116%
6	2.564	472	474	477	rVB3	384	209	0.02%	0.003%
7	2.761	531	535	539	rBV2	575	477	0.05%	0.007%
8	2.857	563	565	569	rVB2	415	184	0.02%	0.003%
9	3.008	608	612	613	rBV	334	199	0.02%	0.003%
10	3.124	642	648	649	rBV	324	231	0.03%	0.004%
11	3.134	649	651	654	rVV2	308	163	0.02%	0.002%
12	3.156	654	658	662	rVV2	284	248	0.03%	0.004%
13	3.317	706	708	711	rVB2	434	241	0.03%	0.004%
14	3.552	780	781	785	rVB	328	157	0.02%	0.002%
15	3.574	785	788	792	rBV	269	211	0.02%	0.003%
16	3.619	799	802	804	rBV2	398	163	0.02%	0.002%
17	3.635	804	807	811	rVB2	313	216	0.02%	0.003%
18	3.802	856	859	862	rVB2	312	130	0.01%	0.002%
19	3.876	872	882	912	rBV	74001	194568	21.83%	2.966%
20	4.281	1006	1008	1010	rBV2	430	212	0.02%	0.003%
21	4.349	1013	1029	1067	rVV	136263	352034	39.50%	5.367%
22	4.587	1100	1103	1105	rBV	413	240	0.03%	0.004%
23	4.616	1110	1112	1115	rBV	264	193	0.02%	0.003%
24	4.677	1128	1131	1135	rBV3	458	298	0.03%	0.005%
25	4.699	1135	1138	1139	rVB	371	198	0.02%	0.003%
26	4.841	1179	1182	1183	rBV	309	174	0.02%	0.003%
27	5.047	1230	1246	1280	rBV2	343027	891200	100.00%	13.587%
28	5.529	1393	1396	1399	rBV2	349	231	0.03%	0.004%
29	5.574	1407	1410	1411	rBV	372	183	0.02%	0.003%
30	5.619	1412	1424	1454	rVV	240304	492926	55.31%	7.515%
31	5.908	1504	1514	1538	rVB4	10680	23704	2.66%	0.361%
32	6.069	1551	1564	1593	rBV	195285	402837	45.20%	6.141%
33	6.368	1655	1657	1661	rVB	343	214	0.02%	0.003%
34	6.445	1677	1681	1683	rBV2	373	312	0.04%	0.005%
35	6.635	1737	1740	1741	rBV2	343	216	0.02%	0.003%
36	6.674	1748	1752	1756	rBV3	391	368	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
 Data File : VV022457.D
 Acq On : 01 Oct 2021 01:42
 Operator : SY/MD
 Sample : M3978-21
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

37	6.989	1839	1850	1879	rBV	93460	176209	19.77%	2.686%
38	7.317	1940	1952	1971	rBV	395691	699655	78.51%	10.666%
39	7.584	2033	2035	2038	rVB	442	217	0.02%	0.003%
40	7.622	2038	2047	2075	rBV	64921	117568	13.19%	1.792%
41	7.831	2110	2112	2118	rVB3	376	282	0.03%	0.004%
42	7.886	2126	2129	2130	rBV2	320	148	0.02%	0.002%
43	7.918	2136	2139	2142	rBV	306	179	0.02%	0.003%
44	7.982	2153	2159	2165	rBV4	1180	1580	0.18%	0.024%
45	8.088	2182	2192	2227	rBV	216953	411944	46.22%	6.280%
46	8.429	2296	2298	2300	rBV2	398	196	0.02%	0.003%
47	8.526	2325	2328	2331	rBV2	499	315	0.04%	0.005%
48	8.709	2382	2385	2390	rVB4	331	247	0.03%	0.004%
49	8.754	2397	2399	2402	rBV2	373	183	0.02%	0.003%
50	8.773	2402	2405	2408	rVV	243	149	0.02%	0.002%
51	8.854	2419	2430	2456	rBV	368109	603050	67.67%	9.194%
52	9.021	2480	2482	2487	rVB3	536	359	0.04%	0.005%
53	9.066	2494	2496	2499	rVB	451	250	0.03%	0.004%
54	9.124	2513	2514	2518	rBV2	343	225	0.03%	0.003%
55	9.239	2547	2550	2552	rBV2	265	187	0.02%	0.003%
56	9.342	2580	2582	2586	rBV	263	129	0.01%	0.002%
57	9.362	2586	2588	2590	rVB	236	130	0.01%	0.002%
58	9.439	2610	2612	2617	rVB2	404	289	0.03%	0.004%
59	9.477	2617	2624	2627	rBV3	344	411	0.05%	0.006%
60	9.690	2688	2690	2692	rBV	301	147	0.02%	0.002%
61	9.799	2722	2724	2729	rVB2	209	131	0.01%	0.002%
62	9.876	2746	2748	2749	rBV2	297	141	0.02%	0.002%
63	9.902	2753	2756	2758	rVB	483	236	0.03%	0.004%
64	9.985	2779	2782	2786	rVB2	394	239	0.03%	0.004%
65	10.037	2794	2798	2800	rBV2	390	305	0.03%	0.005%
66	10.072	2806	2809	2813	rBV3	298	214	0.02%	0.003%
67	10.130	2817	2827	2836	rVB4	1558	2480	0.28%	0.038%
68	10.217	2842	2854	2875	rBV	268126	426419	47.85%	6.501%
69	10.416	2913	2916	2922	rBV3	293	200	0.02%	0.003%
70	10.477	2933	2935	2941	rVB2	338	278	0.03%	0.004%
71	10.709	3005	3007	3014	rVB2	324	261	0.03%	0.004%
72	10.741	3014	3017	3018	rBV	347	176	0.02%	0.003%
73	10.924	3066	3074	3081	rVB5	1476	2428	0.27%	0.037%
74	10.985	3088	3093	3095	rBV2	208	201	0.02%	0.003%
75	11.046	3108	3112	3120	rVB3	579	543	0.06%	0.008%
76	11.075	3120	3121	3126	rBV2	343	195	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
 Data File : VV022457.D
 Acq On : 01 Oct 2021 01:42
 Operator : SY/MD
 Sample : M3978-21
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

77	11.124	3133	3136	3139	rBV	350	167	0.02%	0.003%
78	11.149	3139	3144	3152	rVB4	810	894	0.10%	0.014%
79	11.185	3152	3155	3162	rBV2	287	344	0.04%	0.005%
80	11.252	3165	3176	3196	rBV	330414	519208	58.26%	7.915%
81	11.426	3226	3230	3238	rVB7	1306	1765	0.20%	0.027%
82	11.458	3238	3240	3245	rBV2	506	275	0.03%	0.004%
83	11.522	3257	3260	3262	rBV3	496	286	0.03%	0.004%
84	11.625	3280	3292	3313	rBV	385206	608550	68.28%	9.277%
85	11.960	3393	3396	3400	rBV	6062	3599	0.40%	0.055%
86	12.220	3475	3477	3481	rVB2	509	280	0.03%	0.004%
87	12.243	3481	3484	3487	rBV2	209	152	0.02%	0.002%
88	12.503	3561	3565	3569	rVB3	354	278	0.03%	0.004%
89	12.522	3569	3571	3574	rBV2	264	159	0.02%	0.002%
90	12.802	3655	3658	3664	rBV3	351	324	0.04%	0.005%
91	13.059	3735	3738	3740	rBV	280	208	0.02%	0.003%
92	13.143	3761	3764	3767	rBV2	270	174	0.02%	0.003%
93	13.500	3873	3875	3879	rVB2	366	148	0.02%	0.002%
94	13.677	3926	3930	3933	rBV2	393	306	0.03%	0.005%
95	13.783	3958	3963	3964	rBV2	362	274	0.03%	0.004%
96	13.876	3986	3992	3995	rBV3	359	416	0.05%	0.006%
97	13.892	3995	3997	3999	rBV2	332	165	0.02%	0.003%
98	14.037	4039	4042	4044	rBV	296	218	0.02%	0.003%
99	14.355	4138	4141	4144	rBV3	467	267	0.03%	0.004%
100	15.458	4481	4484	4486	rBV	930	459	0.05%	0.007%




Sum of corrected areas: 6559434

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
Data File : VV022457.D
Acq On : 01 Oct 2021 01:42
Operator : SY/MD
Sample : M3978-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

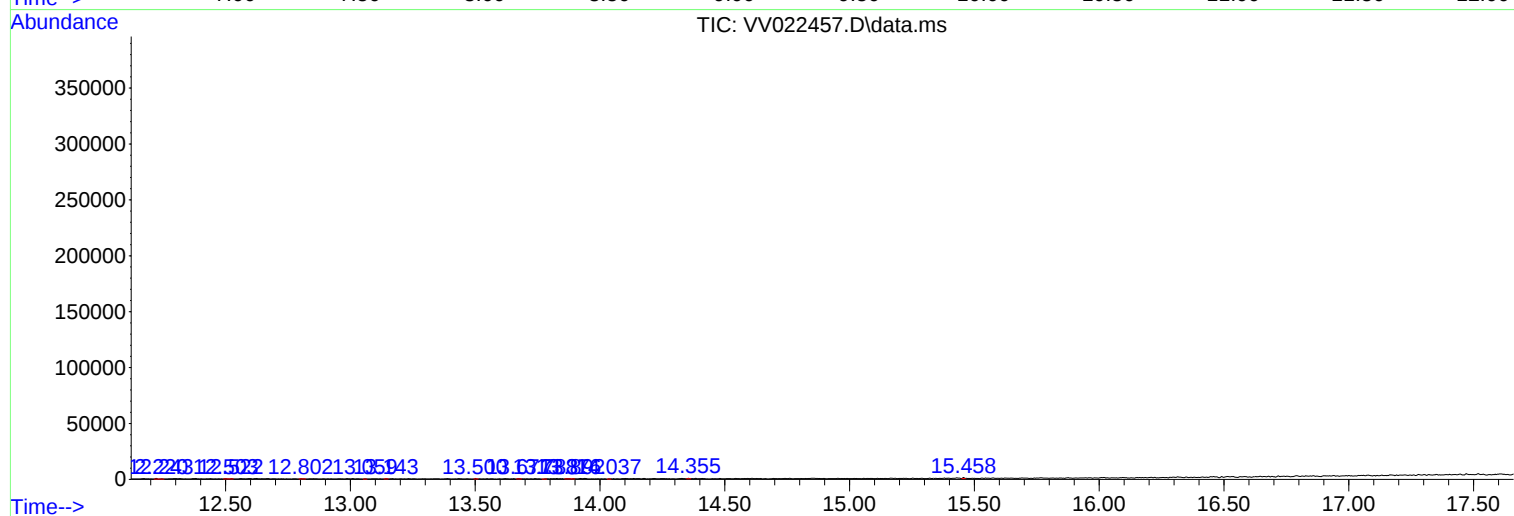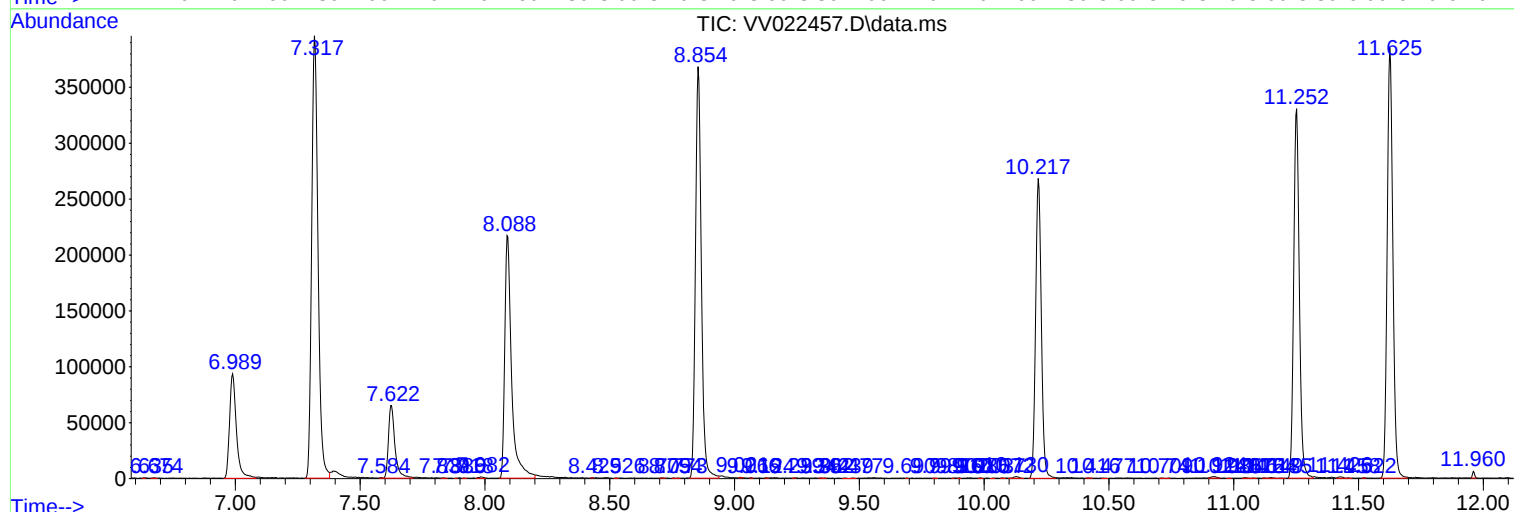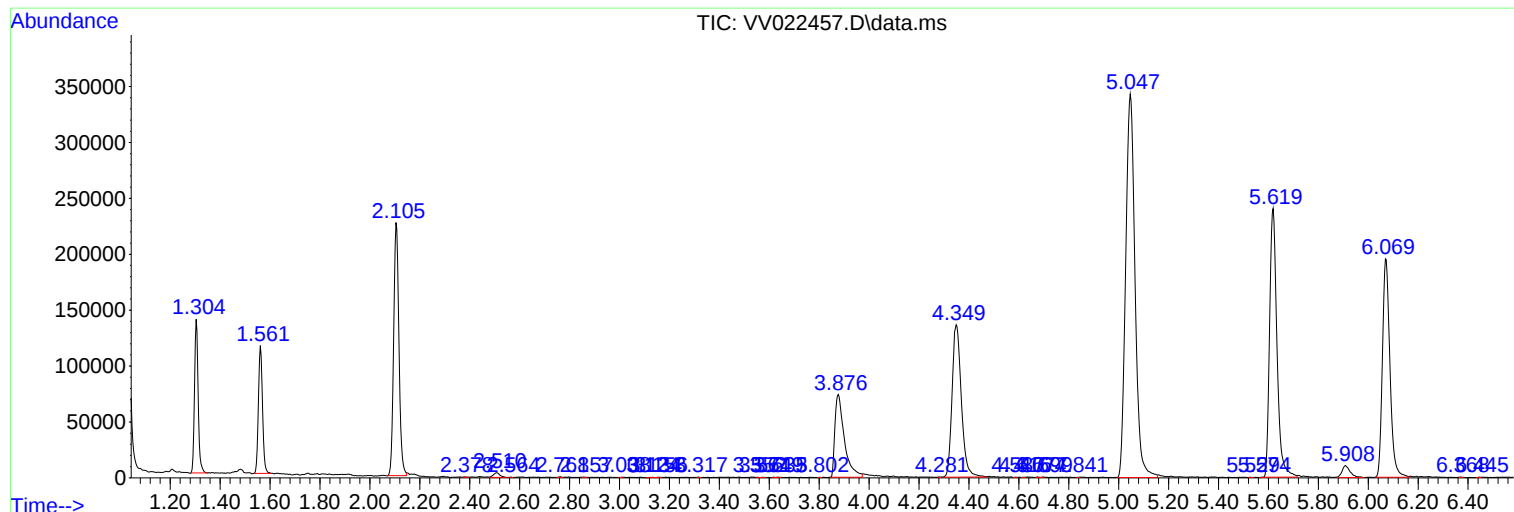

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
Data File : VV022457.D
Acq On : 01 Oct 2021 01:42
Operator : SY/MD
Sample : M3978-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
Data File : VV022457.D
Acq On : 01 Oct 2021 01:42
Operator : SY/MD
Sample : M3978-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
