

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
 Data File : VV022460.D
 Acq On : 01 Oct 2021 02:54
 Operator : SY/MD
 Sample : M3996-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A30

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

Signal : TIC: VV022460.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	94	rVB	138863	139160	12.56%	1.789%
2	1.561	155	162	174	rBV	113620	127281	11.49%	1.636%
3	2.105	321	331	355	rVB	236228	338911	30.59%	4.356%
4	2.571	474	476	478	rBV2	360	196	0.02%	0.003%
5	2.616	482	490	495	rBV4	1858	2704	0.24%	0.035%
6	2.744	527	530	531	rBV2	619	341	0.03%	0.004%
7	2.873	569	570	573	rBV2	234	129	0.01%	0.002%
8	3.198	669	671	675	rVV2	269	140	0.01%	0.002%
9	3.259	689	690	695	rBV2	261	174	0.02%	0.002%
10	3.294	699	701	704	rVB2	530	253	0.02%	0.003%
11	3.310	704	706	710	rBV2	271	188	0.02%	0.002%
12	3.375	724	726	729	rBV	217	136	0.01%	0.002%
13	3.497	761	764	766	rBV2	216	135	0.01%	0.002%
14	3.580	786	790	791	rBV2	281	177	0.02%	0.002%
15	3.625	802	804	807	rBV2	177	140	0.01%	0.002%
16	3.658	812	814	820	rVB2	325	275	0.02%	0.004%
17	3.693	820	825	827	rBV2	403	349	0.03%	0.004%
18	3.748	838	842	844	rBV3	344	278	0.03%	0.004%
19	3.796	855	857	861	rBV2	339	207	0.02%	0.003%
20	3.873	872	881	913	rBV	73430	201724	18.21%	2.593%
21	4.211	984	986	991	rVB2	381	238	0.02%	0.003%
22	4.349	1013	1029	1057	rBV	141107	351650	31.74%	4.520%
23	4.596	1104	1106	1108	rBV	387	188	0.02%	0.002%
24	4.680	1128	1132	1136	rBV	607	612	0.06%	0.008%
25	4.725	1142	1146	1149	rVB2	347	214	0.02%	0.003%
26	4.741	1149	1151	1155	rBV3	281	178	0.02%	0.002%
27	4.899	1198	1200	1203	rBV	615	285	0.03%	0.004%
28	5.047	1229	1246	1273	rBV2	348899	898193	81.08%	11.545%
29	5.400	1351	1356	1361	rBV3	477	535	0.05%	0.007%
30	5.474	1377	1379	1383	rBV	295	164	0.01%	0.002%
31	5.513	1387	1391	1394	rVV3	268	238	0.02%	0.003%
32	5.535	1396	1398	1402	rVB2	441	278	0.03%	0.004%
33	5.619	1411	1424	1447	rBV	260161	532348	48.05%	6.843%
34	5.911	1505	1515	1531	rVB9	6909	15630	1.41%	0.201%
35	5.995	1537	1541	1544	rBV3	457	363	0.03%	0.005%
36	6.072	1550	1565	1596	rBV	191827	405606	36.61%	5.214%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
 Data File : VV022460.D
 Acq On : 01 Oct 2021 02:54
 Operator : SY/MD
 Sample : M3996-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A30

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

37	6.294	1632	1634	1637	rBV2	304	183	0.02%	0.002%
38	6.378	1658	1660	1662	rBV	197	135	0.01%	0.002%
39	6.436	1674	1678	1680	rBV3	339	279	0.03%	0.004%
40	6.574	1716	1721	1724	rBV3	590	496	0.04%	0.006%
41	6.741	1770	1773	1777	rVV2	213	152	0.01%	0.002%
42	6.757	1777	1778	1781	rVB	304	135	0.01%	0.002%
43	6.780	1781	1785	1787	rBV2	425	234	0.02%	0.003%
44	6.989	1839	1850	1869	rBV	96018	175102	15.81%	2.251%
45	7.111	1885	1888	1892	rBV3	783	549	0.05%	0.007%
46	7.217	1918	1921	1923	rBV2	495	376	0.03%	0.005%
47	7.272	1936	1938	1940	rVB	442	178	0.02%	0.002%
48	7.317	1940	1952	1971	rBV	402013	709901	64.08%	9.125%
49	7.622	2037	2047	2069	rBV	66184	118299	10.68%	1.521%
50	7.786	2096	2098	2104	rBV4	494	468	0.04%	0.006%
51	7.976	2145	2157	2178	rBV	658017	1107819	100.00%	14.239%
52	8.088	2183	2192	2228	rVV	205041	377149	34.04%	4.848%
53	8.448	2302	2304	2307	rVB	427	186	0.02%	0.002%
54	8.506	2319	2322	2324	rBV2	312	240	0.02%	0.003%
55	8.651	2363	2367	2372	rBV3	573	534	0.05%	0.007%
56	8.728	2387	2391	2393	rBV2	403	262	0.02%	0.003%
57	8.853	2416	2430	2458	rBV	394218	648892	58.57%	8.341%
58	9.056	2491	2493	2494	rBV2	380	135	0.01%	0.002%
59	9.149	2519	2522	2528	rBV4	798	826	0.07%	0.011%
60	9.522	2636	2638	2643	rVB	267	143	0.01%	0.002%
61	10.037	2796	2798	2804	rVB4	484	285	0.03%	0.004%
62	10.133	2819	2828	2835	rBV4	1260	1953	0.18%	0.025%
63	10.217	2842	2854	2878	rBV	269695	428092	38.64%	5.503%
64	10.323	2883	2887	2889	rBV3	537	441	0.04%	0.006%
65	10.384	2903	2906	2909	rBV2	453	347	0.03%	0.004%
66	10.445	2922	2925	2928	rBV	319	182	0.02%	0.002%
67	10.548	2954	2957	2960	rBV2	226	148	0.01%	0.002%
68	10.567	2961	2963	2964	rBV	418	153	0.01%	0.002%
69	10.644	2984	2987	2992	rBV2	291	270	0.02%	0.003%
70	10.670	2992	2995	2996	rBV	369	184	0.02%	0.002%
71	10.712	3005	3008	3011	rBV	273	199	0.02%	0.003%
72	10.837	3044	3047	3050	rBV2	197	129	0.01%	0.002%
73	10.921	3066	3073	3083	rVB7	1374	2022	0.18%	0.026%
74	10.982	3086	3092	3093	rBV	355	267	0.02%	0.003%
75	11.082	3121	3123	3128	rVB	384	235	0.02%	0.003%
76	11.146	3138	3143	3147	rBV4	662	714	0.06%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
 Data File : VV022460.D
 Acq On : 01 Oct 2021 02:54
 Operator : SY/MD
 Sample : M3996-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A30

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M

Title : VOC Analysis

77	11.252	3164	3176	3197	rBV	359951	561634	50.70%	7.219%
78	11.390	3215	3219	3221	rBV4	724	533	0.05%	0.007%
79	11.506	3253	3255	3257	rBV	203	134	0.01%	0.002%
80	11.625	3280	3292	3318	rBV	380903	614222	55.44%	7.895%
81	11.889	3369	3374	3375	rBV2	239	219	0.02%	0.003%
82	12.088	3433	3436	3437	rBV2	533	220	0.02%	0.003%
83	12.429	3537	3542	3546	rBV2	337	306	0.03%	0.004%
84	12.464	3550	3553	3558	rVB2	315	295	0.03%	0.004%
85	12.535	3574	3575	3579	rBV2	294	154	0.01%	0.002%
86	12.551	3579	3580	3585	rVB	367	261	0.02%	0.003%
87	12.609	3596	3598	3601	rVB2	564	210	0.02%	0.003%
88	12.709	3626	3629	3632	rBV2	184	181	0.02%	0.002%
89	13.114	3751	3755	3756	rBV	273	198	0.02%	0.003%
90	13.162	3763	3770	3776	rBV2	546	592	0.05%	0.008%
91	13.207	3782	3784	3787	rVB3	337	196	0.02%	0.003%
92	13.519	3875	3881	3885	rBV3	517	611	0.06%	0.008%
93	13.670	3924	3928	3930	rBV	382	249	0.02%	0.003%
94	13.924	4005	4007	4010	rBV2	210	149	0.01%	0.002%
95	13.998	4027	4030	4032	rBV	345	275	0.02%	0.004%
96	14.207	4092	4095	4097	rBV	266	193	0.02%	0.002%
97	14.429	4161	4164	4166	rBV2	370	242	0.02%	0.003%
98	14.471	4175	4177	4179	rBV2	345	156	0.01%	0.002%
99	14.512	4186	4190	4193	rBV2	387	405	0.04%	0.005%
100	15.525	4502	4505	4506	rBV2	581	364	0.03%	0.005%




Sum of corrected areas: 7779911

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
Data File : VV022460.D
Acq On : 01 Oct 2021 02:54
Operator : SY/MD
Sample : M3996-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
F4A30

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

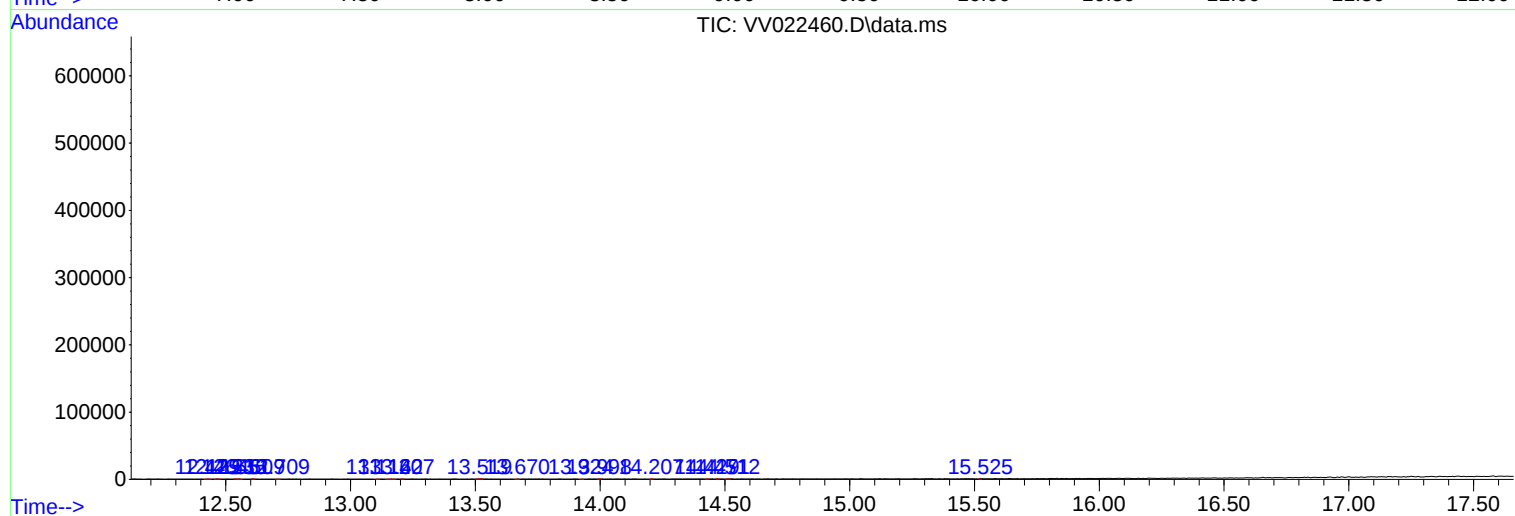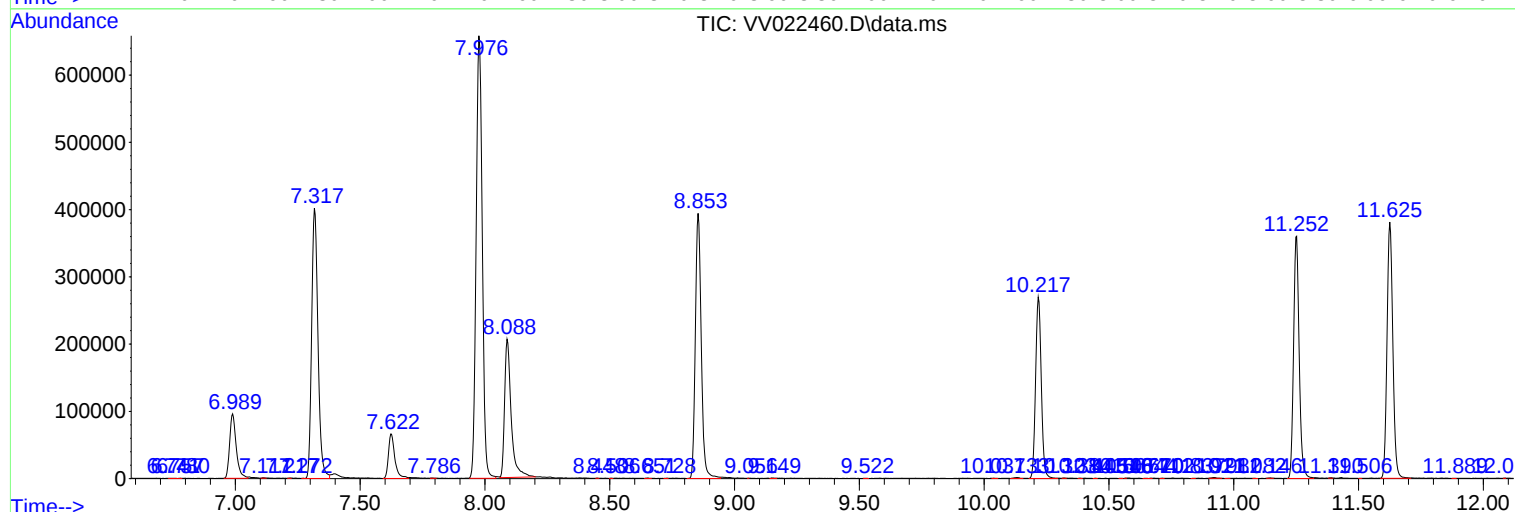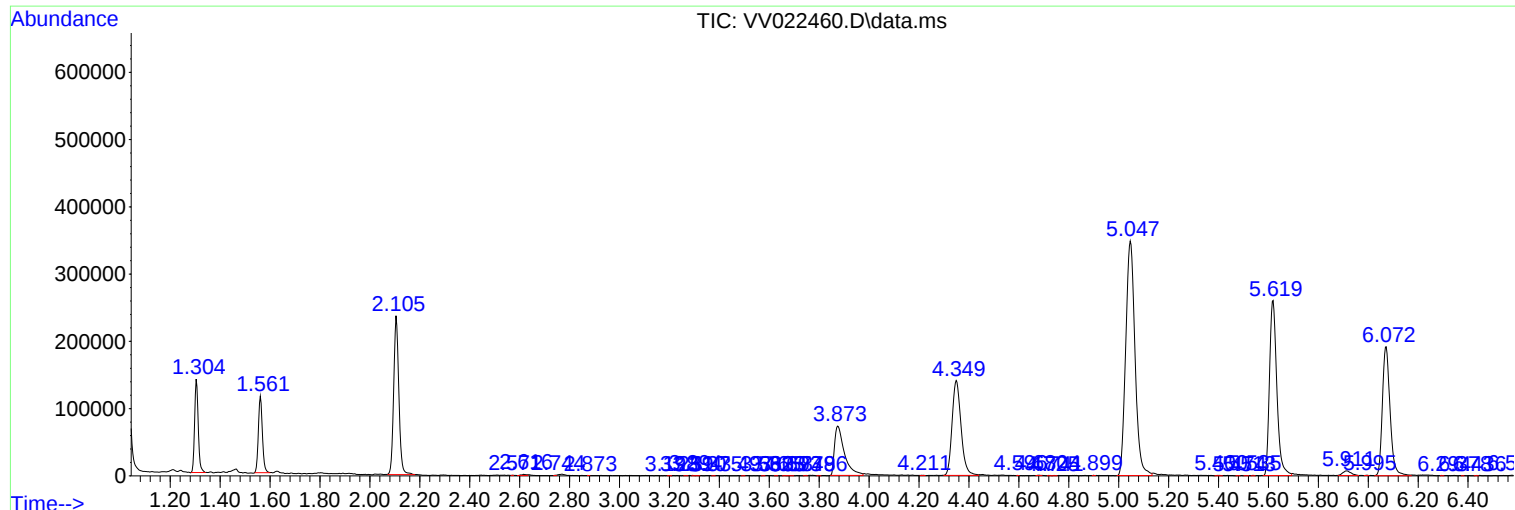

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
Data File : VV022460.D
Acq On : 01 Oct 2021 02:54
Operator : SY/MD
Sample : M3996-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A30

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
Data File : VV022460.D
Acq On : 01 Oct 2021 02:54
Operator : SY/MD
Sample : M3996-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A30

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
