

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
 Data File : VV022461.D
 Acq On : 01 Oct 2021 03:18
 Operator : SY/MD
 Sample : M3996-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A31

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M

Title : VOC Analysis

Signal : TIC: VV022461.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	97	rVB	136360	139212	9.08%	1.700%
2	1.561	155	162	177	rBV	111642	128217	8.36%	1.566%
3	2.105	321	331	347	rBV	223121	329423	21.49%	4.023%
4	2.619	479	491	506	rVB2	5238	11276	0.74%	0.138%
5	2.767	528	537	548	rVB7	2325	4886	0.32%	0.060%
6	2.841	558	560	562	rBV	323	156	0.01%	0.002%
7	2.953	592	595	597	rBV	210	171	0.01%	0.002%
8	3.108	641	643	646	rBV2	292	180	0.01%	0.002%
9	3.185	663	667	670	rVB2	197	155	0.01%	0.002%
10	3.201	670	672	674	rBV2	350	171	0.01%	0.002%
11	3.220	676	678	681	rVB	370	157	0.01%	0.002%
12	3.333	707	713	717	rBV2	303	410	0.03%	0.005%
13	3.355	717	720	722	rBV2	267	203	0.01%	0.002%
14	3.420	738	740	742	rBV2	309	143	0.01%	0.002%
15	3.484	757	760	764	rVB2	378	322	0.02%	0.004%
16	3.510	764	768	770	rBV2	288	238	0.02%	0.003%
17	3.767	846	848	852	rVB	264	146	0.01%	0.002%
18	3.876	871	882	921	rBV2	82731	247774	16.16%	3.026%
19	4.349	1012	1029	1053	rBV	140192	350468	22.86%	4.280%
20	4.567	1094	1097	1103	rVB2	640	521	0.03%	0.006%
21	4.760	1154	1157	1160	rBV2	374	330	0.02%	0.004%
22	4.802	1165	1170	1173	rBV2	401	333	0.02%	0.004%
23	4.841	1180	1182	1186	rVB3	465	250	0.02%	0.003%
24	4.870	1189	1191	1196	rVB4	273	169	0.01%	0.002%
25	4.892	1196	1198	1201	rBV2	370	192	0.01%	0.002%
26	4.989	1224	1228	1230	rBV2	353	198	0.01%	0.002%
27	5.047	1230	1246	1290	rBV2	344402	889150	58.00%	10.858%
28	5.403	1353	1357	1359	rVB	296	147	0.01%	0.002%
29	5.455	1371	1373	1375	rBV2	373	207	0.01%	0.003%
30	5.555	1401	1404	1408	rBV	231	211	0.01%	0.003%
31	5.619	1412	1424	1449	rBV	255349	523169	34.13%	6.389%
32	5.908	1505	1514	1536	rVB7	7428	17713	1.16%	0.216%
33	6.072	1547	1565	1586	rBV	191540	399296	26.05%	4.876%
34	6.211	1606	1608	1610	rBV2	484	266	0.02%	0.003%
35	6.307	1633	1638	1641	rBV2	505	518	0.03%	0.006%
36	6.686	1753	1756	1758	rVB2	471	213	0.01%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
 Data File : VV022461.D
 Acq On : 01 Oct 2021 03:18
 Operator : SY/MD
 Sample : M3996-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A31

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

37	6.744	1772	1774	1779	rVB3	310	186	0.01%	0.002%
38	6.989	1839	1850	1874	rBV	94758	175923	11.48%	2.148%
39	7.214	1917	1920	1922	rBV	355	177	0.01%	0.002%
40	7.262	1931	1935	1937	rBV	327	172	0.01%	0.002%
41	7.317	1938	1952	1972	rBV	404177	699111	45.60%	8.537%
42	7.622	2038	2047	2071	rBV	64869	116384	7.59%	1.421%
43	7.895	2130	2132	2136	rVB2	530	340	0.02%	0.004%
44	7.915	2136	2138	2141	rBV	230	176	0.01%	0.002%
45	7.976	2141	2157	2178	rBV	915696	1533013	100.00%	18.721%
46	8.088	2183	2192	2225	rVV	211695	382975	24.98%	4.677%
47	8.416	2290	2294	2295	rBV	369	279	0.02%	0.003%
48	8.487	2314	2316	2317	rBV	425	178	0.01%	0.002%
49	8.542	2329	2333	2334	rBV3	373	267	0.02%	0.003%
50	8.593	2347	2349	2351	rBV2	342	229	0.01%	0.003%
51	8.683	2375	2377	2381	rBV2	356	235	0.02%	0.003%
52	8.776	2402	2406	2409	rBV3	202	217	0.01%	0.003%
53	8.853	2418	2430	2453	rBV	391942	636535	41.52%	7.773%
54	9.117	2510	2512	2515	rBV2	327	189	0.01%	0.002%
55	9.149	2519	2522	2530	rVV4	835	845	0.06%	0.010%
56	9.178	2530	2531	2534	rVV2	419	222	0.01%	0.003%
57	9.214	2538	2542	2545	rBV3	232	172	0.01%	0.002%
58	9.445	2611	2614	2618	rBV3	315	245	0.02%	0.003%
59	9.468	2618	2621	2625	rVB2	364	259	0.02%	0.003%
60	9.497	2625	2630	2631	rBV	215	190	0.01%	0.002%
61	9.644	2674	2676	2681	rBV2	313	194	0.01%	0.002%
62	9.712	2695	2697	2699	rBV2	231	144	0.01%	0.002%
63	9.796	2721	2723	2725	rVV2	465	240	0.02%	0.003%
64	9.834	2729	2735	2739	rVB2	618	414	0.03%	0.005%
65	9.870	2743	2746	2748	rVV2	476	293	0.02%	0.004%
66	9.889	2748	2752	2753	rVB2	284	181	0.01%	0.002%
67	9.982	2779	2781	2784	rVB	318	156	0.01%	0.002%
68	10.098	2813	2817	2819	rBV2	307	174	0.01%	0.002%
69	10.130	2819	2827	2833	rBV3	1163	1660	0.11%	0.020%
70	10.178	2837	2842	2843	rBV	171	161	0.01%	0.002%
71	10.217	2843	2854	2874	rBV	273318	429798	28.04%	5.249%
72	10.365	2897	2900	2902	rBV2	525	300	0.02%	0.004%
73	10.378	2902	2904	2911	rVB3	555	275	0.02%	0.003%
74	10.445	2923	2925	2928	rBV	374	181	0.01%	0.002%
75	10.519	2947	2948	2954	rVB3	291	217	0.01%	0.003%
76	10.551	2954	2958	2959	rBV	332	182	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
 Data File : VV022461.D
 Acq On : 01 Oct 2021 03:18
 Operator : SY/MD
 Sample : M3996-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A31

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

77	10.606	2973	2975	2978	rBV	317	156	0.01%	0.002%
78	10.641	2983	2986	2989	rBV	200	179	0.01%	0.002%
79	10.918	3068	3072	3073	rBV2	701	458	0.03%	0.006%
80	10.982	3090	3092	3097	rVB2	235	147	0.01%	0.002%
81	11.030	3105	3107	3109	rBV2	348	196	0.01%	0.002%
82	11.069	3117	3119	3122	rBV3	416	204	0.01%	0.002%
83	11.143	3139	3142	3143	rBV	608	294	0.02%	0.004%
84	11.249	3165	3175	3198	rBV	347311	551949	36.00%	6.740%
85	11.570	3273	3275	3278	rBV2	411	199	0.01%	0.002%
86	11.625	3278	3292	3317	rBV	380056	601895	39.26%	7.350%
87	11.747	3326	3330	3332	rBV3	384	284	0.02%	0.003%
88	11.947	3388	3392	3395	rBV	269	172	0.01%	0.002%
89	12.181	3462	3465	3467	rBV	488	274	0.02%	0.003%
90	12.384	3524	3528	3529	rBV	179	148	0.01%	0.002%
91	12.451	3547	3549	3552	rBV	261	171	0.01%	0.002%
92	12.847	3670	3672	3675	rBV2	249	160	0.01%	0.002%
93	13.522	3879	3882	3883	rBV2	513	224	0.01%	0.003%
94	13.885	3993	3995	4000	rBV2	358	258	0.02%	0.003%
95	13.982	4022	4025	4028	rBV3	315	220	0.01%	0.003%
96	14.111	4060	4065	4066	rBV	338	264	0.02%	0.003%
97	14.229	4099	4102	4104	rBV2	361	238	0.02%	0.003%
98	14.258	4109	4111	4114	rBV2	403	192	0.01%	0.002%
99	14.400	4151	4155	4156	rBV	377	295	0.02%	0.004%
100	14.654	4231	4234	4239	rBV3	669	453	0.03%	0.006%


Sum of corrected areas: 8188710

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
Data File : VV022461.D
Acq On : 01 Oct 2021 03:18
Operator : SY/MD
Sample : M3996-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A31

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

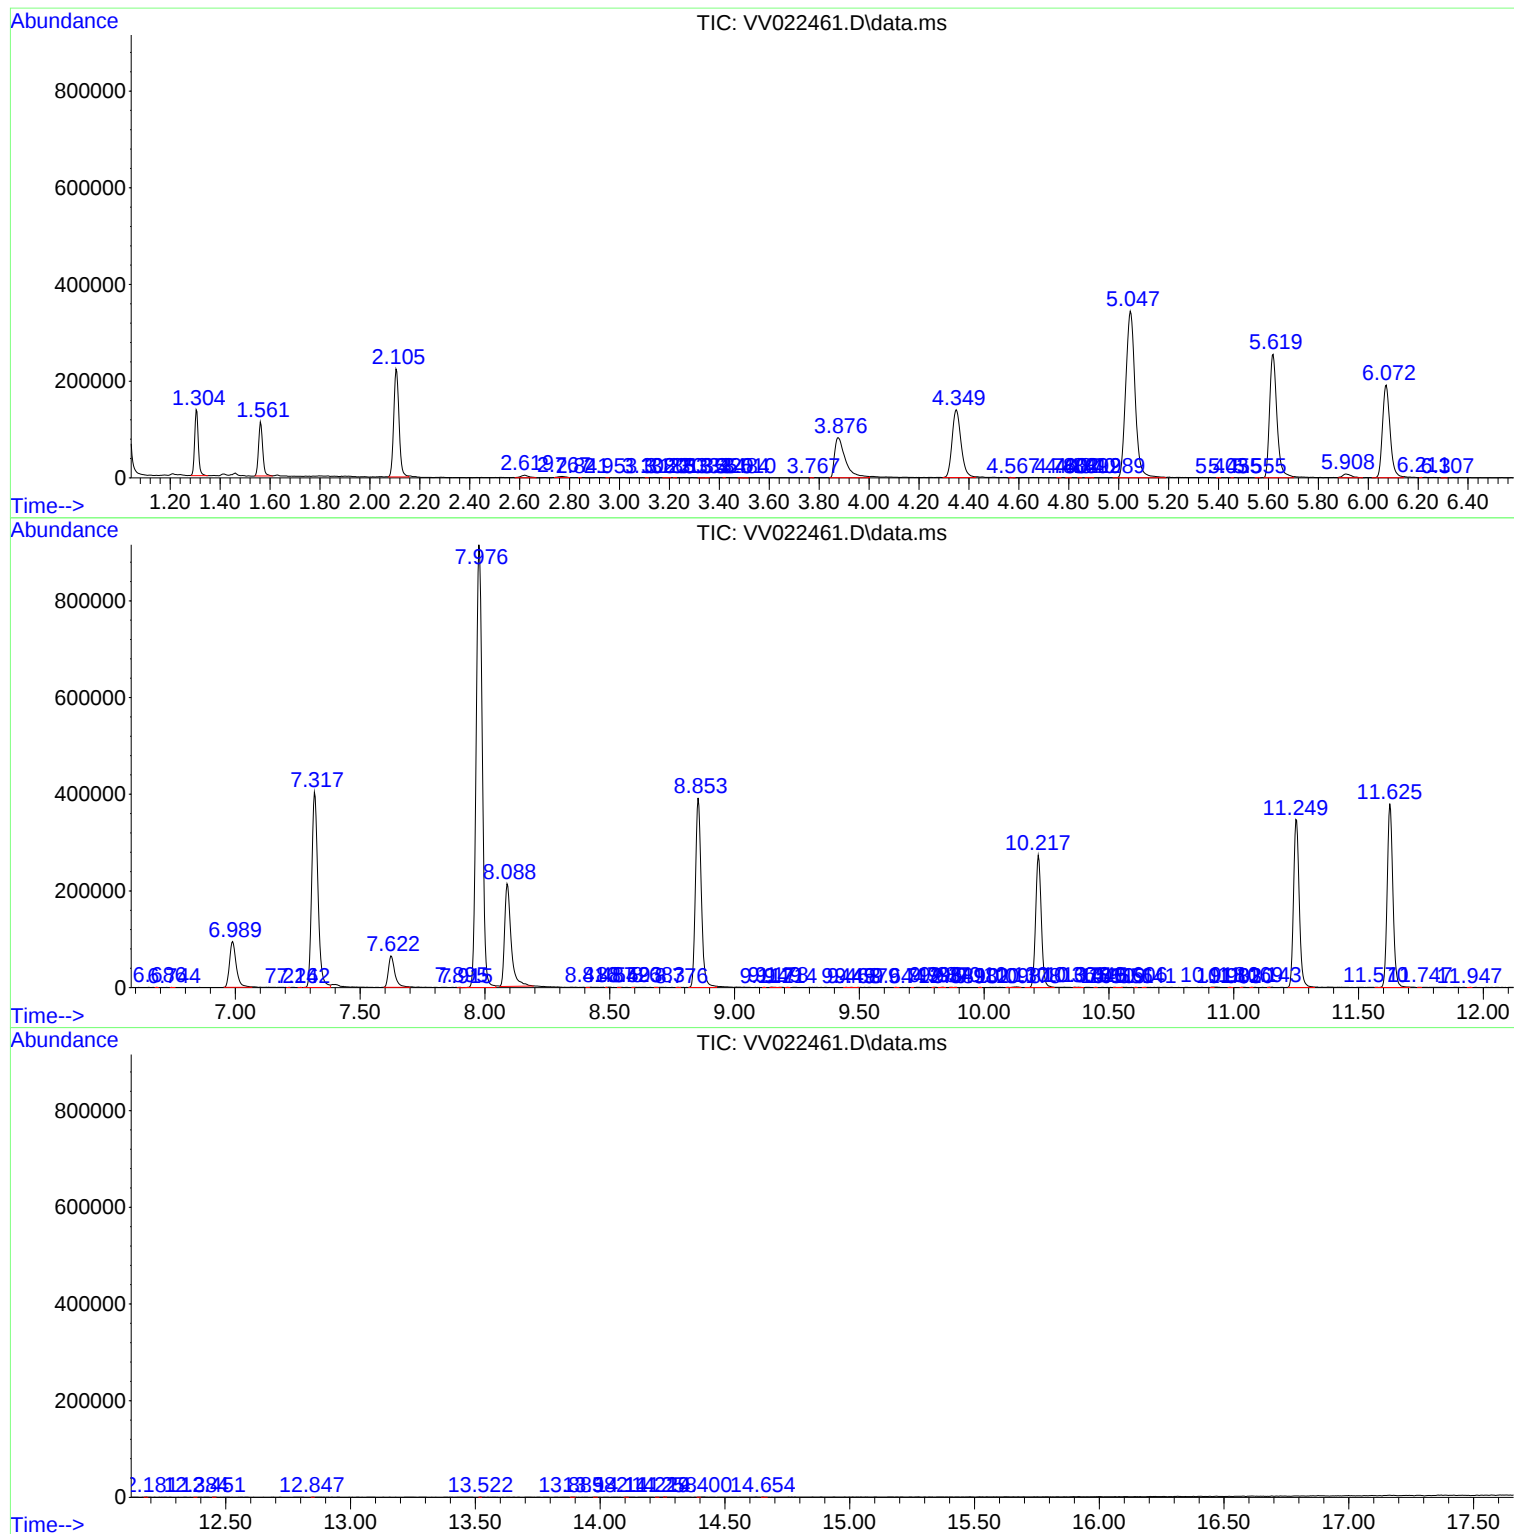

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
Data File : VV022461.D
Acq On : 01 Oct 2021 03:18
Operator : SY/MD
Sample : M3996-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A31

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
Data File : VV022461.D
Acq On : 01 Oct 2021 03:18
Operator : SY/MD
Sample : M3996-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A31

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
