

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
 Data File : VV022462.D
 Acq On : 01 Oct 2021 03:42
 Operator : SY/MD
 Sample : M3996-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A32

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

Signal : TIC: VV022462.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	97	rVB	134240	136015	5.57%	1.509%
2	1.561	155	162	177	rBV	107238	125605	5.14%	1.394%
3	2.105	321	331	348	rBV	219300	327218	13.40%	3.631%
4	2.346	404	406	411	rBV2	514	282	0.01%	0.003%
5	2.767	527	537	547	rBV5	5044	9872	0.40%	0.110%
6	2.973	599	601	604	rVB2	356	160	0.01%	0.002%
7	3.014	610	614	617	rBV2	442	323	0.01%	0.004%
8	3.031	617	619	624	rVB2	385	273	0.01%	0.003%
9	3.101	635	641	643	rBV	180	217	0.01%	0.002%
10	3.256	686	689	691	rBV2	250	204	0.01%	0.002%
11	3.330	709	712	717	rBV3	323	273	0.01%	0.003%
12	3.439	743	746	751	rBV2	244	149	0.01%	0.002%
13	3.497	761	764	772	rVB3	330	284	0.01%	0.003%
14	3.686	821	823	827	rVB3	273	158	0.01%	0.002%
15	3.725	833	835	840	rVB	265	208	0.01%	0.002%
16	3.760	842	846	848	rBV2	298	220	0.01%	0.002%
17	3.783	851	853	856	rBV2	285	196	0.01%	0.002%
18	3.802	857	859	863	rVB2	289	155	0.01%	0.002%
19	3.873	872	881	916	rBV	72598	204613	8.38%	2.271%
20	4.349	1013	1029	1053	rBV	138649	348684	14.27%	3.869%
21	4.619	1109	1113	1114	rBV	250	189	0.01%	0.002%
22	4.654	1118	1124	1127	rVB2	491	391	0.02%	0.004%
23	4.677	1127	1131	1134	rBV2	340	221	0.01%	0.002%
24	4.719	1141	1144	1148	rBV4	435	389	0.02%	0.004%
25	4.757	1153	1156	1161	rVB3	338	221	0.01%	0.002%
26	4.780	1161	1163	1166	rVB2	256	143	0.01%	0.002%
27	4.895	1194	1199	1202	rBV3	493	417	0.02%	0.005%
28	5.047	1229	1246	1276	rBV2	340726	877720	35.93%	9.740%
29	5.503	1386	1388	1392	rBV	442	217	0.01%	0.002%
30	5.539	1395	1399	1402	rBV2	305	196	0.01%	0.002%
31	5.619	1412	1424	1454	rBV2	250943	518627	21.23%	5.755%
32	5.915	1504	1516	1538	rBV8	15395	37823	1.55%	0.420%
33	6.069	1551	1564	1587	rBV	190381	392908	16.08%	4.360%
34	6.252	1619	1621	1624	rVB2	473	263	0.01%	0.003%
35	6.288	1631	1632	1637	rVB2	611	306	0.01%	0.003%
36	6.333	1642	1646	1650	rBV4	444	376	0.02%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
 Data File : VV022462.D
 Acq On : 01 Oct 2021 03:42
 Operator : SY/MD
 Sample : M3996-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A32

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

37	6.548	1710	1713	1716	rVB	221	155	0.01%	0.002%
38	6.567	1716	1719	1723	rVB2	292	165	0.01%	0.002%
39	6.603	1728	1730	1735	rVB2	508	327	0.01%	0.004%
40	6.770	1780	1782	1787	rBV2	370	258	0.01%	0.003%
41	6.870	1810	1813	1816	rBV	293	189	0.01%	0.002%
42	6.989	1840	1850	1870	rBV	94238	172481	7.06%	1.914%
43	7.317	1940	1952	1969	rBV	395971	689099	28.21%	7.647%
44	7.580	2030	2034	2038	rBV3	417	263	0.01%	0.003%
45	7.625	2038	2048	2077	rBV	64169	116915	4.79%	1.297%
46	7.802	2099	2103	2105	rBV2	279	183	0.01%	0.002%
47	7.821	2105	2109	2118	rVB3	579	529	0.02%	0.006%
48	7.908	2133	2136	2138	rBV2	261	169	0.01%	0.002%
49	7.976	2144	2157	2180	rBV	1448881	2442827	100.00%	27.107%
50	8.088	2184	2192	2228	rVB	210754	386633	15.83%	4.290%
51	8.333	2265	2268	2271	rBV3	548	394	0.02%	0.004%
52	8.487	2312	2316	2320	rVB4	393	430	0.02%	0.005%
53	8.506	2320	2322	2326	rBV2	404	286	0.01%	0.003%
54	8.686	2375	2378	2383	rBV2	248	210	0.01%	0.002%
55	8.731	2389	2392	2395	rVB	308	222	0.01%	0.002%
56	8.853	2419	2430	2449	rBV	389953	629375	25.76%	6.984%
57	9.034	2484	2486	2488	rBV3	479	207	0.01%	0.002%
58	9.072	2495	2498	2504	rVB2	673	600	0.02%	0.007%
59	9.104	2504	2508	2509	rBV	264	187	0.01%	0.002%
60	9.136	2516	2518	2520	rBV	364	146	0.01%	0.002%
61	9.323	2573	2576	2580	rVV2	365	290	0.01%	0.003%
62	9.525	2636	2639	2641	rBV2	346	182	0.01%	0.002%
63	9.648	2676	2677	2682	rVB2	275	198	0.01%	0.002%
64	9.715	2696	2698	2701	rBV2	293	172	0.01%	0.002%
65	9.770	2710	2715	2719	rBV3	343	399	0.02%	0.004%
66	9.882	2747	2750	2754	rBV2	198	196	0.01%	0.002%
67	10.005	2784	2788	2790	rBV2	296	235	0.01%	0.003%
68	10.037	2794	2798	2803	rVB	303	260	0.01%	0.003%
69	10.082	2807	2812	2814	rBV2	353	223	0.01%	0.002%
70	10.124	2820	2825	2827	rBV4	1125	919	0.04%	0.010%
71	10.217	2842	2854	2877	rBV	268272	427019	17.48%	4.738%
72	10.358	2896	2898	2902	rBV2	348	177	0.01%	0.002%
73	10.435	2919	2922	2924	rBV3	260	169	0.01%	0.002%
74	10.747	3017	3019	3022	rBV2	280	144	0.01%	0.002%
75	10.921	3067	3073	3081	rVB4	1102	1492	0.06%	0.017%
76	10.960	3082	3085	3089	rVB2	538	326	0.01%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
 Data File : VV022462.D
 Acq On : 01 Oct 2021 03:42
 Operator : SY/MD
 Sample : M3996-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A32

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

77	10.982	3089	3092	3099	rBV2	179	245	0.01%	0.003%
78	11.117	3131	3134	3136	rBV	330	206	0.01%	0.002%
79	11.152	3142	3145	3148	rVB2	929	568	0.02%	0.006%
80	11.172	3148	3151	3153	rBV2	466	310	0.01%	0.003%
81	11.252	3164	3176	3197	rBV	345609	548266	22.44%	6.084%
82	11.503	3251	3254	3257	rBV	362	295	0.01%	0.003%
83	11.561	3269	3272	3275	rVB3	387	236	0.01%	0.003%
84	11.625	3281	3292	3314	rBV	373649	597447	24.46%	6.630%
85	11.760	3331	3334	3336	rBV	374	261	0.01%	0.003%
86	11.914	3380	3382	3388	rVB2	313	271	0.01%	0.003%
87	12.062	3423	3428	3434	rBV2	409	387	0.02%	0.004%
88	12.117	3442	3445	3449	rBV2	439	264	0.01%	0.003%
89	12.140	3449	3452	3455	rBV2	278	210	0.01%	0.002%
90	12.213	3473	3475	3479	rVB2	459	210	0.01%	0.002%
91	12.233	3479	3481	3485	rVB	288	142	0.01%	0.002%
92	13.046	3730	3734	3737	rBV	321	214	0.01%	0.002%
93	13.078	3741	3744	3748	rBV2	222	194	0.01%	0.002%
94	13.500	3872	3875	3878	rBV2	334	212	0.01%	0.002%
95	13.995	4026	4029	4034	rVB	419	272	0.01%	0.003%
96	14.220	4098	4099	4102	rBV2	373	155	0.01%	0.002%
97	14.358	4136	4142	4144	rBV2	400	450	0.02%	0.005%
98	14.577	4208	4210	4212	rBV2	389	147	0.01%	0.002%
99	14.757	4264	4266	4272	rBV3	354	300	0.01%	0.003%
100	14.815	4280	4284	4288	rBV3	439	348	0.01%	0.004%




Sum of corrected areas: 9011777

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
Data File : VV022462.D
Acq On : 01 Oct 2021 03:42
Operator : SY/MD
Sample : M3996-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A32

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

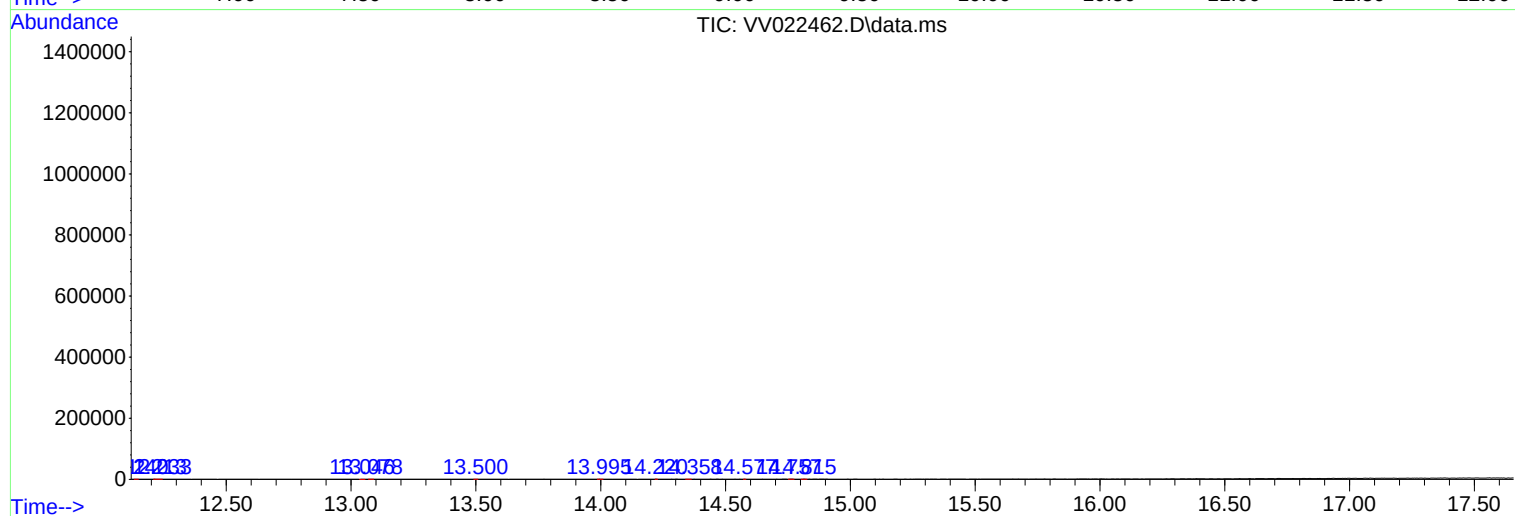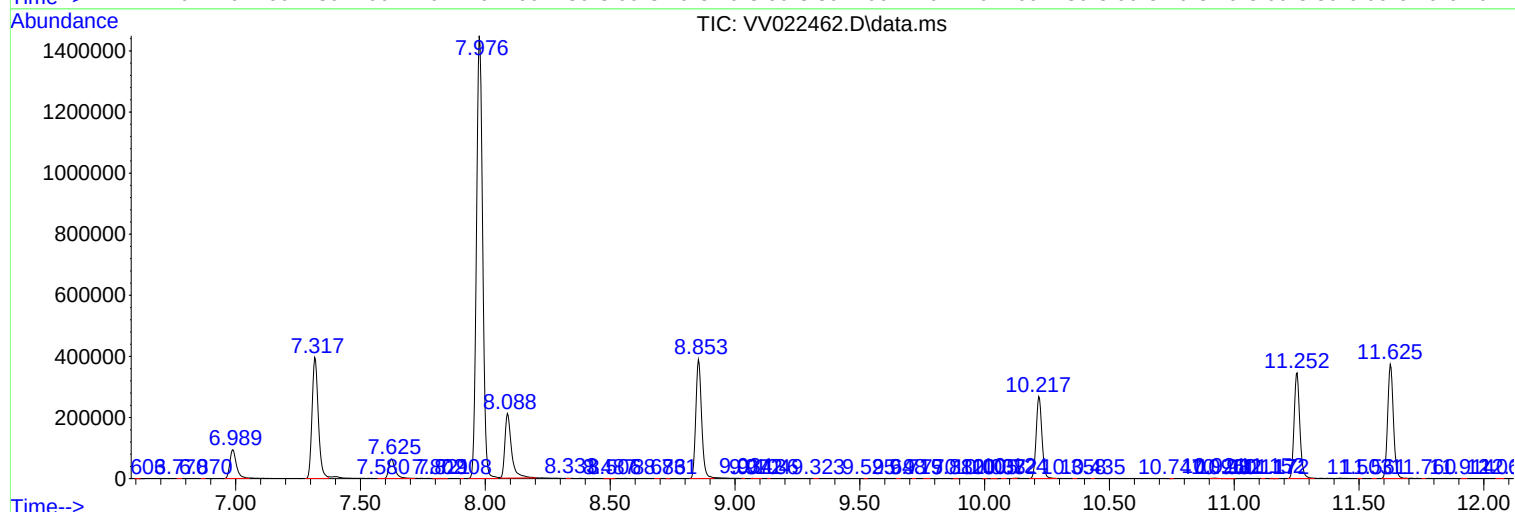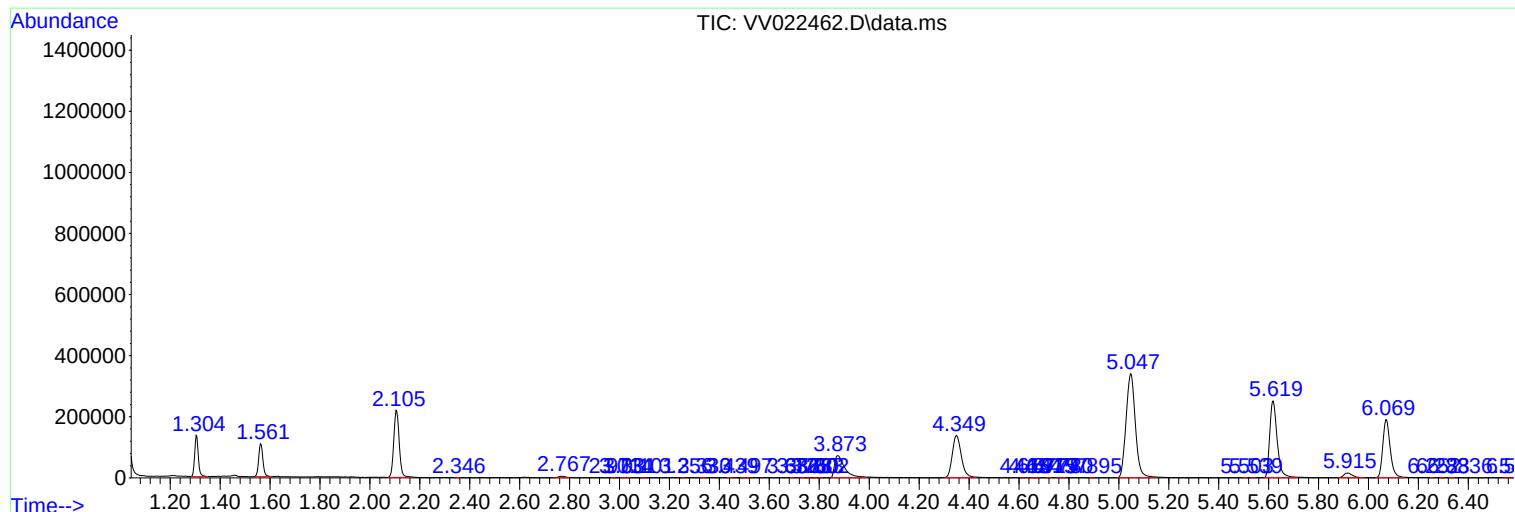

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
Data File : VV022462.D
Acq On : 01 Oct 2021 03:42
Operator : SY/MD
Sample : M3996-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A32

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
Data File : VV022462.D
Acq On : 01 Oct 2021 03:42
Operator : SY/MD
Sample : M3996-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A32

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
