

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
 Data File : VV022464.D
 Acq On : 01 Oct 2021 04:30
 Operator : SY/MD
 Sample : M3996-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A38

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

Signal : TIC: VV022464.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	97	rVB	139027	141591	15.18%	2.067%
2	1.564	157	163	175	rVB	110018	124995	13.40%	1.825%
3	2.105	321	331	346	rBV	228843	329512	35.32%	4.811%
4	2.484	446	449	450	rBV	455	250	0.03%	0.004%
5	2.606	480	487	488	rBV3	890	864	0.09%	0.013%
6	2.716	517	521	522	rBV2	491	355	0.04%	0.005%
7	2.976	600	602	604	rBV2	267	139	0.01%	0.002%
8	3.140	649	653	657	rBV2	235	225	0.02%	0.003%
9	3.166	657	661	664	rBV	317	223	0.02%	0.003%
10	3.243	683	685	688	rVB2	235	126	0.01%	0.002%
11	3.269	691	693	696	rBV2	275	181	0.02%	0.003%
12	3.445	746	748	750	rBV	251	127	0.01%	0.002%
13	3.503	765	766	772	rVB3	282	196	0.02%	0.003%
14	3.532	772	775	777	rBV2	285	202	0.02%	0.003%
15	3.696	823	826	828	rBV	325	186	0.02%	0.003%
16	3.712	828	831	833	rVV2	230	140	0.02%	0.002%
17	3.754	841	844	845	rVB2	287	130	0.01%	0.002%
18	3.912	880	893	938	rBV2	52258	233292	25.01%	3.406%
19	4.349	1012	1029	1060	rBV	142599	368042	39.45%	5.373%
20	4.561	1093	1095	1097	rBV	369	151	0.02%	0.002%
21	4.658	1121	1125	1127	rBV3	439	340	0.04%	0.005%
22	4.715	1140	1143	1145	rBV	228	134	0.01%	0.002%
23	4.748	1150	1153	1159	rBV3	300	345	0.04%	0.005%
24	4.799	1167	1169	1175	rBV	266	248	0.03%	0.004%
25	4.921	1204	1207	1208	rBV2	239	154	0.02%	0.002%
26	4.969	1218	1222	1225	rBV4	424	337	0.04%	0.005%
27	5.047	1230	1246	1283	rBV2	364183	932955	100.00%	13.621%
28	5.268	1313	1315	1318	rBV2	621	349	0.04%	0.005%
29	5.323	1329	1332	1334	rVB3	412	201	0.02%	0.003%
30	5.400	1352	1356	1357	rBV3	325	227	0.02%	0.003%
31	5.429	1364	1365	1368	rVB	372	148	0.02%	0.002%
32	5.519	1389	1393	1395	rVB2	363	211	0.02%	0.003%
33	5.616	1409	1423	1457	rBV	255343	533615	57.20%	7.791%
34	5.912	1504	1515	1531	rVB5	7469	16797	1.80%	0.245%
35	6.072	1551	1565	1586	rBV	202263	414944	44.48%	6.058%
36	6.217	1608	1610	1611	rBV	655	256	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
 Data File : VV022464.D
 Acq On : 01 Oct 2021 04:30
 Operator : SY/MD
 Sample : M3996-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A38

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

37	6.262	1621	1624	1627	rVV3	612	376	0.04%	0.005%
38	6.288	1630	1632	1636	rVB2	321	142	0.02%	0.002%
39	6.307	1636	1638	1646	rVB3	356	329	0.04%	0.005%
40	6.413	1668	1671	1674	rVB	284	162	0.02%	0.002%
41	6.445	1678	1681	1682	rBV	298	134	0.01%	0.002%
42	6.506	1697	1700	1702	rVV2	385	207	0.02%	0.003%
43	6.667	1748	1750	1752	rVB	450	193	0.02%	0.003%
44	6.735	1770	1771	1774	rVB	408	154	0.02%	0.002%
45	6.757	1774	1778	1781	rBV2	450	397	0.04%	0.006%
46	6.818	1795	1797	1800	rVB	287	145	0.02%	0.002%
47	6.847	1803	1806	1809	rBV2	244	185	0.02%	0.003%
48	6.989	1838	1850	1872	rBV	96757	182884	19.60%	2.670%
49	7.236	1923	1927	1931	rBV3	316	292	0.03%	0.004%
50	7.317	1940	1952	1970	rBV	421999	728513	78.09%	10.636%
51	7.545	2021	2023	2025	rBV2	336	197	0.02%	0.003%
52	7.574	2030	2032	2035	rVB2	380	216	0.02%	0.003%
53	7.625	2038	2048	2063	rBV	64644	118225	12.67%	1.726%
54	7.873	2123	2125	2131	rBV2	389	232	0.02%	0.003%
55	7.934	2140	2144	2145	rBV2	442	308	0.03%	0.004%
56	7.979	2149	2158	2181	rVB2	25628	45531	4.88%	0.665%
57	8.095	2183	2194	2233	rBV	214409	423418	45.38%	6.182%
58	8.426	2295	2297	2299	rVB2	485	157	0.02%	0.002%
59	8.503	2317	2321	2324	rBV3	389	282	0.03%	0.004%
60	8.522	2324	2327	2328	rBV2	302	127	0.01%	0.002%
61	8.699	2379	2382	2390	rVB2	555	493	0.05%	0.007%
62	8.767	2400	2403	2407	rVV2	250	196	0.02%	0.003%
63	8.854	2419	2430	2456	rBV	386653	637906	68.37%	9.313%
64	9.079	2496	2500	2502	rBV	403	315	0.03%	0.005%
65	9.111	2508	2510	2515	rVB4	458	394	0.04%	0.006%
66	9.153	2520	2523	2525	rBV	329	209	0.02%	0.003%
67	9.185	2530	2533	2536	rBV2	453	276	0.03%	0.004%
68	9.278	2559	2562	2565	rBV	383	249	0.03%	0.004%
69	9.397	2597	2599	2603	rBV2	179	148	0.02%	0.002%
70	9.583	2653	2657	2658	rBV	295	179	0.02%	0.003%
71	9.603	2659	2663	2668	rVB2	475	453	0.05%	0.007%
72	9.693	2688	2691	2693	rBV2	210	135	0.01%	0.002%
73	9.969	2774	2777	2784	rBV2	475	339	0.04%	0.005%
74	10.130	2822	2827	2835	rVB4	1024	1324	0.14%	0.019%
75	10.217	2843	2854	2874	rBV	283498	444394	47.63%	6.488%
76	10.317	2883	2885	2888	rBV2	311	199	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
 Data File : VV022464.D
 Acq On : 01 Oct 2021 04:30
 Operator : SY/MD
 Sample : M3996-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A38

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

77	10.362	2897	2899	2901	rVB	415	153	0.02%	0.002%
78	10.378	2901	2904	2907	rBV2	598	474	0.05%	0.007%
79	10.458	2927	2929	2931	rBV	247	169	0.02%	0.002%
80	10.535	2949	2953	2954	rBV	288	135	0.01%	0.002%
81	10.757	3020	3022	3023	rBV	292	127	0.01%	0.002%
82	10.863	3052	3055	3057	rBV	270	191	0.02%	0.003%
83	11.149	3140	3144	3147	rBV2	780	570	0.06%	0.008%
84	11.252	3165	3176	3197	rBV	344606	539806	57.86%	7.881%
85	11.538	3262	3265	3268	rBV2	1257	1163	0.12%	0.017%
86	11.625	3280	3292	3312	rBV	383994	611387	65.53%	8.926%
87	11.773	3336	3338	3342	rVB3	415	267	0.03%	0.004%
88	11.792	3342	3344	3347	rBV2	289	173	0.02%	0.003%
89	11.905	3376	3379	3382	rBV2	303	219	0.02%	0.003%
90	11.966	3396	3398	3406	rBV2	339	267	0.03%	0.004%
91	12.358	3518	3520	3524	rBV	357	301	0.03%	0.004%
92	12.432	3541	3543	3547	rBV2	276	170	0.02%	0.002%
93	12.474	3553	3556	3559	rBV2	228	145	0.02%	0.002%
94	12.943	3697	3702	3706	rBV2	356	290	0.03%	0.004%
95	13.030	3727	3729	3735	rVB2	383	256	0.03%	0.004%
96	13.664	3924	3926	3929	rBV	373	188	0.02%	0.003%
97	13.956	4014	4017	4020	rBV2	425	332	0.04%	0.005%
98	13.992	4025	4028	4030	rBV	277	189	0.02%	0.003%
99	14.474	4176	4178	4179	rBV	343	128	0.01%	0.002%
100	15.538	4507	4509	4510	rBV	562	234	0.03%	0.003%




Sum of corrected areas: 6849537

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
Data File : VV022464.D
Acq On : 01 Oct 2021 04:30
Operator : SY/MD
Sample : M3996-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A38

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

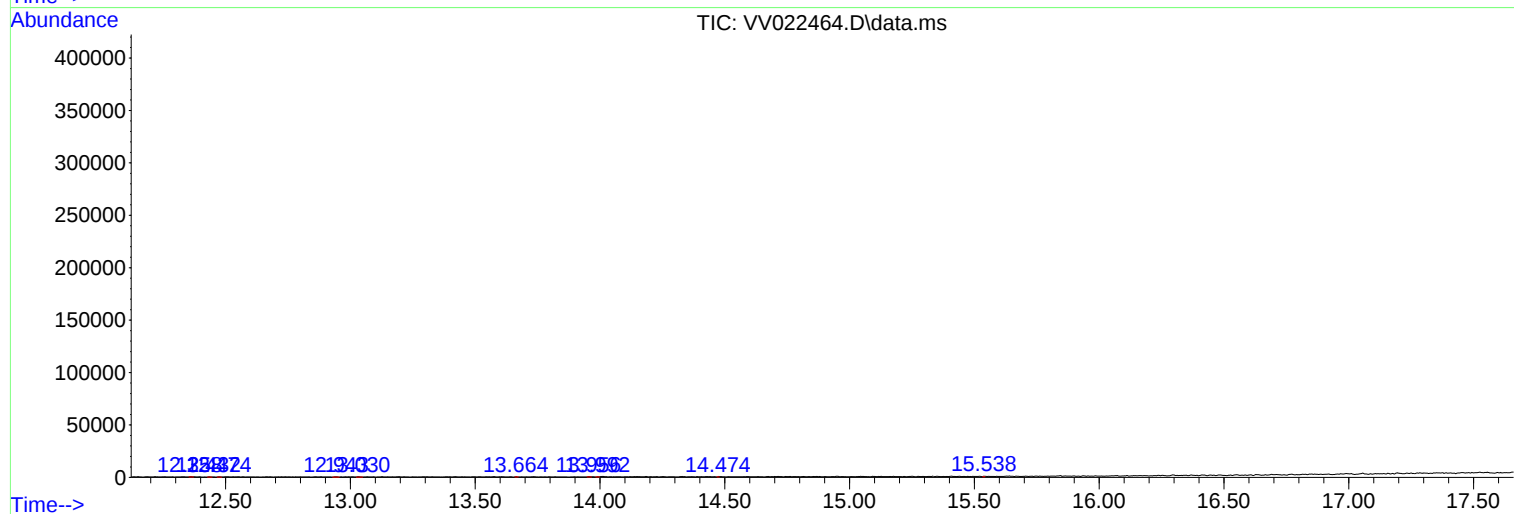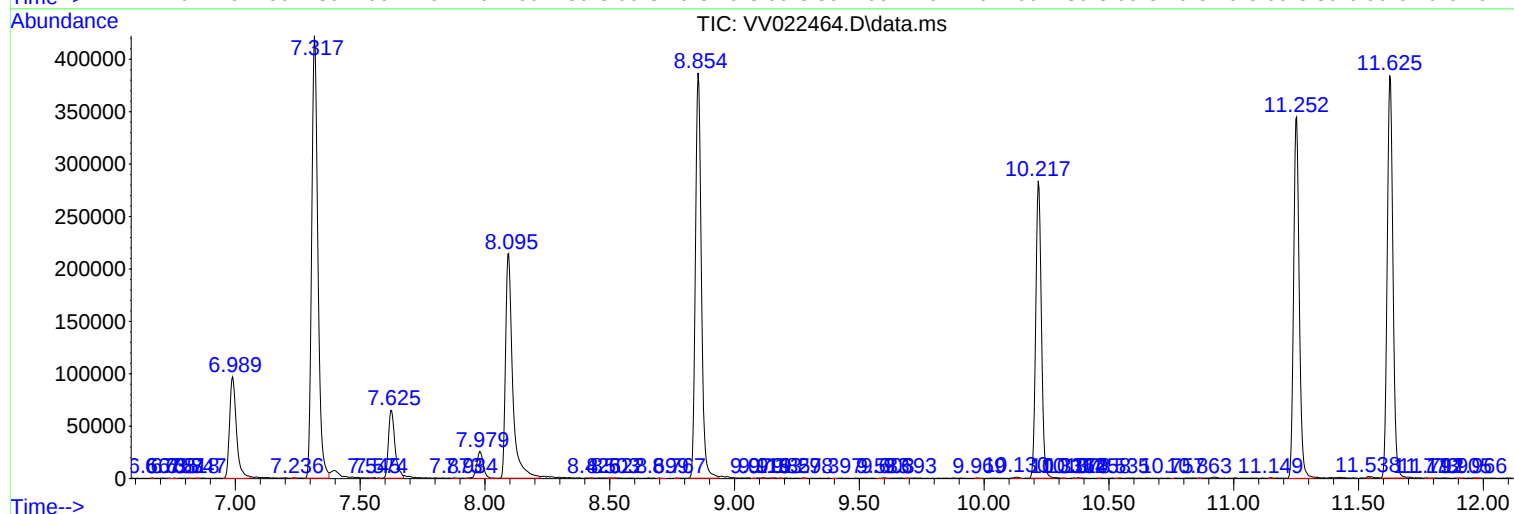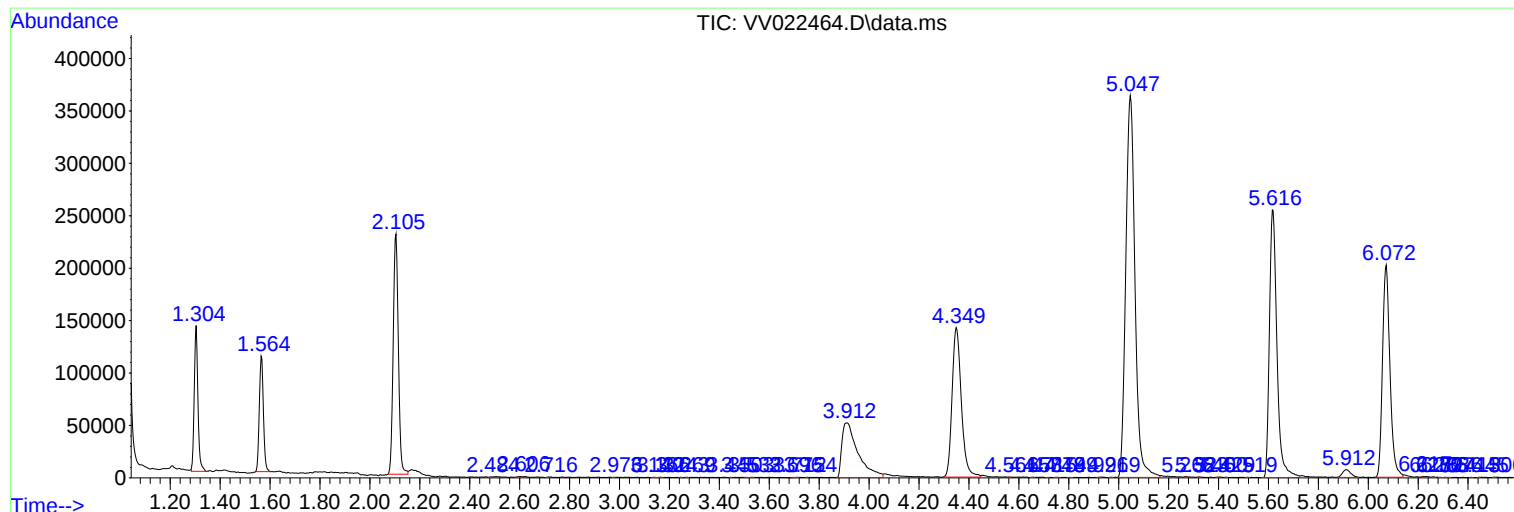

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
Data File : VV022464.D
Acq On : 01 Oct 2021 04:30
Operator : SY/MD
Sample : M3996-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A38

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
Data File : VV022464.D
Acq On : 01 Oct 2021 04:30
Operator : SY/MD
Sample : M3996-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A38

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------