

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
 Data File : VV022465.D
 Acq On : 01 Oct 2021 04:54
 Operator : SY/MD
 Sample : M3996-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A41

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

Signal : TIC: VV022465.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	93	rVB	132656	130540	5.96%	1.466%
2	1.565	157	163	184	rVB	109452	126275	5.77%	1.418%
3	2.105	321	331	347	rBV	222195	322028	14.71%	3.616%
4	2.622	481	492	502	rVB5	2162	4610	0.21%	0.052%
5	2.770	525	538	553	rBV3	12063	26540	1.21%	0.298%
6	2.854	562	564	566	rBV3	281	124	0.01%	0.001%
7	2.970	597	600	603	rBV	274	233	0.01%	0.003%
8	3.015	611	614	615	rBV	242	147	0.01%	0.002%
9	3.163	658	660	665	rBV2	259	169	0.01%	0.002%
10	3.214	673	676	680	rVB2	350	232	0.01%	0.003%
11	3.494	762	763	764	rBV2	305	96	0.00%	0.001%
12	3.597	790	795	797	rBV2	308	263	0.01%	0.003%
13	3.699	825	827	831	rVB	324	234	0.01%	0.003%
14	3.841	868	871	874	rBV2	202	101	0.00%	0.001%
15	3.905	879	891	943	rBV2	59513	257059	11.74%	2.887%
16	4.349	1015	1029	1056	rBV	138642	343860	15.71%	3.861%
17	4.728	1145	1147	1153	rVB4	336	246	0.01%	0.003%
18	4.818	1172	1175	1176	rBV	189	91	0.00%	0.001%
19	4.928	1208	1209	1212	rBV	257	119	0.01%	0.001%
20	4.963	1217	1220	1226	rVB2	397	312	0.01%	0.004%
21	5.047	1229	1246	1288	rBV2	353316	891171	40.70%	10.008%
22	5.439	1365	1368	1370	rBV2	294	195	0.01%	0.002%
23	5.487	1381	1383	1386	rBV2	354	244	0.01%	0.003%
24	5.506	1386	1389	1392	rVV2	254	218	0.01%	0.002%
25	5.551	1401	1403	1406	rVB2	286	150	0.01%	0.002%
26	5.616	1412	1423	1449	rBV	258341	523727	23.92%	5.881%
27	5.851	1493	1496	1498	rVB	353	153	0.01%	0.002%
28	5.863	1498	1500	1502	rBV	308	120	0.01%	0.001%
29	5.918	1504	1517	1542	rVV4	45327	102967	4.70%	1.156%
30	6.072	1551	1565	1590	rBV	191499	399035	18.23%	4.481%
31	6.285	1627	1631	1635	rBV3	723	515	0.02%	0.006%
32	6.307	1635	1638	1639	rVB2	201	87	0.00%	0.001%
33	6.381	1659	1661	1664	rVB	320	204	0.01%	0.002%
34	6.400	1664	1667	1674	rBV3	359	345	0.02%	0.004%
35	6.426	1674	1675	1677	rBV3	205	79	0.00%	0.001%
36	6.545	1708	1712	1713	rBV	402	226	0.01%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
 Data File : VV022465.D
 Acq On : 01 Oct 2021 04:54
 Operator : SY/MD
 Sample : M3996-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A41

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

37	6.593	1723	1727	1728	rBV2	290	132	0.01%	0.001%
38	6.625	1733	1737	1740	rVV2	302	196	0.01%	0.002%
39	6.728	1766	1769	1770	rBV2	461	196	0.01%	0.002%
40	6.838	1801	1803	1811	rBV2	246	315	0.01%	0.004%
41	6.989	1839	1850	1868	rBV	91562	171040	7.81%	1.921%
42	7.252	1930	1932	1935	rBV2	364	177	0.01%	0.002%
43	7.268	1935	1937	1939	rBV	297	129	0.01%	0.001%
44	7.317	1940	1952	1971	rBV	400112	695187	31.75%	7.807%
45	7.561	2026	2028	2030	rBV3	357	171	0.01%	0.002%
46	7.625	2038	2048	2069	rBV2	64275	113857	5.20%	1.279%
47	7.825	2108	2110	2111	rBV	338	112	0.01%	0.001%
48	7.902	2131	2134	2136	rBV	382	166	0.01%	0.002%
49	7.976	2141	2157	2176	rBV	1310901	2189411	100.00%	24.586%
50	8.092	2184	2193	2227	rVB	211648	397403	18.15%	4.463%
51	8.461	2306	2308	2312	rBV2	367	264	0.01%	0.003%
52	8.516	2323	2325	2328	rVB	284	110	0.01%	0.001%
53	8.690	2375	2379	2380	rBV	403	312	0.01%	0.004%
54	8.796	2411	2412	2413	rBV	237	81	0.00%	0.001%
55	8.854	2419	2430	2451	rBV	388930	633690	28.94%	7.116%
56	9.088	2501	2503	2504	rVB2	426	118	0.01%	0.001%
57	9.146	2516	2521	2523	rBV2	634	474	0.02%	0.005%
58	9.207	2535	2540	2542	rBV2	302	344	0.02%	0.004%
59	9.256	2553	2555	2562	rVB3	520	382	0.02%	0.004%
60	9.288	2562	2565	2567	rBV2	395	198	0.01%	0.002%
61	9.384	2594	2595	2599	rVB	311	127	0.01%	0.001%
62	9.555	2646	2648	2653	rVB	325	149	0.01%	0.002%
63	9.683	2685	2688	2694	rBV3	518	515	0.02%	0.006%
64	9.757	2709	2711	2712	rBV3	206	108	0.00%	0.001%
65	9.799	2720	2724	2725	rBV	319	163	0.01%	0.002%
66	9.831	2733	2734	2736	rBV	234	93	0.00%	0.001%
67	9.937	2765	2767	2770	rBV	204	124	0.01%	0.001%
68	9.992	2781	2784	2785	rBV	157	90	0.00%	0.001%
69	10.217	2841	2854	2876	rBV	271985	425710	19.44%	4.781%
70	10.384	2902	2906	2913	rVB4	865	1019	0.05%	0.011%
71	10.538	2952	2954	2956	rBV	349	191	0.01%	0.002%
72	10.577	2962	2966	2968	rBV3	425	295	0.01%	0.003%
73	10.600	2971	2973	2976	rBV2	331	213	0.01%	0.002%
74	10.664	2991	2993	2995	rVB	307	108	0.00%	0.001%
75	10.751	3016	3020	3021	rBV	176	115	0.01%	0.001%
76	10.764	3021	3024	3026	rVV	324	140	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
 Data File : VV022465.D
 Acq On : 01 Oct 2021 04:54
 Operator : SY/MD
 Sample : M3996-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A41

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

77	10.892	3062	3064	3065	rBV	273	96	0.00%	0.001%
78	10.915	3068	3071	3075	rVV3	977	845	0.04%	0.009%
79	11.008	3095	3100	3103	rBV2	278	327	0.01%	0.004%
80	11.034	3107	3108	3109	rBV	256	82	0.00%	0.001%
81	11.153	3140	3145	3146	rBV2	514	418	0.02%	0.005%
82	11.249	3164	3175	3193	rBV	340602	542865	24.80%	6.096%
83	11.548	3266	3268	3271	rVB2	488	232	0.01%	0.003%
84	11.625	3280	3292	3309	rBV	369542	589500	26.93%	6.620%
85	11.834	3354	3357	3360	rBV3	319	256	0.01%	0.003%
86	11.921	3378	3384	3388	rBV2	584	636	0.03%	0.007%
87	12.349	3515	3517	3525	rVB3	613	458	0.02%	0.005%
88	12.381	3525	3527	3528	rBV	269	91	0.00%	0.001%
89	12.455	3548	3550	3553	rVB2	276	126	0.01%	0.001%
90	12.500	3563	3564	3568	rBV3	340	206	0.01%	0.002%
91	12.574	3585	3587	3589	rVB2	311	141	0.01%	0.002%
92	12.706	3625	3628	3631	rVB2	333	254	0.01%	0.003%
93	12.731	3631	3636	3640	rBV3	383	412	0.02%	0.005%
94	12.767	3645	3647	3649	rBV	277	117	0.01%	0.001%
95	12.831	3664	3667	3670	rVB	206	102	0.00%	0.001%
96	13.062	3736	3739	3741	rBV	474	238	0.01%	0.003%
97	13.175	3768	3774	3777	rBV2	394	470	0.02%	0.005%
98	13.374	3833	3836	3840	rBV	191	190	0.01%	0.002%
99	14.284	4117	4119	4121	rBV2	304	116	0.01%	0.001%
100	14.329	4128	4133	4136	rBV2	463	468	0.02%	0.005%




Sum of corrected areas: 8904986

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
Data File : VV022465.D
Acq On : 01 Oct 2021 04:54
Operator : SY/MD
Sample : M3996-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A41

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

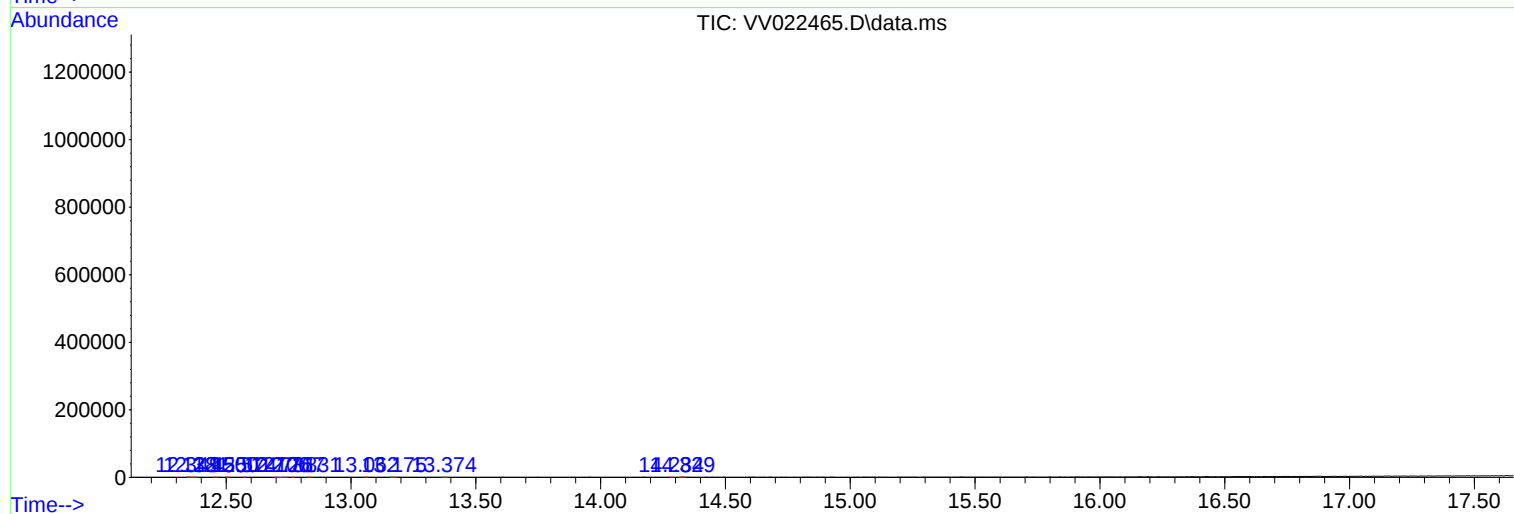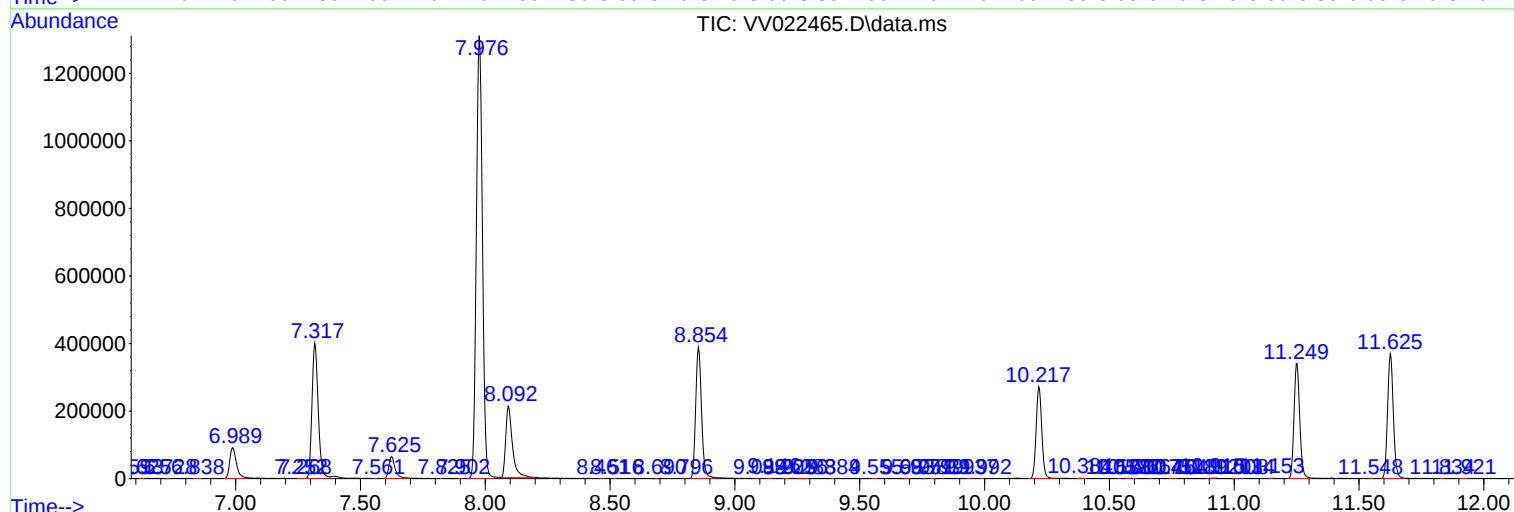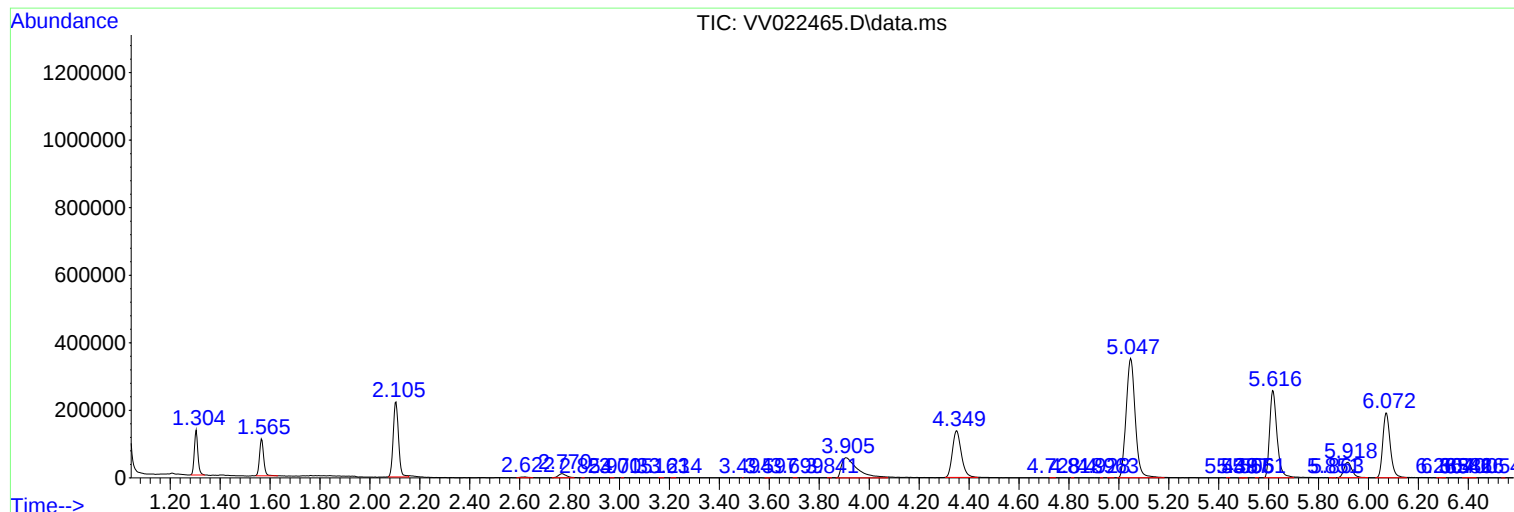

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
Data File : VV022465.D
Acq On : 01 Oct 2021 04:54
Operator : SY/MD
Sample : M3996-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A41

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
Data File : VV022465.D
Acq On : 01 Oct 2021 04:54
Operator : SY/MD
Sample : M3996-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A41

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
