

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
 Data File : VV022466.D
 Acq On : 01 Oct 2021 05:18
 Operator : SY/MD
 Sample : M3997-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A47

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

Signal : TIC: VV022466.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	77	82	89	rBV	128312	130952	15.00%	1.849%
2	2.105	323	331	345	rVB	228162	338297	38.75%	4.776%
3	2.761	523	535	561	rBV2	91981	182021	20.85%	2.570%
4	3.288	696	699	702	rBV2	393	217	0.02%	0.003%
5	3.362	718	722	724	rVB2	254	183	0.02%	0.003%
6	3.391	729	731	736	rVV2	250	122	0.01%	0.002%
7	3.429	742	743	746	rBV	189	112	0.01%	0.002%
8	3.545	778	779	783	rVB	281	100	0.01%	0.001%
9	3.619	798	802	806	rVB3	299	224	0.03%	0.003%
10	3.667	815	817	821	rBV2	257	93	0.01%	0.001%
11	3.735	835	838	842	rBV2	291	220	0.03%	0.003%
12	3.764	845	847	851	rVV	375	210	0.02%	0.003%
13	3.876	871	882	923	rBV4	75288	287028	32.88%	4.052%
14	4.349	1014	1029	1055	rBV	136664	339714	38.91%	4.796%
15	4.770	1158	1160	1164	rVB	347	230	0.03%	0.003%
16	4.786	1164	1165	1168	rBV2	332	214	0.02%	0.003%
17	4.934	1207	1211	1212	rBV	459	280	0.03%	0.004%
18	4.944	1212	1214	1218	rVV	362	289	0.03%	0.004%
19	5.047	1229	1246	1275	rBV2	338298	873087	100.00%	12.326%
20	5.330	1333	1334	1338	rVB	477	204	0.02%	0.003%
21	5.490	1382	1384	1387	rVV2	279	106	0.01%	0.001%
22	5.532	1396	1397	1402	rBV2	291	163	0.02%	0.002%
23	5.616	1405	1423	1448	rBV	252912	516174	59.12%	7.287%
24	5.905	1507	1513	1534	rVB5	9352	21344	2.44%	0.301%
25	6.069	1550	1564	1589	rBV2	191660	396272	45.39%	5.595%
26	6.355	1650	1653	1654	rBV	361	176	0.02%	0.002%
27	6.400	1665	1667	1672	rVB2	415	229	0.03%	0.003%
28	6.448	1679	1682	1683	rBV	156	103	0.01%	0.001%
29	6.580	1719	1723	1726	rBV3	664	586	0.07%	0.008%
30	6.686	1752	1756	1758	rBV3	480	276	0.03%	0.004%
31	6.706	1760	1762	1764	rBV	240	109	0.01%	0.002%
32	6.831	1799	1801	1802	rVB	331	108	0.01%	0.002%
33	6.847	1802	1806	1808	rBV	361	189	0.02%	0.003%
34	6.944	1833	1836	1837	rBV	239	111	0.01%	0.002%
35	6.989	1839	1850	1871	rVV	88668	164712	18.87%	2.325%
36	7.204	1914	1917	1918	rBV	404	241	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
 Data File : VV022466.D
 Acq On : 01 Oct 2021 05:18
 Operator : SY/MD
 Sample : M3997-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A47

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

37	7.272	1936	1938	1940	rBV	379	187	0.02%	0.003%
38	7.317	1940	1952	1971	rBV	392723	685956	78.57%	9.684%
39	7.625	2038	2048	2065	rBV	59923	106433	12.19%	1.503%
40	7.792	2098	2100	2102	rBV3	384	205	0.02%	0.003%
41	7.828	2108	2111	2113	rBV3	233	127	0.01%	0.002%
42	7.860	2119	2121	2122	rBV3	336	139	0.02%	0.002%
43	7.892	2129	2131	2133	rBV	246	155	0.02%	0.002%
44	7.931	2141	2143	2145	rBV	316	162	0.02%	0.002%
45	7.976	2145	2157	2176	rVV	265485	449379	51.47%	6.344%
46	8.088	2183	2192	2227	rBV	185159	361689	41.43%	5.106%
47	8.471	2309	2311	2314	rBV2	424	213	0.02%	0.003%
48	8.506	2320	2322	2325	rVV3	307	121	0.01%	0.002%
49	8.529	2325	2329	2332	rVB3	460	363	0.04%	0.005%
50	8.625	2357	2359	2360	rBV3	292	93	0.01%	0.001%
51	8.722	2387	2389	2394	rVB2	412	336	0.04%	0.005%
52	8.767	2401	2403	2408	rVB2	204	98	0.01%	0.001%
53	8.792	2408	2411	2414	rVB2	308	205	0.02%	0.003%
54	8.812	2414	2417	2418	rBV	351	201	0.02%	0.003%
55	8.854	2418	2430	2455	rBV	385139	626950	71.81%	8.851%
56	9.143	2516	2520	2521	rBV	647	350	0.04%	0.005%
57	9.194	2534	2536	2538	rVV2	243	102	0.01%	0.001%
58	9.226	2544	2546	2547	rBV	597	289	0.03%	0.004%
59	9.358	2585	2587	2588	rBV	287	116	0.01%	0.002%
60	9.423	2604	2607	2610	rBV2	191	157	0.02%	0.002%
61	9.545	2643	2645	2647	rBV2	514	222	0.03%	0.003%
62	9.702	2692	2694	2699	rVB3	359	231	0.03%	0.003%
63	9.731	2701	2703	2706	rVB2	303	108	0.01%	0.002%
64	9.757	2706	2711	2712	rBV2	305	183	0.02%	0.003%
65	9.834	2733	2735	2738	rBV	340	155	0.02%	0.002%
66	9.860	2742	2743	2744	rBV	361	99	0.01%	0.001%
67	9.956	2771	2773	2775	rBV	274	121	0.01%	0.002%
68	10.014	2781	2791	2807	rBV2	4415	9015	1.03%	0.127%
69	10.130	2819	2827	2830	rBV4	1845	2351	0.27%	0.033%
70	10.217	2842	2854	2876	rBV	262633	413567	47.37%	5.839%
71	10.487	2935	2938	2940	rBV2	185	152	0.02%	0.002%
72	10.567	2960	2963	2965	rBV2	375	277	0.03%	0.004%
73	10.580	2965	2967	2969	rVB	357	160	0.02%	0.002%
74	10.648	2985	2988	2990	rBV	197	111	0.01%	0.002%
75	10.664	2990	2993	2995	rBV2	413	254	0.03%	0.004%
76	10.738	3015	3016	3019	rVB2	248	100	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
 Data File : VV022466.D
 Acq On : 01 Oct 2021 05:18
 Operator : SY/MD
 Sample : M3997-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A47

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

77	10.770	3023	3026	3027	rBV	305	141	0.02%	0.002%
78	10.805	3035	3037	3038	rBV	365	143	0.02%	0.002%
79	10.879	3059	3060	3064	rVB	238	121	0.01%	0.002%
80	10.915	3064	3071	3083	rVB6	1316	2195	0.25%	0.031%
81	10.995	3094	3096	3100	rBV2	214	86	0.01%	0.001%
82	11.040	3105	3110	3113	rBV3	360	350	0.04%	0.005%
83	11.201	3158	3160	3162	rBV	210	110	0.01%	0.002%
84	11.249	3164	3175	3197	rVV	350305	547105	62.66%	7.724%
85	11.458	3237	3240	3243	rBV2	451	309	0.04%	0.004%
86	11.474	3243	3245	3251	rVV3	481	400	0.05%	0.006%
87	11.506	3253	3255	3257	rBV2	295	146	0.02%	0.002%
88	11.529	3260	3262	3264	rVV2	311	126	0.01%	0.002%
89	11.625	3279	3292	3311	rVV	384600	605326	69.33%	8.546%
90	11.969	3395	3399	3401	rBV	283	224	0.03%	0.003%
91	12.130	3447	3449	3453	rVB2	547	245	0.03%	0.003%
92	12.619	3599	3601	3605	rBV2	441	265	0.03%	0.004%
93	12.754	3638	3643	3646	rBV3	371	373	0.04%	0.005%
94	12.924	3693	3696	3699	rBV3	321	208	0.02%	0.003%
95	12.966	3707	3709	3712	rBV2	303	111	0.01%	0.002%
96	12.985	3712	3715	3717	rBV2	311	181	0.02%	0.003%
97	13.545	3887	3889	3890	rBV	277	114	0.01%	0.002%
98	14.400	4153	4155	4156	rBV	350	106	0.01%	0.001%
99	15.217	4407	4409	4413	rVB2	641	336	0.04%	0.005%
100	16.184	4703	4710	4718	rVB8	5982	8592	0.98%	0.121%




Sum of corrected areas: 7083141

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
Data File : VV022466.D
Acq On : 01 Oct 2021 05:18
Operator : SY/MD
Sample : M3997-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A47

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

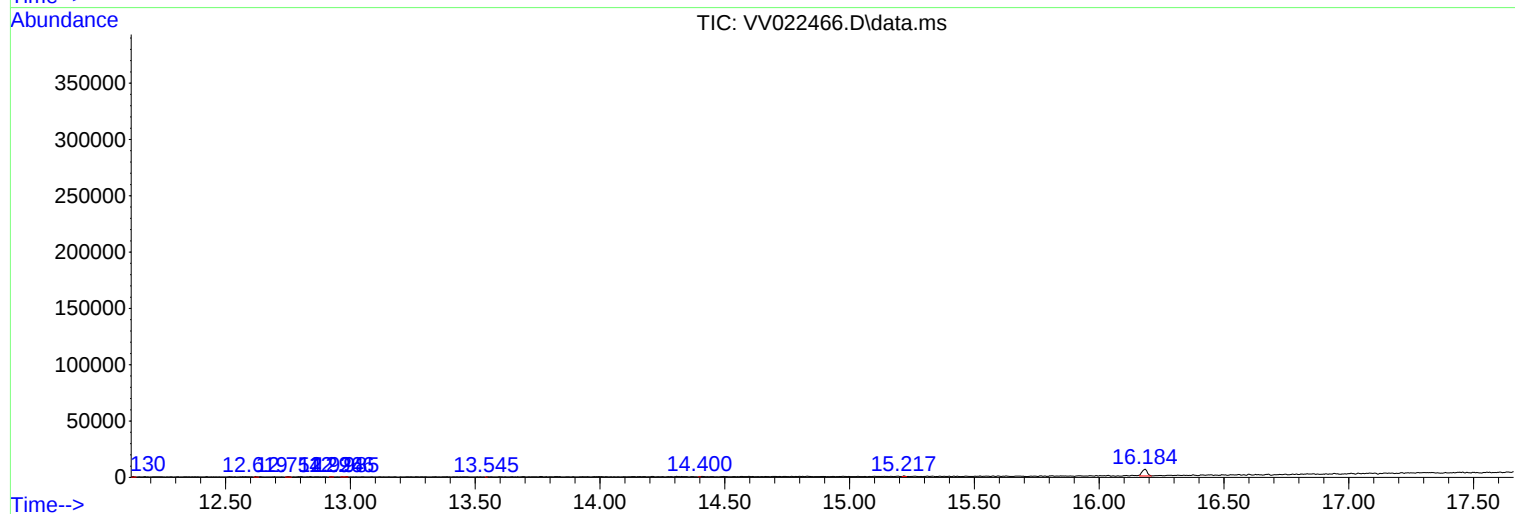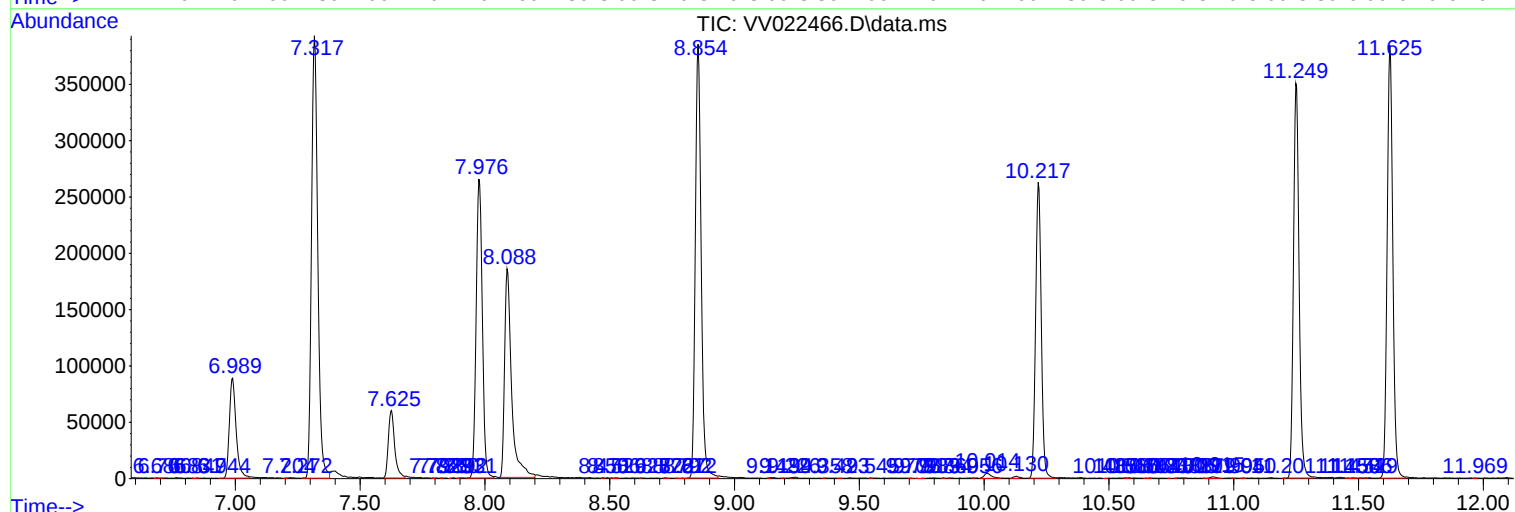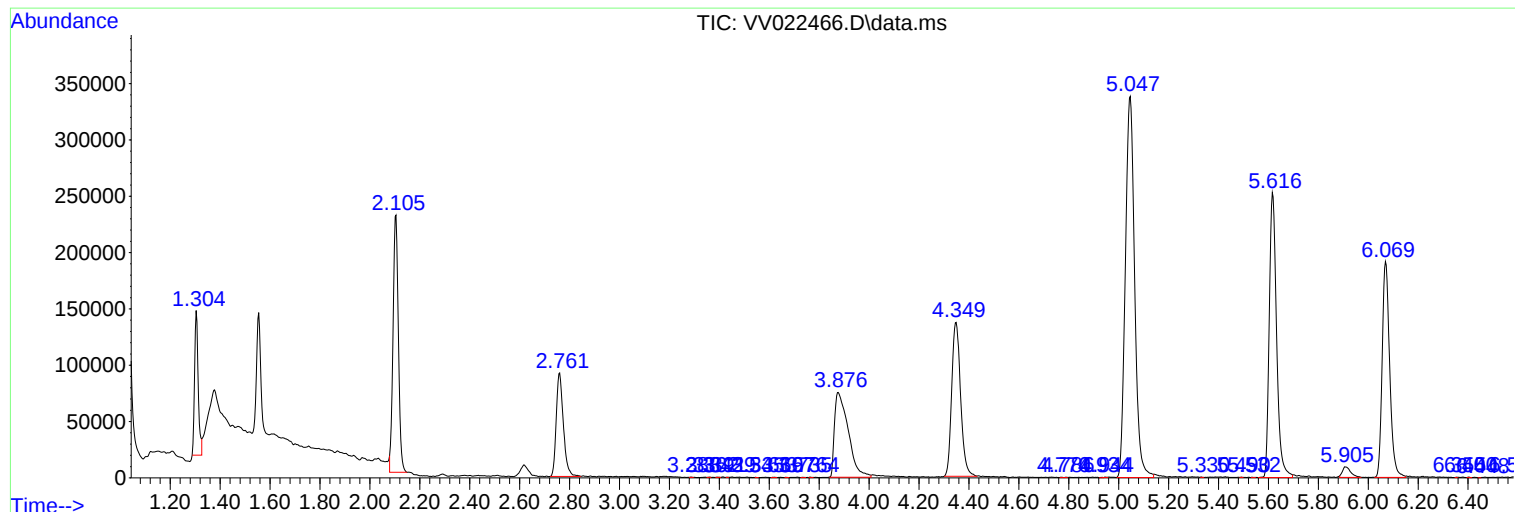

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
Data File : VV022466.D
Acq On : 01 Oct 2021 05:18
Operator : SY/MD
Sample : M3997-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A47

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
Data File : VV022466.D
Acq On : 01 Oct 2021 05:18
Operator : SY/MD
Sample : M3997-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A47

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
