

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
 Data File : VV022467.D
 Acq On : 01 Oct 2021 05:41
 Operator : SY/MD
 Sample : M3997-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A48

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

Signal : TIC: VV022467.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	77	82	97	rVB	129927	134433	5.79%	1.494%
2	1.564	158	163	179	rVB	107599	122334	5.27%	1.359%
3	2.101	321	330	342	rVB	223655	317134	13.66%	3.524%
4	2.500	451	454	456	rBV3	776	579	0.02%	0.006%
5	2.616	479	490	509	rBV	11178	23666	1.02%	0.263%
6	2.928	584	587	593	rBV2	390	278	0.01%	0.003%
7	3.011	610	613	617	rBV2	335	238	0.01%	0.003%
8	3.304	702	704	706	rBV2	165	118	0.01%	0.001%
9	3.352	716	719	723	rBV2	247	204	0.01%	0.002%
10	3.452	748	750	752	rBV2	308	123	0.01%	0.001%
11	3.481	756	759	760	rBV2	283	116	0.00%	0.001%
12	3.625	801	804	805	rBV	365	155	0.01%	0.002%
13	3.712	827	831	835	rBV3	350	260	0.01%	0.003%
14	3.773	846	850	851	rBV	334	204	0.01%	0.002%
15	3.912	881	893	927	rBV3	50820	221197	9.53%	2.458%
16	4.349	1013	1029	1058	rBV	141245	354846	15.29%	3.943%
17	4.577	1099	1100	1104	rBV	338	217	0.01%	0.002%
18	4.648	1120	1122	1124	rBV2	481	241	0.01%	0.003%
19	4.715	1138	1143	1148	rBV	528	536	0.02%	0.006%
20	4.770	1157	1160	1162	rVV3	314	185	0.01%	0.002%
21	4.796	1165	1168	1170	rBV2	184	123	0.01%	0.001%
22	4.841	1180	1182	1186	rVB3	294	160	0.01%	0.002%
23	4.902	1197	1201	1204	rBV2	298	218	0.01%	0.002%
24	4.985	1225	1227	1229	rBV	289	167	0.01%	0.002%
25	5.047	1229	1246	1274	rBV2	359050	902853	38.90%	10.031%
26	5.410	1356	1359	1363	rVB	403	241	0.01%	0.003%
27	5.461	1372	1375	1378	rBV	398	204	0.01%	0.002%
28	5.571	1406	1409	1411	rBV	588	350	0.02%	0.004%
29	5.616	1411	1423	1449	rBV	263251	533382	22.98%	5.926%
30	5.908	1505	1514	1515	rBV4	6714	6864	0.30%	0.076%
31	6.069	1551	1564	1593	rBV	193605	406512	17.51%	4.517%
32	6.201	1603	1605	1607	rBV2	423	152	0.01%	0.002%
33	6.384	1660	1662	1666	rVB2	322	200	0.01%	0.002%
34	6.432	1673	1677	1679	rBV2	196	124	0.01%	0.001%
35	6.545	1709	1712	1715	rBV2	286	200	0.01%	0.002%
36	6.651	1743	1745	1748	rBV2	505	203	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
 Data File : VV022467.D
 Acq On : 01 Oct 2021 05:41
 Operator : SY/MD
 Sample : M3997-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A48

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

37	6.670	1748	1751	1752	rBV	379	264	0.01%	0.003%
38	6.731	1767	1770	1772	rBV2	231	118	0.01%	0.001%
39	6.837	1799	1803	1804	rBV	215	145	0.01%	0.002%
40	6.854	1806	1808	1811	rVV2	301	166	0.01%	0.002%
41	6.876	1813	1815	1819	rVB2	358	202	0.01%	0.002%
42	6.989	1838	1850	1874	rBV	94051	176019	7.58%	1.956%
43	7.191	1911	1913	1915	rBV	363	131	0.01%	0.001%
44	7.230	1923	1925	1927	rBV	246	114	0.00%	0.001%
45	7.317	1941	1952	1972	rBV	403984	703914	30.33%	7.821%
46	7.625	2035	2048	2065	rBV	64258	115194	4.96%	1.280%
47	7.812	2104	2106	2109	rBV2	321	167	0.01%	0.002%
48	7.895	2127	2132	2133	rBV	419	267	0.01%	0.003%
49	7.976	2137	2157	2183	rVV	1376335	2321012	100.00%	25.788%
50	8.095	2185	2194	2233	rVB	207180	402810	17.35%	4.475%
51	8.435	2298	2300	2304	rBV3	432	189	0.01%	0.002%
52	8.503	2316	2321	2323	rBV3	580	572	0.02%	0.006%
53	8.670	2371	2373	2379	rBV4	350	284	0.01%	0.003%
54	8.776	2403	2406	2407	rBV2	305	191	0.01%	0.002%
55	8.853	2418	2430	2452	rBV	395736	647677	27.90%	7.196%
56	9.072	2497	2498	2501	rBV2	355	136	0.01%	0.002%
57	9.146	2517	2521	2528	rBV2	672	833	0.04%	0.009%
58	9.252	2552	2554	2556	rVB	300	125	0.01%	0.001%
59	9.313	2570	2573	2574	rBV	379	194	0.01%	0.002%
60	9.374	2589	2592	2595	rBV3	467	255	0.01%	0.003%
61	9.622	2666	2669	2673	rBV2	234	169	0.01%	0.002%
62	9.670	2682	2684	2690	rBV2	241	167	0.01%	0.002%
63	9.718	2697	2699	2704	rVB2	353	252	0.01%	0.003%
64	9.760	2711	2712	2715	rBV	241	107	0.00%	0.001%
65	9.844	2734	2738	2739	rBV	450	283	0.01%	0.003%
66	9.898	2753	2755	2759	rBV	298	172	0.01%	0.002%
67	10.101	2815	2818	2820	rBV2	268	145	0.01%	0.002%
68	10.130	2820	2827	2828	rBV3	1099	1000	0.04%	0.011%
69	10.217	2840	2854	2870	rBV	277862	433851	18.69%	4.820%
70	10.384	2905	2906	2911	rVB2	567	375	0.02%	0.004%
71	10.580	2961	2967	2969	rBV	386	340	0.01%	0.004%
72	10.741	3015	3017	3019	rBV2	374	105	0.00%	0.001%
73	10.831	3042	3045	3047	rBV2	340	225	0.01%	0.002%
74	10.914	3067	3071	3074	rBV3	744	694	0.03%	0.008%
75	11.001	3096	3098	3106	rBV	296	334	0.01%	0.004%
76	11.249	3164	3175	3195	rBV	350891	547648	23.60%	6.085%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
 Data File : VV022467.D
 Acq On : 01 Oct 2021 05:41
 Operator : SY/MD
 Sample : M3997-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A48

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M

Title : VOC Analysis

77	11.625	3279	3292	3316	rBV	378404	605957	26.11%	6.733%
78	11.995	3405	3407	3410	rBV	297	219	0.01%	0.002%
79	12.104	3438	3441	3445	rVB3	363	273	0.01%	0.003%
80	12.210	3472	3474	3481	rVB2	315	236	0.01%	0.003%
81	12.239	3481	3483	3486	rBV2	424	236	0.01%	0.003%
82	12.348	3514	3517	3518	rBV2	500	193	0.01%	0.002%
83	12.435	3541	3544	3546	rBV	305	155	0.01%	0.002%
84	12.516	3566	3569	3574	rBV3	317	170	0.01%	0.002%
85	12.725	3630	3634	3635	rBV	625	425	0.02%	0.005%
86	12.850	3670	3673	3676	rBV	199	120	0.01%	0.001%
87	13.056	3734	3737	3739	rBV2	294	222	0.01%	0.002%
88	13.159	3763	3769	3778	rVB7	2371	3334	0.14%	0.037%
89	13.323	3817	3820	3822	rBV2	330	172	0.01%	0.002%
90	13.410	3845	3847	3851	rBV2	291	201	0.01%	0.002%
91	13.438	3854	3856	3858	rVB2	401	137	0.01%	0.002%
92	13.464	3858	3864	3870	rBV3	456	655	0.03%	0.007%
93	13.548	3888	3890	3892	rBV	256	112	0.00%	0.001%
94	13.593	3902	3904	3906	rBV2	455	222	0.01%	0.002%
95	13.606	3906	3908	3911	rBV2	245	101	0.00%	0.001%
96	13.750	3952	3953	3955	rBV2	309	116	0.00%	0.001%
97	13.789	3963	3965	3967	rBV2	212	103	0.00%	0.001%
98	13.844	3977	3982	3985	rBV3	472	505	0.02%	0.006%
99	13.863	3985	3988	3989	rBV2	448	239	0.01%	0.003%
100	14.133	4069	4072	4078	rVV3	386	395	0.02%	0.004%




Sum of corrected areas: 9000361

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
Data File : VV022467.D
Acq On : 01 Oct 2021 05:41
Operator : SY/MD
Sample : M3997-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A48

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

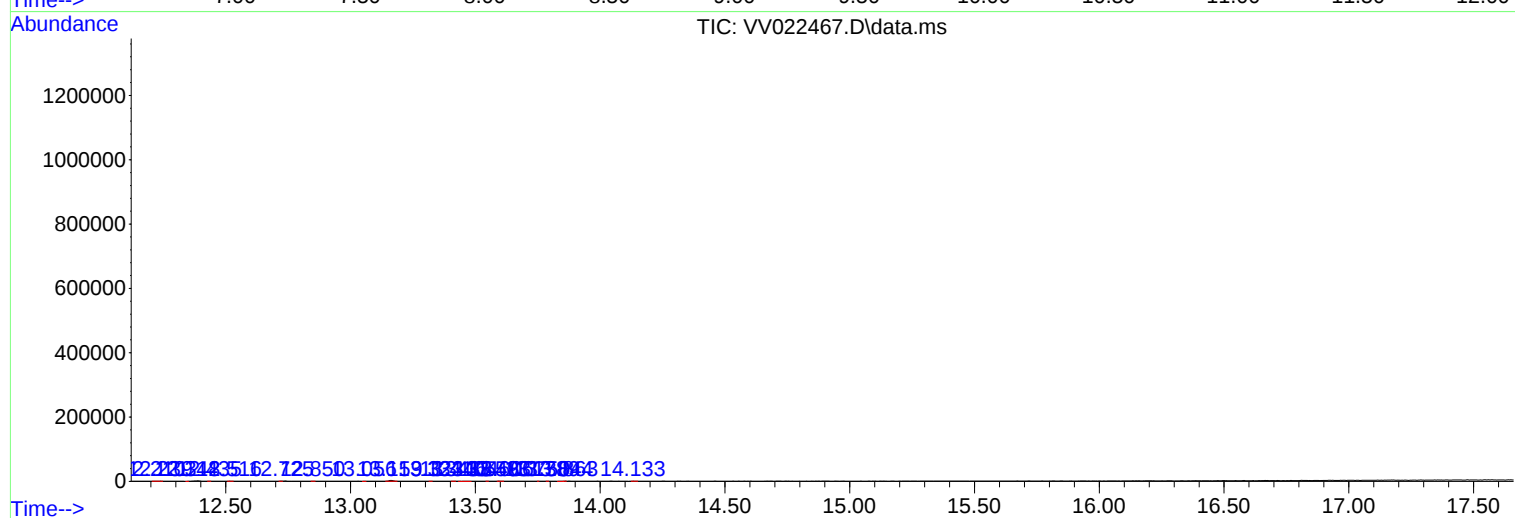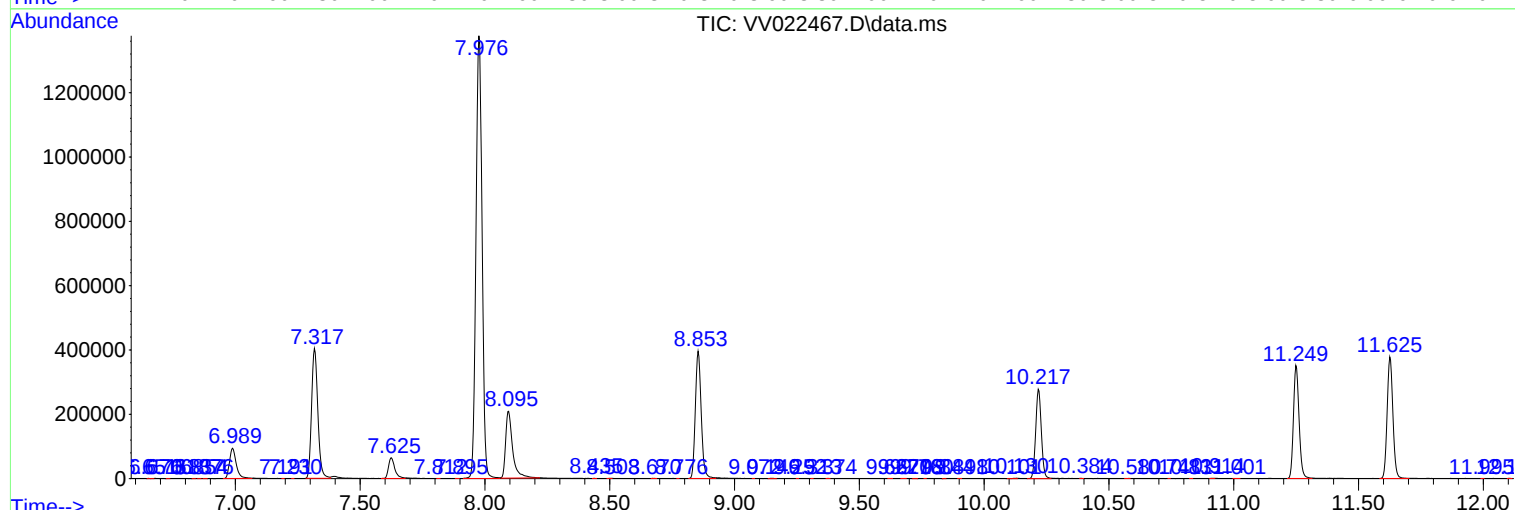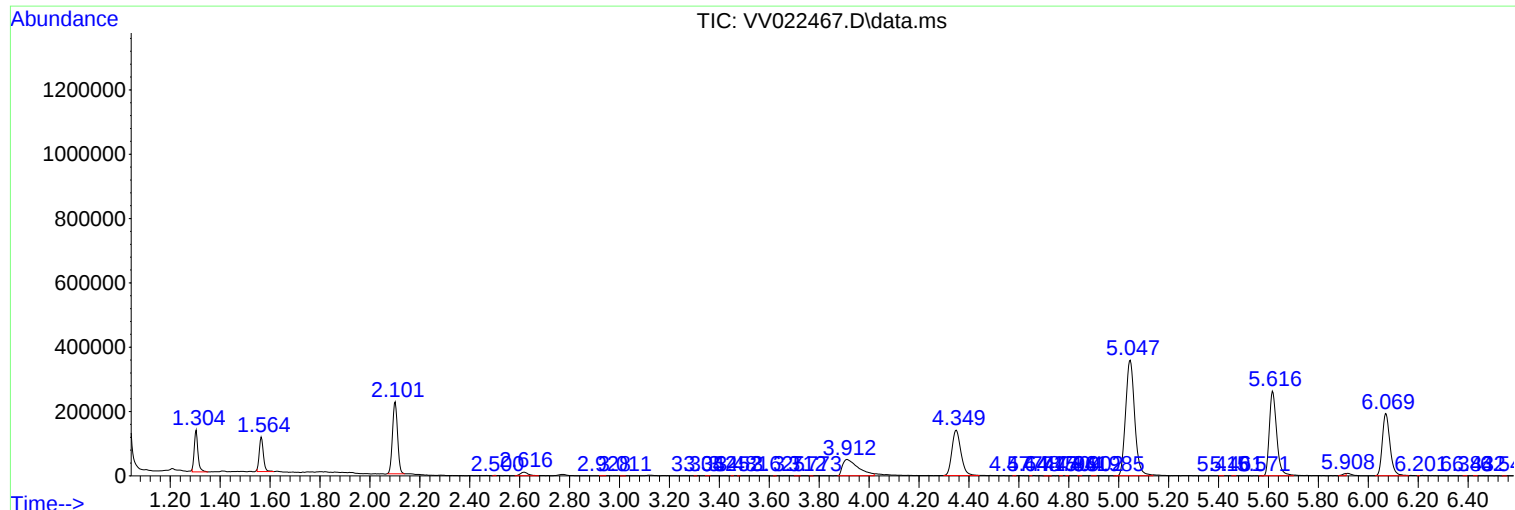

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
Data File : VV022467.D
Acq On : 01 Oct 2021 05:41
Operator : SY/MD
Sample : M3997-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A48

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
Data File : VV022467.D
Acq On : 01 Oct 2021 05:41
Operator : SY/MD
Sample : M3997-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A48

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------