

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
 Data File : VV022468.D
 Acq On : 01 Oct 2021 06:05
 Operator : SY/MD
 Sample : M3997-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A53

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M

Title : VOC Analysis

Signal : TIC: VV022468.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	77	82	94	rVB	122306	122273	3.56%	1.246%
2	1.542	151	156	172	rVB	101944	123130	3.58%	1.254%
3	2.101	320	330	347	rVB	209433	308476	8.98%	3.142%
4	2.327	398	400	401	rBV	422	150	0.00%	0.002%
5	2.503	450	455	460	rVB4	1076	907	0.03%	0.009%
6	2.532	460	464	468	rBV3	328	365	0.01%	0.004%
7	2.616	476	490	511	rBV2	21961	47277	1.38%	0.482%
8	2.844	557	561	563	rBV2	306	268	0.01%	0.003%
9	2.931	586	588	590	rBV	253	126	0.00%	0.001%
10	2.976	599	602	606	rBV	354	245	0.01%	0.002%
11	3.230	679	681	684	rBV	286	165	0.00%	0.002%
12	3.285	696	698	702	rBV	146	129	0.00%	0.001%
13	3.436	742	745	749	rBV2	240	177	0.01%	0.002%
14	3.516	767	770	772	rBV	505	256	0.01%	0.003%
15	3.626	801	804	810	rBV2	286	264	0.01%	0.003%
16	3.687	820	823	827	rBV	361	265	0.01%	0.003%
17	3.876	871	882	918	rBV3	72948	281598	8.19%	2.869%
18	4.346	1014	1028	1052	rBV2	130154	325352	9.47%	3.314%
19	4.613	1110	1111	1114	rBV	316	165	0.00%	0.002%
20	4.632	1115	1117	1121	rVB2	325	175	0.01%	0.002%
21	4.654	1121	1124	1128	rVB3	466	406	0.01%	0.004%
22	4.674	1128	1130	1134	rBV2	267	225	0.01%	0.002%
23	4.744	1150	1152	1155	rVB	331	166	0.00%	0.002%
24	4.773	1159	1161	1166	rVV	347	231	0.01%	0.002%
25	4.812	1169	1173	1176	rBV2	333	278	0.01%	0.003%
26	4.867	1188	1190	1194	rVB	331	158	0.00%	0.002%
27	4.886	1194	1196	1198	rBV2	283	139	0.00%	0.001%
28	4.937	1209	1212	1214	rBV	414	184	0.01%	0.002%
29	5.043	1229	1245	1269	rBV2	329605	834558	24.28%	8.502%
30	5.375	1345	1348	1349	rBV2	492	201	0.01%	0.002%
31	5.500	1385	1387	1391	rBV2	217	159	0.00%	0.002%
32	5.616	1412	1423	1443	rBV	243148	488395	14.21%	4.975%
33	5.918	1505	1517	1535	rVB8	9753	24640	0.72%	0.251%
34	6.069	1548	1564	1584	rBV	184152	378666	11.02%	3.858%
35	6.211	1606	1608	1611	rBV3	718	337	0.01%	0.003%
36	6.359	1649	1654	1657	rBV2	261	218	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
 Data File : VV022468.D
 Acq On : 01 Oct 2021 06:05
 Operator : SY/MD
 Sample : M3997-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A53

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

37	6.378	1657	1660	1663	rVB2	219	128	0.00%	0.001%
38	6.548	1710	1713	1716	rBV2	297	191	0.01%	0.002%
39	6.625	1735	1737	1740	rVB2	373	178	0.01%	0.002%
40	6.744	1772	1774	1777	rVB	416	227	0.01%	0.002%
41	6.815	1792	1796	1799	rBV3	324	270	0.01%	0.003%
42	6.863	1809	1811	1817	rVB2	451	299	0.01%	0.003%
43	6.928	1829	1831	1833	rBV	325	138	0.00%	0.001%
44	6.989	1838	1850	1872	rBV	86525	163668	4.76%	1.667%
45	7.214	1919	1920	1922	rBV2	410	161	0.00%	0.002%
46	7.317	1940	1952	1971	rBV	381899	661283	19.24%	6.737%
47	7.622	2037	2047	2073	rBV	59308	108201	3.15%	1.102%
48	7.976	2142	2157	2182	rBV	2039918	3436736	100.00%	35.010%
49	8.088	2184	2192	2222	rVB	200701	362408	10.55%	3.692%
50	8.465	2308	2309	2311	rBV2	344	136	0.00%	0.001%
51	8.600	2349	2351	2353	rBV2	379	164	0.00%	0.002%
52	8.648	2362	2366	2368	rBV3	303	227	0.01%	0.002%
53	8.686	2375	2378	2380	rBV2	314	158	0.00%	0.002%
54	8.773	2403	2405	2410	rVB3	500	369	0.01%	0.004%
55	8.854	2419	2430	2450	rBV	368507	601681	17.51%	6.129%
56	9.133	2514	2517	2520	rBV3	366	327	0.01%	0.003%
57	9.188	2531	2534	2536	rBV	329	218	0.01%	0.002%
58	9.301	2566	2569	2573	rBV2	298	244	0.01%	0.002%
59	9.400	2597	2600	2604	rVB2	334	247	0.01%	0.003%
60	9.423	2604	2607	2609	rBV	208	181	0.01%	0.002%
61	9.442	2609	2613	2617	rVV2	440	432	0.01%	0.004%
62	9.465	2618	2620	2623	rVV2	258	132	0.00%	0.001%
63	9.555	2645	2648	2652	rVB2	375	279	0.01%	0.003%
64	9.577	2652	2655	2657	rBV2	368	229	0.01%	0.002%
65	9.641	2673	2675	2678	rBV2	265	147	0.00%	0.001%
66	9.789	2719	2721	2726	rVB2	474	285	0.01%	0.003%
67	9.915	2755	2760	2762	rBV3	385	327	0.01%	0.003%
68	10.005	2784	2788	2791	rBV	355	307	0.01%	0.003%
69	10.165	2836	2838	2842	rVB2	372	156	0.00%	0.002%
70	10.217	2842	2854	2872	rBV	259608	407223	11.85%	4.148%
71	10.310	2881	2883	2886	rBV3	490	289	0.01%	0.003%
72	10.349	2891	2895	2899	rBV3	809	816	0.02%	0.008%
73	10.419	2915	2917	2924	rVB4	453	379	0.01%	0.004%
74	10.481	2933	2936	2939	rVB2	367	186	0.01%	0.002%
75	10.497	2939	2941	2946	rBV2	294	207	0.01%	0.002%
76	10.583	2963	2968	2972	rBV5	616	475	0.01%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
 Data File : VV022468.D
 Acq On : 01 Oct 2021 06:05
 Operator : SY/MD
 Sample : M3997-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A53

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

77	10.603	2972	2974	2978	rVV3	383	210	0.01%	0.002%
78	10.792	3031	3033	3036	rBV2	227	148	0.00%	0.002%
79	10.809	3036	3038	3041	rVV3	284	126	0.00%	0.001%
80	10.847	3046	3050	3055	rBV2	301	269	0.01%	0.003%
81	10.908	3065	3069	3070	rBV2	486	280	0.01%	0.003%
82	11.249	3164	3175	3194	rBV	341332	532150	15.48%	5.421%
83	11.484	3244	3248	3250	rBV3	279	195	0.01%	0.002%
84	11.532	3260	3263	3264	rBV	299	168	0.00%	0.002%
85	11.625	3280	3292	3314	rBV	375470	589201	17.14%	6.002%
86	11.976	3397	3401	3403	rBV3	344	234	0.01%	0.002%
87	12.143	3450	3453	3455	rBV2	284	184	0.01%	0.002%
88	12.249	3483	3486	3490	rBV2	223	158	0.00%	0.002%
89	12.284	3495	3497	3498	rBV2	301	153	0.00%	0.002%
90	12.329	3509	3511	3515	rBV	401	300	0.01%	0.003%
91	12.509	3564	3567	3571	rBV2	307	266	0.01%	0.003%
92	12.596	3592	3594	3596	rVB	360	141	0.00%	0.001%
93	12.886	3682	3684	3687	rBV2	295	131	0.00%	0.001%
94	12.947	3701	3703	3705	rVB	496	177	0.01%	0.002%
95	12.966	3705	3709	3711	rBV	244	211	0.01%	0.002%
96	13.281	3805	3807	3811	rVB2	343	122	0.00%	0.001%
97	13.403	3843	3845	3848	rBV	283	175	0.01%	0.002%
98	13.706	3937	3939	3943	rVB3	560	201	0.01%	0.002%
99	13.882	3992	3994	3998	rBV2	368	227	0.01%	0.002%
100	14.792	4272	4277	4280	rBV2	378	443	0.01%	0.005%




Sum of corrected areas: 9816303

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
Data File : VV022468.D
Acq On : 01 Oct 2021 06:05
Operator : SY/MD
Sample : M3997-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 52 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A53

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

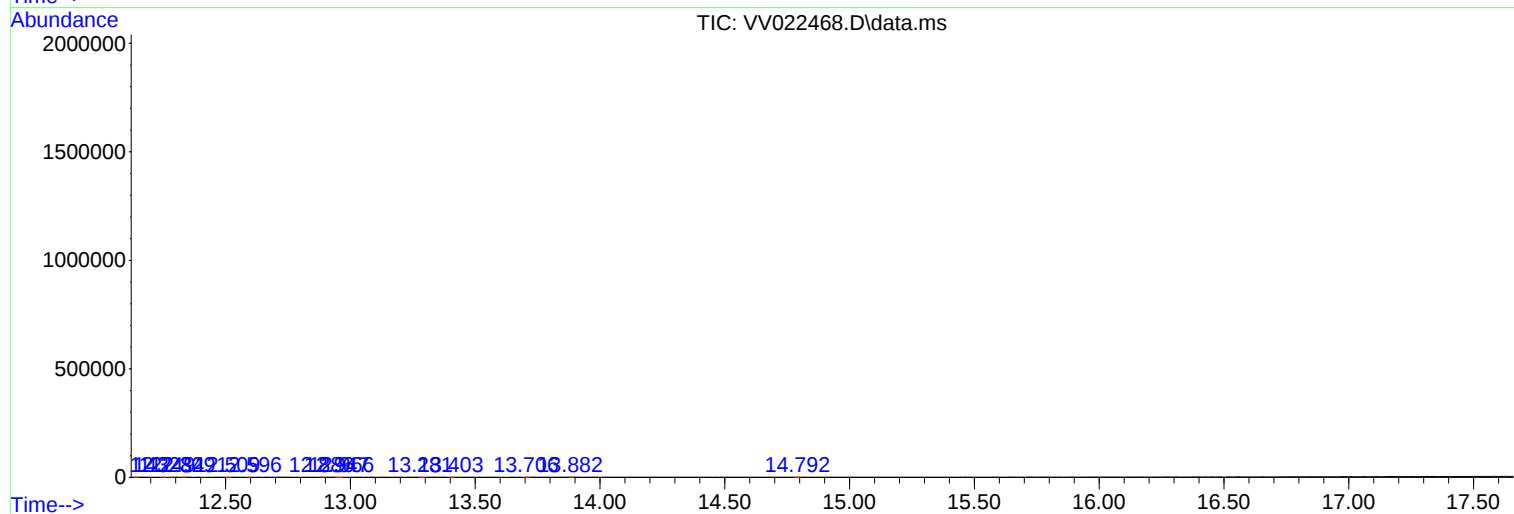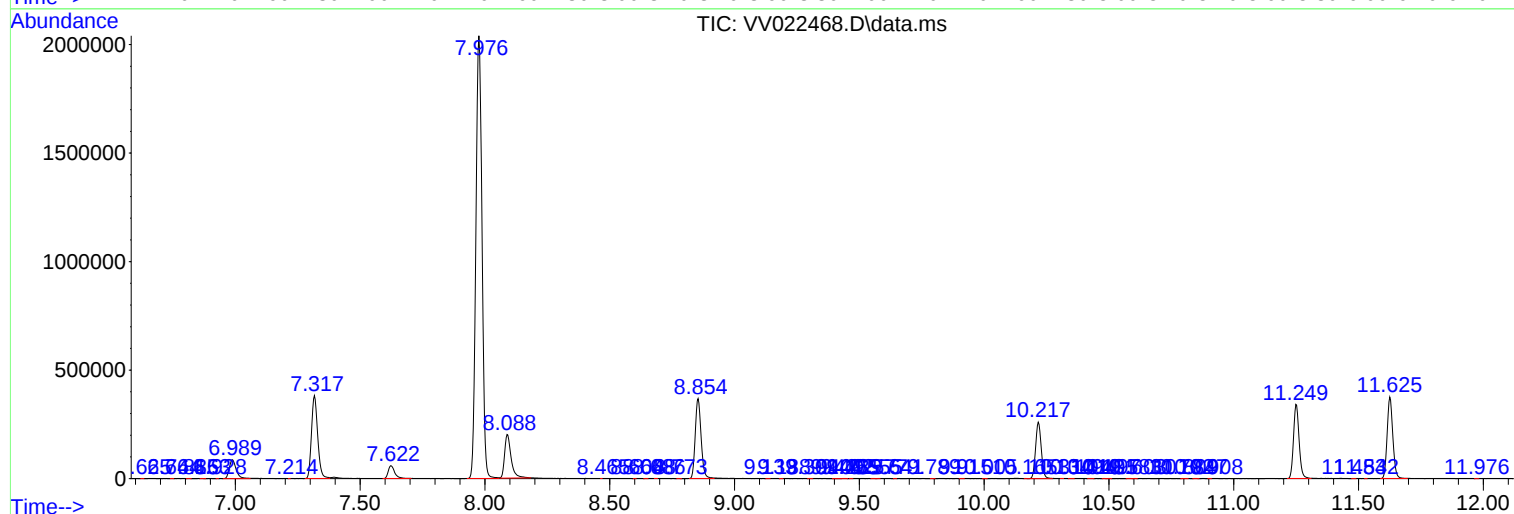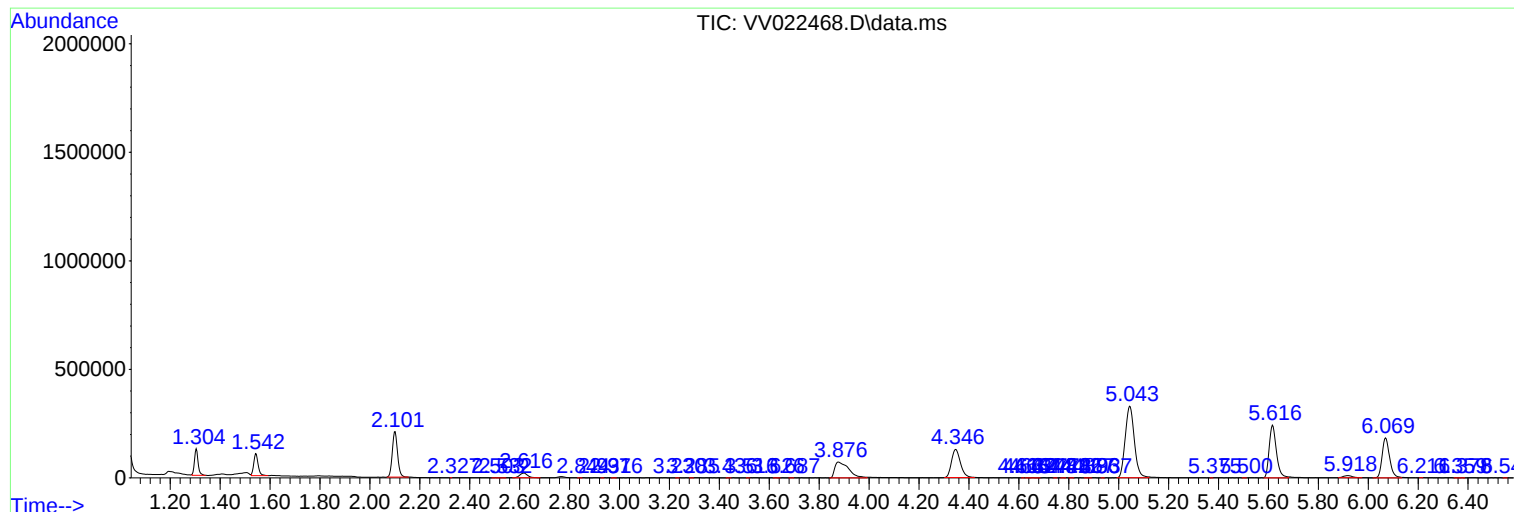

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
Data File : VV022468.D
Acq On : 01 Oct 2021 06:05
Operator : SY/MD
Sample : M3997-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 52 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A53

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
Data File : VV022468.D
Acq On : 01 Oct 2021 06:05
Operator : SY/MD
Sample : M3997-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 52 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A53

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
