

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
 Data File : VV022469.D
 Acq On : 01 Oct 2021 06:29
 Operator : SY/MD
 Sample : M3997-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A55

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M

Title : VOC Analysis

Signal : TIC: VV022469.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	95	rVB	127263	128150	14.03%	1.730%
2	1.564	157	163	177	rVB	103397	121951	13.35%	1.646%
3	2.098	320	329	343	rBV	228409	328267	35.93%	4.432%
4	2.371	411	414	417	rBV	486	295	0.03%	0.004%
5	2.616	480	490	499	rBV6	1690	3507	0.38%	0.047%
6	2.770	530	538	550	rVB3	3994	8084	0.88%	0.109%
7	2.931	585	588	589	rVB	367	144	0.02%	0.002%
8	2.973	599	601	602	rBV	284	134	0.01%	0.002%
9	3.095	636	639	643	rBV	183	148	0.02%	0.002%
10	3.223	672	679	683	rBV4	355	411	0.04%	0.006%
11	3.252	686	688	691	rVB	281	132	0.01%	0.002%
12	3.365	721	723	724	rBV2	239	136	0.01%	0.002%
13	3.523	770	772	775	rVB2	322	159	0.02%	0.002%
14	3.548	775	780	783	rBV2	389	350	0.04%	0.005%
15	3.661	813	815	817	rVB	380	140	0.02%	0.002%
16	3.825	862	866	868	rBV3	220	146	0.02%	0.002%
17	3.847	869	873	878	rVB2	396	288	0.03%	0.004%
18	3.905	879	891	939	rBV2	52299	202677	22.19%	2.736%
19	4.265	999	1003	1007	rBV3	394	344	0.04%	0.005%
20	4.349	1015	1029	1061	rVB2	139142	352687	38.61%	4.761%
21	4.551	1089	1092	1093	rBV2	366	253	0.03%	0.003%
22	4.593	1101	1105	1111	rVB2	505	450	0.05%	0.006%
23	4.622	1111	1114	1117	rBV2	362	287	0.03%	0.004%
24	4.693	1131	1136	1138	rVB3	354	243	0.03%	0.003%
25	4.709	1138	1141	1145	rVV3	299	250	0.03%	0.003%
26	4.738	1147	1150	1154	rVB3	647	407	0.04%	0.005%
27	4.799	1165	1169	1171	rBV3	327	255	0.03%	0.003%
28	4.841	1180	1182	1185	rBV	266	157	0.02%	0.002%
29	4.860	1186	1188	1195	rVB2	453	415	0.05%	0.006%
30	4.892	1195	1198	1201	rBV3	239	237	0.03%	0.003%
31	4.989	1225	1228	1229	rBV	408	217	0.02%	0.003%
32	5.043	1229	1245	1275	rVV2	363026	913526	100.00%	12.332%
33	5.323	1330	1332	1340	rVB4	486	529	0.06%	0.007%
34	5.391	1351	1353	1360	rBV3	418	506	0.06%	0.007%
35	5.481	1379	1381	1384	rBV2	292	190	0.02%	0.003%
36	5.510	1387	1390	1392	rBV	260	182	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
 Data File : VV022469.D
 Acq On : 01 Oct 2021 06:29
 Operator : SY/MD
 Sample : M3997-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A55

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

37	5.616	1409	1423	1452	rBV	266746	544381	59.59%	7.349%
38	5.918	1503	1517	1540	rVB5	23874	57826	6.33%	0.781%
39	6.069	1551	1564	1586	rBV2	201898	410791	44.97%	5.546%
40	6.426	1671	1675	1678	rBV2	200	207	0.02%	0.003%
41	6.506	1695	1700	1705	rVB3	257	301	0.03%	0.004%
42	6.542	1705	1711	1713	rBV2	419	347	0.04%	0.005%
43	6.661	1744	1748	1752	rBV2	285	293	0.03%	0.004%
44	6.821	1796	1798	1803	rVB2	349	206	0.02%	0.003%
45	6.866	1809	1812	1814	rBV2	195	137	0.01%	0.002%
46	6.928	1829	1831	1836	rVB2	381	223	0.02%	0.003%
47	6.989	1836	1850	1875	rBV	93947	177724	19.45%	2.399%
48	7.201	1915	1916	1921	rVB2	565	282	0.03%	0.004%
49	7.249	1929	1931	1937	rVB3	415	222	0.02%	0.003%
50	7.317	1940	1952	1972	rBV	412490	716596	78.44%	9.674%
51	7.535	2016	2020	2023	rBV4	405	405	0.04%	0.005%
52	7.622	2038	2047	2069	rBV	64513	116730	12.78%	1.576%
53	7.976	2142	2157	2176	rBV	393910	658895	72.13%	8.895%
54	8.095	2184	2194	2225	rBV	200555	396173	43.37%	5.348%
55	8.474	2310	2312	2313	rBV	392	150	0.02%	0.002%
56	8.583	2342	2346	2350	rBV2	497	319	0.03%	0.004%
57	8.632	2359	2361	2364	rBV2	286	185	0.02%	0.002%
58	8.667	2369	2372	2374	rBV	182	129	0.01%	0.002%
59	8.718	2386	2388	2391	rBV3	289	177	0.02%	0.002%
60	8.760	2399	2401	2404	rVB	328	134	0.01%	0.002%
61	8.853	2419	2430	2458	rBV	403080	644222	70.52%	8.697%
62	9.124	2512	2514	2516	rBV2	283	162	0.02%	0.002%
63	9.291	2562	2566	2569	rBV3	237	248	0.03%	0.003%
64	9.972	2776	2778	2784	rVB2	383	167	0.02%	0.002%
65	10.034	2794	2797	2802	rBV3	208	201	0.02%	0.003%
66	10.127	2820	2826	2837	rBV4	1756	2737	0.30%	0.037%
67	10.217	2843	2854	2873	rBV	271743	434406	47.55%	5.864%
68	10.342	2890	2893	2897	rBV3	529	364	0.04%	0.005%
69	10.384	2900	2906	2918	rVB5	1191	1547	0.17%	0.021%
70	10.451	2925	2927	2931	rBV2	252	160	0.02%	0.002%
71	10.529	2946	2951	2954	rBV2	528	483	0.05%	0.007%
72	10.577	2962	2966	2970	rBV5	458	503	0.06%	0.007%
73	10.603	2972	2974	2977	rVB2	307	144	0.02%	0.002%
74	10.683	2997	2999	3002	rBV2	196	129	0.01%	0.002%
75	10.918	3065	3072	3080	rBV4	1296	1815	0.20%	0.025%
76	11.095	3123	3127	3131	rBV	413	361	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
 Data File : VV022469.D
 Acq On : 01 Oct 2021 06:29
 Operator : SY/MD
 Sample : M3997-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A55

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis

77	11.133	3136	3139	3140	rBV	237	132	0.01%	0.002%
78	11.249	3163	3175	3202	rBV	346071	557618	61.04%	7.528%
79	11.509	3253	3256	3259	rVB2	247	141	0.02%	0.002%
80	11.577	3273	3277	3280	rBV3	442	410	0.04%	0.006%
81	11.625	3280	3292	3310	rBV	387034	608070	66.56%	8.209%
82	11.828	3351	3355	3357	rBV3	348	256	0.03%	0.003%
83	11.998	3404	3408	3410	rBV	319	190	0.02%	0.003%
84	12.040	3417	3421	3424	rBV2	392	350	0.04%	0.005%
85	12.085	3433	3435	3439	rBV2	285	179	0.02%	0.002%
86	12.246	3483	3485	3487	rBV2	397	202	0.02%	0.003%
87	12.320	3506	3508	3512	rBV2	225	181	0.02%	0.002%
88	12.342	3513	3515	3520	rVB2	258	154	0.02%	0.002%
89	12.898	3687	3688	3691	rVB2	329	129	0.01%	0.002%
90	13.165	3769	3771	3775	rVB2	437	257	0.03%	0.003%
91	13.188	3775	3778	3780	rBV	296	129	0.01%	0.002%
92	13.300	3811	3813	3816	rVB2	305	128	0.01%	0.002%
93	13.332	3820	3823	3824	rBV	407	196	0.02%	0.003%
94	13.442	3854	3857	3860	rBV	272	144	0.02%	0.002%
95	13.503	3874	3876	3880	rVB2	358	195	0.02%	0.003%
96	13.831	3975	3978	3983	rBV2	283	333	0.04%	0.004%
97	13.972	4019	4022	4025	rBV	271	172	0.02%	0.002%
98	14.590	4211	4214	4217	rBV2	370	318	0.03%	0.004%
99	15.847	4602	4605	4607	rBV	636	484	0.05%	0.007%
100	16.117	4687	4689	4691	rBV	798	463	0.05%	0.006%




Sum of corrected areas: 7407567

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
Data File : VV022469.D
Acq On : 01 Oct 2021 06:29
Operator : SY/MD
Sample : M3997-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 53 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A55

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

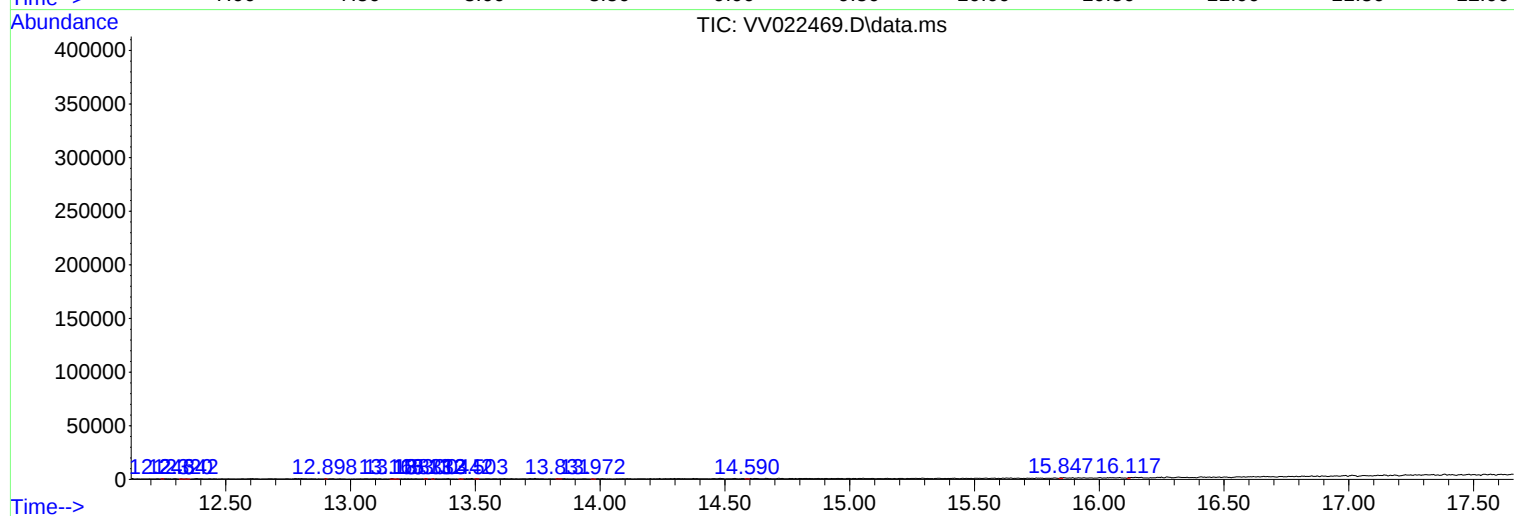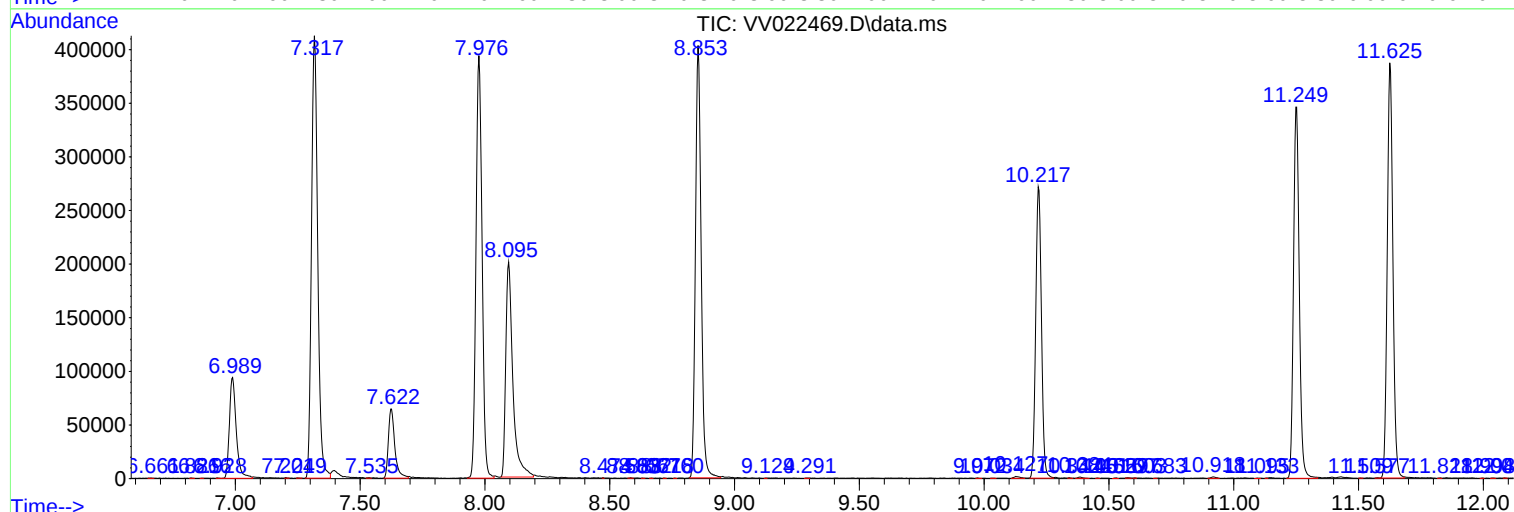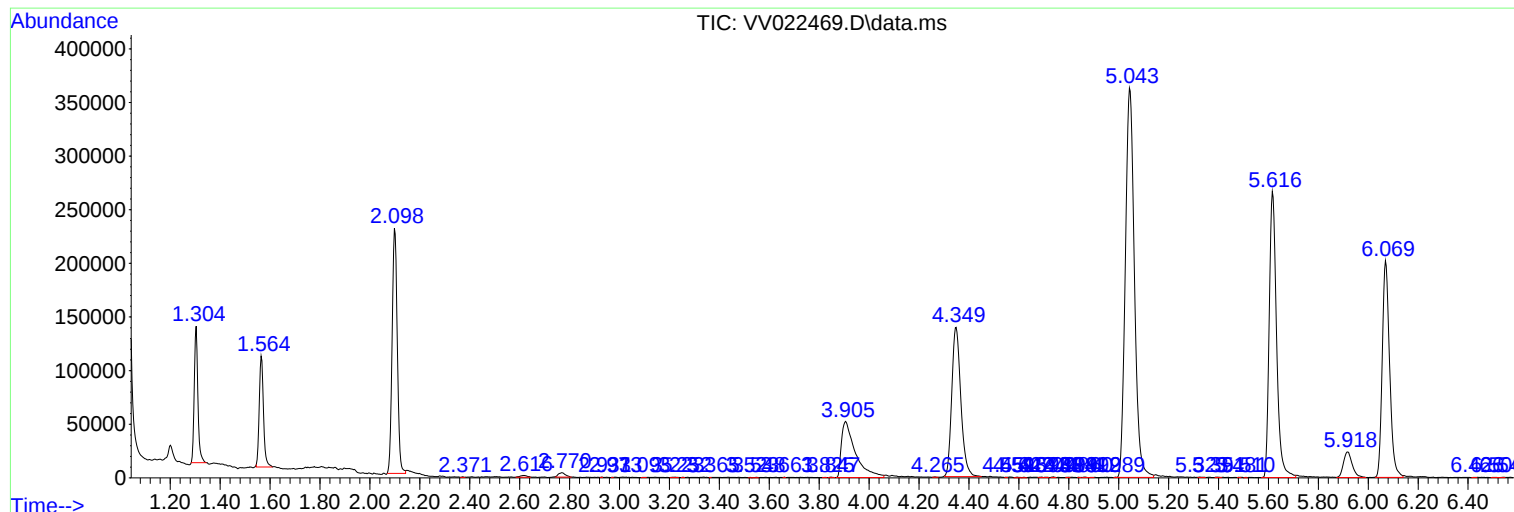

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
Data File : VV022469.D
Acq On : 01 Oct 2021 06:29
Operator : SY/MD
Sample : M3997-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 53 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A55

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
Data File : VV022469.D
Acq On : 01 Oct 2021 06:29
Operator : SY/MD
Sample : M3997-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 53 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A55

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc