


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
 Data File : VV022418.D
 Acq On : 30 Sep 2021 09:07
 Operator : SY/MD
 Sample : BFB238
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB238

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Title : VOC Analysis
 Last Update : Fri Oct 01 04:27:45 2021

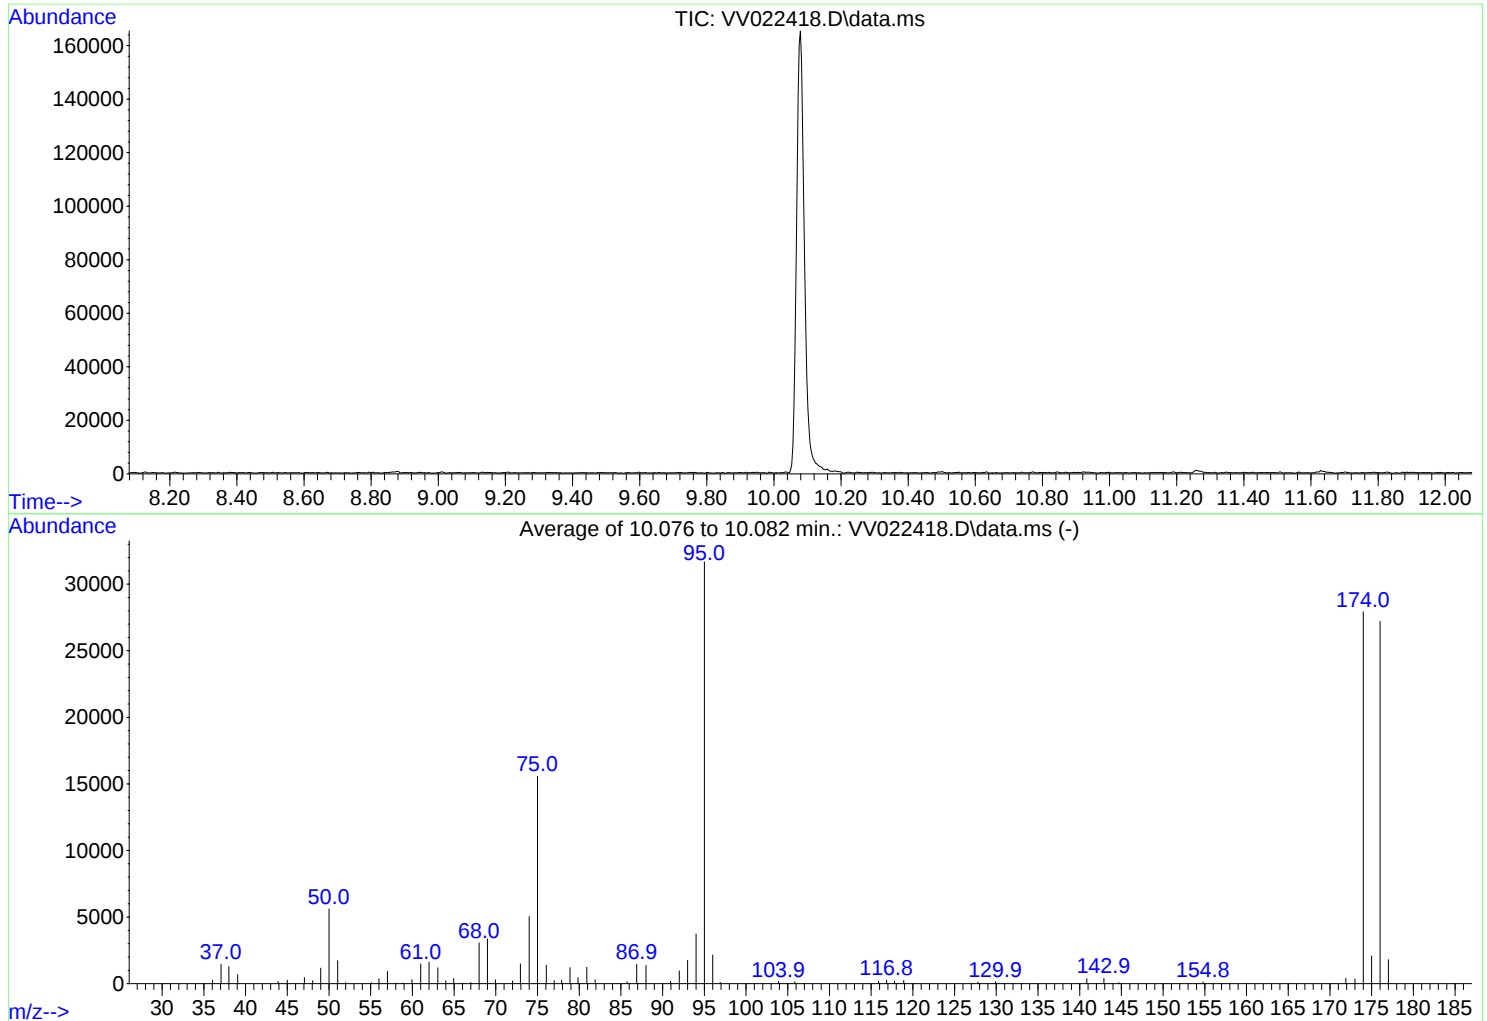

AutoFind: Scans 2810, 2811, 2812; Background Corrected with Scan 2800

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	5606	PASS
75	95	30	80	49.1	15568	PASS
95	95	100	100	100.0	31677	PASS
96	95	5	9	6.8	2157	PASS
173	174	0.00	2	1.3	352	PASS
174	95	50	120	88.1	27923	PASS
175	174	5	9	7.4	2074	PASS
176	174	95	105	97.5	27211	PASS
177	176	5	10	6.6	1805	PASS

Scan 2800 (10.043 min): VV022418.D\data.ms
BFB238

m/z	Abundance
40.00	207.0
43.90	210.0

Instrument :
MSVOA_V
ClientSampleId :
BFB238

m/z	Abundance
36.10	243.0
37.10	1572.0
38.00	1209.0
39.00	705.0
39.80	168.0
44.00	402.0
45.00	275.0
47.10	502.0
48.10	222.0
49.00	1185.0
50.00	5800.0
51.00	1856.0
52.00	138.0
55.10	112.0
56.00	399.0
57.00	956.0
58.00	109.0
60.00	329.0
61.00	1443.0
62.00	1646.0
63.10	1175.0
64.00	270.0
64.90	393.0
68.00	2981.0
69.00	3353.0
70.00	302.0
72.00	251.0
73.00	1467.0
74.00	5073.0
75.00	15961.0
76.10	1347.0
77.00	265.0
77.90	246.0
78.90	1211.0
79.80	429.0
80.90	1272.0
81.90	323.0
85.80	150.0
86.90	1501.0
88.00	1438.0
90.90	143.0
92.00	1045.0
93.00	1710.0
94.00	3709.0
95.00	32040.0
96.00	2257.0
96.90	169.0
103.90	177.0
105.80	144.0
115.90	147.0
116.80	273.0
117.80	203.0
118.80	231.0
127.80	125.0
130.00	147.0
140.80	355.0
142.90	350.0
154.80	125.0
171.90	367.0
173.00	360.0
174.00	27584.0
175.00	2009.0
176.00	26904.0
177.00	1846.0

Instrument :
MSVOA_V
ClientSampleId :
BFB238

m/z	Abundance
36.00	250.0
37.10	1495.0
38.00	1334.0
39.00	695.0
39.90	155.0
44.00	362.0
45.00	273.0
47.00	481.0
48.00	241.0
49.00	1186.0
50.00	5799.0
51.10	1758.0
52.00	116.0
55.10	109.0
56.00	366.0
57.00	985.0
59.90	296.0
61.00	1552.0
62.00	1691.0
63.00	1224.0
64.00	239.0
65.00	421.0
67.00	121.0
68.00	3124.0
69.00	3478.0
69.90	294.0
72.00	208.0
72.90	1515.0
74.00	5253.0
75.00	16156.0
76.00	1449.0
77.00	230.0
77.90	275.0
78.90	1256.0
79.90	450.0
80.90	1264.0
81.90	289.0
85.80	149.0
86.90	1494.0
88.00	1407.0
91.00	179.0
92.00	980.0
93.00	1800.0
94.00	3833.0
95.00	32640.0
96.00	2236.0
96.90	135.0
103.90	165.0
105.80	145.0
115.90	179.0
116.90	259.0
117.80	211.0
118.90	245.0
127.80	132.0
129.90	156.0
140.90	388.0
142.90	410.0
144.70	107.0
154.80	140.0
171.90	412.0
173.00	362.0
174.00	28720.0
175.00	2152.0
176.00	28136.0
177.00	1891.0

Instrument :
MSVOA_V
ClientSampleId :
BFB238

m/z	Abundance
36.00	259.0
37.00	1289.0
38.00	1327.0
39.10	634.0
40.00	132.0
43.90	369.0
45.00	258.0
47.00	393.0
48.00	232.0
49.00	1131.0
50.00	5218.0
51.10	1581.0
56.00	353.0
57.00	803.0
58.80	114.0
59.90	292.0
61.00	1436.0
62.00	1542.0
63.00	1157.0
64.00	170.0
65.00	356.0
66.00	105.0
67.00	120.0
68.00	3074.0
69.00	3228.0
69.90	256.0
72.00	156.0
73.00	1461.0
74.00	4764.0
75.00	14586.0
76.00	1342.0
77.00	192.0
77.90	234.0
78.90	1147.0
79.90	445.0
80.90	1186.0
81.90	273.0
85.70	138.0
86.90	1385.0
88.00	1276.0
91.00	189.0
92.00	851.0
93.00	1730.0
94.00	3632.0
95.00	30352.0
96.00	1978.0
103.90	166.0
105.90	141.0
115.90	186.0
116.90	231.0
117.80	175.0
119.00	253.0
127.80	114.0
129.80	137.0
140.90	382.0
142.90	436.0
144.70	125.0
154.80	137.0
171.90	435.0
173.00	335.0
174.00	27464.0
175.00	2062.0
176.00	26592.0
177.00	1679.0

Instrument :
MSVOA_V
ClientSampleId :
BFB238