

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100118\  
 Data File : VV008002.D  
 Acq On : 01 Oct 2018 18:42  
 Operator : SY/MD  
 Sample : J5091-05DL 20X  
 Misc : 25.0 mL/MSVOA V/WATER  
 ALS Vial : 15 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 E62S8DL

Quant Time: Oct 02 04:18:21 2018  
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_V\METHOD\SOMVTR092718WMA.M  
 Quant Title : TRACE VOA SOM01.0  
 QLast Update : Tue Oct 02 04:17:24 2018  
 Response via : Initial Calibration

| Internal Standards         | R.T.  | QIon | Response | Conc | Units | Dev(Min) |
|----------------------------|-------|------|----------|------|-------|----------|
| 1) 1,4-Difluorobenzene     | 5.67  | 114  | 88580    | 5.00 | ug/L  | 0.00     |
| 28) Chlorobenzene-d5       | 8.90  | 117  | 84583    | 5.00 | ug/L  | 0.00     |
| 60) 1,4-Dichlorobenzene-d4 | 11.30 | 152  | 41053    | 5.00 | ug/L  | 0.00     |

## System Monitoring Compounds

|                                |        |       |          |          |      |         |
|--------------------------------|--------|-------|----------|----------|------|---------|
| 4) Vinyl Chloride-d3           | 1.32   | 65    | 17881    | 3.76     | ug/L | 0.00    |
| Spiked Amount                  | 5.000  | Range | 40 - 130 | Recovery | =    | 75.20%  |
| 7) Chloroethane-d5             | 1.59   | 69    | 17610    | 4.29     | ug/L | 0.00    |
| Spiked Amount                  | 5.000  | Range | 65 - 130 | Recovery | =    | 85.80%  |
| 11) 1,1-Dichloroethene-d2      | 2.13   | 63    | 31360    | 2.92     | ug/L | 0.00    |
| Spiked Amount                  | 5.000  | Range | 60 - 125 | Recovery | =    | 58.40%# |
| 20) 2-Butanone-d5              | 3.97   | 46    | 77530    | 54.28    | ug/L | 0.00    |
| Spiked Amount                  | 50.000 | Range | 40 - 130 | Recovery | =    | 108.56% |
| 24) Chloroform-d               | 4.41   | 84    | 51474    | 4.76     | ug/L | 0.00    |
| Spiked Amount                  | 5.000  | Range | 70 - 125 | Recovery | =    | 95.20%  |
| 26) 1,2-Dichloroethane-d4      | 5.09   | 65    | 28316    | 4.76     | ug/L | 0.00    |
| Spiked Amount                  | 5.000  | Range | 70 - 130 | Recovery | =    | 95.20%  |
| 32) Benzene-d6                 | 5.10   | 84    | 94314    | 4.67     | ug/L | 0.00    |
| Spiked Amount                  | 5.000  | Range | 70 - 125 | Recovery | =    | 93.40%  |
| 36) 1,2-Dichloropropane-d6     | 6.12   | 67    | 31656    | 4.94     | ug/L | 0.00    |
| Spiked Amount                  | 5.000  | Range | 60 - 140 | Recovery | =    | 98.80%  |
| 41) Toluene-d8                 | 7.36   | 98    | 86386    | 4.20     | ug/L | 0.00    |
| Spiked Amount                  | 5.000  | Range | 70 - 130 | Recovery | =    | 84.00%  |
| 43) trans-1,3-Dichloropropene- | 7.67   | 79    | 10289    | 4.17     | ug/L | 0.00    |
| Spiked Amount                  | 5.000  | Range | 55 - 130 | Recovery | =    | 83.40%  |
| 46) 2-Hexanone-d5              | 8.14   | 63    | 54603    | 50.19    | ug/L | 0.00    |
| Spiked Amount                  | 50.000 | Range | 45 - 130 | Recovery | =    | 100.38% |
| 57) 1,1,2,2-Tetrachloroethane- | 10.27  | 84    | 25073    | 5.08     | ug/L | 0.00    |
| Spiked Amount                  | 5.000  | Range | 65 - 120 | Recovery | =    | 101.60% |
| 64) 1,2-Dichlorobenzene-d4     | 11.68  | 152   | 38483    | 4.84     | ug/L | 0.00    |
| Spiked Amount                  | 5.000  | Range | 80 - 120 | Recovery | =    | 96.80%  |

## Target Compounds


|                             |      |     |        |              | Ovalue |
|-----------------------------|------|-----|--------|--------------|--------|
| 12) 1,1-Dichloroethene      | 2.15 | 96  | 1248   | 0.213 ug/L # | 1      |
| 16) Methylene chloride      | 2.54 | 84  | 3076   | 0.473 ug/L   | 90     |
| 19) 1,1-Dichloroethane      | 3.23 | 63  | 2836   | 0.258 ug/L   | 95     |
| 34) Trichloroethene         | 5.96 | 95  | 13127  | 1.893 ug/L   | 99     |
| 35) Methylcyclohexane       | 6.12 | 83  | 7402   | 0.712 ug/L # | 18     |
| 37) 1,2-Dichloropropane     | 6.12 | 63  | 3608   | 0.583 ug/L # | 87     |
| 39) cis-1,3-Dichloropropene | 7.03 | 75  | 822    | 0.099 ug/L # | 54     |
| 51) Chlorobenzene           | 8.93 | 112 | 201207 | 11.044 ug/L  | 99     |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV100118\  
Data File : VV008002.D  
Acq On : 01 Oct 2018 18:42  
Operator : SY/MD  
Sample : J5091-05DL 20X  
Misc : 25.0 mL/MSVOA V/WATER  
ALS Vial : 15 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
E62S8DL

Quant Time: Oct 02 04:18:21 2018  
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_V\METHOD\SOMVTR092718WMA.M  
Quant Title : TRACE VOA SOM01.0  
QLast Update : Tue Oct 02 04:17:24 2018  
Response via : Initial Calibration

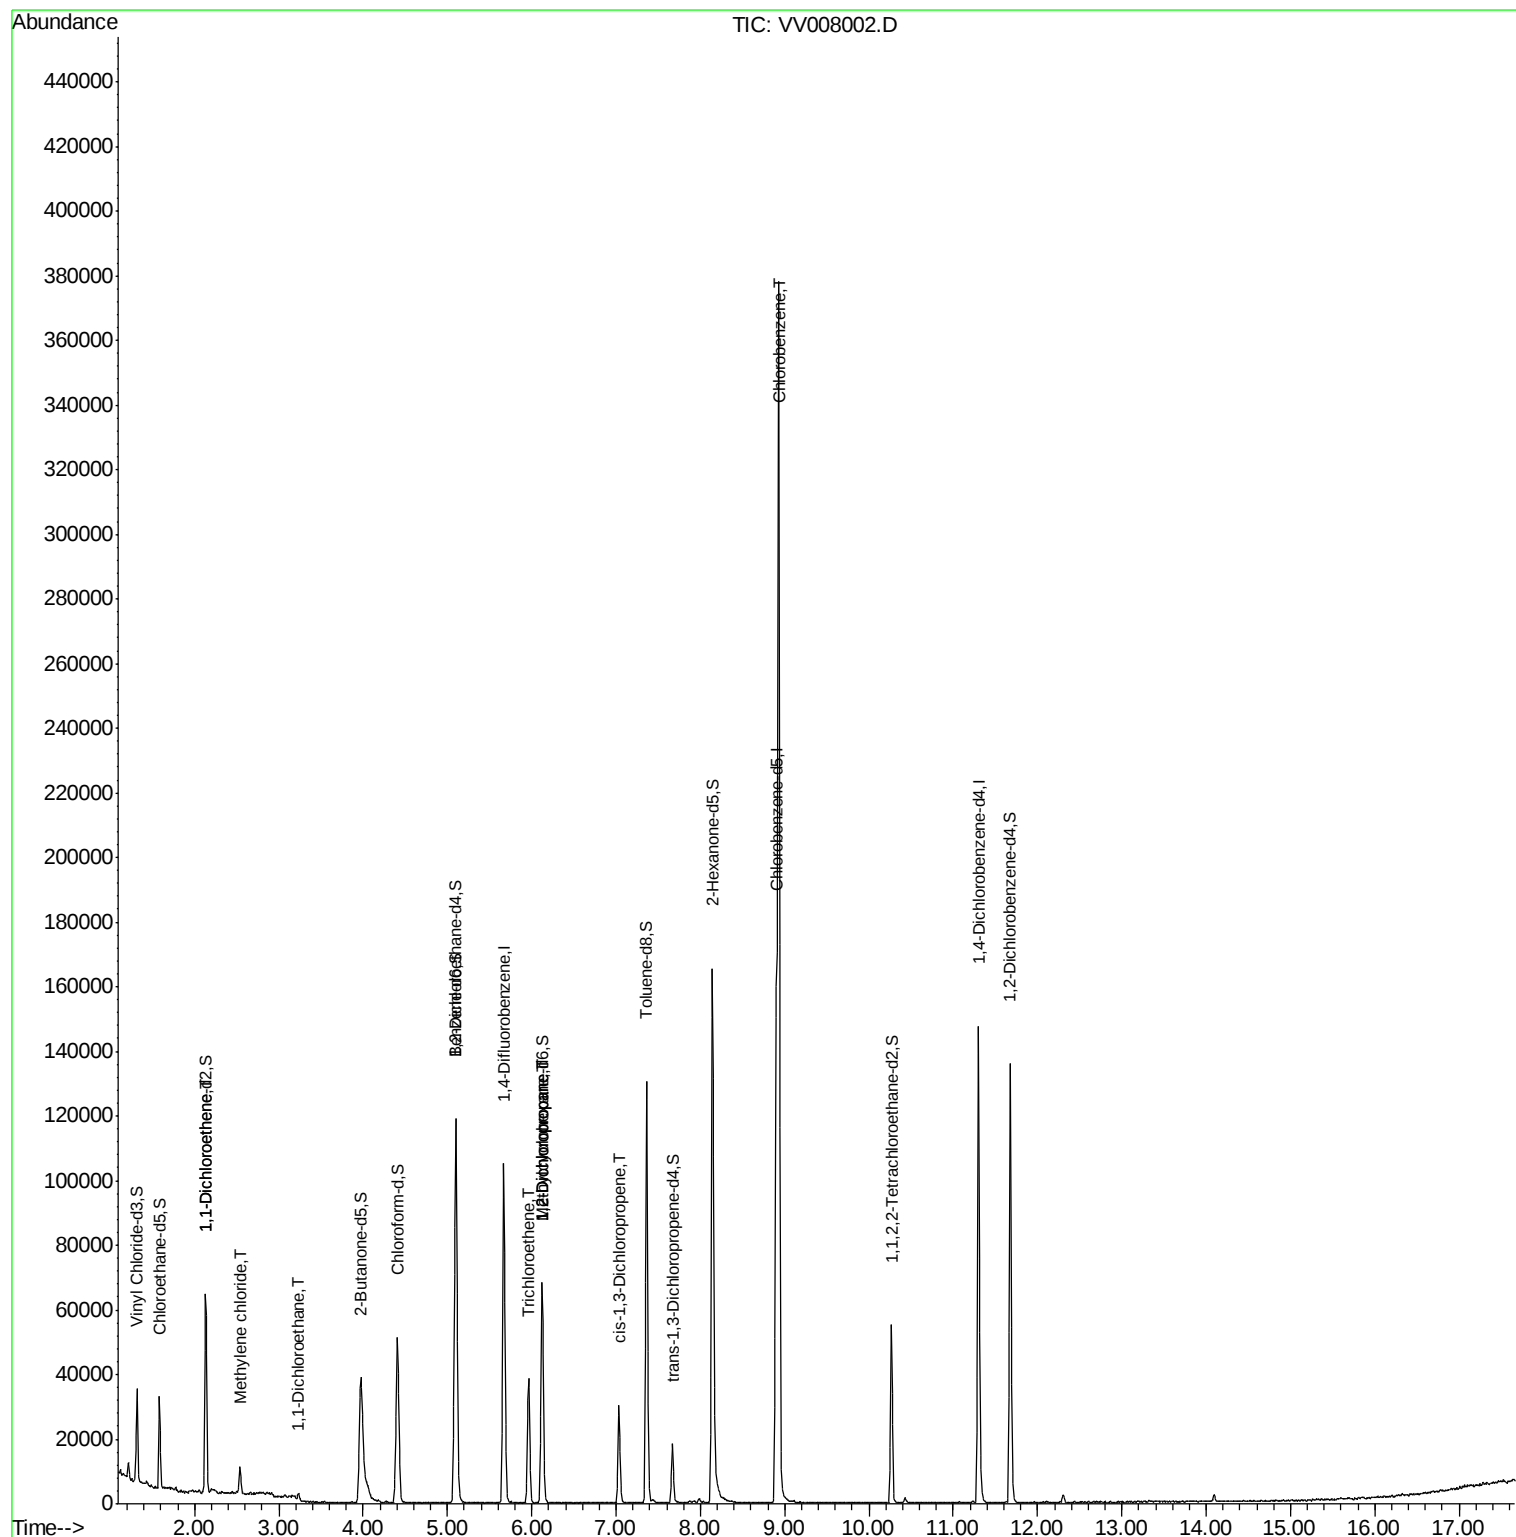

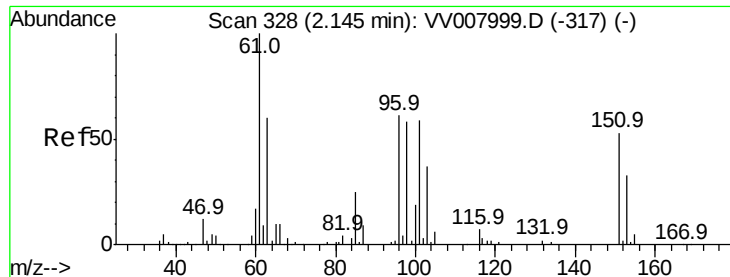

#12

1,1-Dichloroethene

Concen: 0.213 ug/L

RT: 2.15 min Scan# 328

Delta R.T. 0.00 min

Lab File: VV008002.D

Acq: 01 Oct 2018 18:42

Instrument :

MSVOA\_V

ClientSampleId :

E62S8DL





Tot Ion: 96 Resp: 1248

Ion Ratio Lower Upper

96 100

61 272.7 114.1 211.9#

63 1202.0 81.5 151.3#

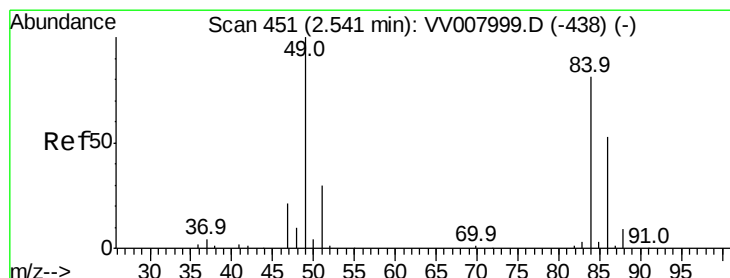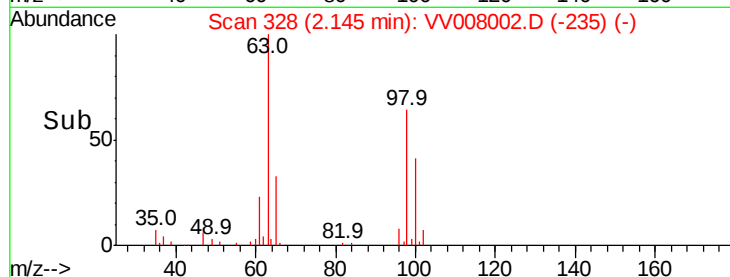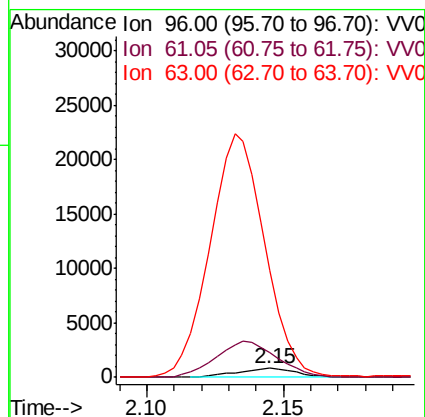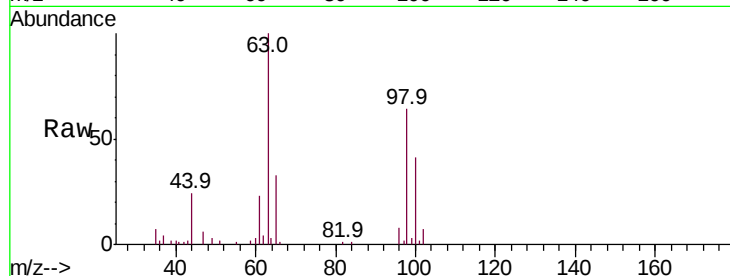

#16

Methylene chloride

Concen: 0.473 ug/L

RT: 2.54 min Scan# 451

Delta R.T. 0.00 min

Lab File: VV008002.D

Acq: 01 Oct 2018 18:42




Tgt Ion: 84 Resp: 3076


Ion Ratio Lower Upper

84 100

86 60.3 47.3 87.8

49 115.6 90.0 167.2


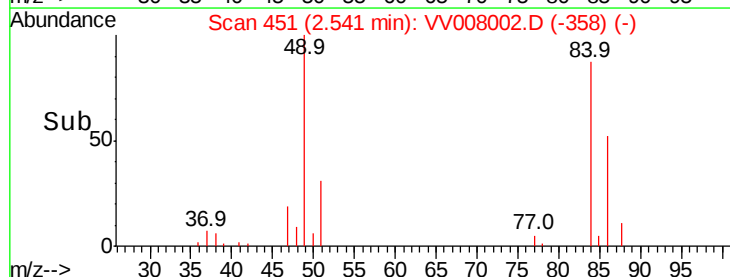
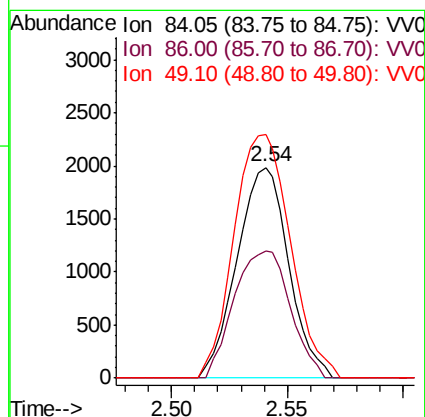
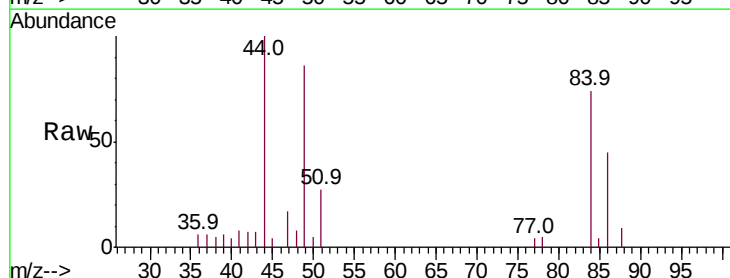


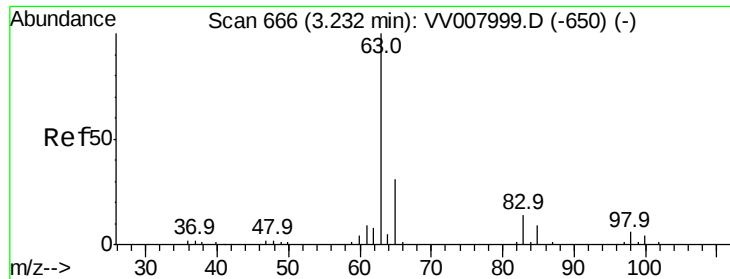

#19  
1,1-Dichloroethane  
Concen: 0.258 ug/L  
RT: 3.23 min Scan# 666  
Delta R.T. 0.00 min  
Lab File: VV008002.D  
Acq: 01 Oct 2018 18:42




Instrument :  
MSVOA\_V  
ClientSampleId :  
E62S8DL


Tot Ion: 63 Resp: 2836  
Ion Ratio Lower Upper  
63 100  
65 30.4 22.3 41.5  
83 17.8 9.8 18.2

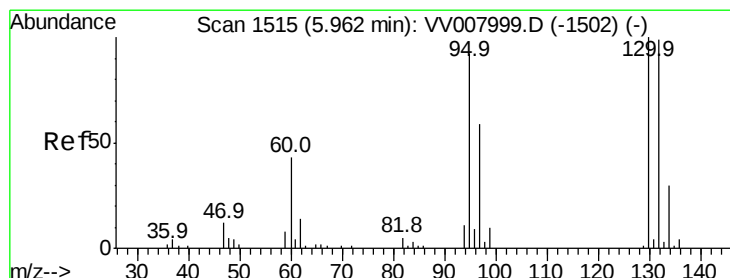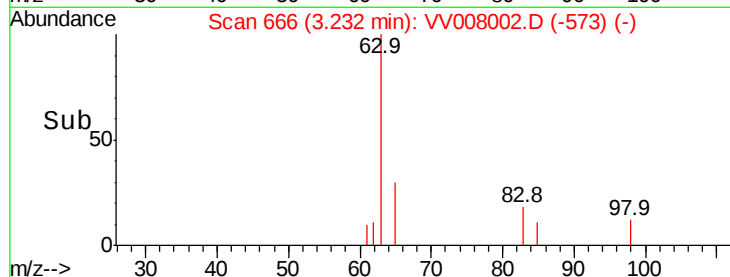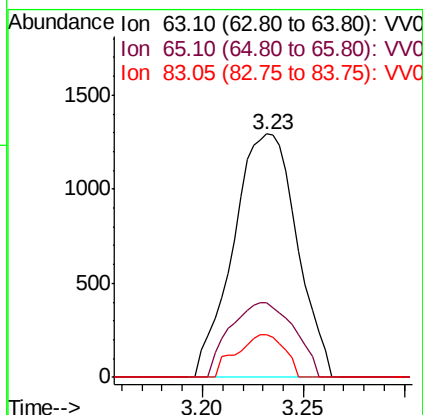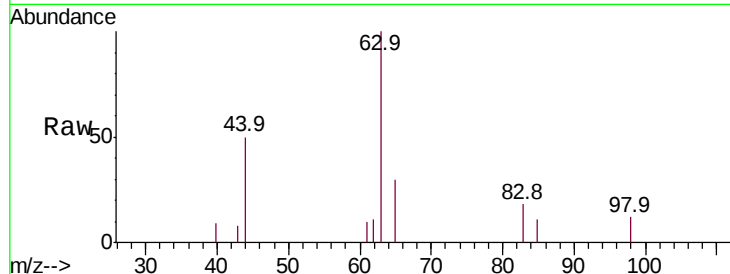

#34  
Trichloroethene  
Concen: 1.893 ug/L  
RT: 5.96 min Scan# 1515  
Delta R.T. 0.00 min  
Lab File: VV008002.D  
Acq: 01 Oct 2018 18:42

Tgt Ion: 95 Resp: 13127  
Ion Ratio Lower Upper  
95 100  
97 62.4 43.6 81.0  
132 100.9 69.9 129.9  
130 105.1 71.7 133.3

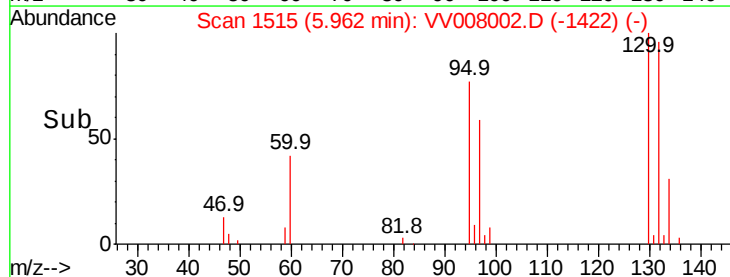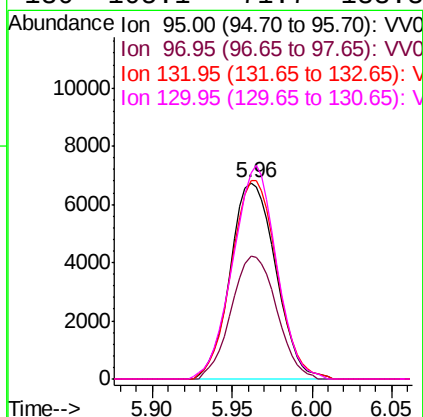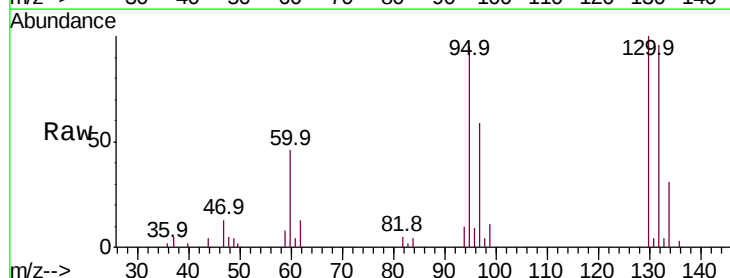


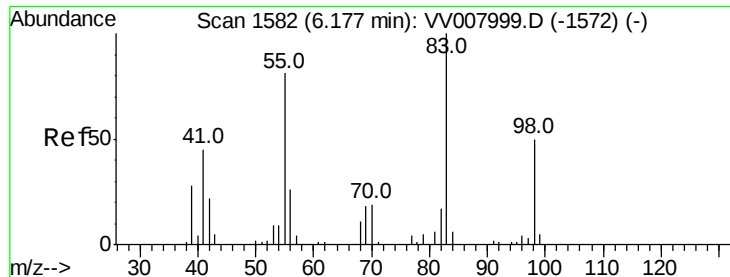




#35  
Methvlcvclohexane  
Concen: 0.712 ug/L  
RT: 6.12 min Scan# 1565  
Delta R.T. -0.05 min  
Lab File: VV008002.D  
Acq: 01 Oct 2018 18:42

Instrument :  
MSVOA\_V  
ClientSampleId :  
E62S8DL

Tot Ion: 83 Resp: 7402  
Ion Ratio Lower Upper  
83 100  
55 0.0 62.2 93.2#  
98 0.0 38.0 57.0#

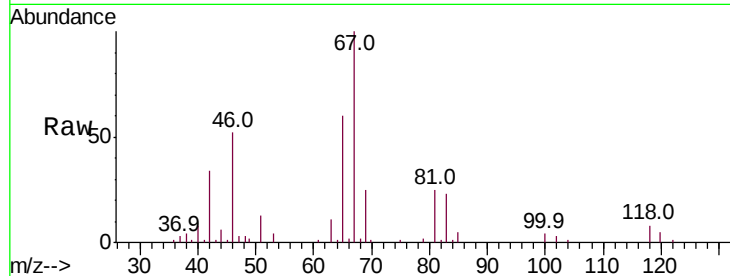


Abundance Ion 83.15 (82.85 to 83.85): VV0  
Ion 55.10 (54.80 to 55.80): VV0  
Ion 98.15 (97.85 to 98.85): VV0

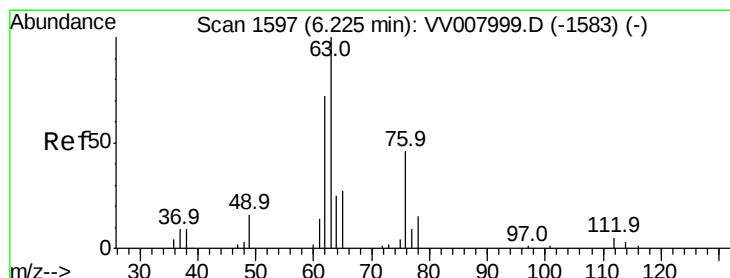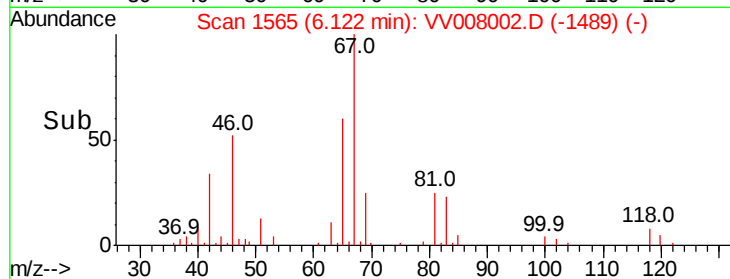
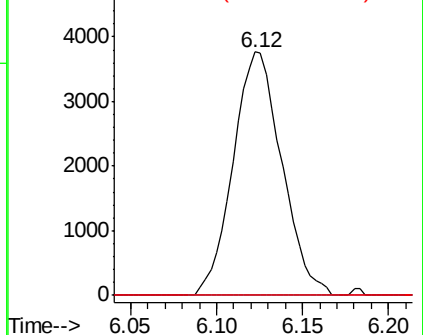



#37  
1,2-Dichloropropane  
Concen: 0.583 ug/L  
RT: 6.12 min Scan# 1565  
Delta R.T. -0.10 min  
Lab File: VV008002.D  
Acq: 01 Oct 2018 18:42

Tgt Ion: 63 Resp: 3608  
Ion Ratio Lower Upper  
63 100  
112 0.0 3.4 5.0#

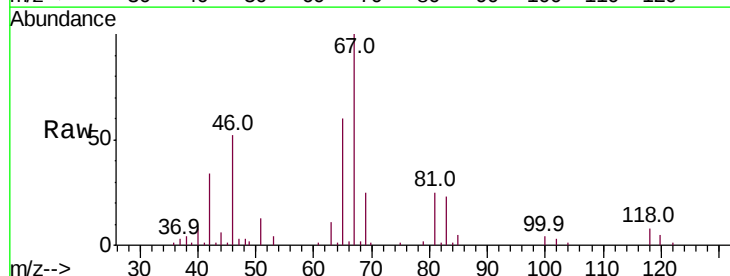

Abundance Ion 63.10 (62.80 to 63.80): VV0  
Ion 112.10 (111.80 to 112.80): V



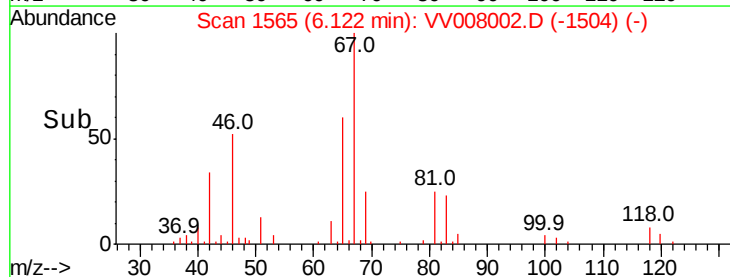
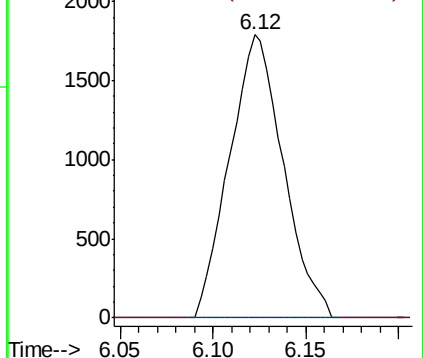


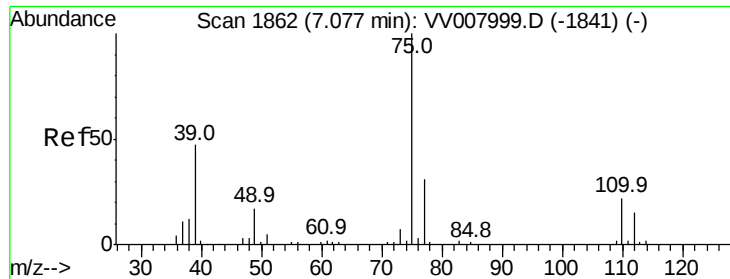

#39  
 cis-1,3-Dichloropropene  
 Concen: 0.099 ug/L  
 RT: 7.03 min Scan# 1847  
 Delta R.T. -0.05 min  
 Lab File: VV008002.D  
 Acq: 01 Oct 2018 18:42

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 E62S8DL

Tot Ion: 75 Resp: 822  
 Ion Ratio Lower Upper  
 75 100  
 77 58.8 22.9 42.5#

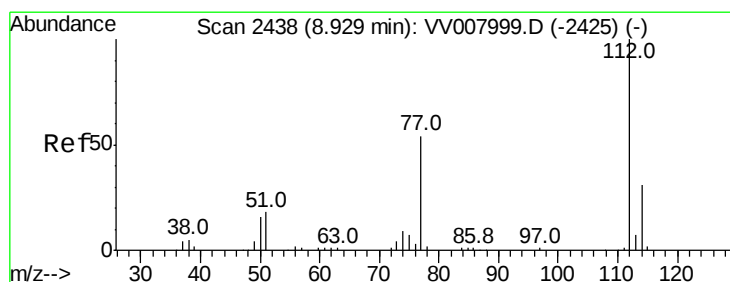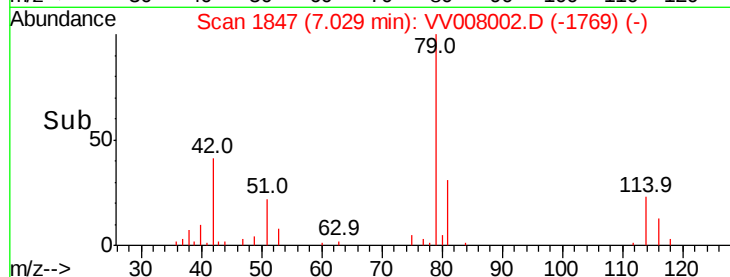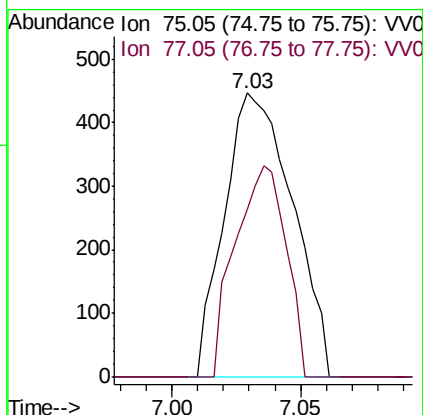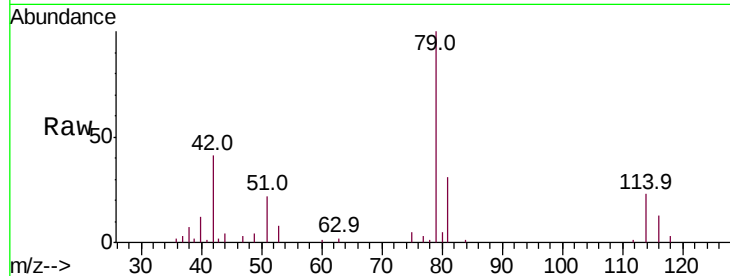

#51  
 Chlorobenzene  
 Concen: 11.044 ug/L  
 RT: 8.93 min Scan# 2438  
 Delta R.T. -0.00 min  
 Lab File: VV008002.D  
 Acq: 01 Oct 2018 18:42

Tgt Ion: 112 Resp: 201207  
 Ion Ratio Lower Upper  
 112 100  
 114 32.5 22.4 41.6  
 77 55.4 45.0 67.6

