

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100118\
 Data File : VV007991.D
 Acq On : 01 Oct 2018 13:33
 Operator : SY/MD
 Sample : J5062-17DL 200X
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GAC17DL

Quant Time: Oct 02 03:05:15 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR092718WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Oct 02 02:56:09 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	89658	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	86299	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	42563	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	17960	3.74	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	74.80%
7) Chloroethane-d5	1.59	69	18728	4.51	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	90.20%
11) 1,1-Dichloroethene-d2	2.13	63	30322	2.79	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	55.80%#
20) 2-Butanone-d5	3.98	46	76124	52.66	ug/L	0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	105.32%
24) Chloroform-d	4.41	84	51000	4.66	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.20%
26) 1,2-Dichloroethane-d4	5.09	65	28208	4.68	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.60%
32) Benzene-d6	5.10	84	96855	4.70	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.00%
36) 1,2-Dichloropropane-d6	6.12	67	31649	4.85	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	97.00%
41) Toluene-d8	7.36	98	89646	4.27	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	85.40%
43) trans-1,3-Dichloropropene-	7.67	79	10858	4.32	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	86.40%
46) 2-Hexanone-d5	8.14	63	53887	48.54	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	97.08%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	24191	4.80	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	96.00%
64) 1,2-Dichlorobenzene-d4	11.68	152	39370	4.78	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	95.60%


Target Compounds					Ovalue
31) Carbon tetrachloride	4.87	117	52394	5.727 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV100118\
Data File : VV007991.D
Acq On : 01 Oct 2018 13:33
Operator : SY/MD
Sample : J5062-17DL 200X
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GAC17DL

Quant Time: Oct 02 03:05:15 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR092718WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Oct 02 02:56:09 2018
Response via : Initial Calibration

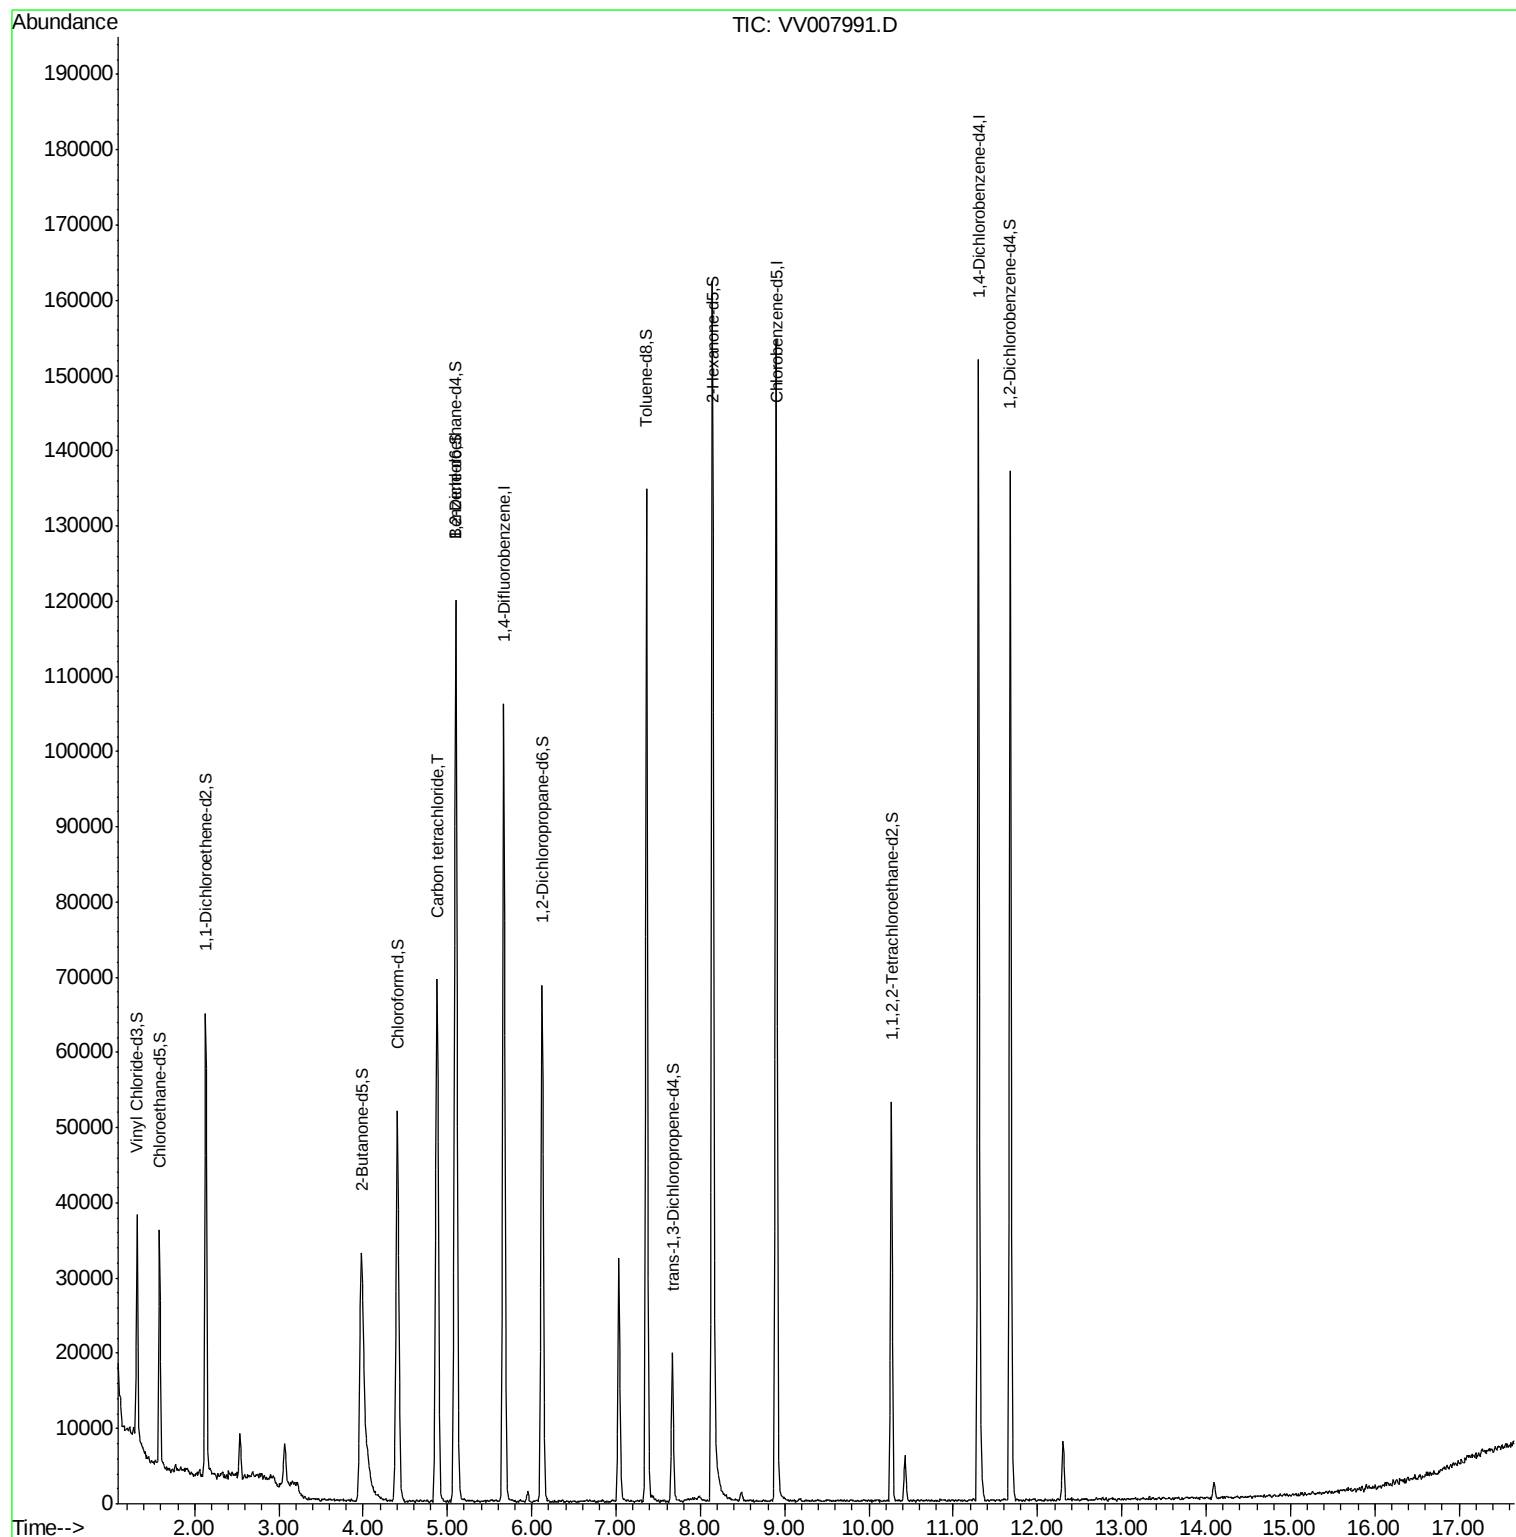

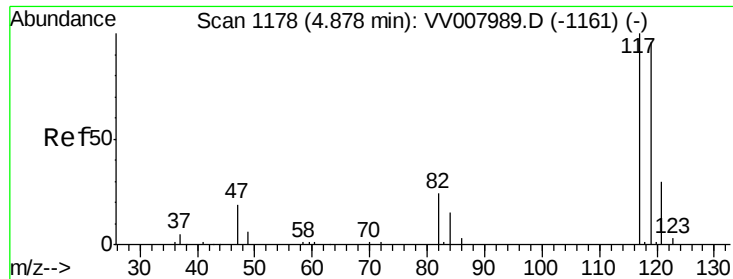

#31

Carbon tetrachloride

Concen: 5.727 ug/L

RT: 4.87 min Scan# 1177

Delta R.T. -0.00 min

Lab File: VV007991.D

Acq: 01 Oct 2018 13:33

Instrument :

MSVOA_V

ClientSampleId :

GAC17DL

Tot Ion:117 Resp: 52394

Ion Ratio Lower Upper

117 100

119 95.7 77.8 116.8

