

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100118\
 Data File : VV007992.D
 Acq On : 01 Oct 2018 14:00
 Operator : SY/MD
 Sample : J5062-18DL 10X
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GAC18DL

Quant Time: Oct 02 03:08:01 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR092718WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Oct 02 02:56:09 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	94185	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	88839	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	42409	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	18845	3.73	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	74.60%
7) Chloroethane-d5	1.59	69	19075	4.37	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	87.40%
11) 1,1-Dichloroethene-d2	2.14	63	32588	2.86	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	57.20%#
20) 2-Butanone-d5	3.97	46	78348	51.59	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	103.18%
24) Chloroform-d	4.41	84	54435	4.73	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.60%
26) 1,2-Dichloroethane-d4	5.09	65	29672	4.69	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.80%
32) Benzene-d6	5.10	84	101605	4.79	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.80%
36) 1,2-Dichloropropane-d6	6.12	67	33263	4.95	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	99.00%
41) Toluene-d8	7.36	98	92240	4.27	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	85.40%
43) trans-1,3-Dichloropropene-	7.67	79	11016	4.25	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	85.00%
46) 2-Hexanone-d5	8.14	63	55009	48.14	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	96.28%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	25000	4.82	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	96.40%
64) 1,2-Dichlorobenzene-d4	11.68	152	39829	4.85	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	97.00%


Target Compounds					Ovalue
31) Carbon tetrachloride	4.88	117	72545	7.703 ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV100118\
Data File : VV007992.D
Acq On : 01 Oct 2018 14:00
Operator : SY/MD
Sample : J5062-18DL 10X
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GAC18DL

Quant Time: Oct 02 03:08:01 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR092718WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Oct 02 02:56:09 2018
Response via : Initial Calibration

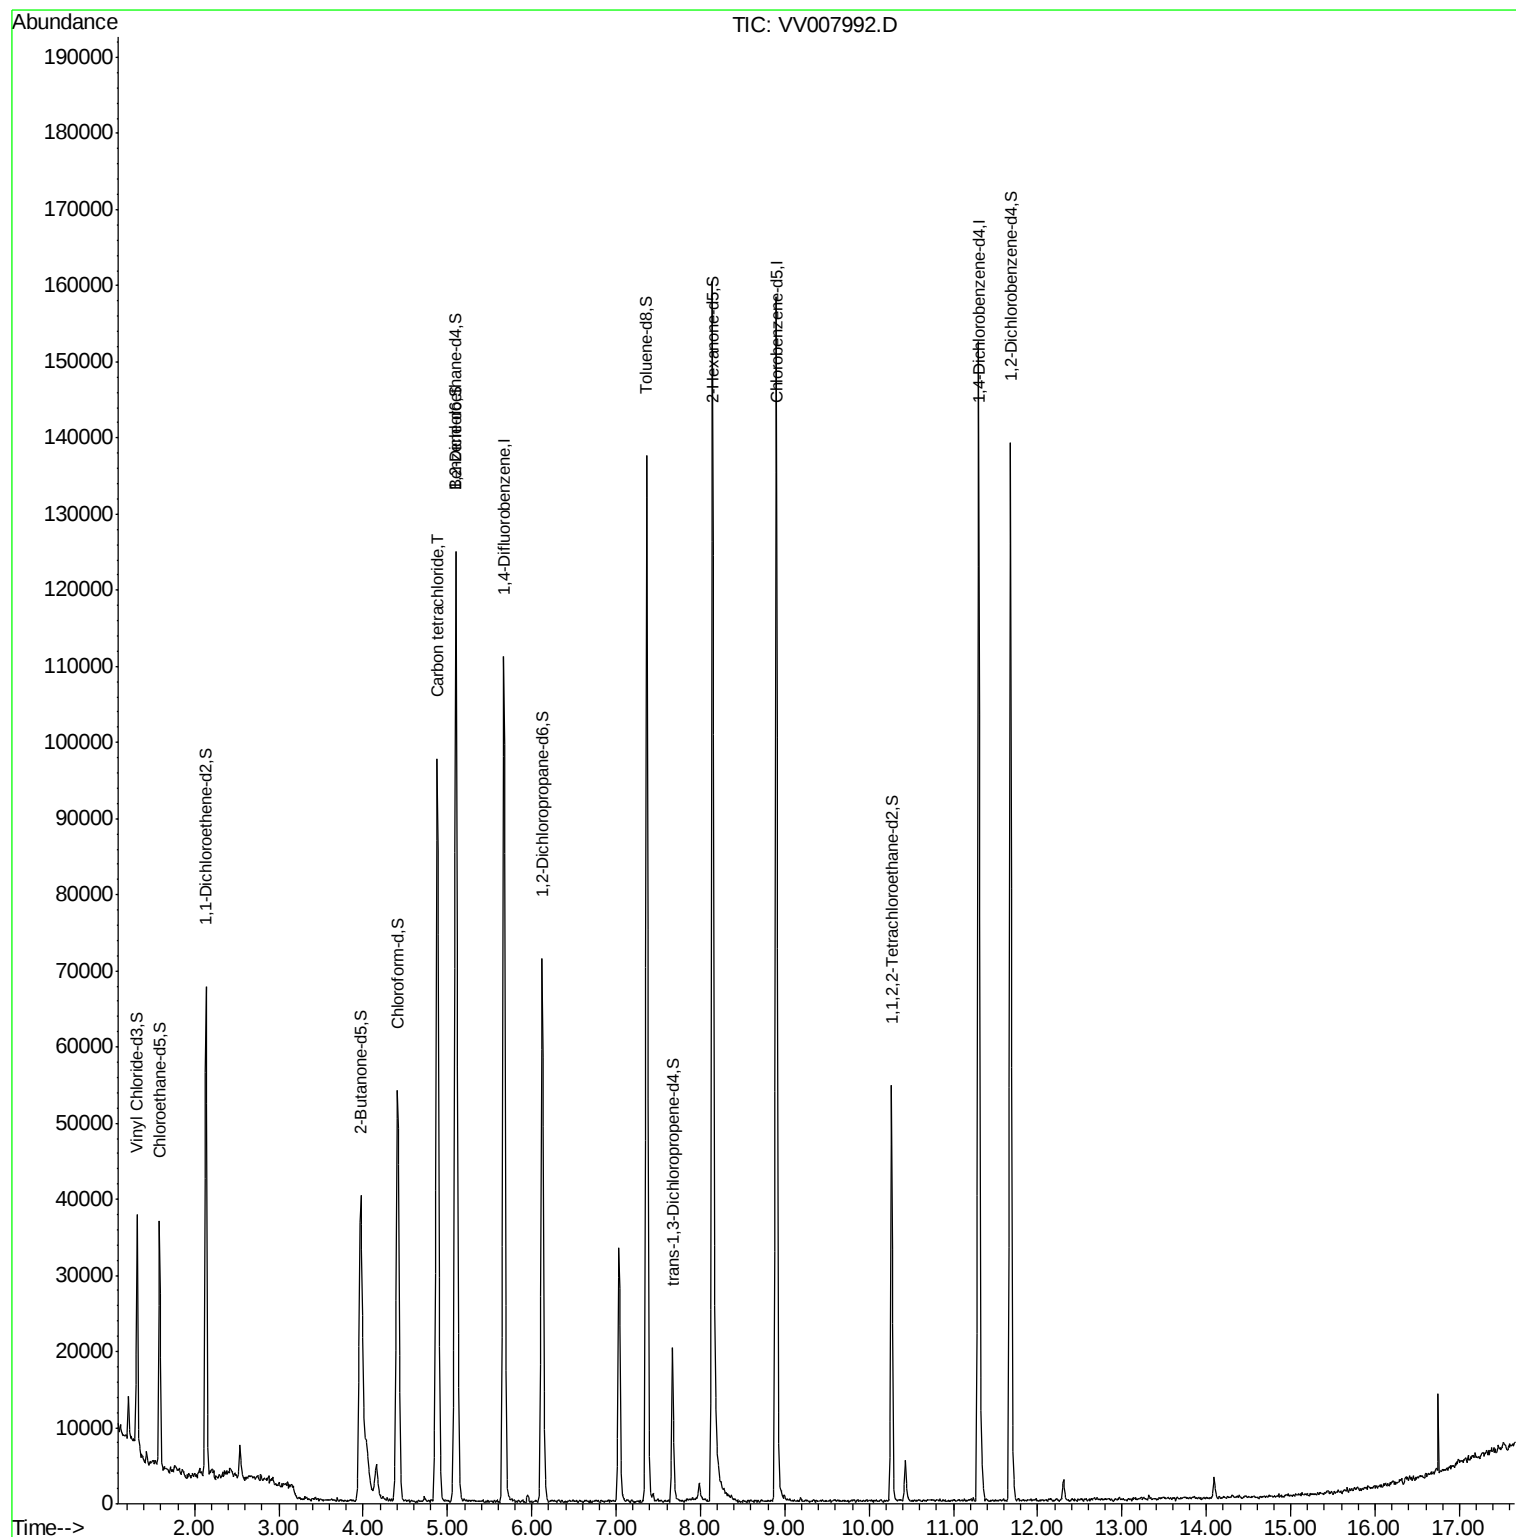

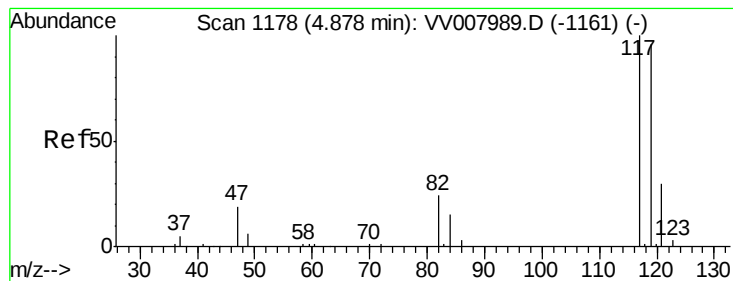

#31

Carbon tetrachloride

Concen: 7.703 ug/L

RT: 4.88 min Scan# 1179

Delta R.T. 0.00 min

Lab File: VV007992.D

Acq: 01 Oct 2018 14:00

Instrument :

MSVOA_V

ClientSampleId :

GAC18DL

Tot Ion:117 Resp: 72545

Ion Ratio Lower Upper

117 100

119 97.5 77.8 116.8

