

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100118\
 Data File : VV007997.D
 Acq On : 01 Oct 2018 16:17
 Operator : SY/MD
 Sample : J5091-05RE
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E62S9RE

Quant Time: Oct 02 04:08:20 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR092718WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Oct 02 02:56:09 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	91400	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	87261	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	42843	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	24322	4.96	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	99.20%
7) Chloroethane-d5	1.59	69	21301	5.03	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	100.60%
11) 1,1-Dichloroethene-d2	2.14	63	38637	3.49	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	69.80%
20) 2-Butanone-d5	3.97	46	67529	45.82	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	91.64%
24) Chloroform-d	4.41	84	52942	4.74	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.80%
26) 1,2-Dichloroethane-d4	5.09	65	28586	4.66	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.20%
32) Benzene-d6	5.10	84	104852	5.03	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.60%
36) 1,2-Dichloropropane-d6	6.12	67	32882	4.98	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	99.60%
41) Toluene-d8	7.36	98	98501	4.64	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.80%
43) trans-1,3-Dichloropropene-	7.67	79	11298	4.44	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	88.80%
46) 2-Hexanone-d5	8.14	63	48700	43.39	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	86.78%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	22838	4.48	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	89.60%
64) 1,2-Dichlorobenzene-d4	11.68	152	40723	4.91	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	98.20%


Target Compounds					Ovalue
13) Acetone	2.22	43	17381	16.187 ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV100118\
Data File : VV007997.D
Acq On : 01 Oct 2018 16:17
Operator : SY/MD
Sample : J5091-05RE
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E62S9RE

Quant Time: Oct 02 04:08:20 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR092718WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Oct 02 02:56:09 2018
Response via : Initial Calibration

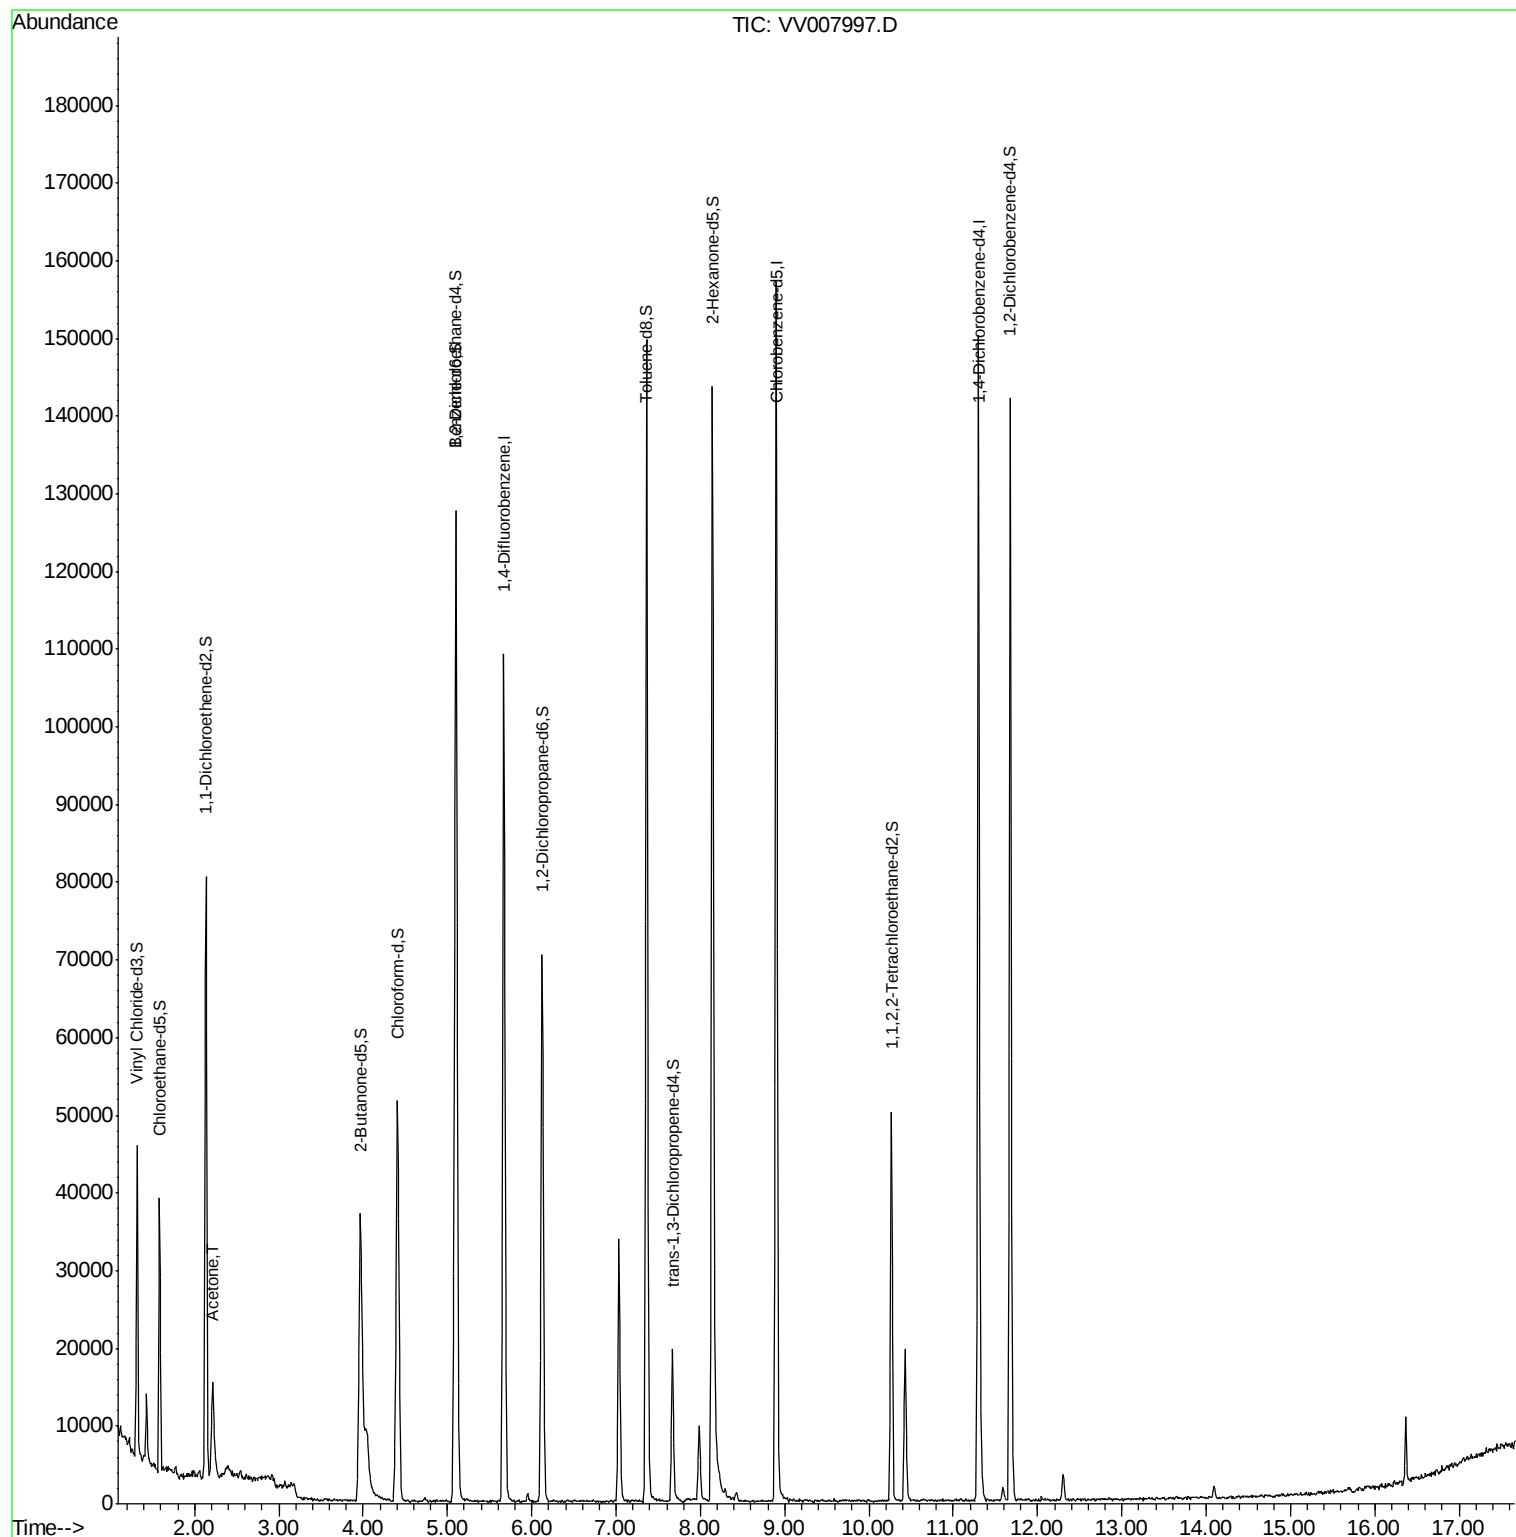

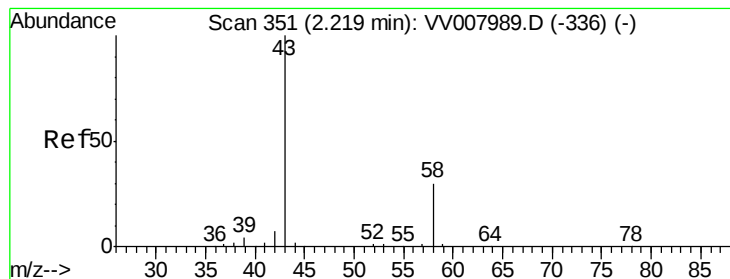

#13
 Acetone
 Concen: 16.187 ug/L
 RT: 2.22 min Scan# 350
 Delta R.T. -0.00 min
 Lab File: VV007997.D
 Acq: 01 Oct 2018 16:17

Instrument :
 MSVOA_V
 ClientSampleId :
 E62S9RE

Tot Ion: 43 Resp: 17381
 Ion Ratio Lower Upper
 43 100
 58 31.6 0.0 62.0

