

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100118\
 Data File : VV008006.D
 Acq On : 01 Oct 2018 20:31
 Operator : SY/MD
 Sample : J5159-10
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GAC96

Quant Time: Oct 02 04:58:49 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR092718WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Oct 02 04:17:24 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	90826	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	85824	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	41668	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	23792	4.89	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	97.80%
7) Chloroethane-d5	1.59	69	20514	4.88	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	97.60%
11) 1,1-Dichloroethene-d2	2.13	63	38036	3.46	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	69.20%
20) 2-Butanone-d5	3.97	46	65514	44.73	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	89.46%
24) Chloroform-d	4.41	84	52618	4.74	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.80%
26) 1,2-Dichloroethane-d4	5.09	65	28316	4.64	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.80%
32) Benzene-d6	5.10	84	102442	5.00	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.00%
36) 1,2-Dichloropropane-d6	6.12	67	31974	4.92	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	98.40%
41) Toluene-d8	7.36	98	95563	4.58	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.60%
43) trans-1,3-Dichloropropene-	7.67	79	10587	4.23	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	84.60%
46) 2-Hexanone-d5	8.14	63	47735	43.24	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	86.48%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	22618	4.51	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	90.20%
64) 1,2-Dichlorobenzene-d4	11.68	152	39364	4.88	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	97.60%


Target Compounds					Ovalue
31) Carbon tetrachloride	4.88	117	10896	1.198 ug/L	99
47) Tetrachloroethene	8.02	164	14998	2.300 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV100118\
Data File : VV008006.D
Acq On : 01 Oct 2018 20:31
Operator : SY/MD
Sample : J5159-10
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GAC96

Quant Time: Oct 02 04:58:49 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR092718WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Oct 02 04:17:24 2018
Response via : Initial Calibration

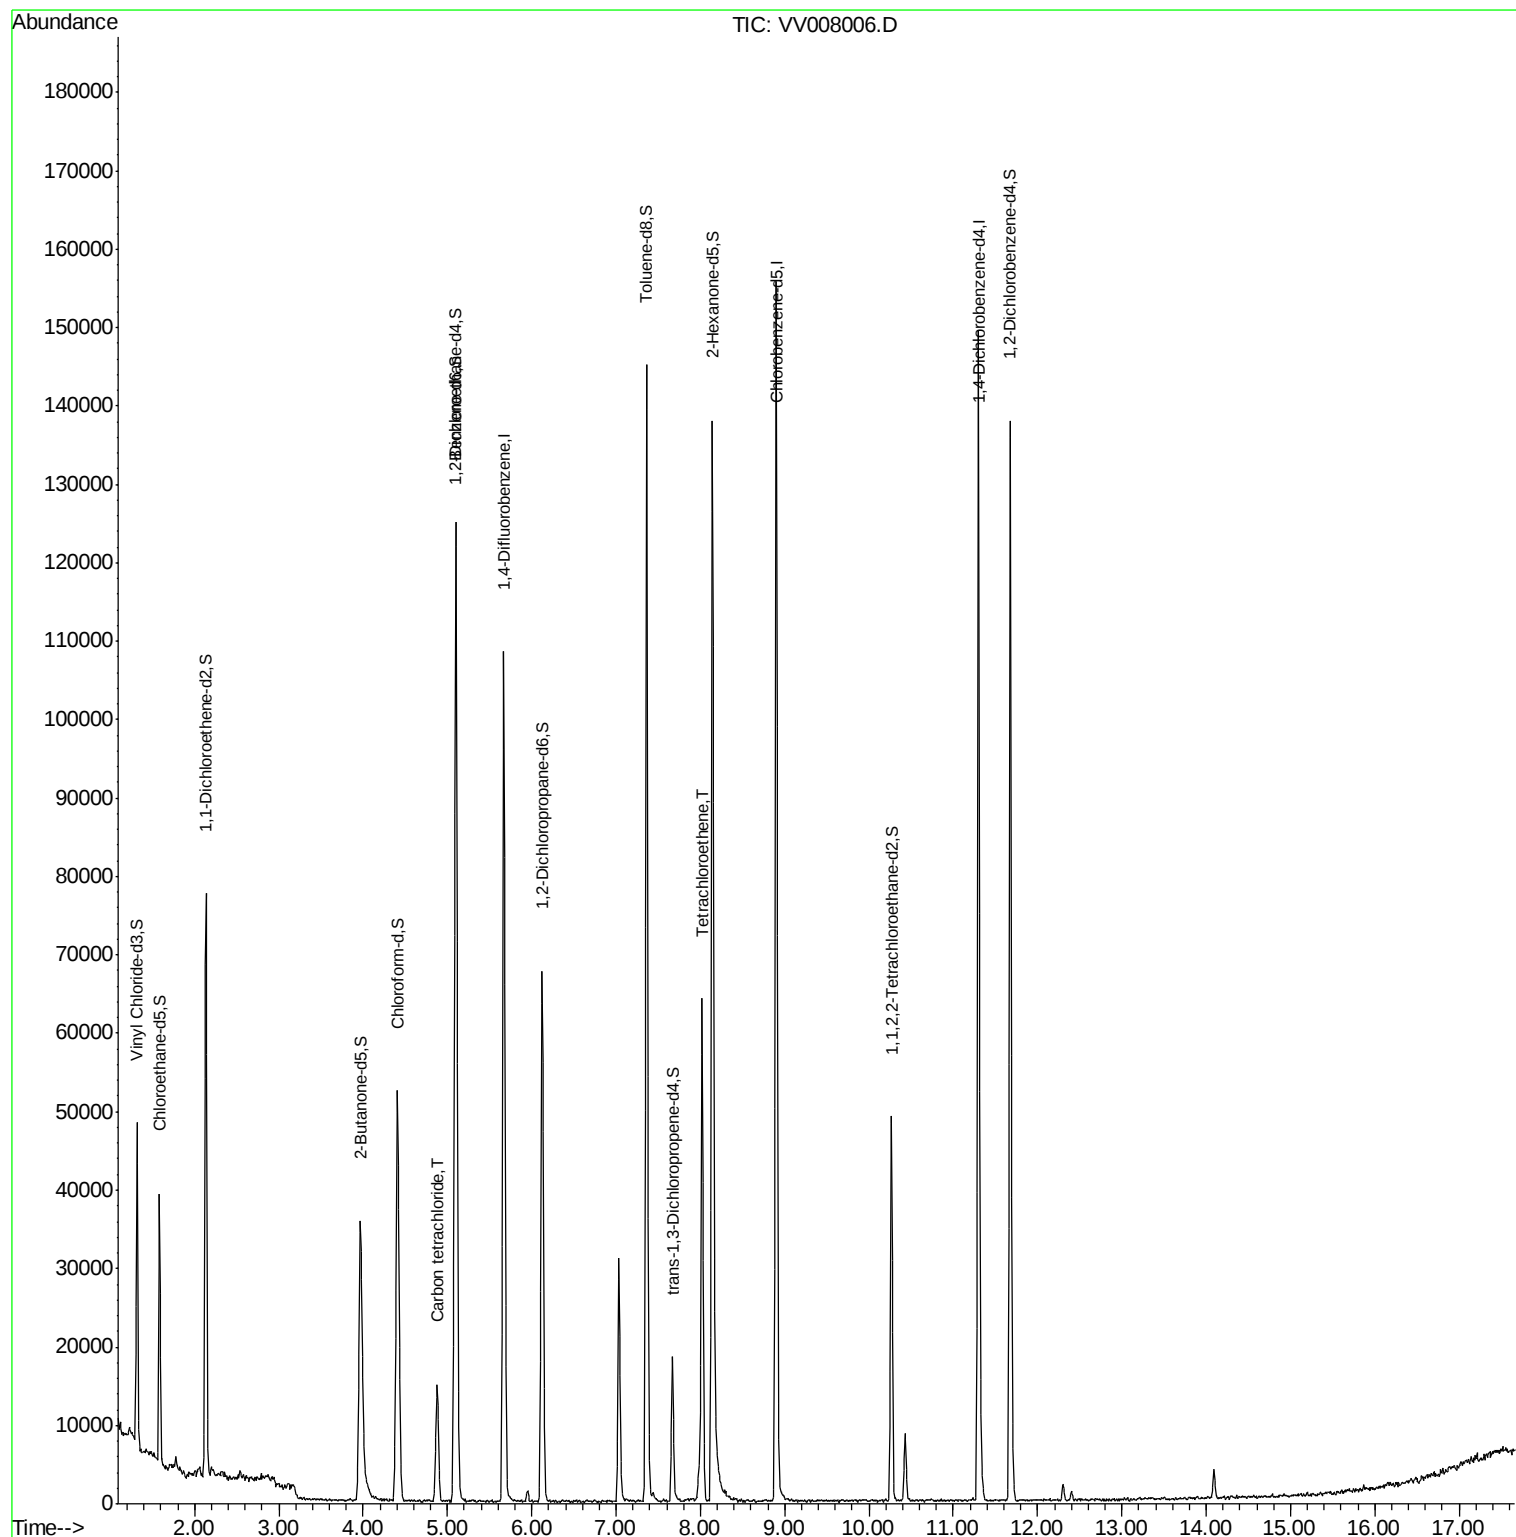


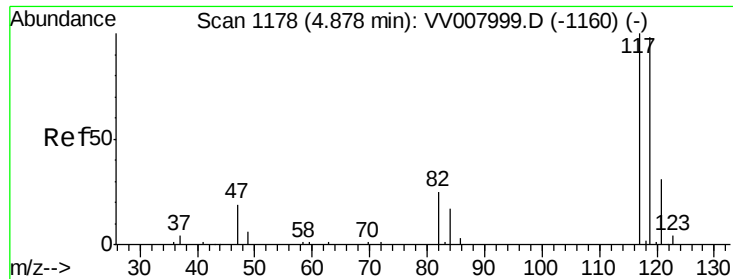




#31
Carbon tetrachloride
Concen: 1.198 ug/L
RT: 4.88 min Scan# 1178
Delta R.T. 0.00 min
Lab File: VV008006.D
Acq: 01 Oct 2018 20:31

Instrument :
MSVOA_V
ClientSampled :
GAC96

Tot Ion:117 Resp: 10896
Ion Ratio Lower Upper
117 100
119 98.0 77.8 116.8

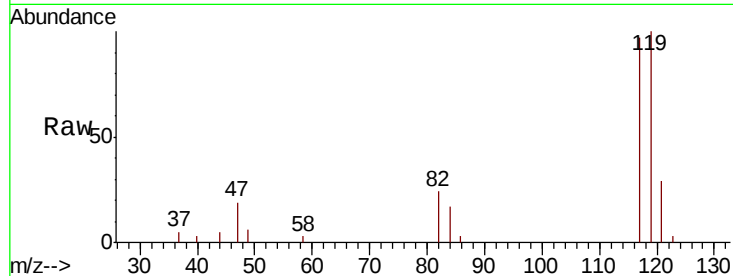


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 118.90 (118.60 to 119.60): V

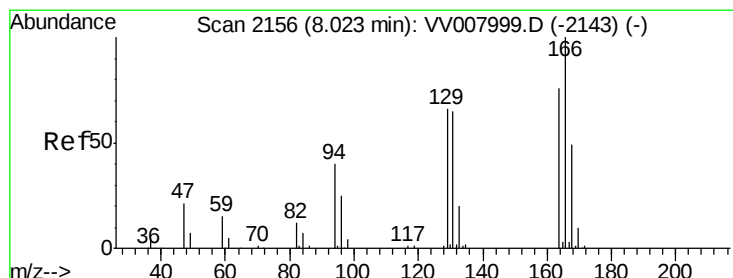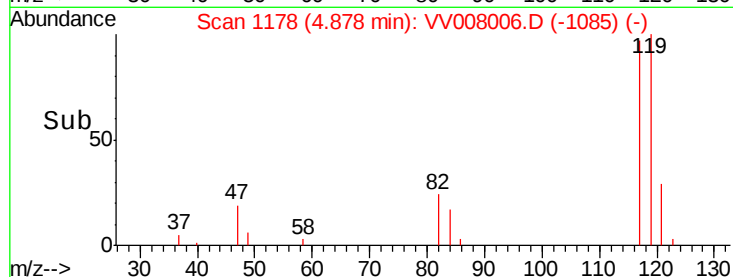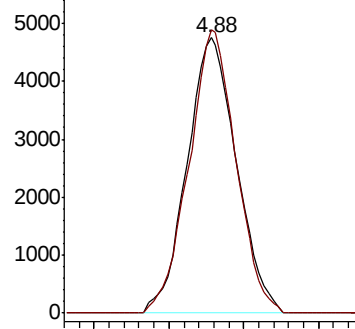

#47
Tetrachloroethene
Concen: 2.300 ug/L
RT: 8.02 min Scan# 2155
Delta R.T. -0.00 min
Lab File: VV008006.D
Acq: 01 Oct 2018 20:31

Tgt Ion:164 Resp: 14998
Ion Ratio Lower Upper
164 100
129 84.1 59.2 110.0
131 80.8 57.1 106.1
166 122.2 88.6 164.6

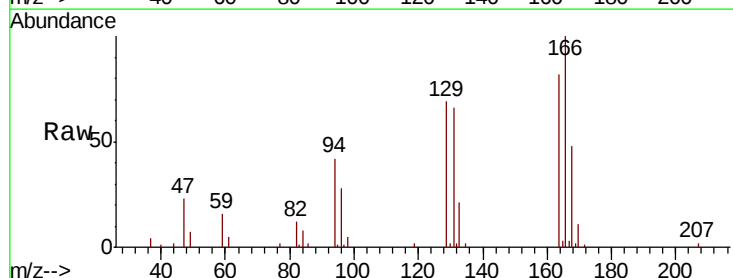

Abundance Ion 163.90 (163.60 to 164.60): V
Ion 128.95 (128.65 to 129.65): V
Ion 130.95 (130.65 to 131.65): V
Ion 165.90 (165.60 to 166.60): V

